

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
 Data File : PD069128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 10:56
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 23:58:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 15 23:58:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	100.3E6	804.8E6	81.049	73.655
28)	SA Decachlor...	8.201	9.365	91965631	481.1E6	73.158	72.100
Target Compounds							
23)	Chlordane-1	4.314	5.193	31531184	333.2E6	765.845	754.044
24)	Chlordane-2	4.815	5.666	36763419	316.5E6	766.239	753.634
25)	Chlordane-3	5.382	6.321	105.8E6	1163.3E6	768.931	755.944
26)	Chlordane-4	5.441	6.399	87431881	1344.4E6	766.069	750.781
27)	Chlordane-5	6.279	7.210	36139704	260.8E6	760.567	755.854



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
Data File : PD069128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 10:56
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 23:58:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Fri Apr 15 23:58:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

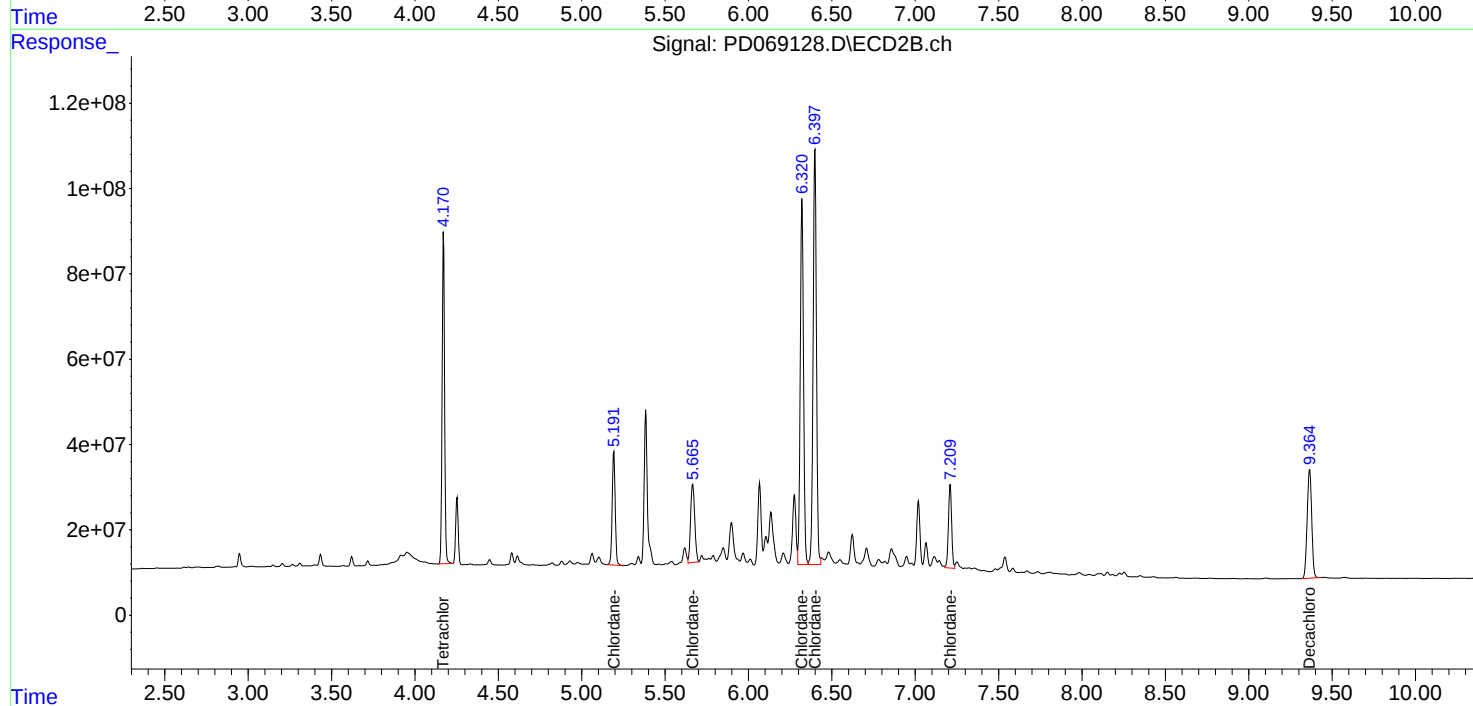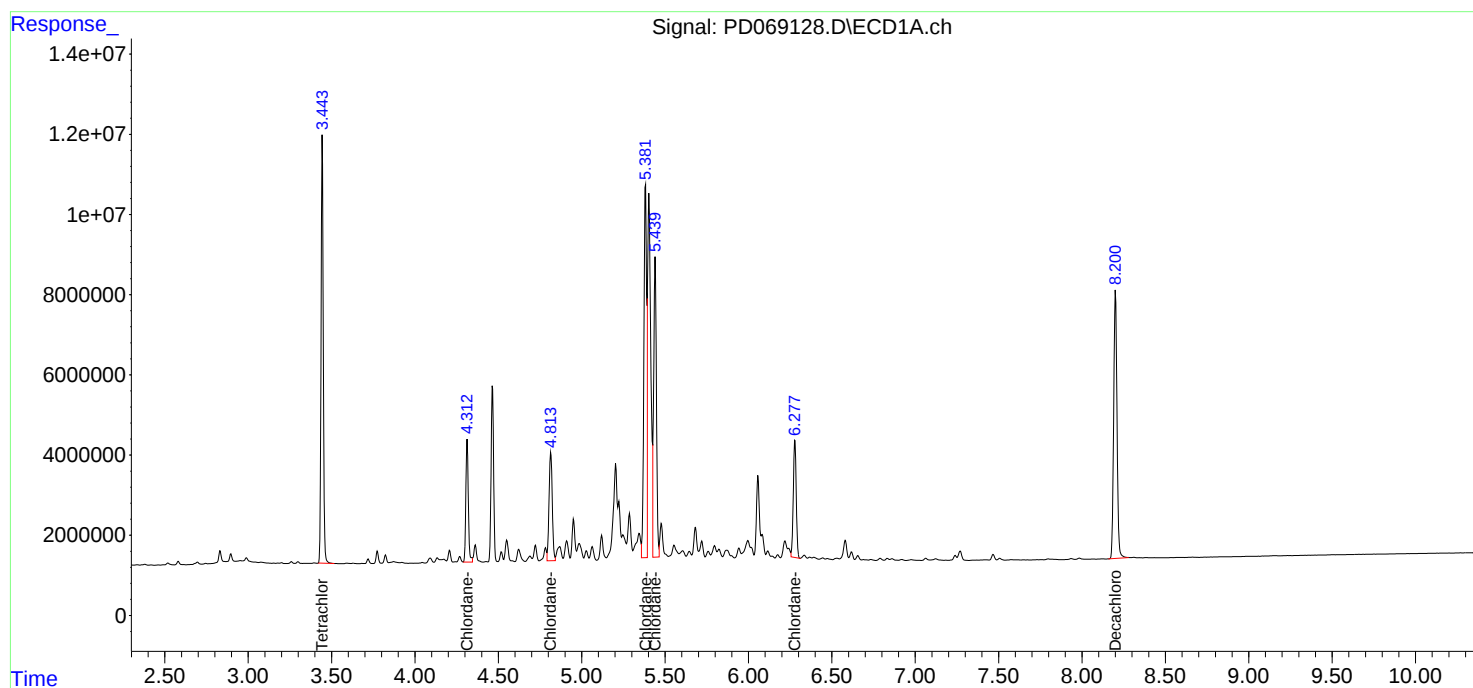


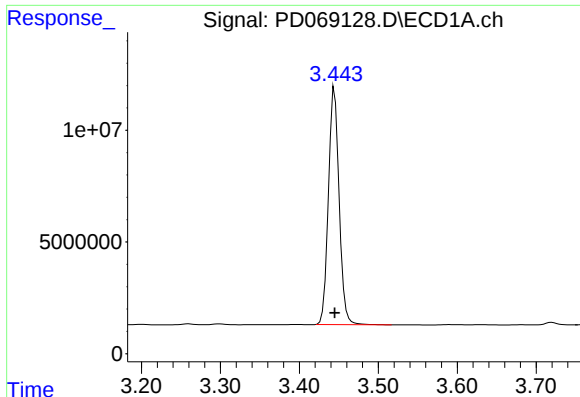

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 100253998
Conc: 81.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

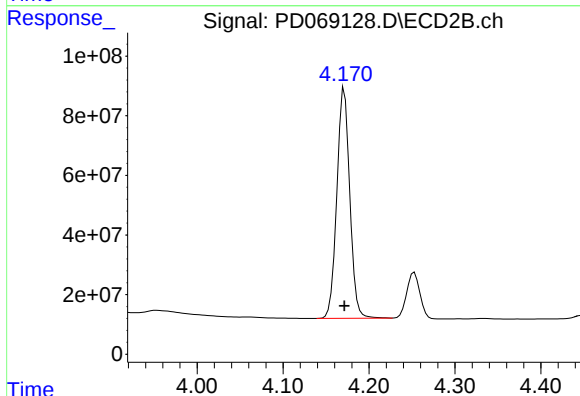


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 804757447
Conc: 73.66 ng/ml

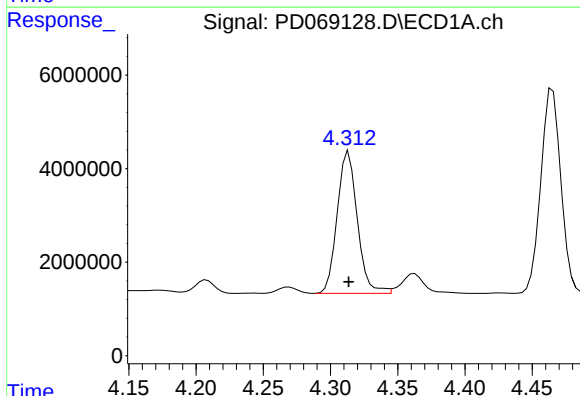


#23 Chlordane-1

R.T.: 4.314 min
Delta R.T.: 0.000 min
Response: 31531184
Conc: 765.85 ng/ml

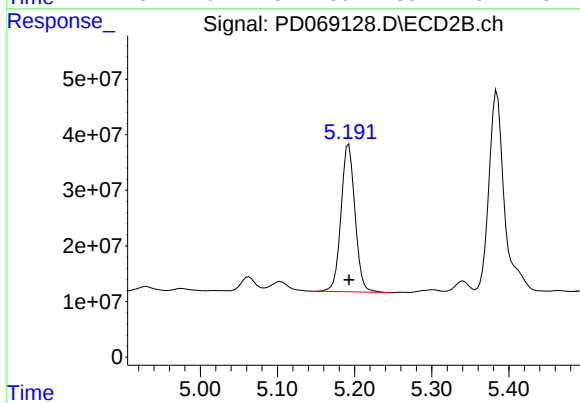

#23 Chlordane-1


R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 333220698
Conc: 754.04 ng/ml

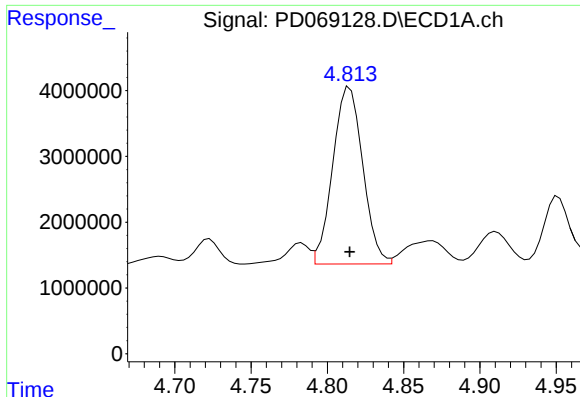

#24 Chlordane-2


R.T.: 4.815 min
Delta R.T.: 0.000 min
Response: 36763419
Conc: 766.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

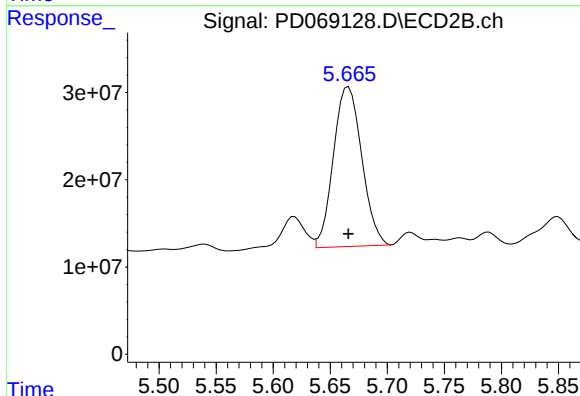


#24 Chlordane-2

R.T.: 5.666 min
Delta R.T.: 0.000 min
Response: 316549760
Conc: 753.63 ng/ml

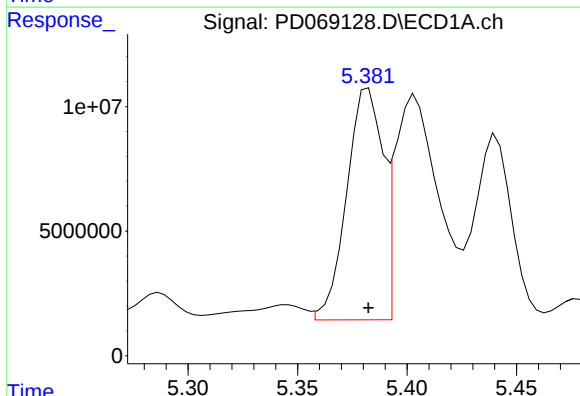


#25 Chlordane-3

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 105778186
Conc: 768.93 ng/ml

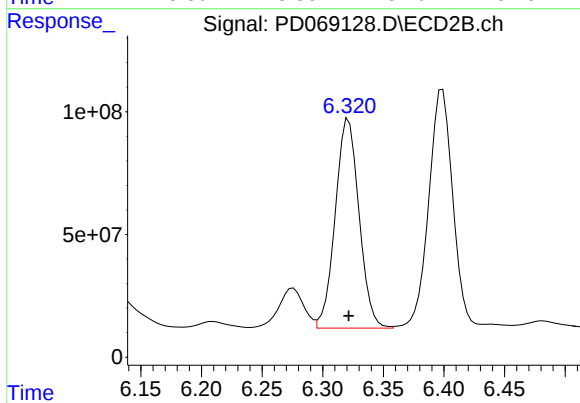

#25 Chlordane-3


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 1163323374
Conc: 755.94 ng/ml

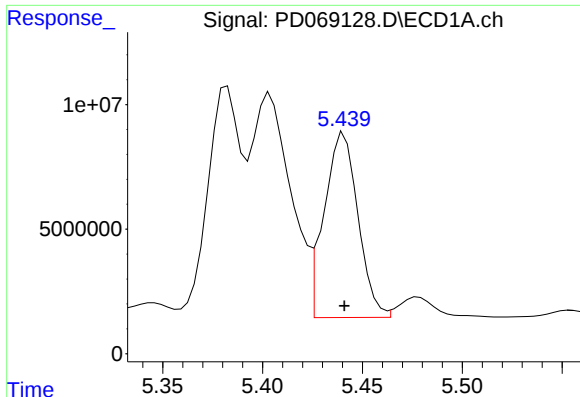

#26 Chlordane-4


R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 87431881
Conc: 766.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

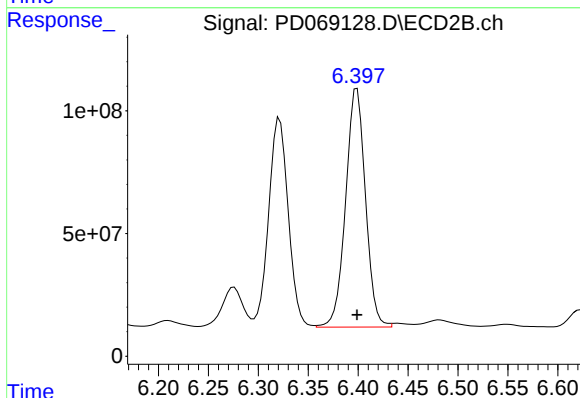


#26 Chlordane-4

R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 1344412494
Conc: 750.78 ng/ml

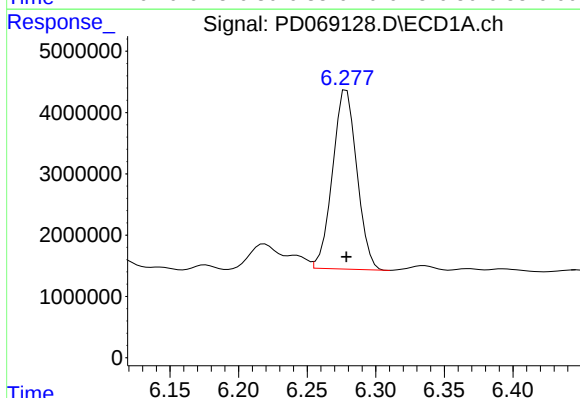


#27 Chlordane-5

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 36139704
Conc: 760.57 ng/ml

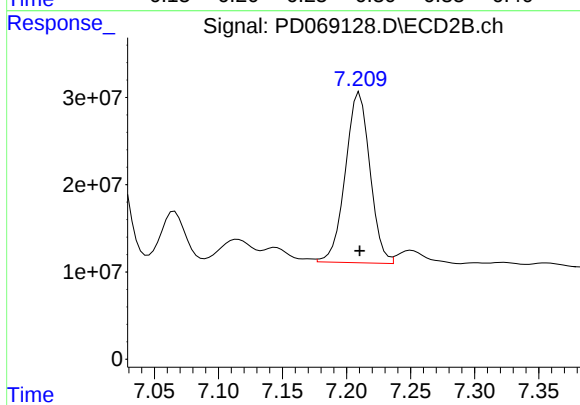

#27 Chlordane-5


R.T.: 7.210 min
Delta R.T.: 0.000 min
Response: 260774207
Conc: 755.85 ng/ml

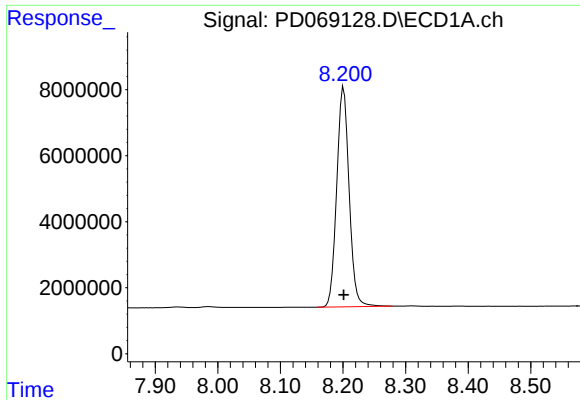

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 91965631
Conc: 73.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

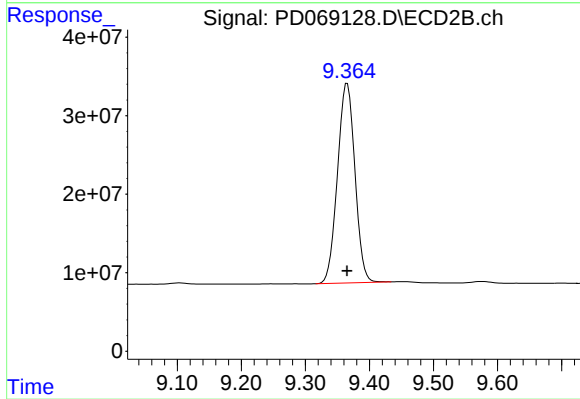

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.000 min
Response: 481104750
Conc: 72.10 ng/ml