

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
 Data File : PD069131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 11:38
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 15:38:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 15 15:37:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	6295470	62964471	4.913	5.813
28)	SA Decachlor...	8.199	9.365	7175614	39512934	6.071	5.996
Target Compounds							
23)	Chlordane-1	4.313	5.193	2115663	27842687	53.009	61.627
24)	Chlordane-2	4.814	5.666	2696317	26643767	56.588	61.263
25)	Chlordane-3	5.381	6.321	6733579	90265314	51.273	58.199
26)	Chlordane-4	5.440	6.399	5812085	107.3E6	53.099	58.775
27)	Chlordane-5	6.277	7.210	2120032	20031054	46.329	56.921



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
Data File : PD069131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 11:38
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 15:38:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Fri Apr 15 15:37:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

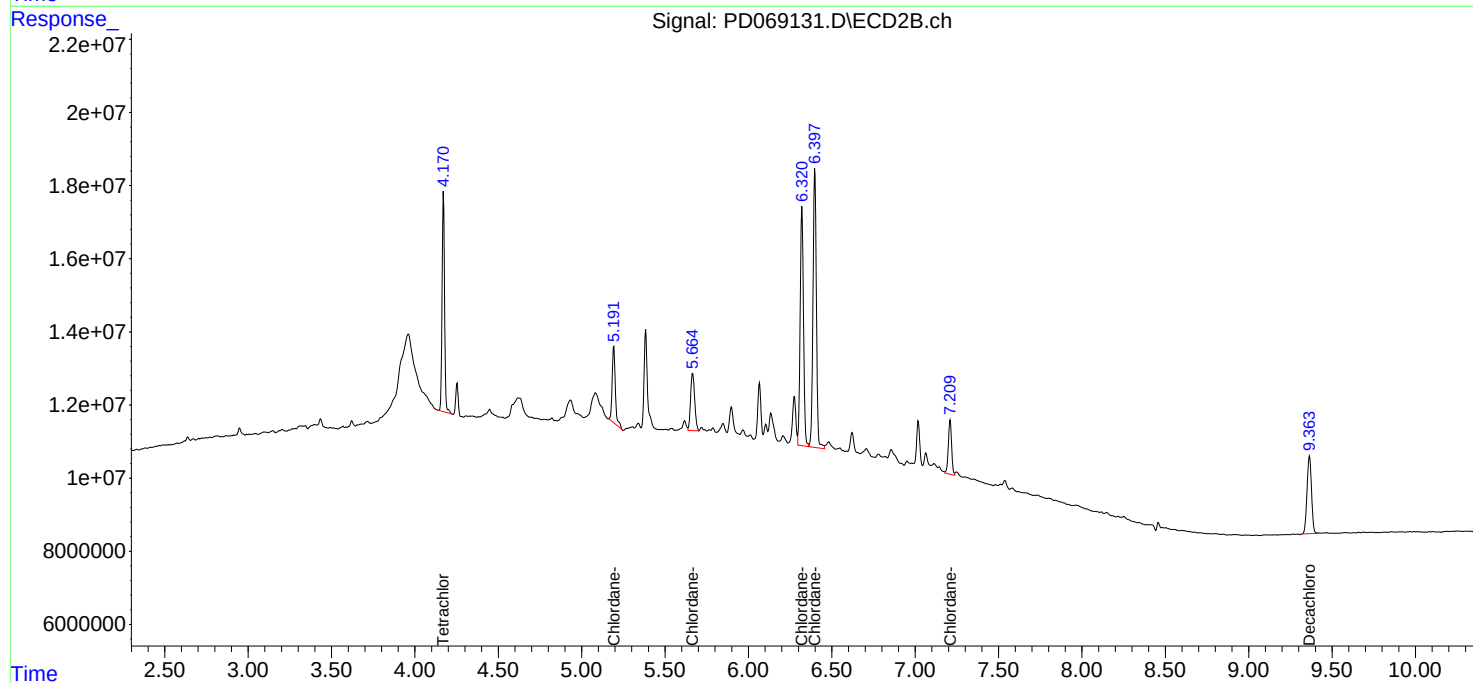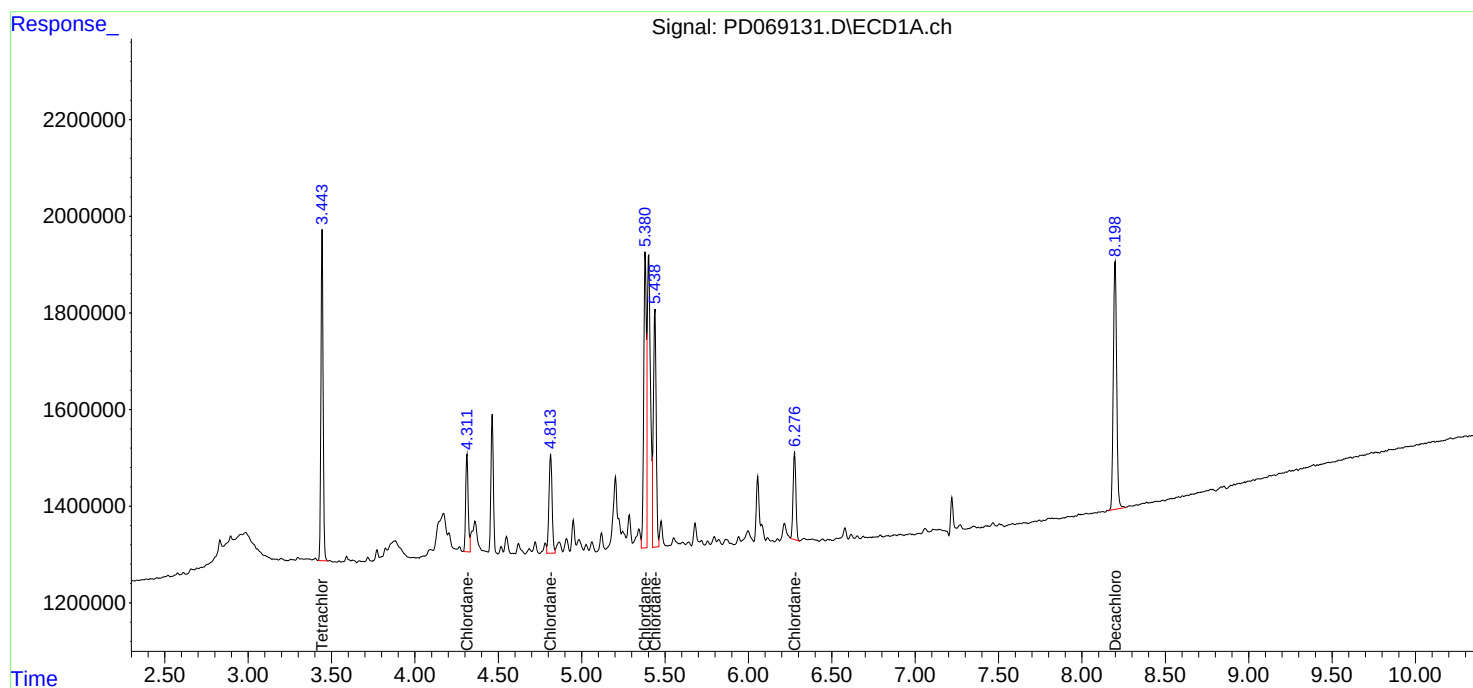


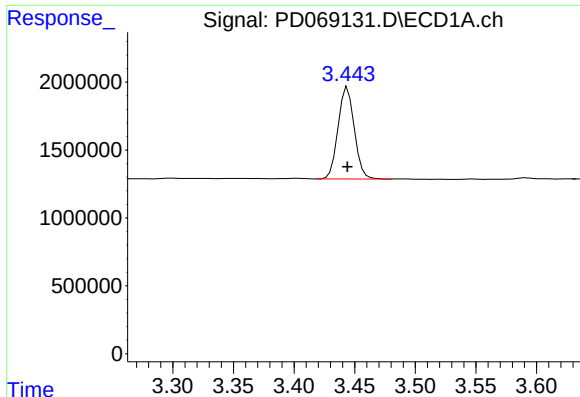

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 6295470
Conc: 4.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

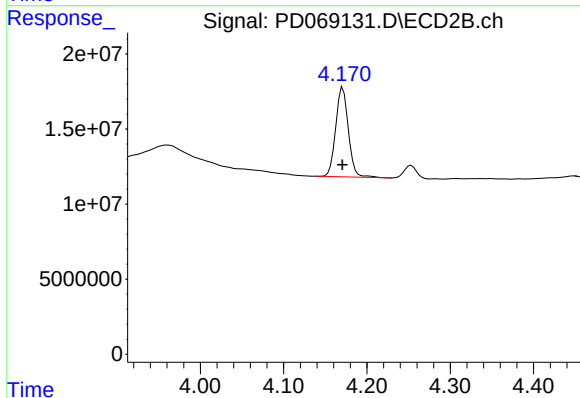


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 62964471
Conc: 5.81 ng/ml

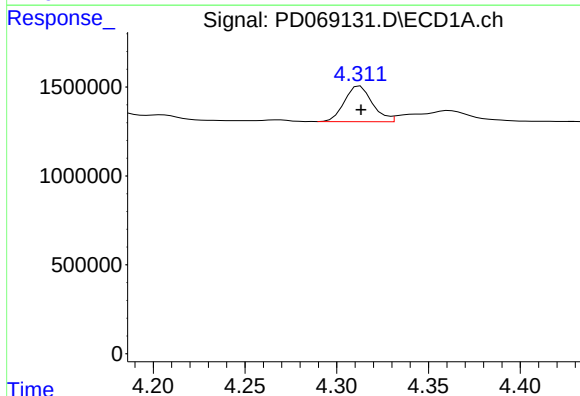


#23 Chlordane-1

R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 2115663
Conc: 53.01 ng/ml

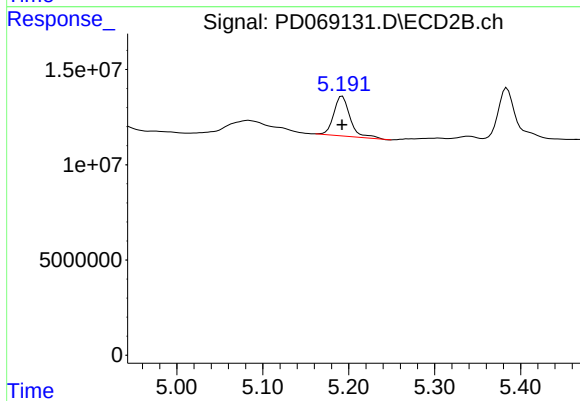

#23 Chlordane-1


R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 27842687
Conc: 61.63 ng/ml

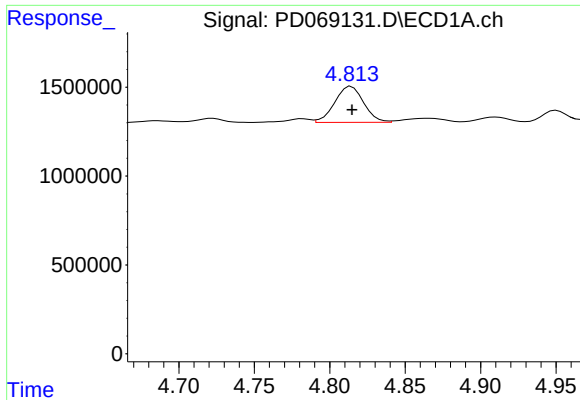

#24 Chlordane-2


R.T.: 4.814 min
Delta R.T.: 0.000 min
Response: 2696317
Conc: 56.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

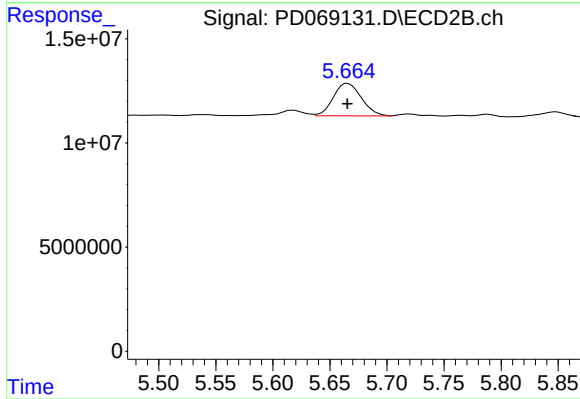


#24 Chlordane-2

R.T.: 5.666 min
Delta R.T.: 0.000 min
Response: 26643767
Conc: 61.26 ng/ml

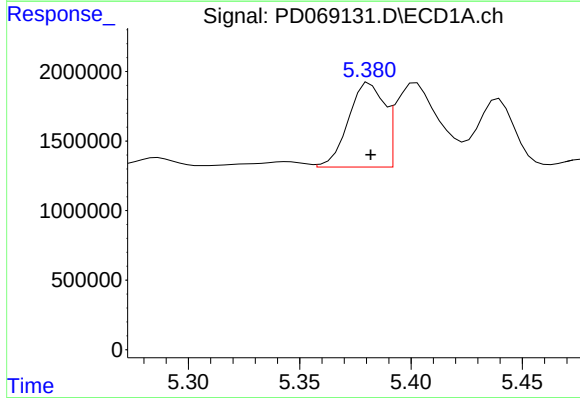


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 6733579
Conc: 51.27 ng/ml

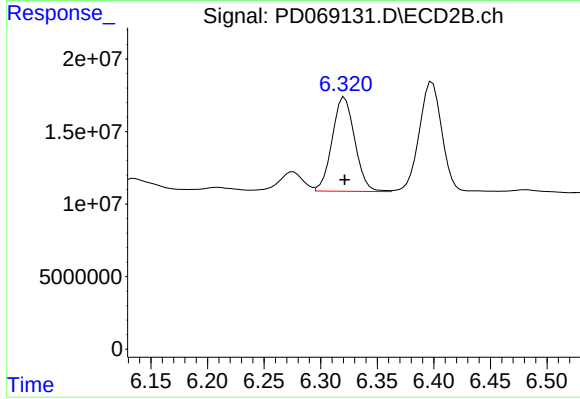

#25 Chlordane-3


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 90265314
Conc: 58.20 ng/ml

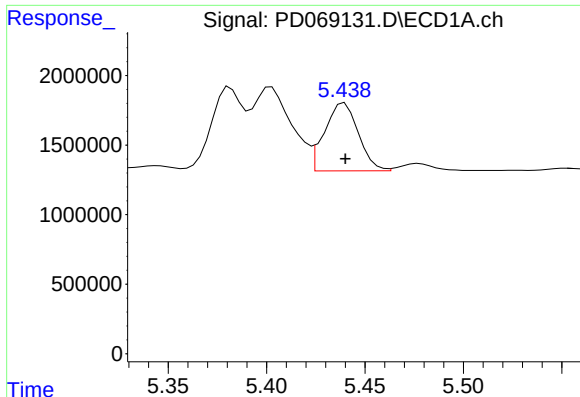

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 5812085
Conc: 53.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

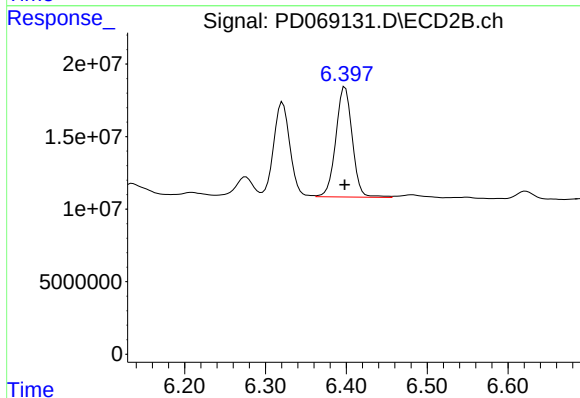


#26 Chlordane-4

R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 107318469
Conc: 58.77 ng/ml

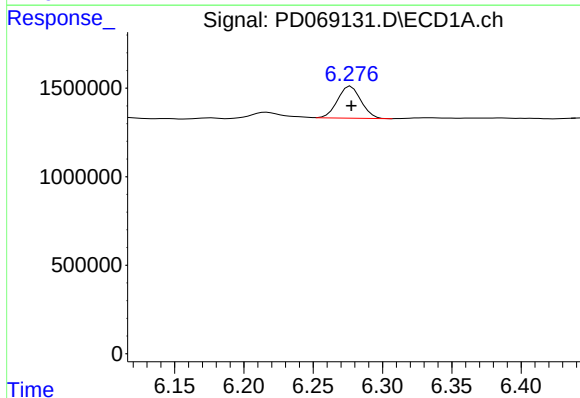


#27 Chlordane-5

R.T.: 6.277 min
Delta R.T.: 0.000 min
Response: 2120032
Conc: 46.33 ng/ml

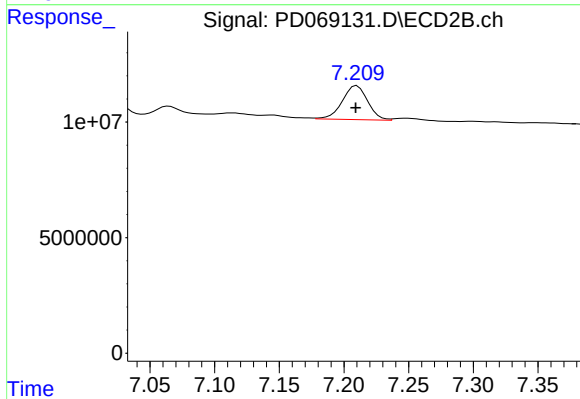

#27 Chlordane-5


R.T.: 7.210 min
Delta R.T.: 0.000 min
Response: 20031054
Conc: 56.92 ng/ml

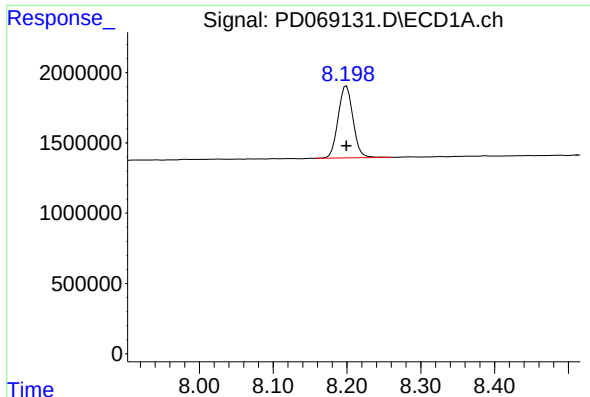

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 7175614
Conc: 6.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

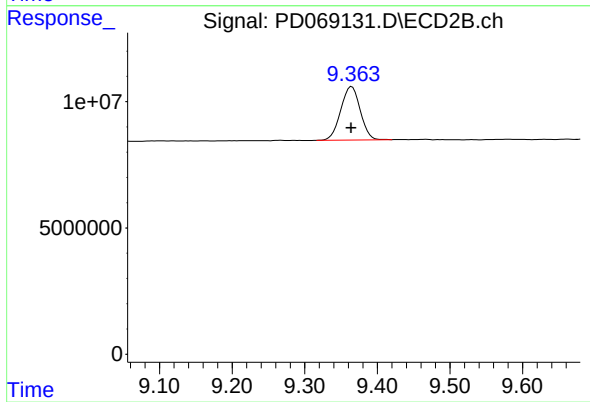

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.000 min
Response: 39512934
Conc: 6.00 ng/ml