

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
 Data File : PD069138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 13:15
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD041622

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 16:20:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 15 16:15:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	65529575	539.8E6	59.031	50.351
28)	SA Decachlor...	8.200	9.365	63406380	331.2E6	50.780	50.614
Target Compounds							
23)	Chlordane-1	4.313	5.192	21026053	226.7E6	526.816	501.820
24)	Chlordane-2	4.815	5.666	25165034	218.4E6	528.138	502.226
25)	Chlordane-3	5.382	6.321	68454501	778.3E6	521.249	501.819
26)	Chlordane-4	5.440	6.399	57585716	904.4E6	526.099	495.287
27)	Chlordane-5	6.278	7.210	23997209	176.2E6	524.409	500.823



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
Data File : PD069138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 13:15
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD041622

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 16:20:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Fri Apr 15 16:15:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

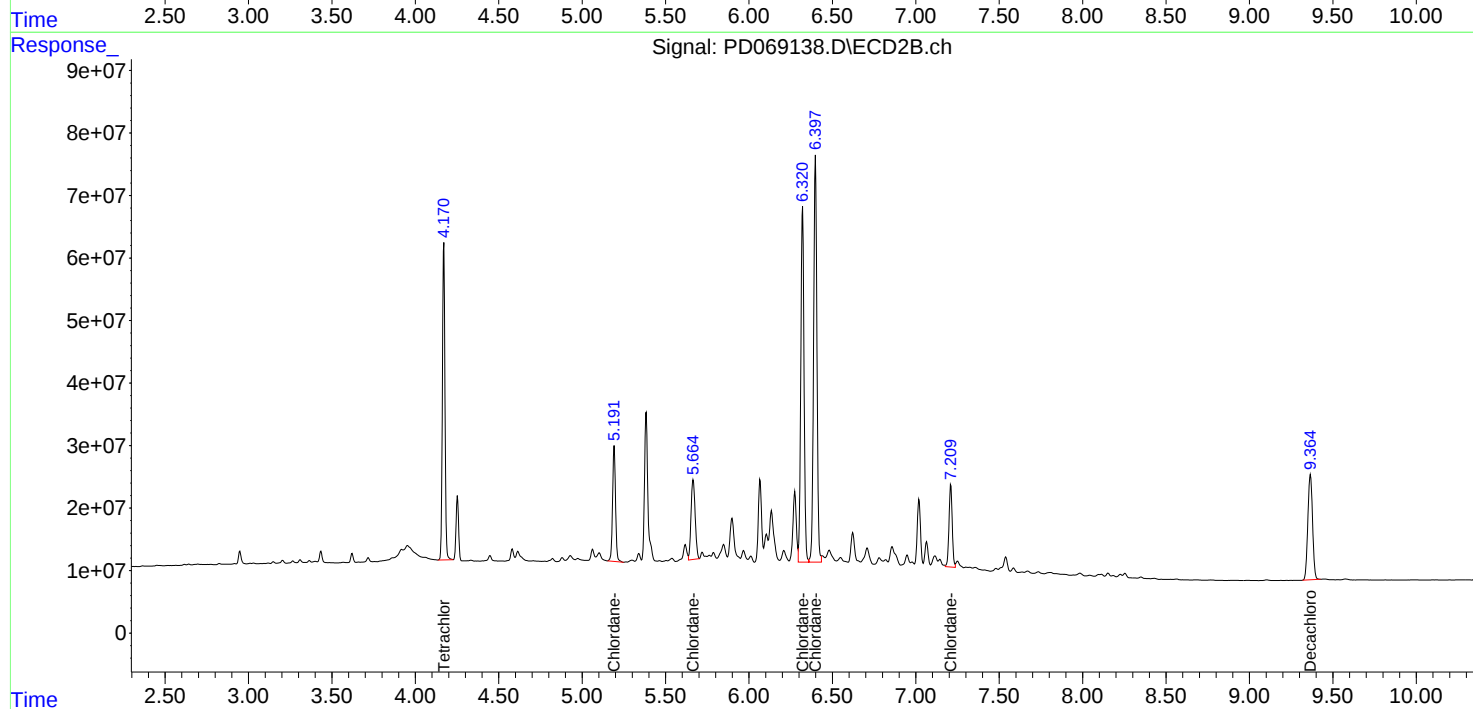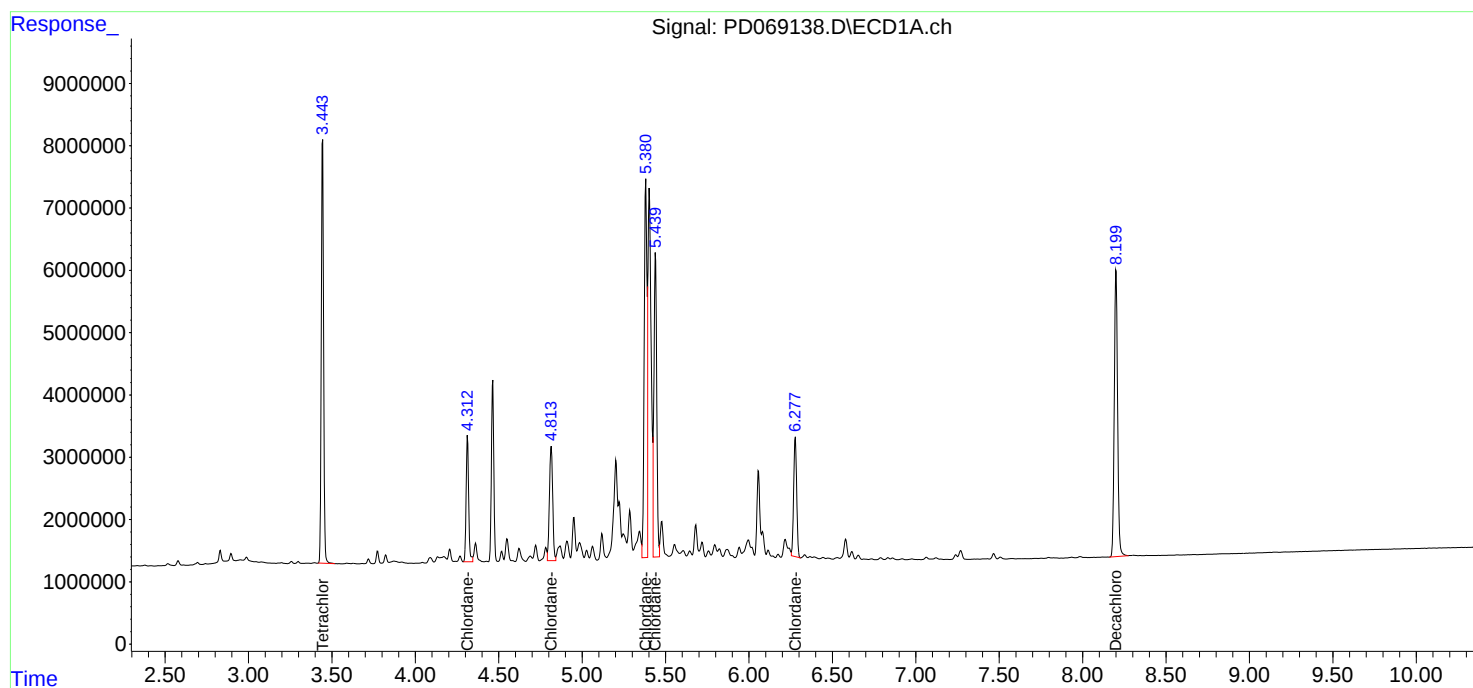


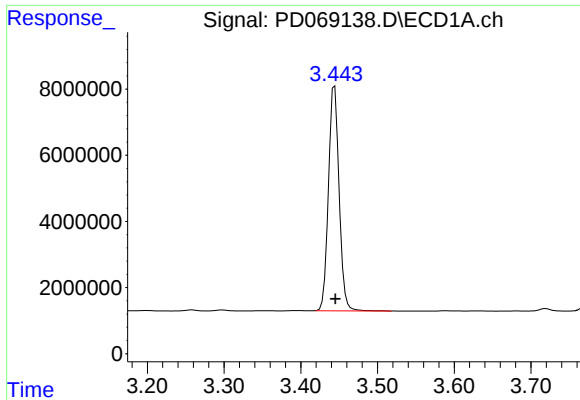

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 65529575
Conc: 59.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD041622

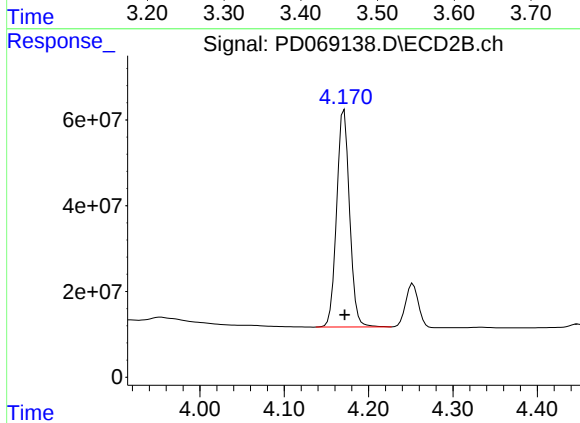


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 539846699
Conc: 50.35 ng/ml

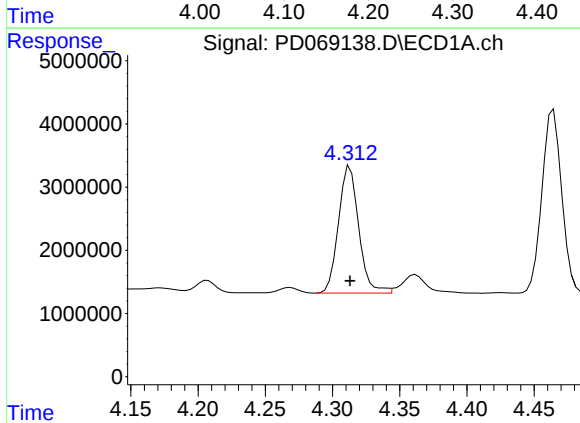


#23 Chlordane-1

R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 21026053
Conc: 526.82 ng/ml

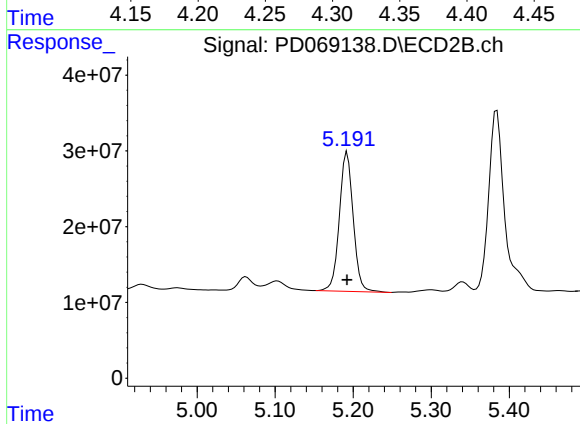

#23 Chlordane-1


R.T.: 5.192 min
Delta R.T.: 0.000 min
Response: 226717615
Conc: 501.82 ng/ml

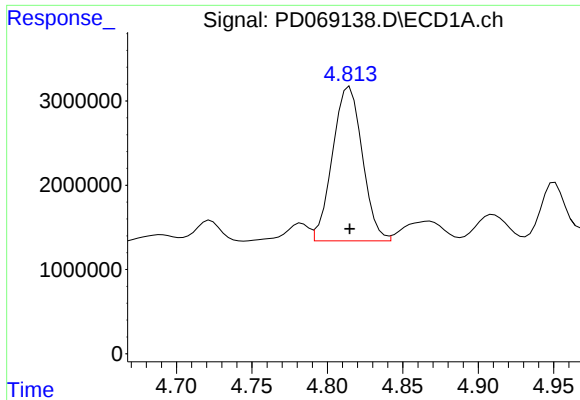

#24 Chlordane-2


R.T.: 4.815 min
Delta R.T.: 0.000 min
Response: 25165034
Conc: 528.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD041622

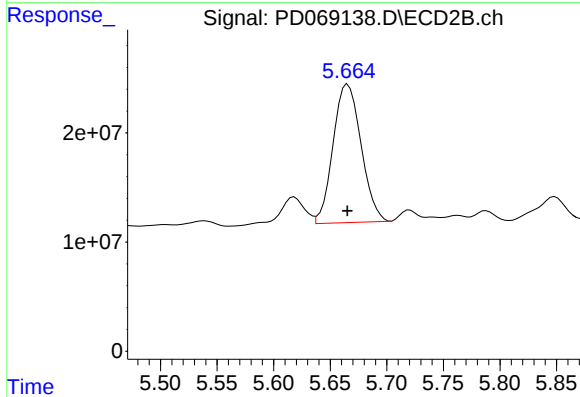


#24 Chlordane-2

R.T.: 5.666 min
Delta R.T.: 0.000 min
Response: 218423616
Conc: 502.23 ng/ml

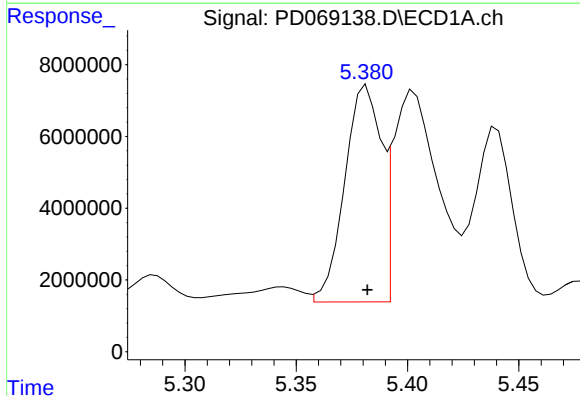


#25 Chlordane-3

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 68454501
Conc: 521.25 ng/ml

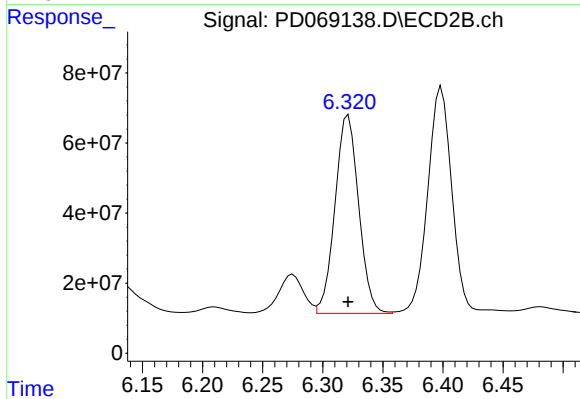

#25 Chlordane-3


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 778304637
Conc: 501.82 ng/ml

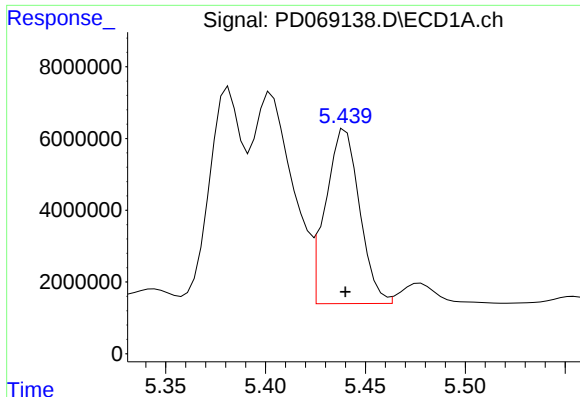

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 57585716
Conc: 526.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD041622

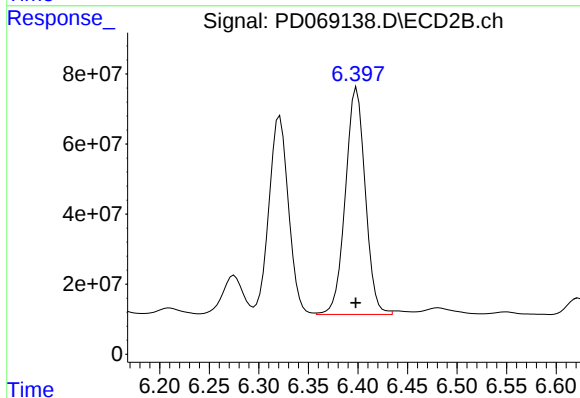


#26 Chlordane-4

R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 904359517
Conc: 495.29 ng/ml

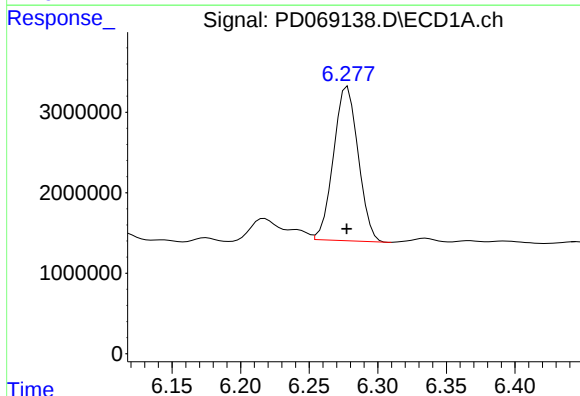


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 23997209
Conc: 524.41 ng/ml

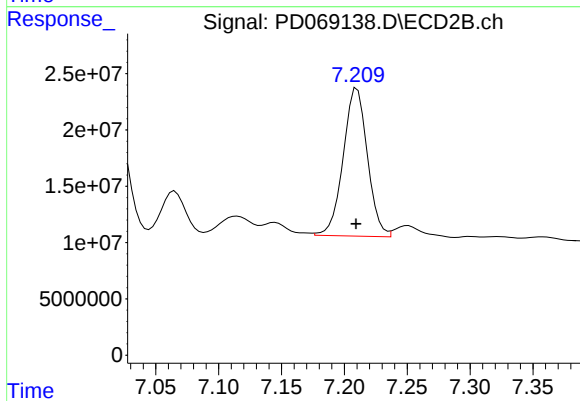

#27 Chlordane-5

R.T.: 7.210 min
Delta R.T.: 0.001 min
Response: 176243863
Conc: 500.82 ng/ml

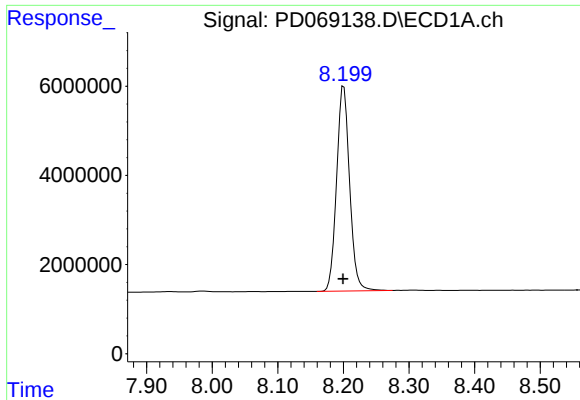

#28 Decachlorobiphenyl


R.T.: 8.200 min

Delta R.T.: 0.001 min

Response: 63406380

Conc: 50.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD041622

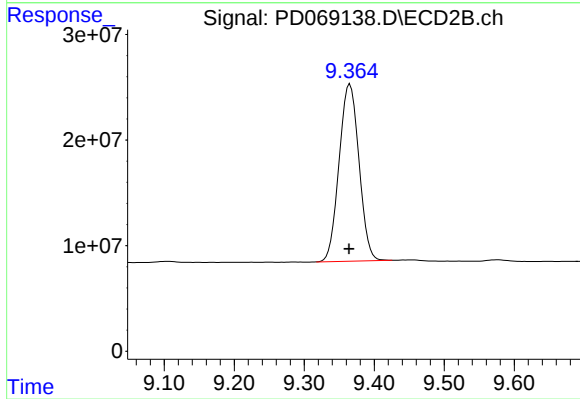

#28 Decachlorobiphenyl

R.T.: 9.365 min

Delta R.T.: 0.001 min

Response: 331217006

Conc: 50.61 ng/ml