

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041624\
 Data File : PD082463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2024 18:50
 Operator : AR\AJ
 Sample : P2060-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1D01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 21:32:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 02:08:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.776	25328799	58042892	16.703	16.835
27)	SA Decachlor...	9.119	7.910	31612565	51222240	16.166	15.742
Target Compounds							
3)	MA gamma-BHC...	0.000	3.601	0	444108	N.D.	<MDL
4)	MA Heptachlor	4.936	0.000	3535689	0	1.400	N.D. #
5)	MB Aldrin	0.000	4.247	0	14921771	N.D.	3.246
6)	B beta-BHC	0.000	3.860f	0	78150510	N.D.	37.591
7)	B delta-BHC	4.793	0.000	70123632	0	29.043	N.D. #
9)	A Endosulfan I	0.000	5.112	0	168712	N.D.	<MDL
10)	B trans-Chl...	5.963	0.000	1632763	0	0.795	N.D. #
11)	B cis-Chlor...	0.000	5.057	0	3074582	N.D.	0.744
14)	MA Endrin	0.000	5.654	0	215996	N.D.	<MDL
15)	B Endosulfa...	0.000	5.959	0	346890	N.D.	0.100
17)	MA 4,4'-DDT	0.000	6.071f	0	89272	N.D.	<MDL
18)	B Endrin al...	0.000	6.127	0	128105	N.D.	<MDL
19)	B Endosulfa...	0.000	6.339	0	130573	N.D.	<MDL
20)	A Methoxychlor	0.000	6.605	0	425239	N.D.	0.254
22)	Toxaphene-1	0.000	5.057f	0	3074582	N.D.	148.813
24)	Toxaphene-3	0.000	6.605	0	425239	N.D.	5.602
25)	Toxaphene-4	0.000	6.756	0	180086	N.D.	1.719
26)	Toxaphene-5	0.000	6.977f	0	2381127	N.D.	58.414


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041624\
Data File : PD082463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2024 18:50
Operator : AR\AJ
Sample : P2060-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 21:32:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 02:08:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

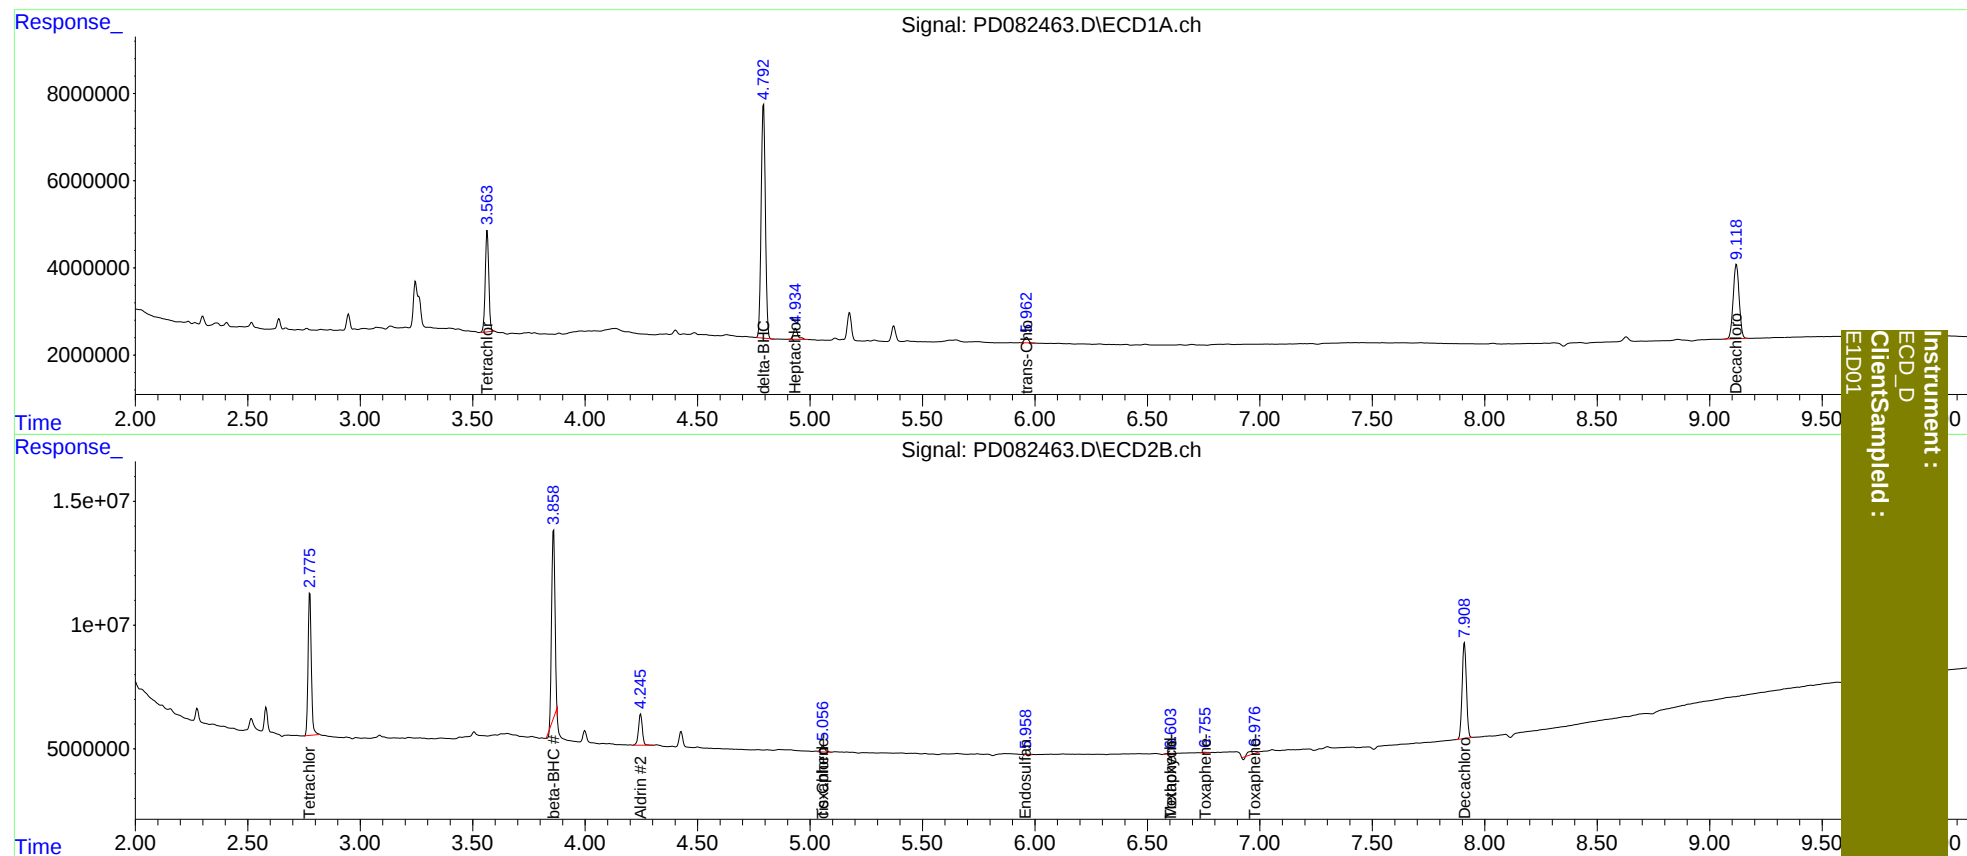


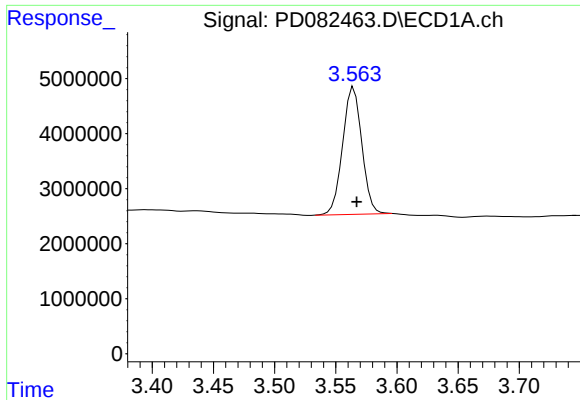

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: -0.002 min
Response: 25328799
Conc: 16.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
E1D01

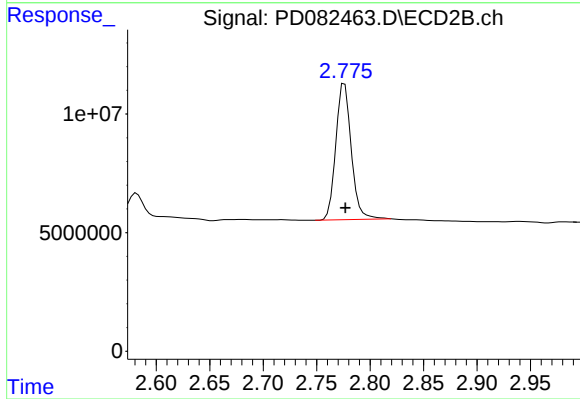


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 58042892
Conc: 16.84 ng/ml

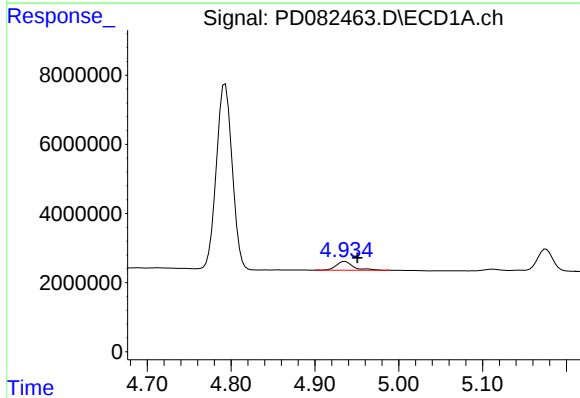


#4 Heptachlor

R.T.: 4.936 min
Delta R.T.: -0.015 min
Response: 3535689
Conc: 1.40 ng/ml

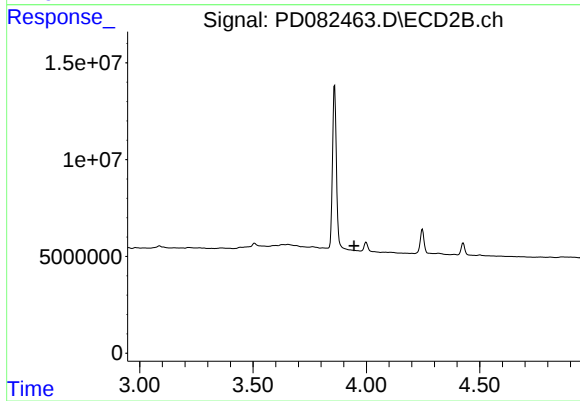

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.946 min
Response: 0
Conc: N.D.

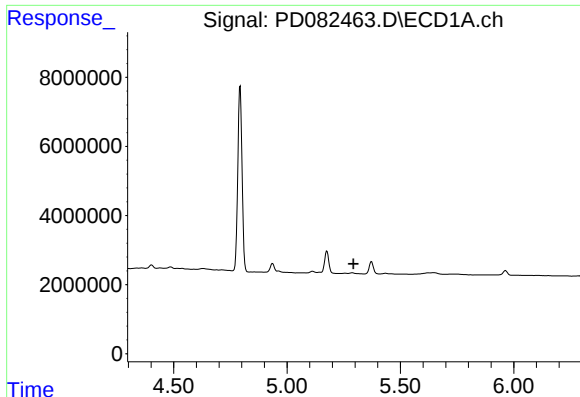

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E1D01

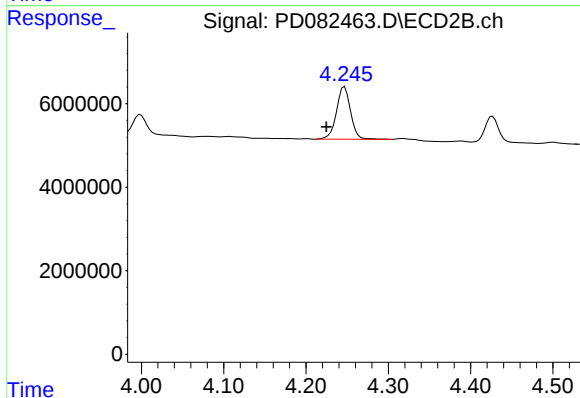


#5 Aldrin

R.T.: 4.247 min
Delta R.T.: 0.022 min
Response: 14921771
Conc: 3.25 ng/ml

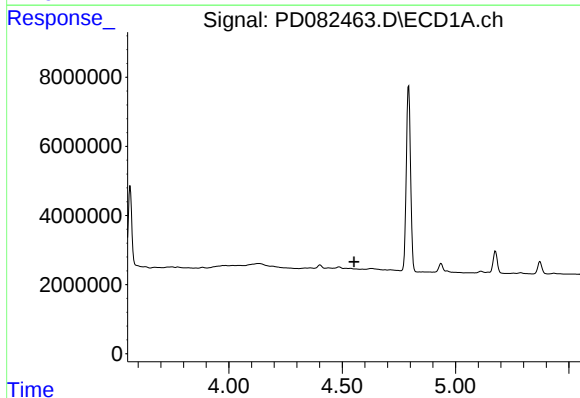


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.553 min
Response: 0
Conc: N.D.

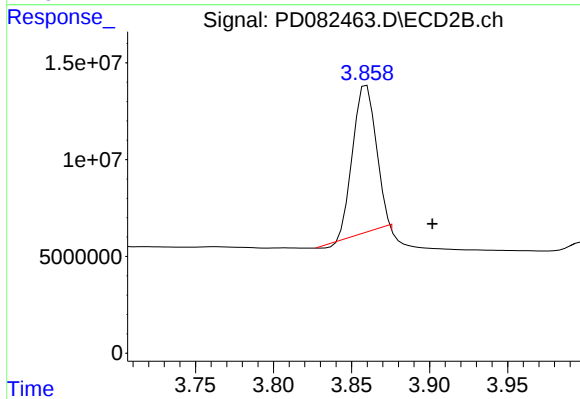

#6 beta-BHC


R.T.: 3.860 min
Delta R.T.: -0.042 min
Response: 78150510
Conc: 37.59 ng/ml

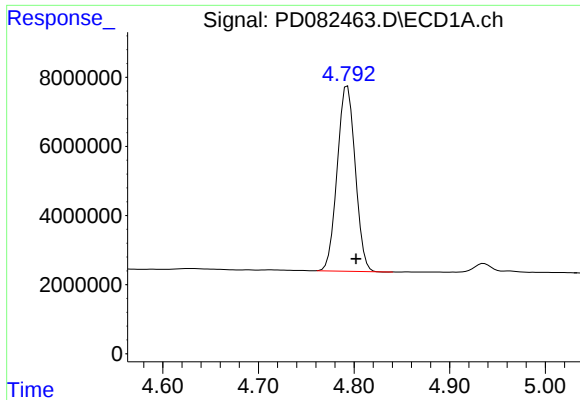

#7 delta-BHC


R.T.: 4.793 min
Delta R.T.: -0.009 min
Response: 70123632
Conc: 29.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
E1D01

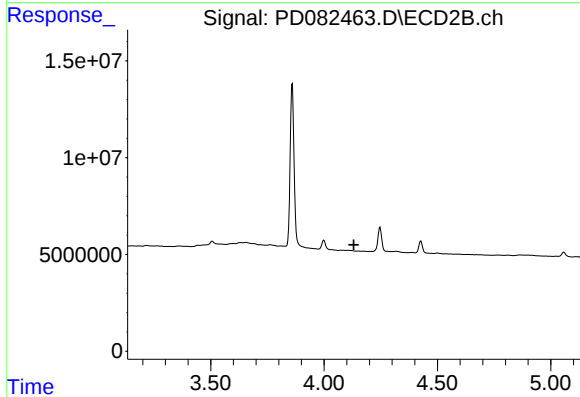


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.131 min
Response: 0
Conc: N.D.

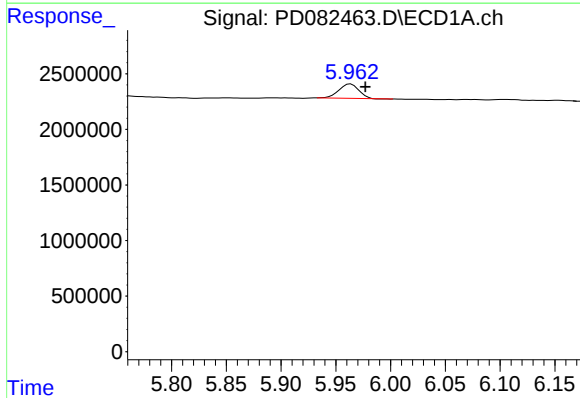


#10 trans-Chlordane

R.T.: 5.963 min
Delta R.T.: -0.013 min
Response: 1632763
Conc: 0.80 ng/ml

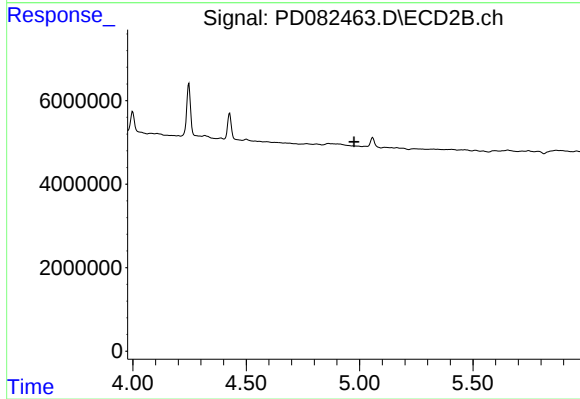

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.976 min
Response: 0
Conc: N.D.

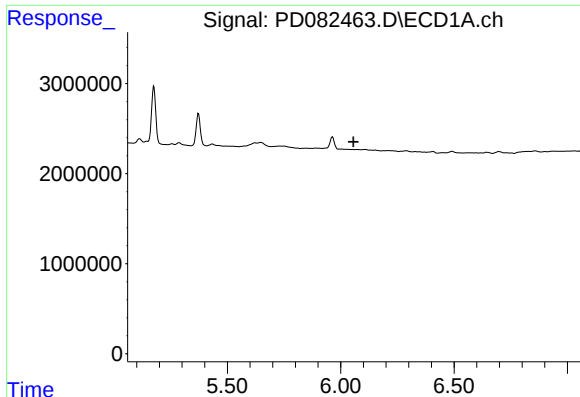

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E1D01

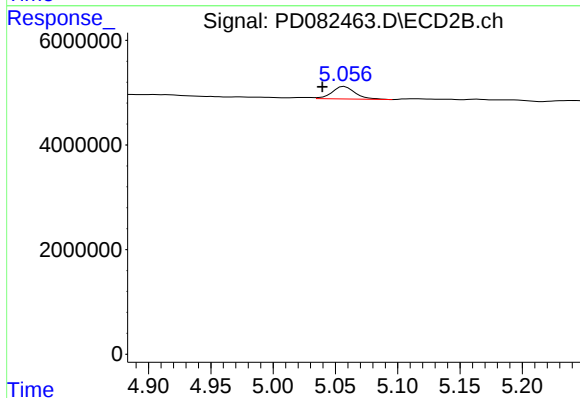


#11 cis-Chlordane

R.T.: 5.057 min
Delta R.T.: 0.018 min
Response: 3074582
Conc: 0.74 ng/ml

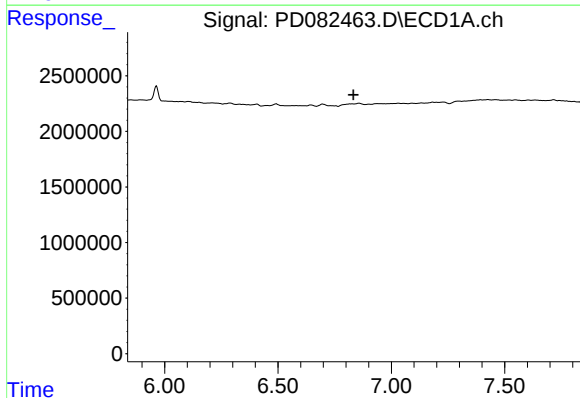


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.833 min
Response: 0
Conc: N.D.

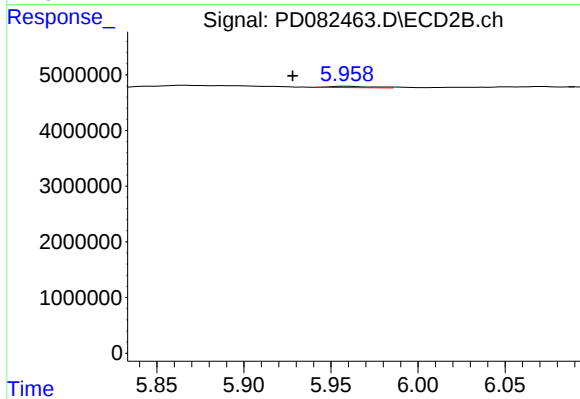

#15 Endosulfan II


R.T.: 5.959 min
Delta R.T.: 0.031 min
Response: 346890
Conc: 0.10 ng/ml

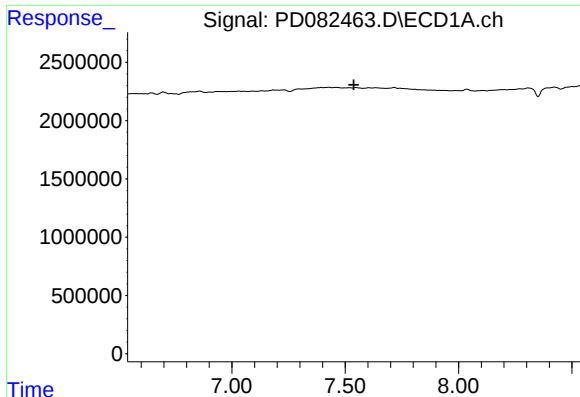

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.538 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E1D01

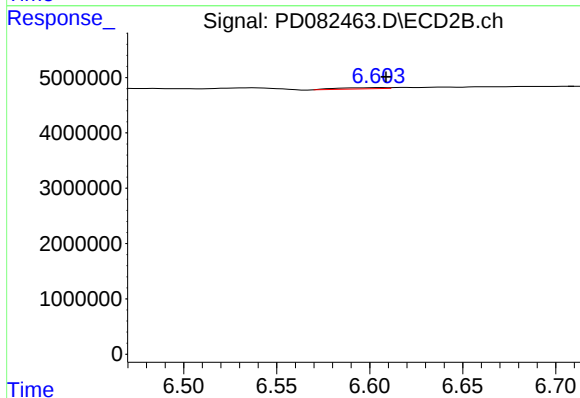


#20 Methoxychlor

R.T.: 6.605 min
Delta R.T.: -0.003 min
Response: 425239
Conc: 0.25 ng/ml

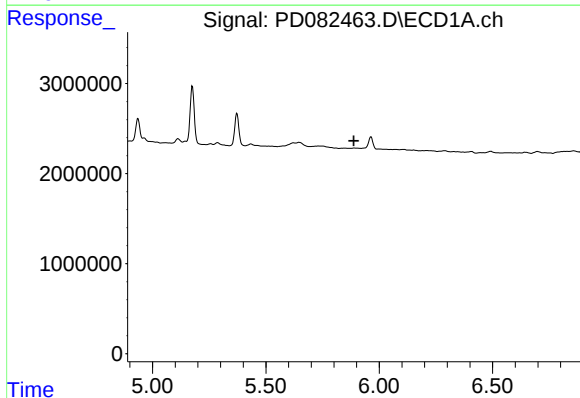


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.888 min
Response: 0
Conc: N.D.

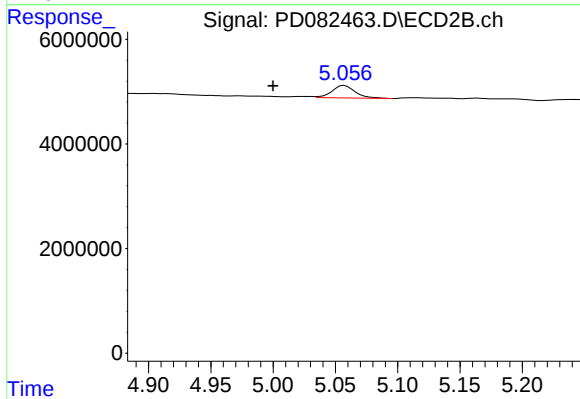

#22 Toxaphene-1


R.T.: 5.057 min
Delta R.T.: 0.057 min
Response: 3074582
Conc: 148.81 ng/ml

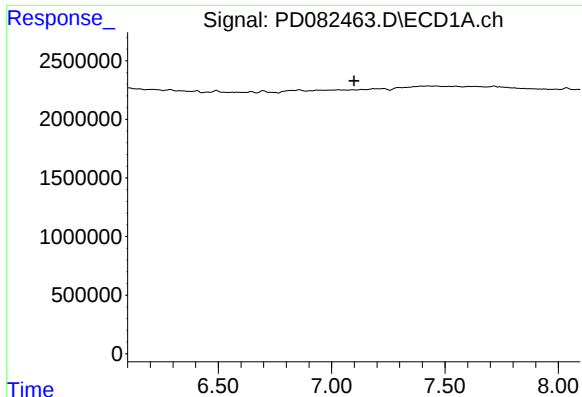

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E1D01

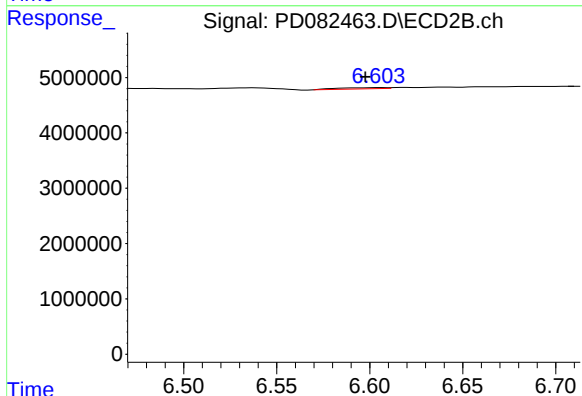


#24 Toxaphene-3

R.T.: 6.605 min
Delta R.T.: 0.008 min
Response: 425239
Conc: 5.60 ng/ml

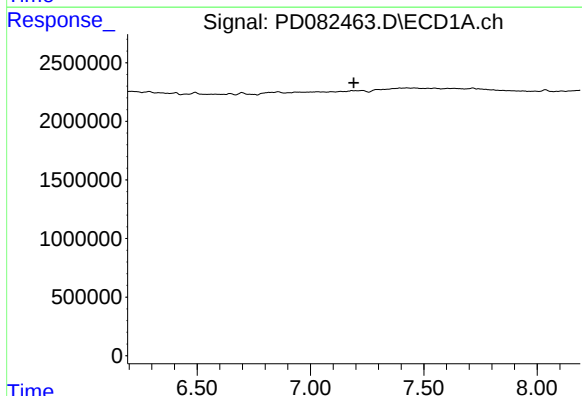


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

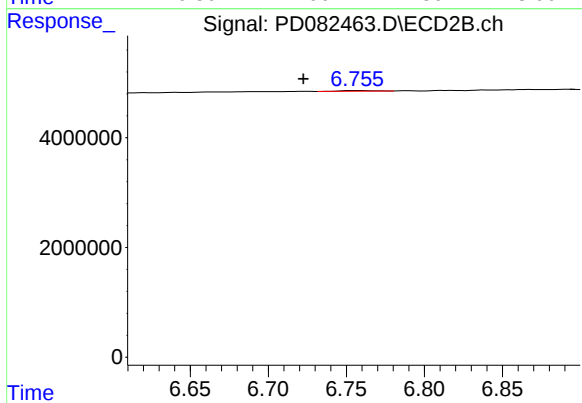

#25 Toxaphene-4


R.T.: 6.756 min
Delta R.T.: 0.034 min
Response: 180086
Conc: 1.72 ng/ml

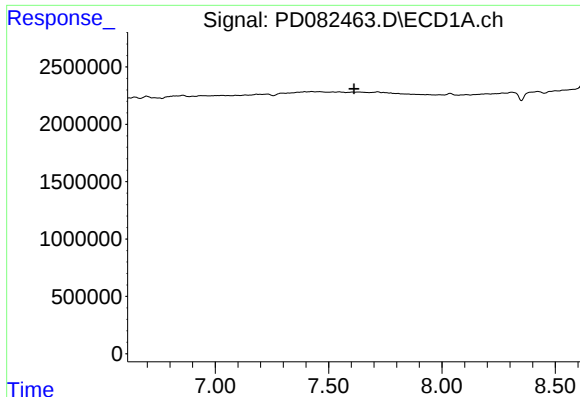

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E1D01

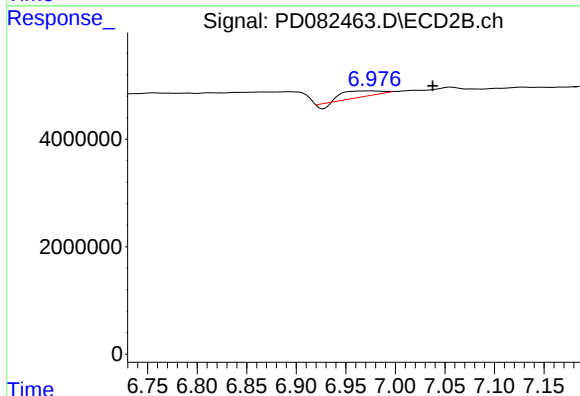


#26 Toxaphene-5

R.T.: 6.977 min
Delta R.T.: -0.060 min
Response: 2381127
Conc: 58.41 ng/ml

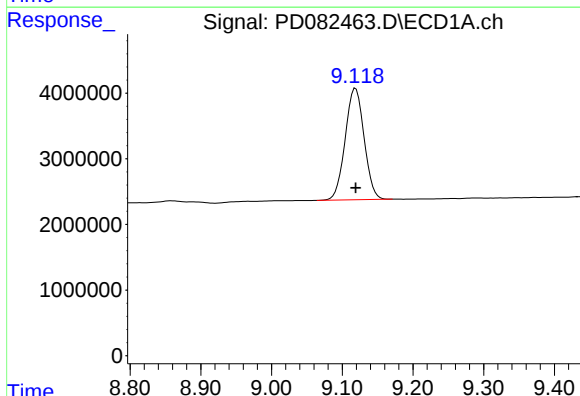

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 31612565
Conc: 16.17 ng/ml

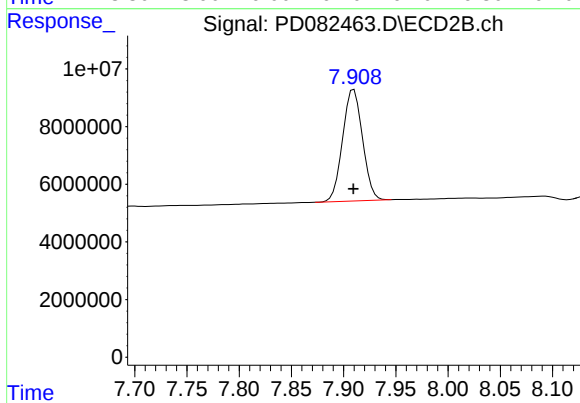

#27 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.000 min
Response: 51222240
Conc: 15.74 ng/ml