

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041719\
 Data File : PD052961.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Apr 2019 8:02
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 02:03:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) MA	gamma-BHC...	3.939f	0.000	715069	0	0.327	N.D. #
4) MA	Heptachlor	0.000	5.235	0	2850672	N.D.	0.072 #
5) MB	Aldrin	4.443f	0.000	4447546	0	2.209	N.D. #
7) B	delta-BHC	4.330	0.000	6830815	0	3.349	N.D. #
8) B	Heptachlo...	0.000	5.922	0	10572994	N.D.	0.328 #
9) A	Endosulfan I	0.000	6.284	0	12698991	N.D.	0.435 #
11) B	alpha-Chl...	0.000	6.258f	0	5697647	N.D.	0.182 #
17) MA	4,4'-DDT	0.000	7.164f	0	54318812	N.D.	2.915 #
19) B	Endosulfa...	6.296	0.000	1850178	0	1.207	N.D. #
24)	Chlordane-2	4.508f	0.000	1582289	0	21.263	N.D. #
26)	Chlordane-4	0.000	6.258f	0	5697647	N.D.	1.120 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041719\
Data File : PD052961.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Apr 2019 8:02
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 02:03:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

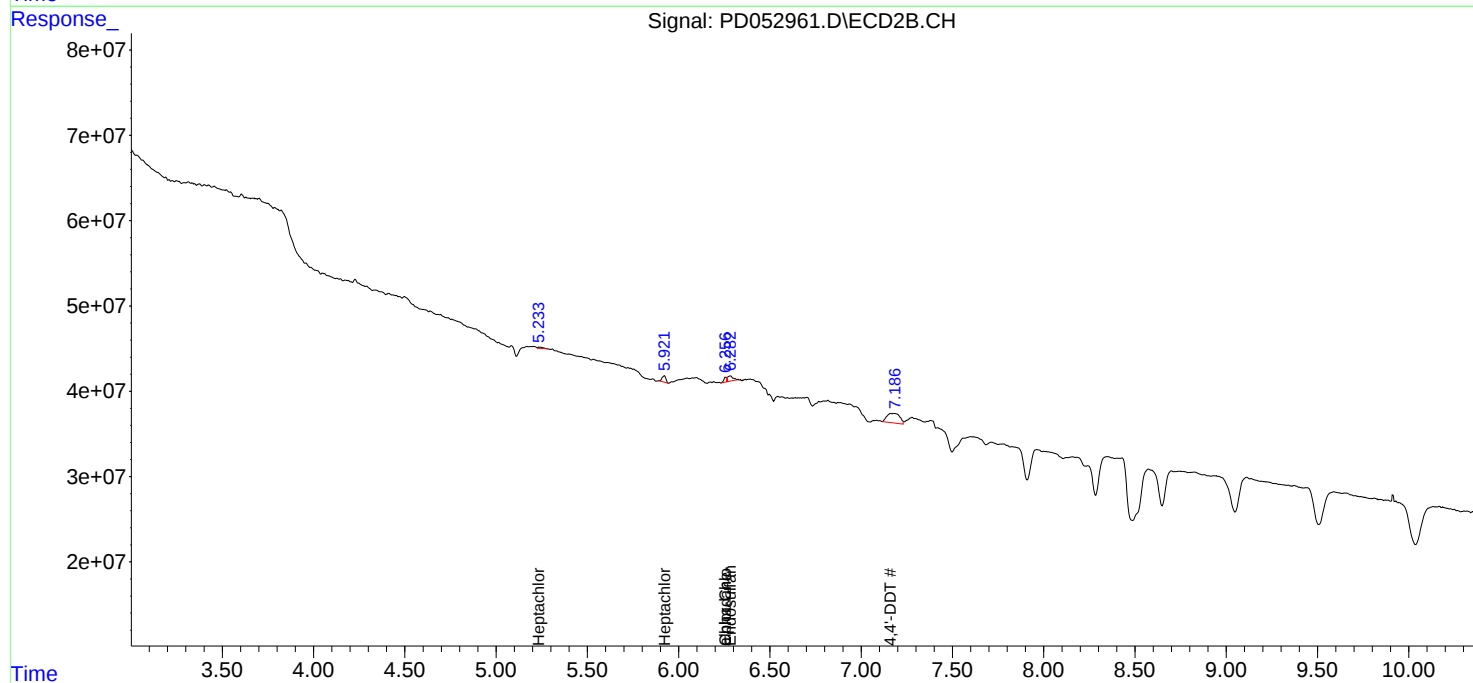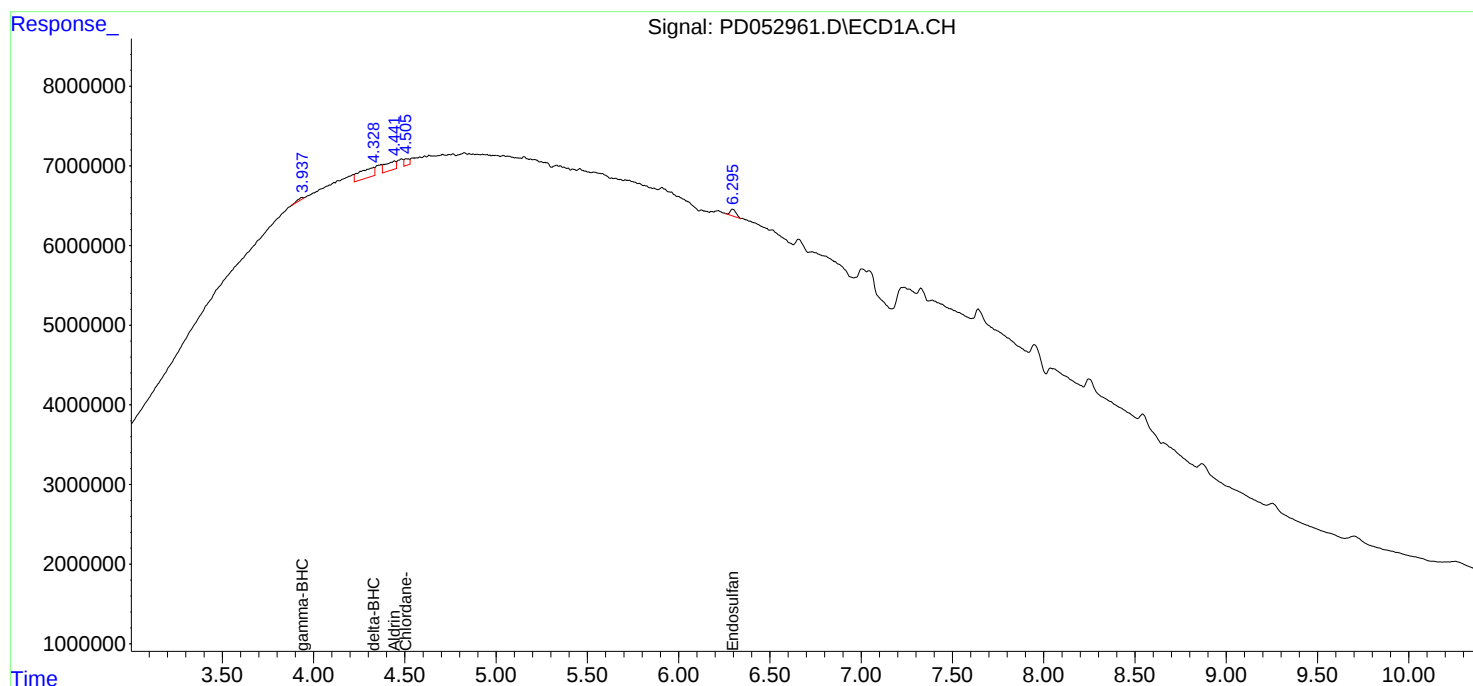


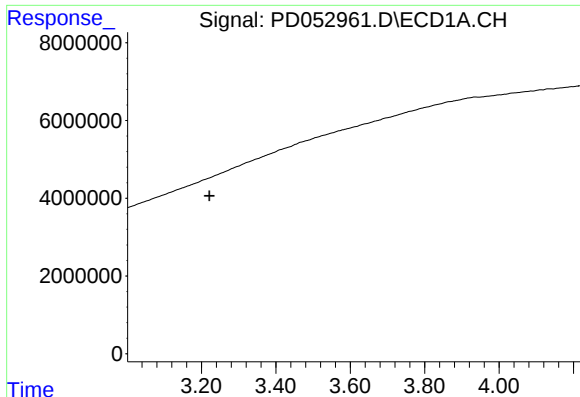

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

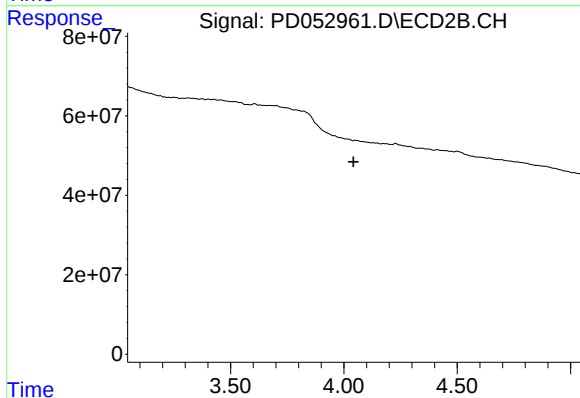


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.043 min
Response: 0
Conc: N.D.

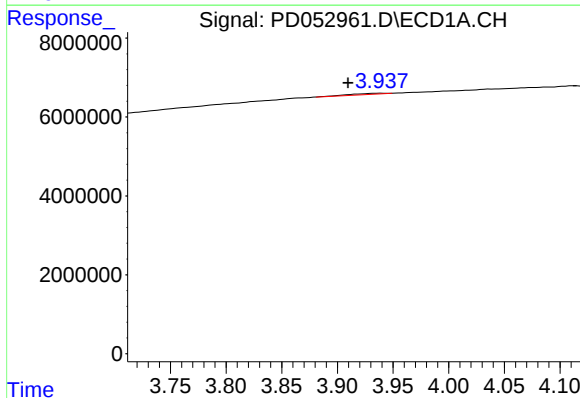


#3 gamma-BHC (Lindane)

R.T.: 3.939 min
Delta R.T.: 0.029 min
Response: 715069
Conc: 0.33 ng/ml

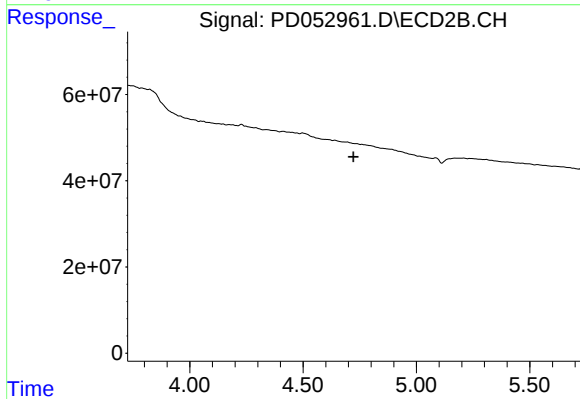

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

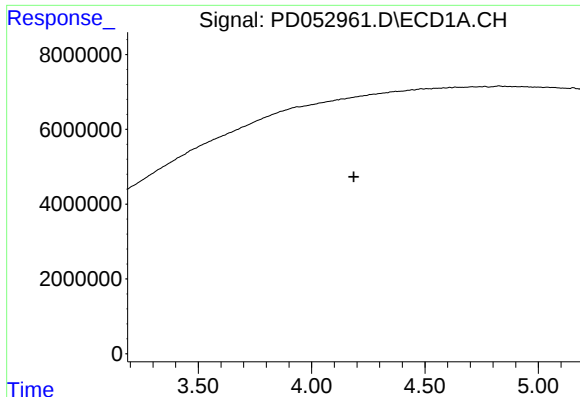

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

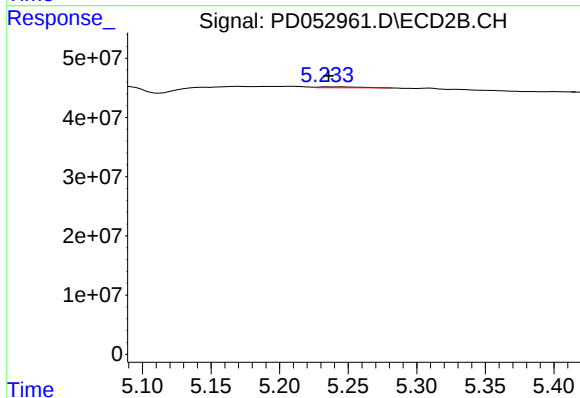


#4 Heptachlor

R.T.: 5.235 min
Delta R.T.: -0.001 min
Response: 2850672
Conc: 0.07 ng/ml

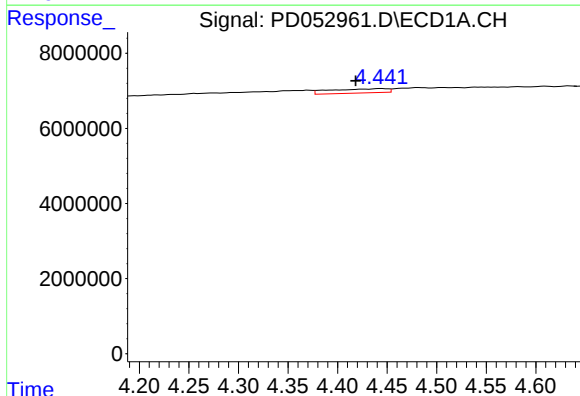


#5 Aldrin

R.T.: 4.443 min
Delta R.T.: 0.025 min
Response: 4447546
Conc: 2.21 ng/ml

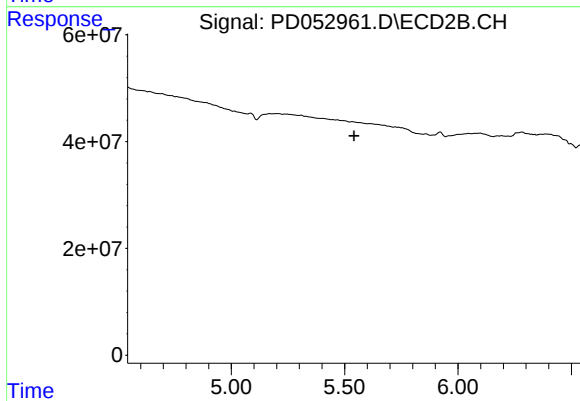

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.542 min
Response: 0
Conc: N.D.

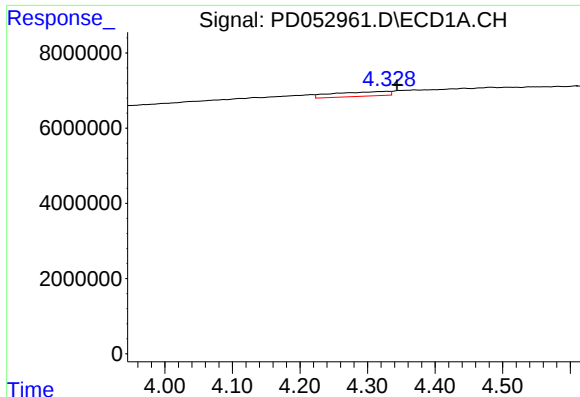

#7 delta-BHC


R.T.: 4.330 min
Delta R.T.: -0.014 min
Response: 6830815
Conc: 3.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

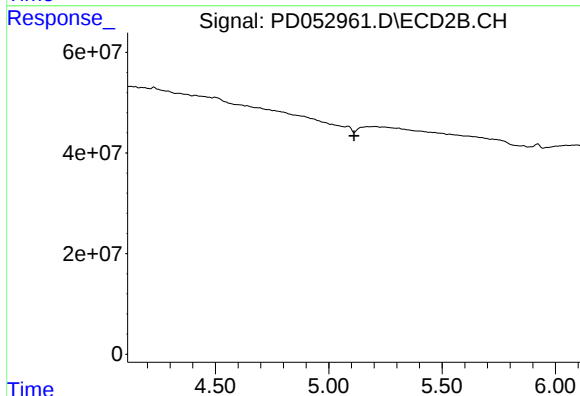


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

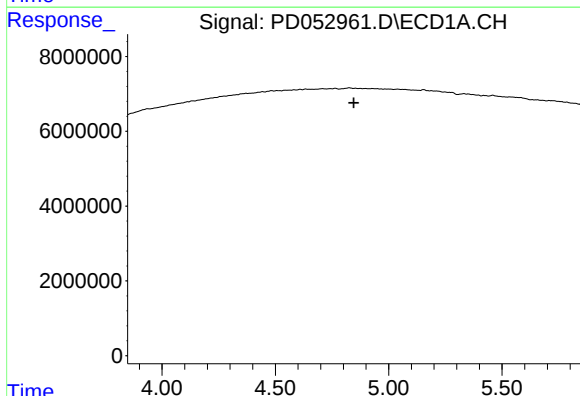


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

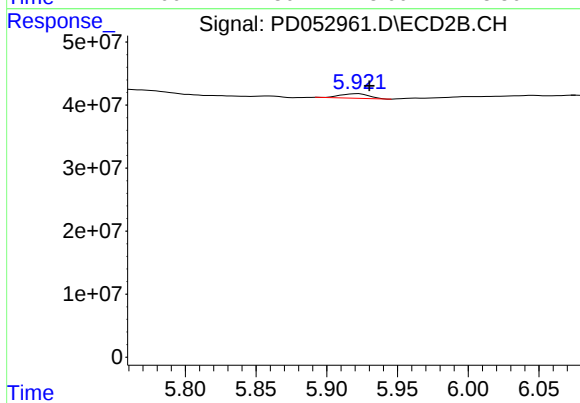

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.008 min
Response: 10572994
Conc: 0.33 ng/ml

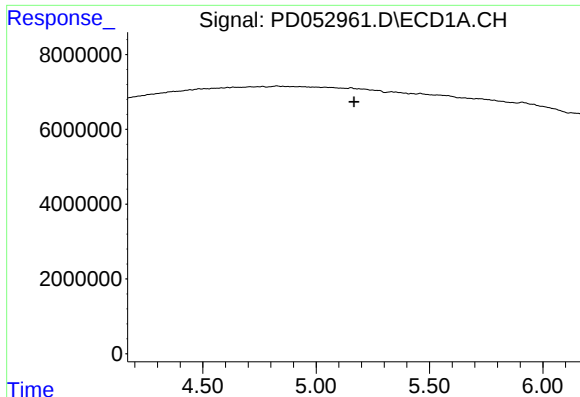

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

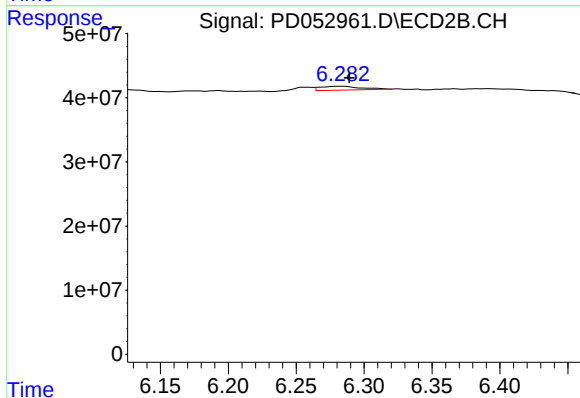


#9 Endosulfan I

R.T.: 6.284 min
Delta R.T.: -0.005 min
Response: 12698991
Conc: 0.43 ng/ml

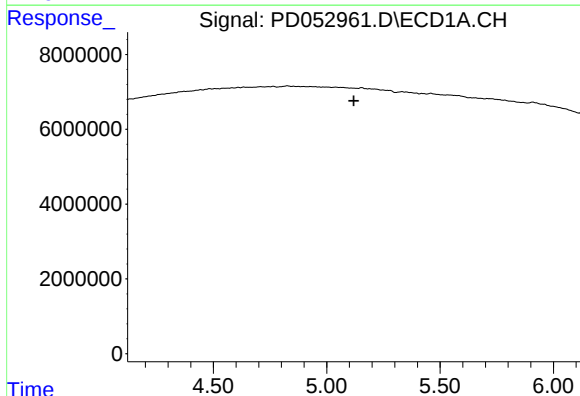


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

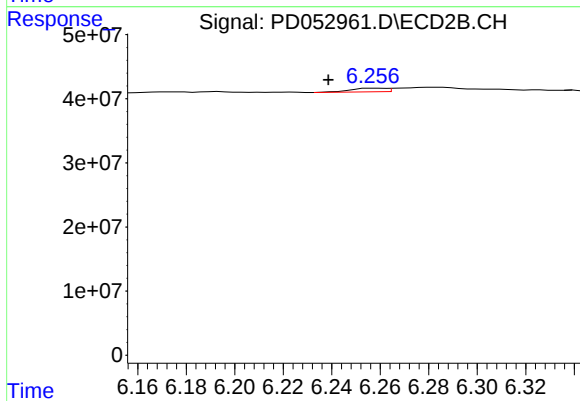

#11 alpha-Chlordane


R.T.: 6.258 min
Delta R.T.: 0.019 min
Response: 5697647
Conc: 0.18 ng/ml

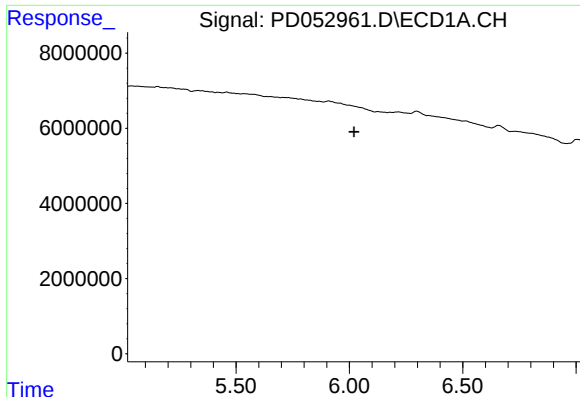

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

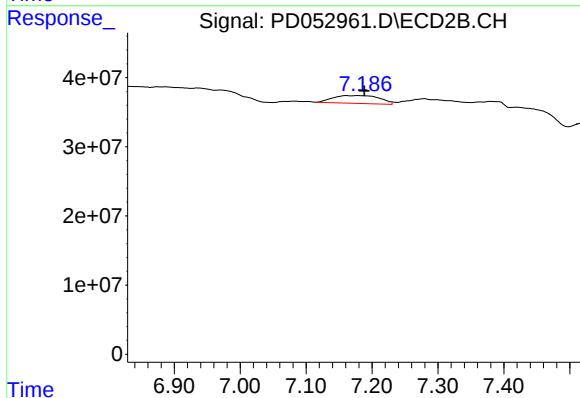


#17 4,4'-DDT

R.T.: 7.164 min
Delta R.T.: -0.024 min
Response: 54318812
Conc: 2.92 ng/ml

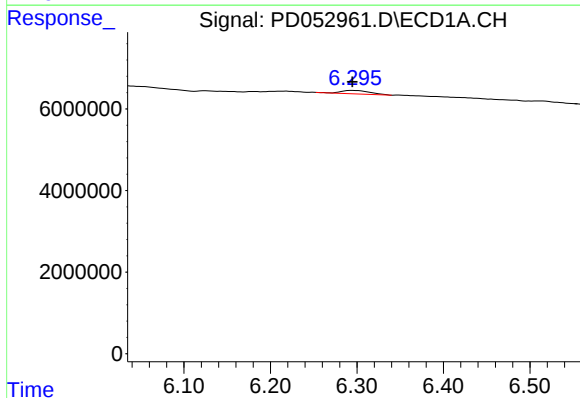


#19 Endosulfan Sulfate

R.T.: 6.296 min
Delta R.T.: 0.001 min
Response: 1850178
Conc: 1.21 ng/ml

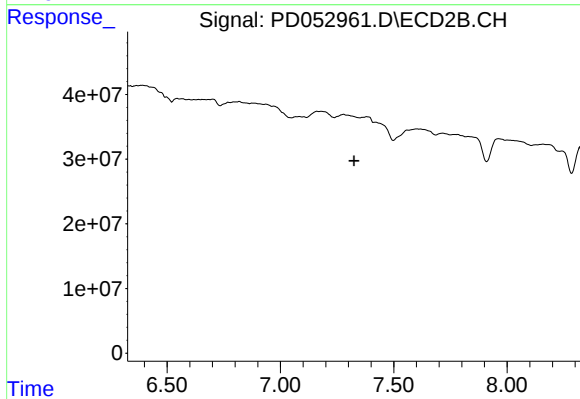

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.326 min
Response: 0
Conc: N.D.

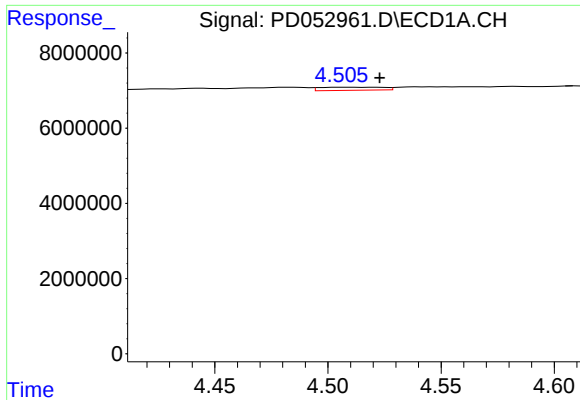

#24 Chlordane-2


R.T.: 4.508 min
Delta R.T.: -0.015 min
Response: 1582289
Conc: 21.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

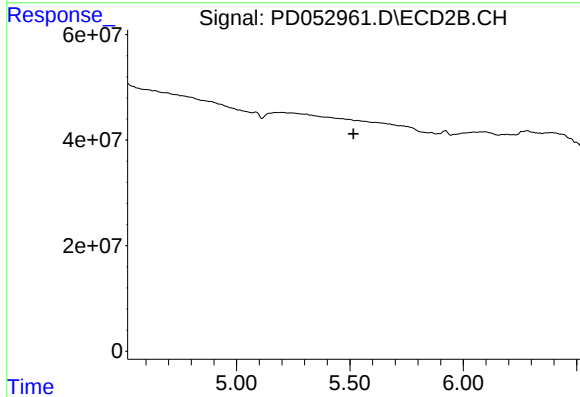


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.516 min
Response: 0
Conc: N.D.

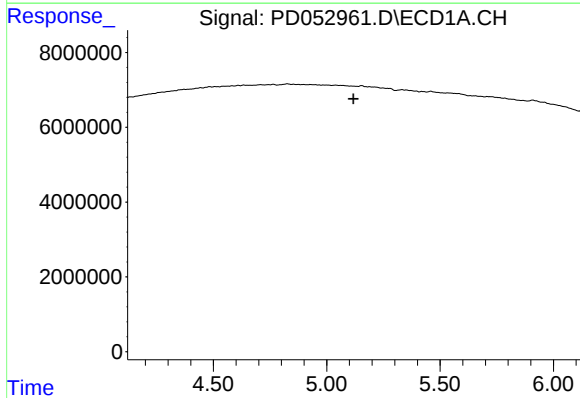


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

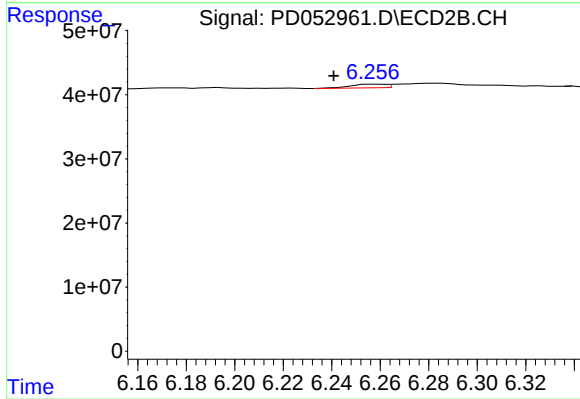

#26 Chlordane-4


R.T.: 6.258 min
Delta R.T.: 0.017 min
Response: 5697647
Conc: 1.12 ng/ml

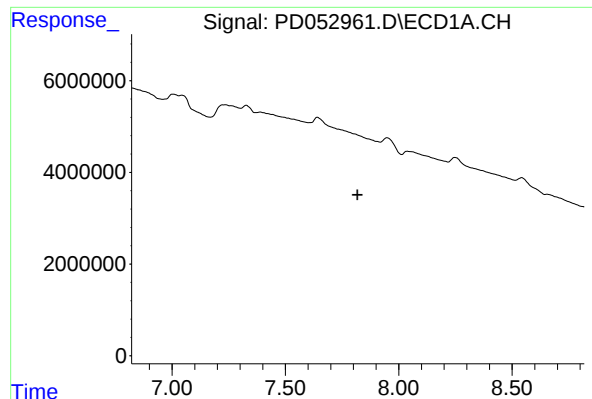

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

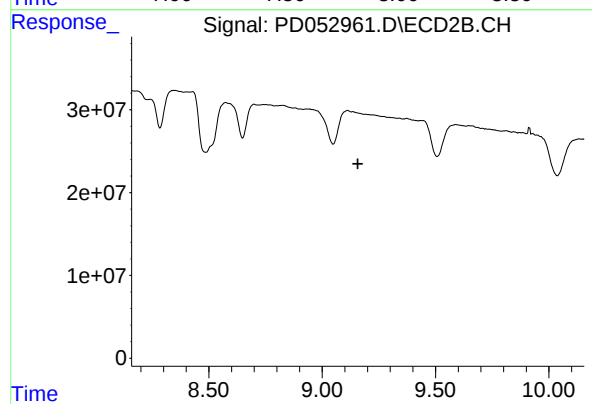

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.156 min
Response: 0
Conc: N.D.