

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041719\
 Data File : PD052975.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Apr 2019 11:36
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 02:05:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.042	28531702	588.9E6	20.447	20.319
28)	SA Decachlor...	7.813	9.160	31329902	403.3E6	23.508	25.933
Target Compounds							
3)	MA gamma-BHC...	3.926f	0.000	2063172	0	0.944	N.D. #
4)	MA Heptachlor	0.000	5.242	0	601185	N.D.	0.015 #
8)	B Heptachlo...	4.866f	5.922	920115	23912817	0.484	0.741 #
10)	B gamma-Chl...	0.000	6.166	0	20408153	N.D.	0.638 #
14)	MA Endrin	0.000	6.762	0	61149050	N.D.	2.440 #
17)	MA 4,4'-DDT	0.000	7.168f	0	24305360	N.D.	1.304 #
19)	B Endosulfa...	6.318f	0.000	1251989	0	0.816	N.D. #
25)	Chlordane-3	0.000	6.166	0	20408153	N.D.	4.625 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041719\
Data File : PD052975.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Apr 2019 11:36
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 02:05:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

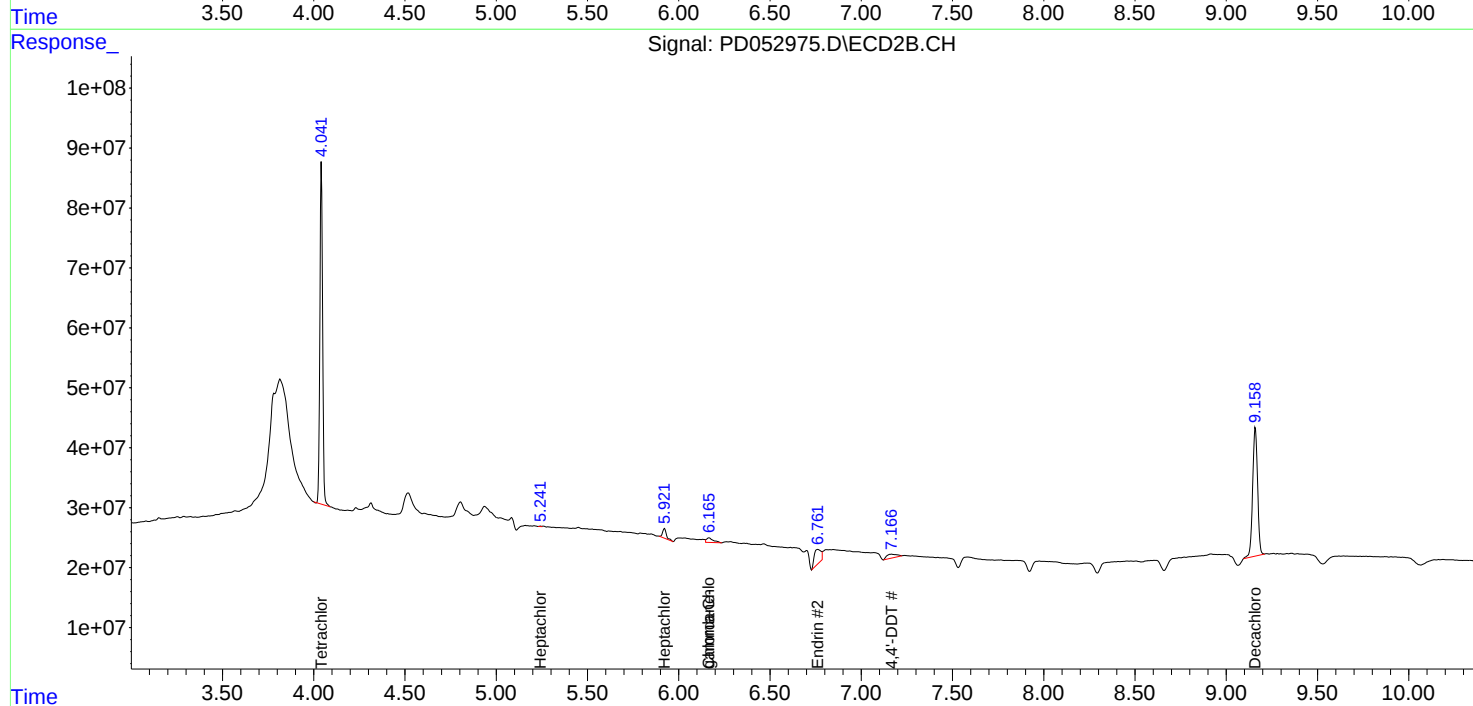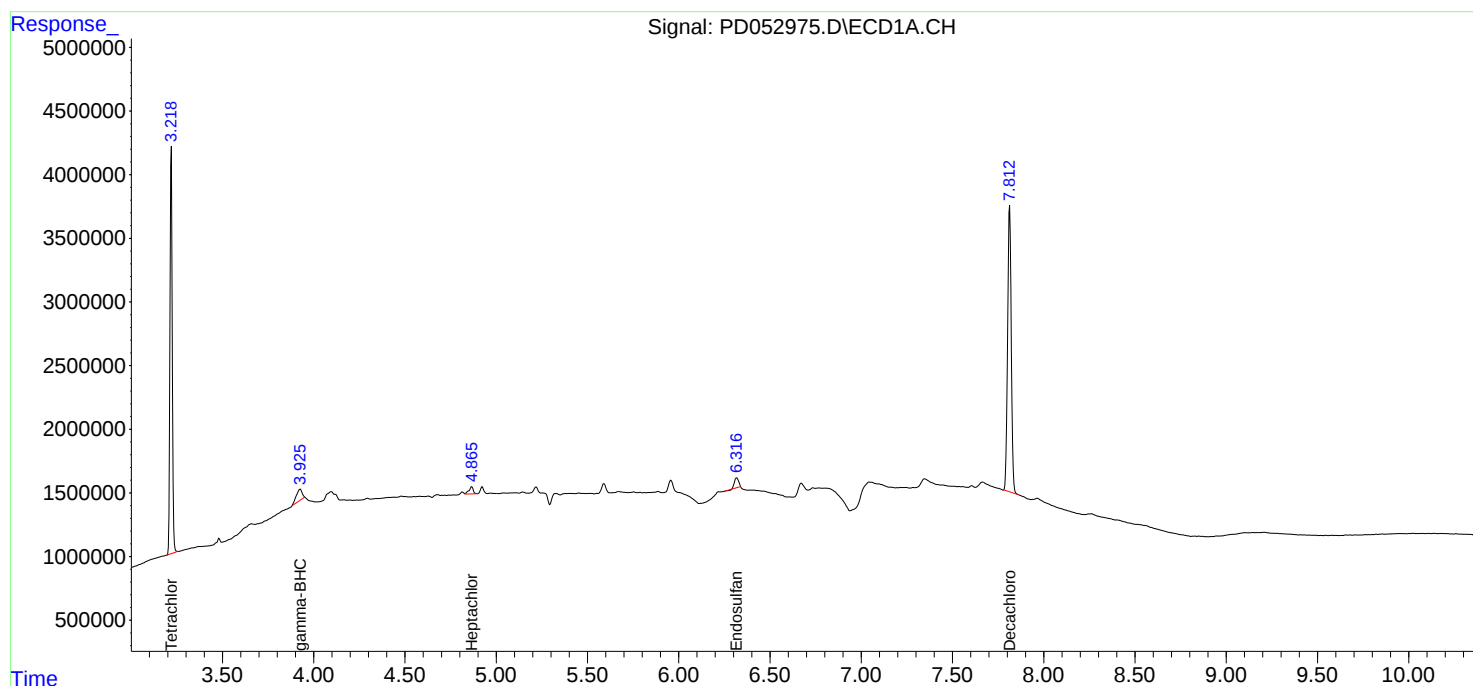


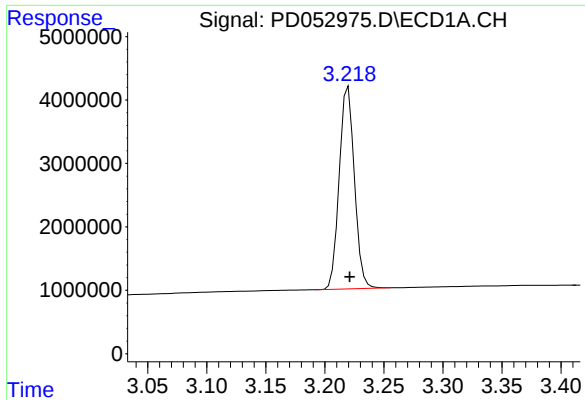

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: -0.001 min
Response: 28531702
Conc: 20.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

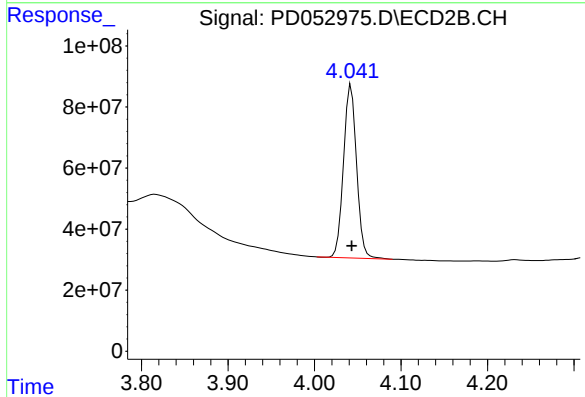


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 588929077
Conc: 20.32 ng/ml

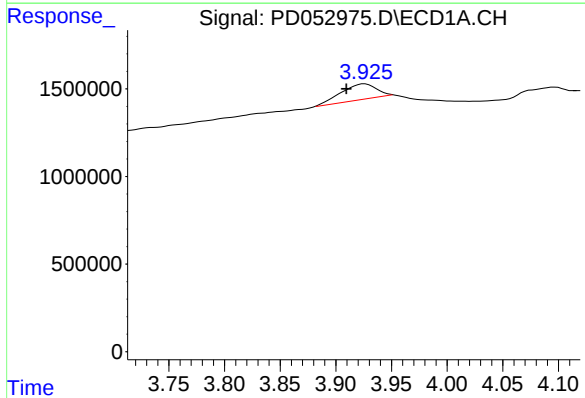


#3 gamma-BHC (Lindane)

R.T.: 3.926 min
Delta R.T.: 0.016 min
Response: 2063172
Conc: 0.94 ng/ml

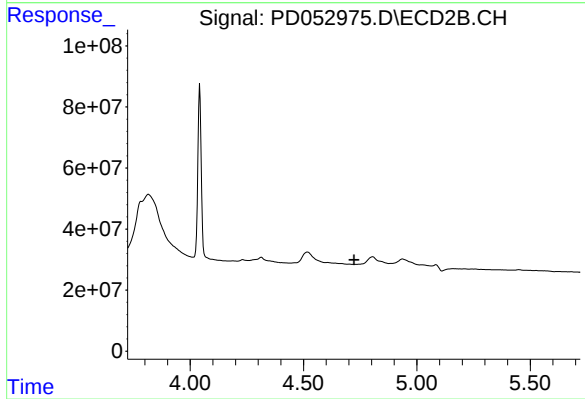

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

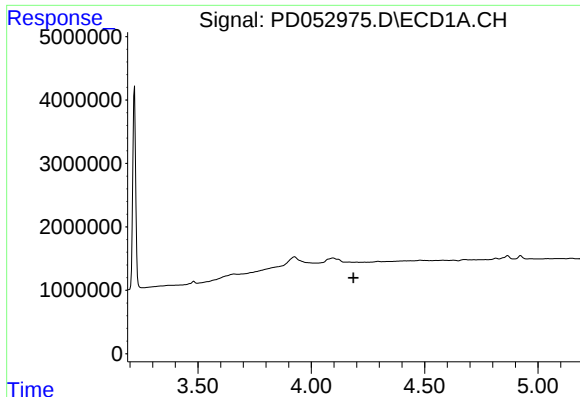

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

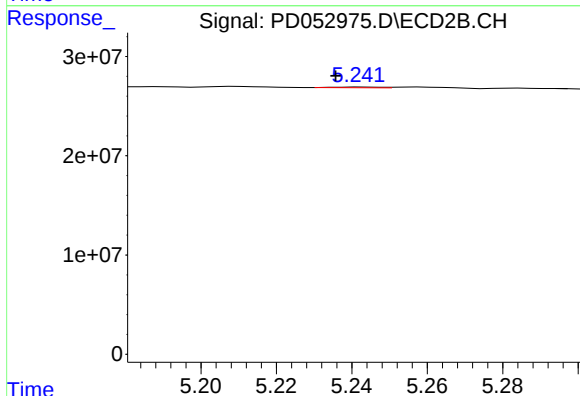


#4 Heptachlor

R.T.: 5.242 min
Delta R.T.: 0.007 min
Response: 601185
Conc: 0.02 ng/ml

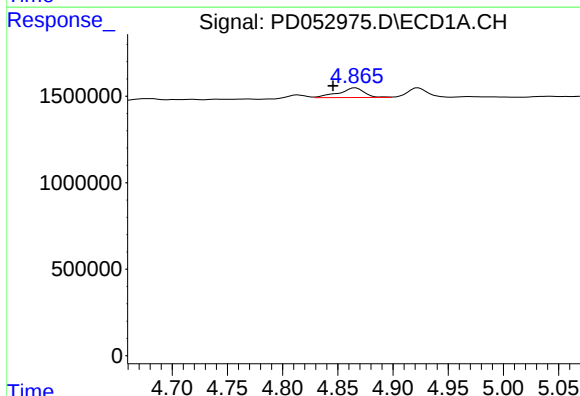


#8 Heptachlor epoxide

R.T.: 4.866 min
Delta R.T.: 0.021 min
Response: 920115
Conc: 0.48 ng/ml

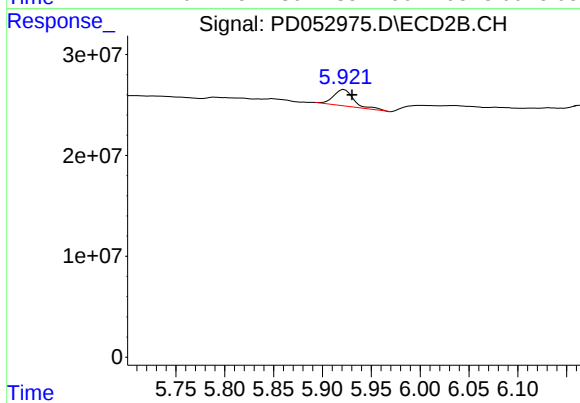

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.008 min
Response: 23912817
Conc: 0.74 ng/ml

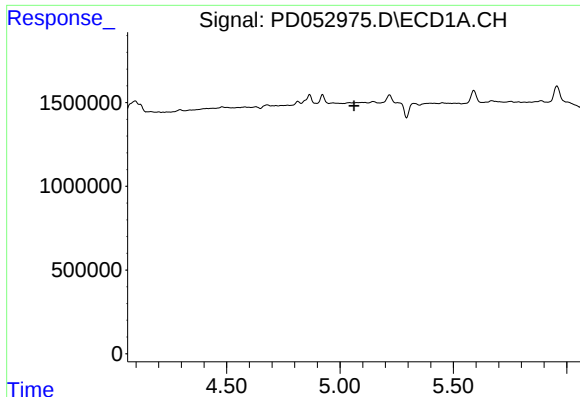

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

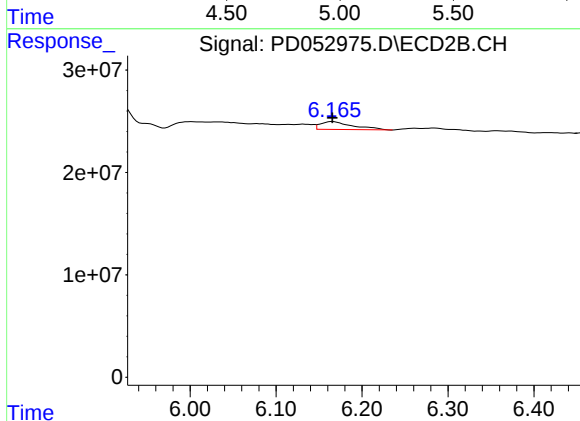


#10 gamma-Chlordane

R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 20408153
Conc: 0.64 ng/ml

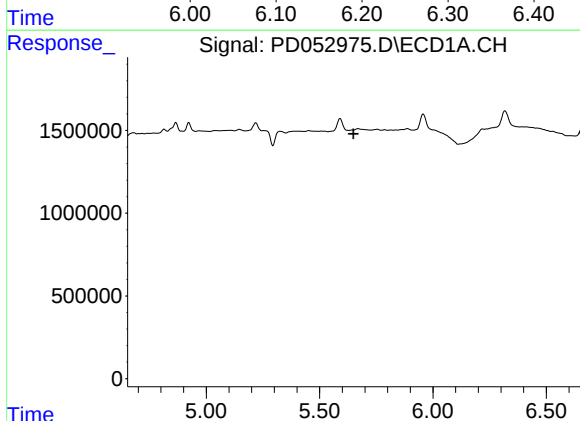


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.650 min
Response: 0
Conc: N.D.

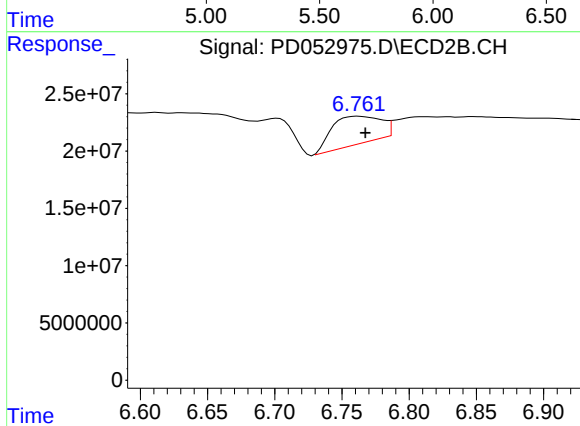

#14 Endrin


R.T.: 6.762 min
Delta R.T.: -0.005 min
Response: 61149050
Conc: 2.44 ng/ml

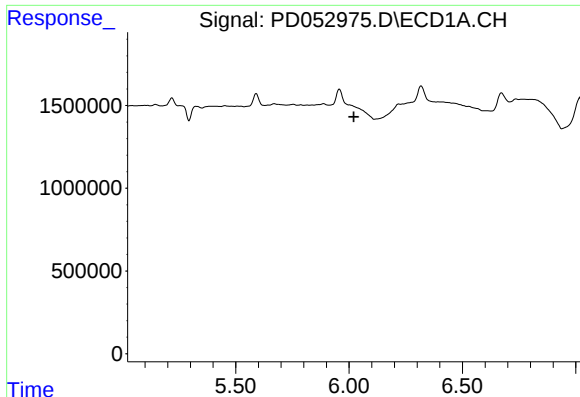

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

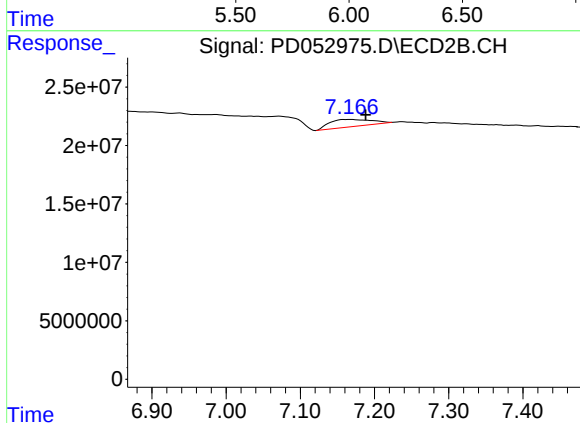


#17 4,4'-DDT

R.T.: 7.168 min
Delta R.T.: -0.020 min
Response: 24305360
Conc: 1.30 ng/ml

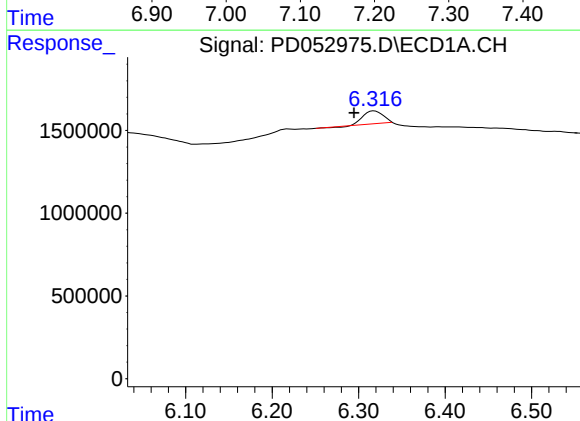


#19 Endosulfan Sulfate

R.T.: 6.318 min
Delta R.T.: 0.023 min
Response: 1251989
Conc: 0.82 ng/ml

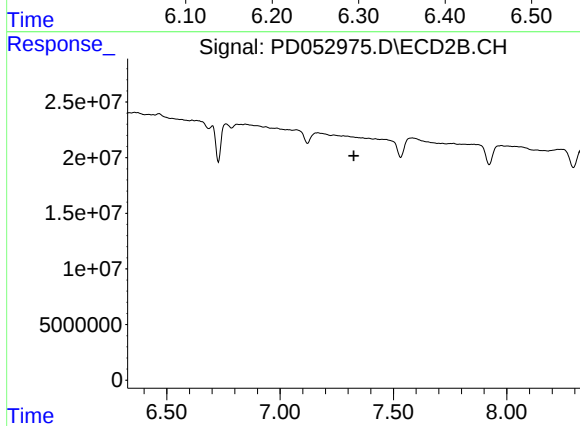

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.326 min
Response: 0
Conc: N.D.

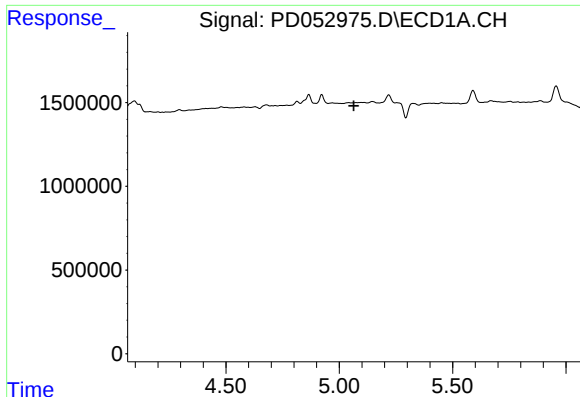

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

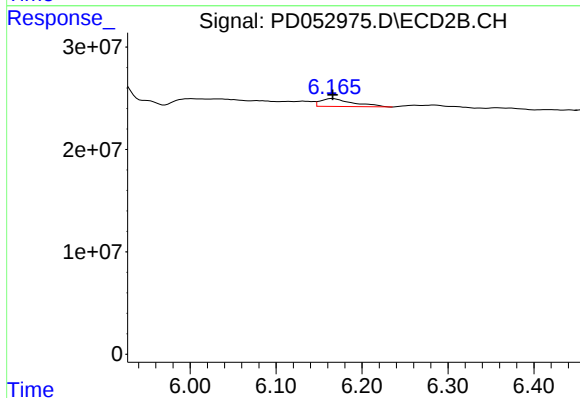


#25 Chlordane-3

R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 20408153
Conc: 4.62 ng/ml

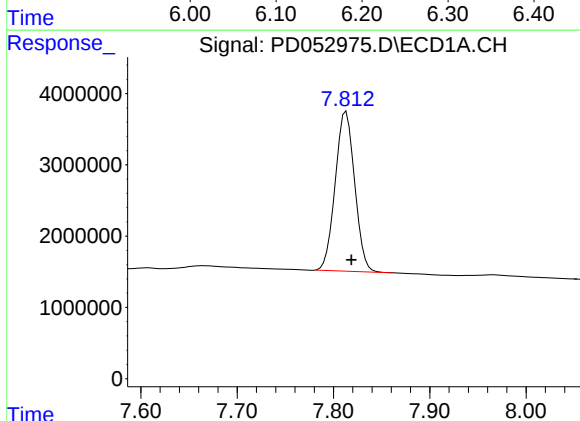

#28 Decachlorobiphenyl

R.T.: 7.813 min
Delta R.T.: -0.005 min
Response: 31329902
Conc: 23.51 ng/ml

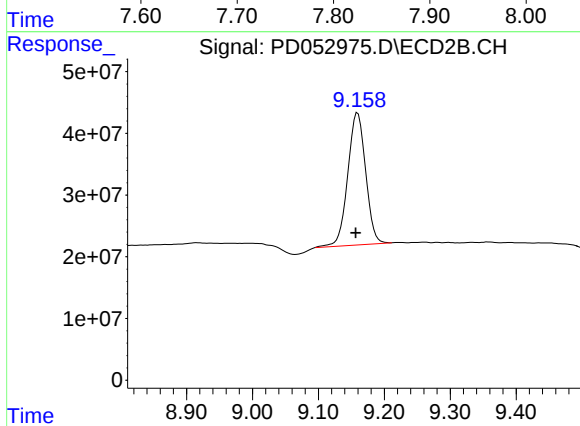

#28 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: 0.003 min
Response: 403296300
Conc: 25.93 ng/ml