

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
 Data File : PD057782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 13:50
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:07:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.894	14403169	19995801	20.173	25.487 #
28)	SA Decachlor...	7.869	8.895	15384433	21421403	20.206	24.355
Target Compounds							
3)	MA gamma-BHC...	3.932	0.000	1021629	0	0.949	N.D. #
8)	B Heptachlo...	0.000	5.742	0	7788008	N.D.	7.771 #
11)	B alpha-Chl...	5.160f	0.000	1712125	0	1.869	N.D. #
14)	MA Endrin	5.708f	0.000	1178480	0	1.622	N.D. #
16)	A 4,4'-DDD	5.795f	0.000	74430	0	0.130	N.D. #
21)	B Endrin ke...	6.847f	0.000	1009444	0	1.235	N.D. #
23)	Chlordane-1	4.064	0.000	166674	0	6.696	N.D. #
26)	Chlordane-4	5.160f	0.000	1712125	0	21.172	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
Data File : PD057782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 13:50
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:07:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

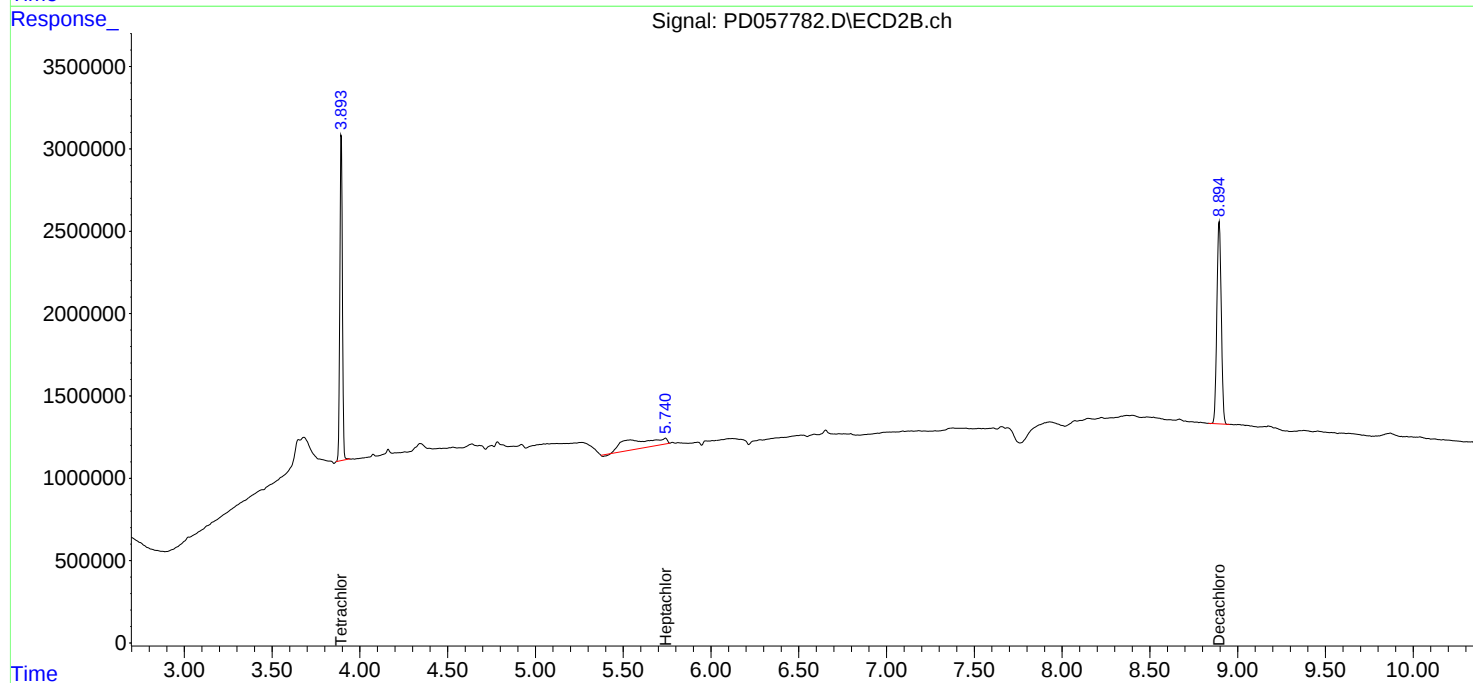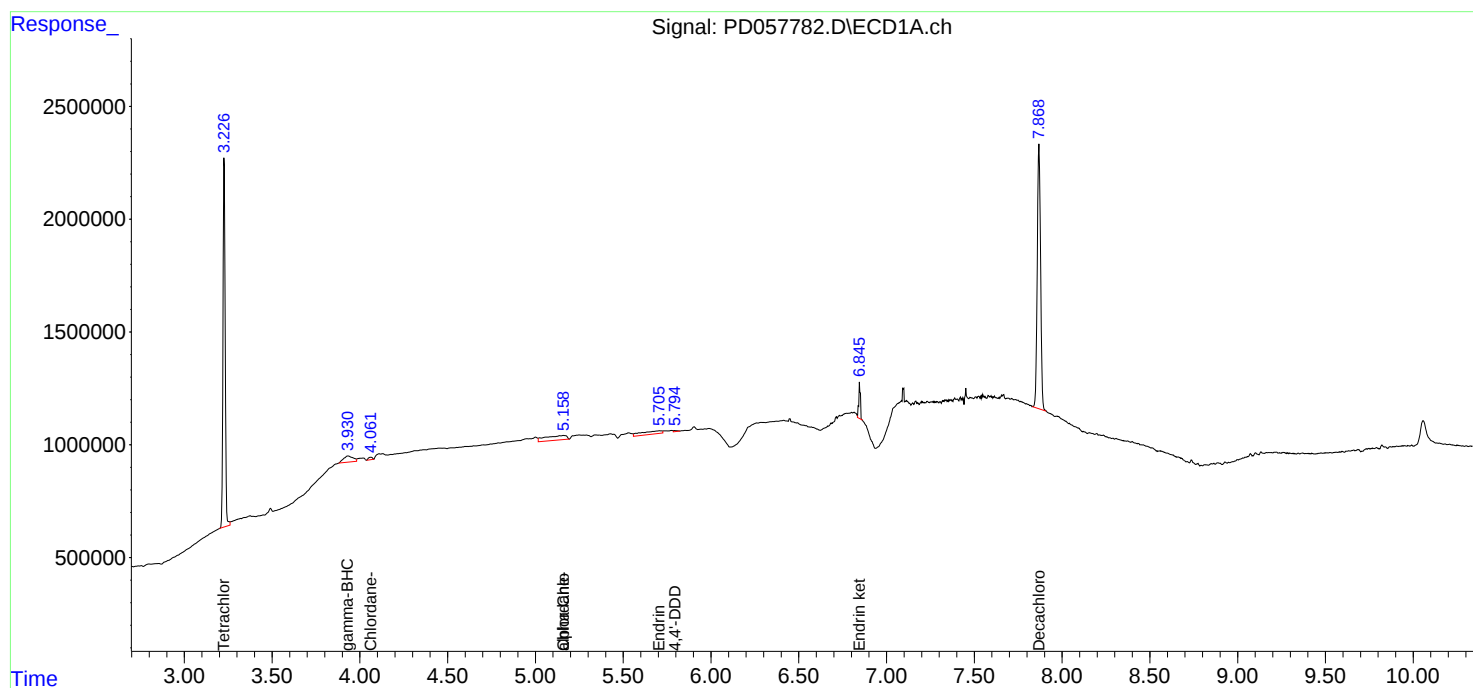


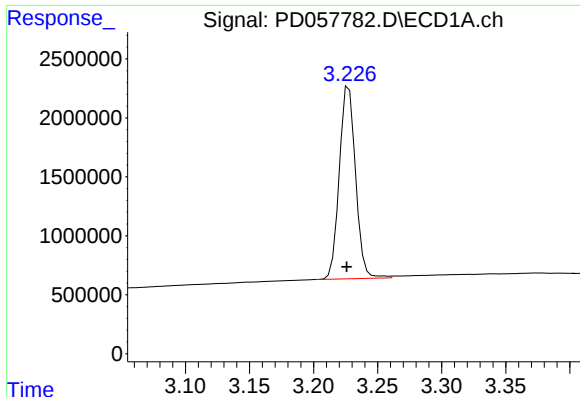

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.002 min
Response: 14403169
Conc: 20.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

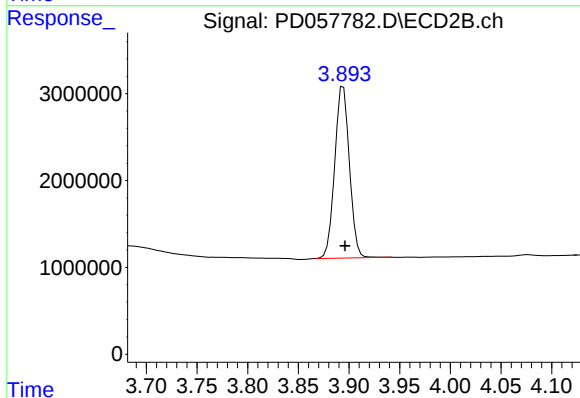


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.002 min
Response: 19995801
Conc: 25.49 ng/ml

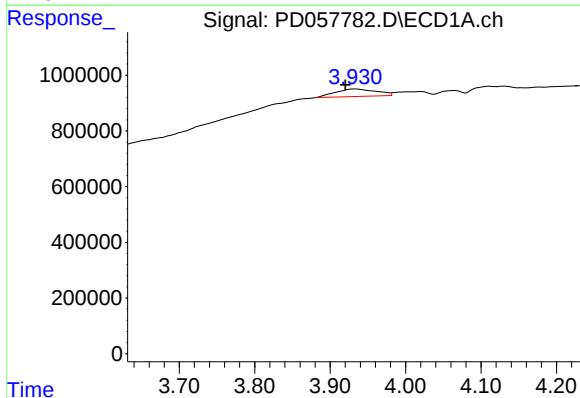


#3 gamma-BHC (Lindane)

R.T.: 3.932 min
Delta R.T.: 0.012 min
Response: 1021629
Conc: 0.95 ng/ml

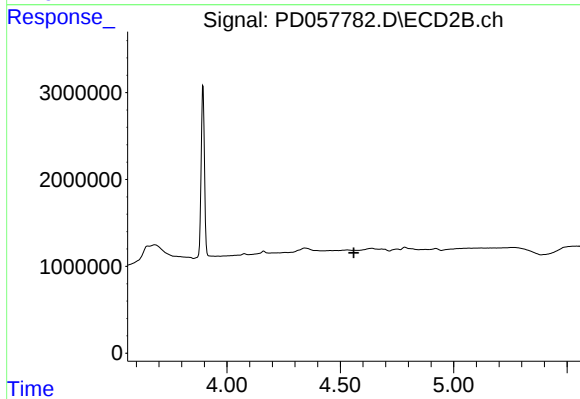

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.560 min
Response: 0
Conc: N.D.

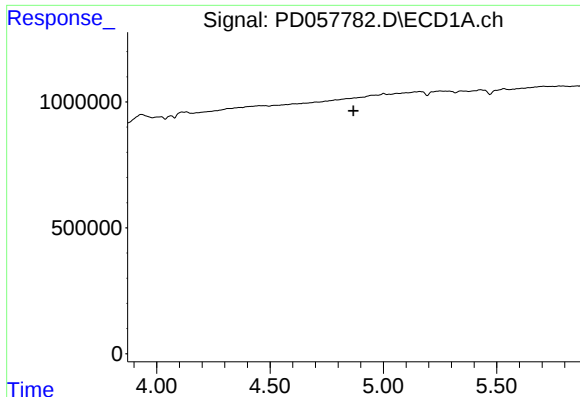

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.869 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

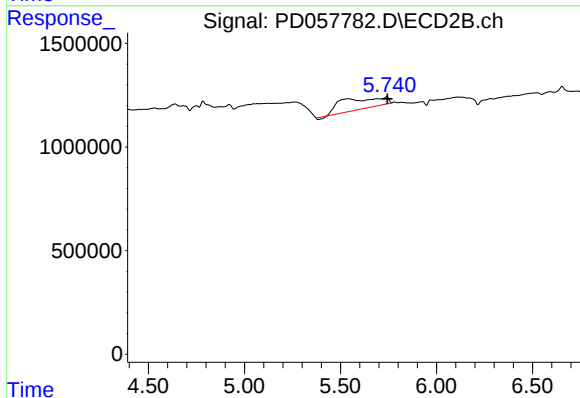


#8 Heptachlor epoxide

R.T.: 5.742 min
Delta R.T.: -0.003 min
Response: 7788008
Conc: 7.77 ng/ml

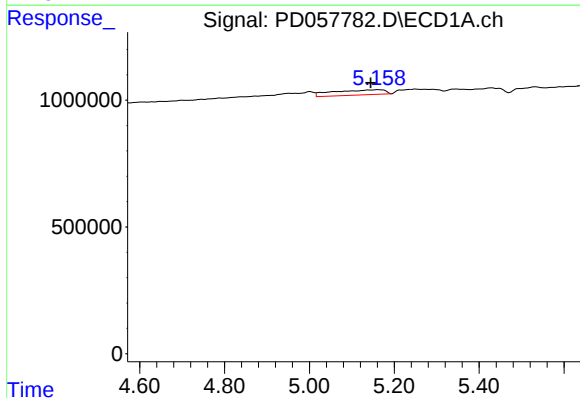


#11 alpha-Chlordane

R.T.: 5.160 min
Delta R.T.: 0.015 min
Response: 1712125
Conc: 1.87 ng/ml

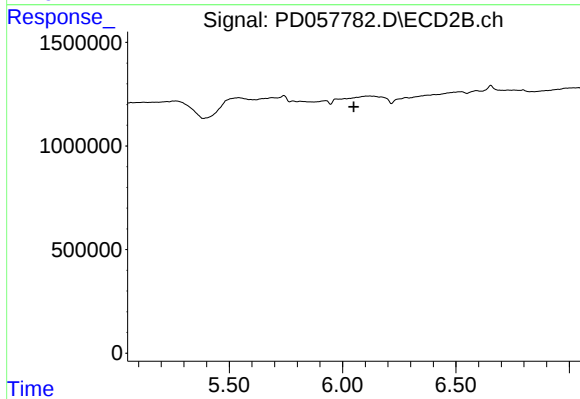

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.050 min
Response: 0
Conc: N.D.

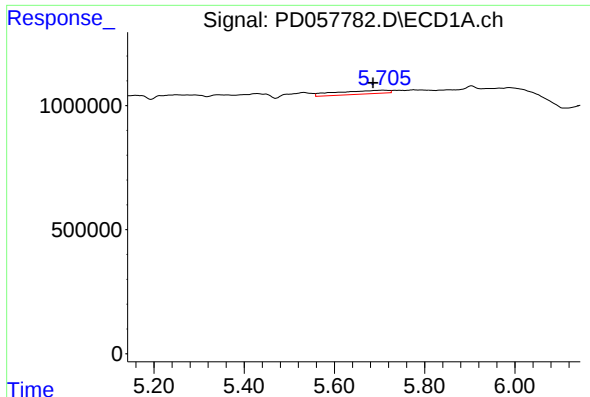

#14 Endrin


R.T.: 5.708 min
Delta R.T.: 0.022 min
Response: 1178480
Conc: 1.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

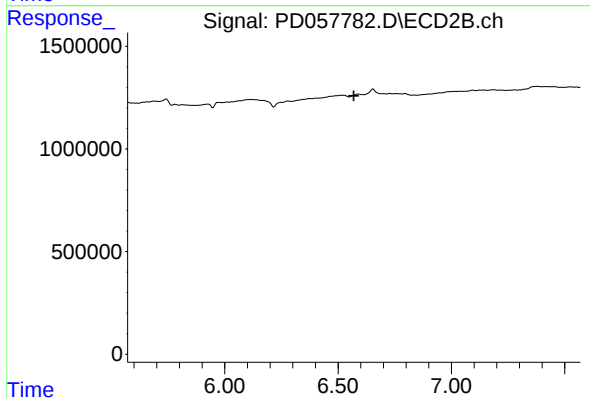


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

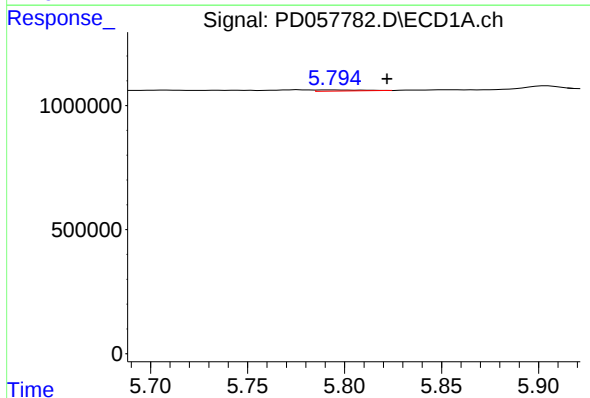


#16 4,4'-DDD

R.T.: 5.795 min
Delta R.T.: -0.027 min
Response: 74430
Conc: 0.13 ng/ml

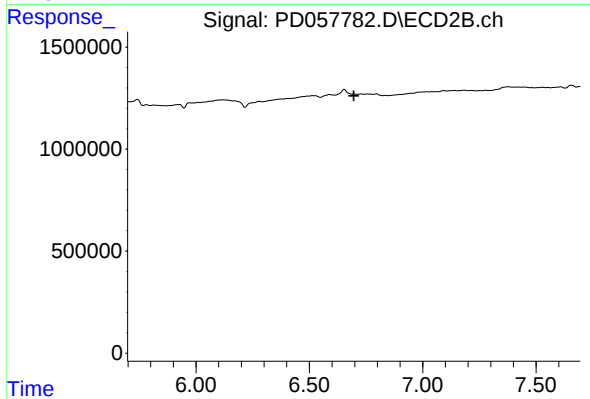

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.696 min
Response: 0
Conc: N.D.

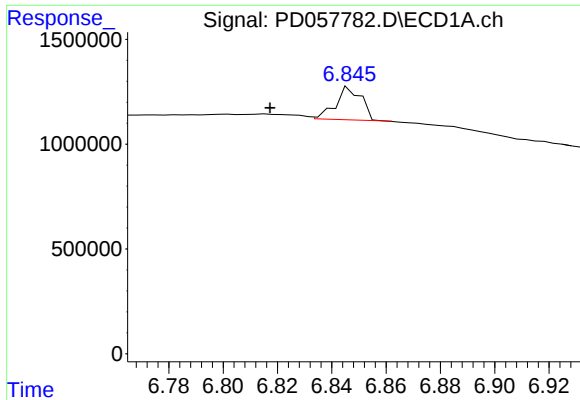

#21 Endrin ketone


R.T.: 6.847 min
Delta R.T.: 0.030 min
Response: 1009444
Conc: 1.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

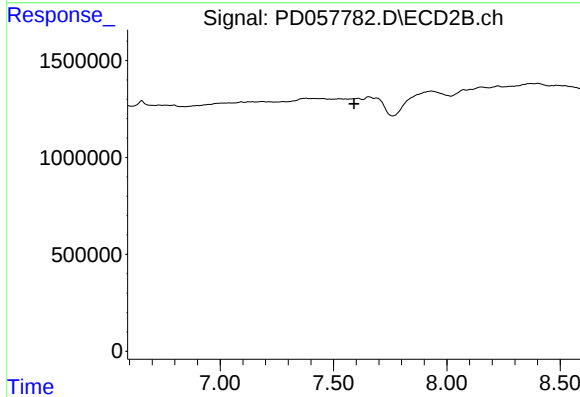


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.591 min
Response: 0
Conc: N.D.

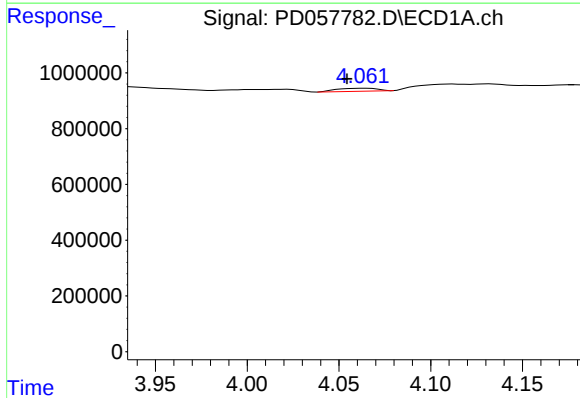


#23 Chlordane-1

R.T.: 4.064 min
Delta R.T.: 0.009 min
Response: 166674
Conc: 6.70 ng/ml

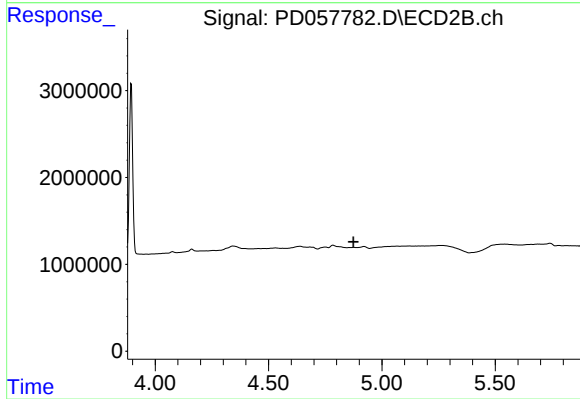

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.875 min
Response: 0
Conc: N.D.

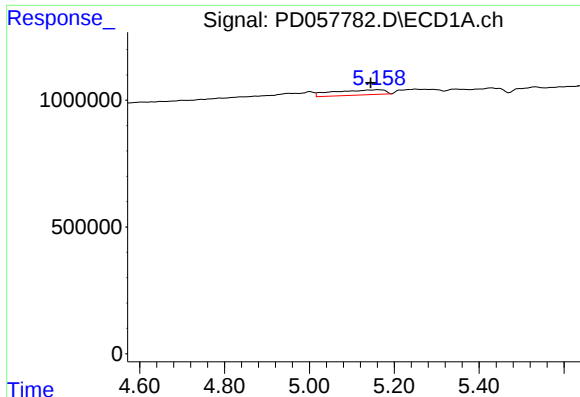

#26 Chlordane-4


R.T.: 5.160 min
Delta R.T.: 0.015 min
Response: 1712125
Conc: 21.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

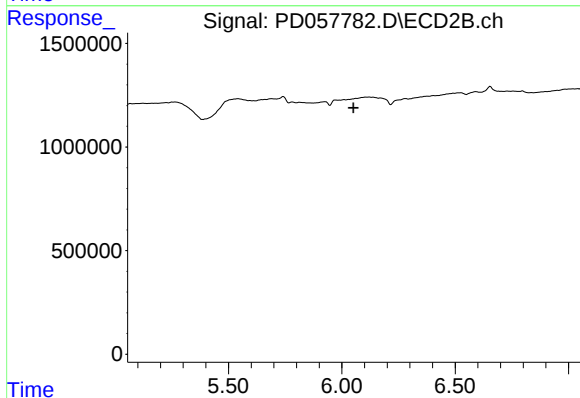


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.052 min
Response: 0
Conc: N.D.

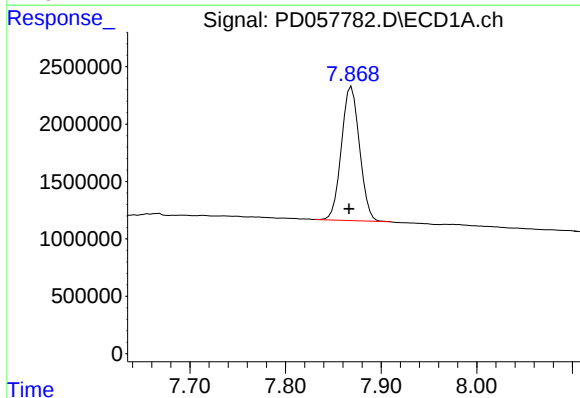

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: 0.002 min
Response: 15384433
Conc: 20.21 ng/ml

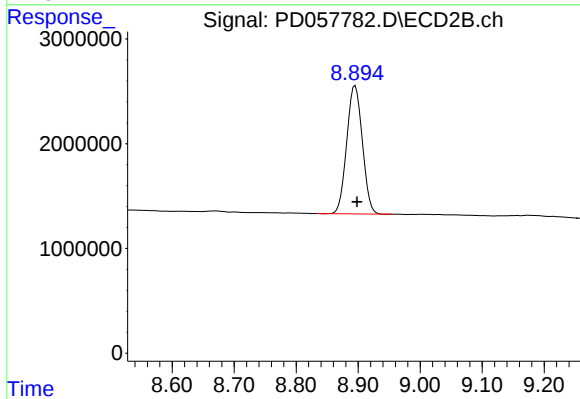

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: -0.003 min
Response: 21421403
Conc: 24.36 ng/ml