

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
 Data File : PD057794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 18:50
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:08:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 14:08:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.896	15500800	21025350	21.710	26.799
28)	SA Decachlor...	7.871	8.898	16962371	23991460	22.278	27.278
Target Compounds							
3)	MA gamma-BHC...	3.932	0.000	1389033	0	1.290	N.D. #
10)	B gamma-Chl...	5.061f	0.000	88745	0	0.097	N.D. #
24)	Chlordane-2	4.548	0.000	199912	0	6.973	N.D. #
25)	Chlordane-3	5.061f	0.000	88745	0	1.011	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
Data File : PD057794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 18:50
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:08:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 14:08:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

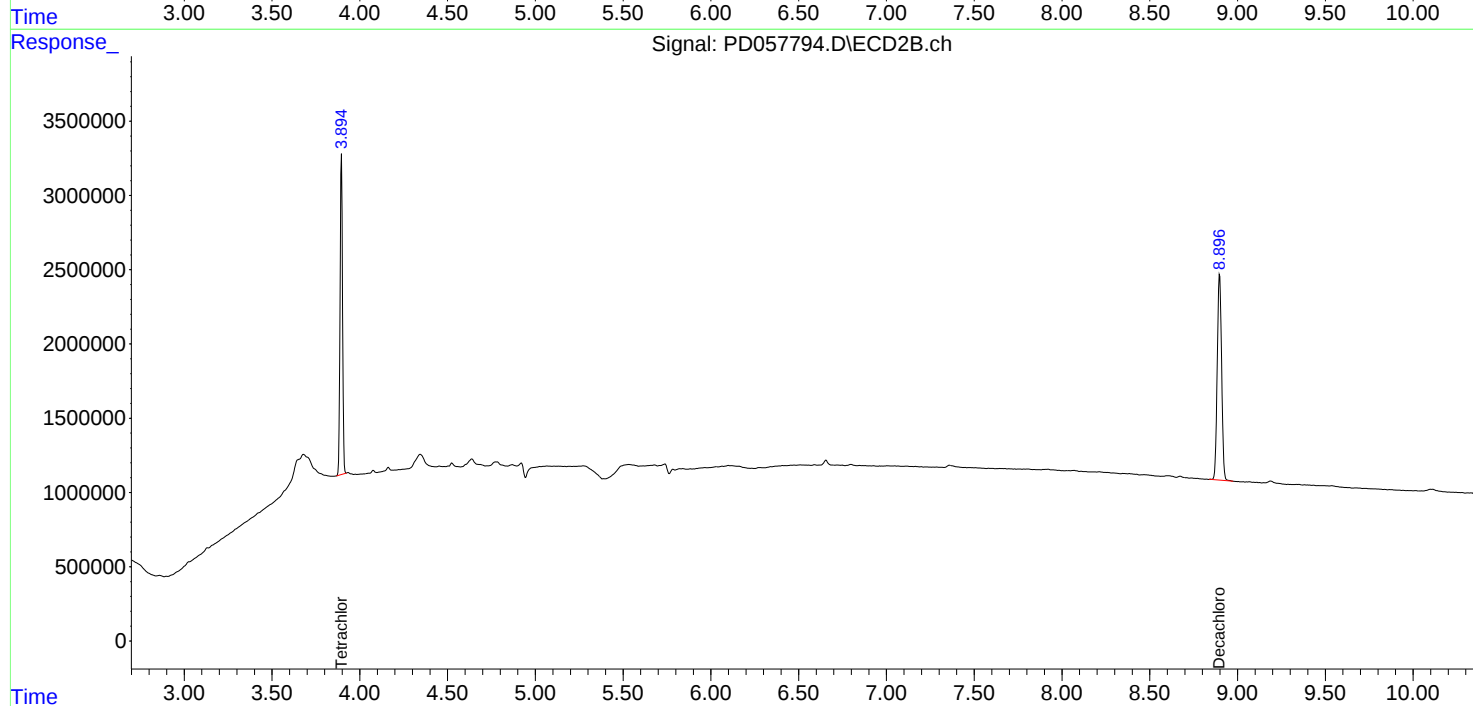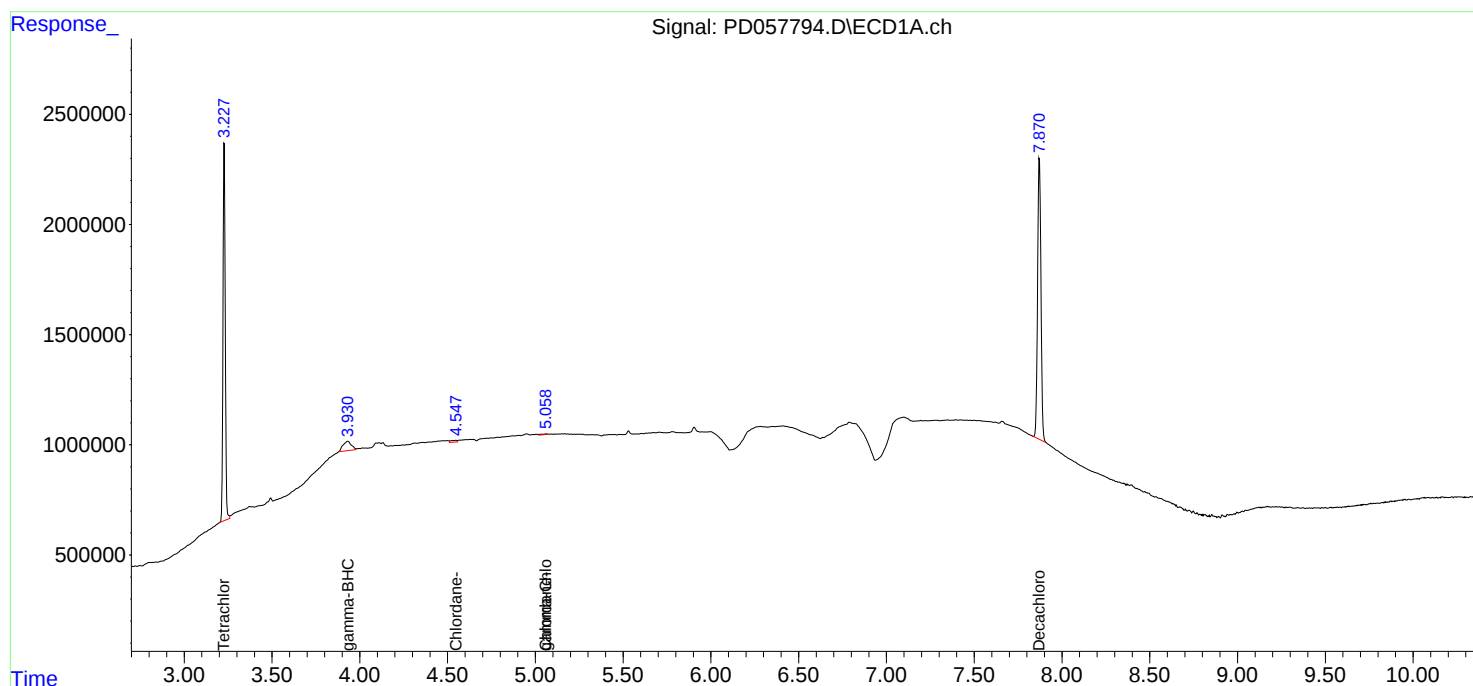


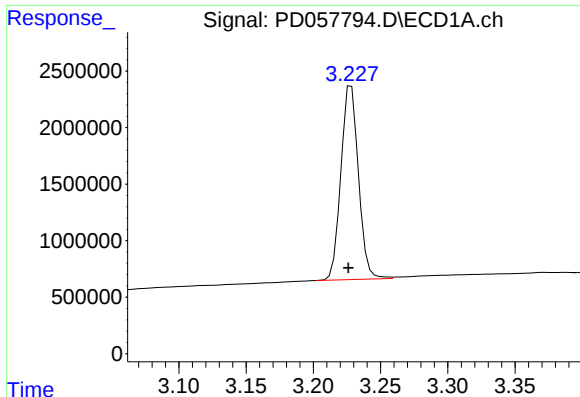

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.002 min
Response: 15500800
Conc: 21.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

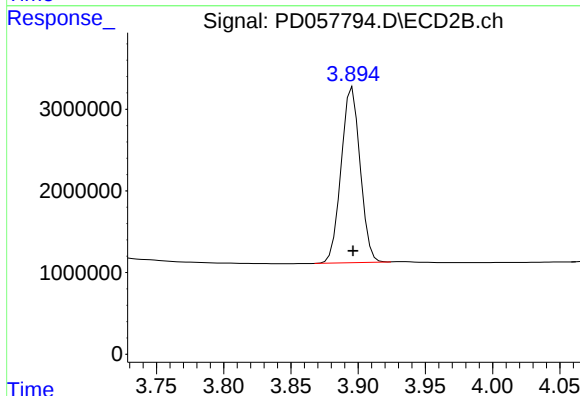


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 21025350
Conc: 26.80 ng/ml

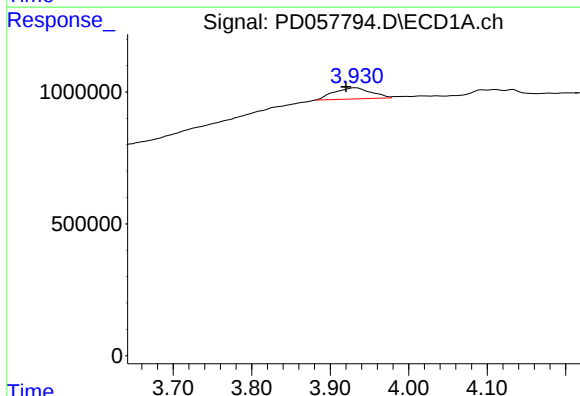


#3 gamma-BHC (Lindane)

R.T.: 3.932 min
Delta R.T.: 0.012 min
Response: 1389033
Conc: 1.29 ng/ml

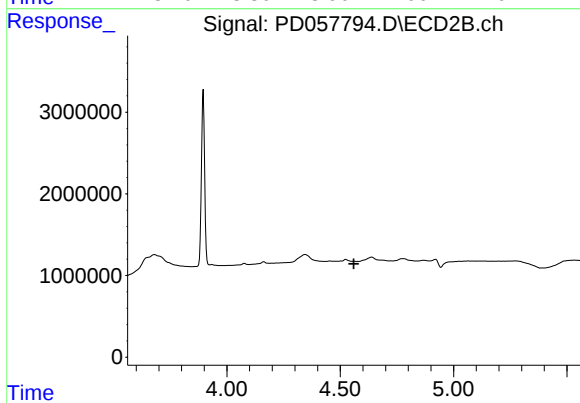

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

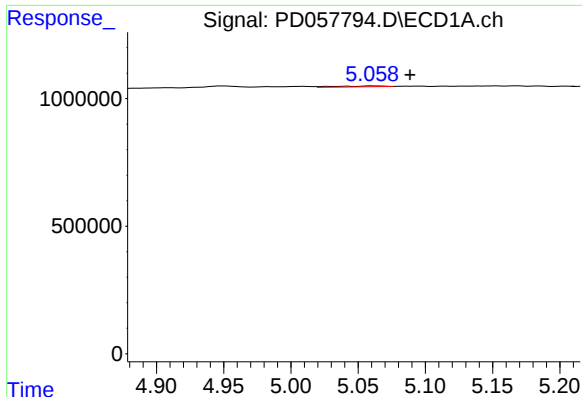

#10 gamma-Chlordane


R.T.: 5.061 min
Delta R.T.: -0.027 min
Response: 88745
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

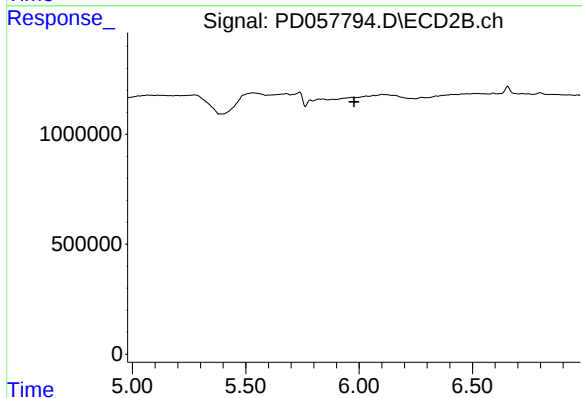


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

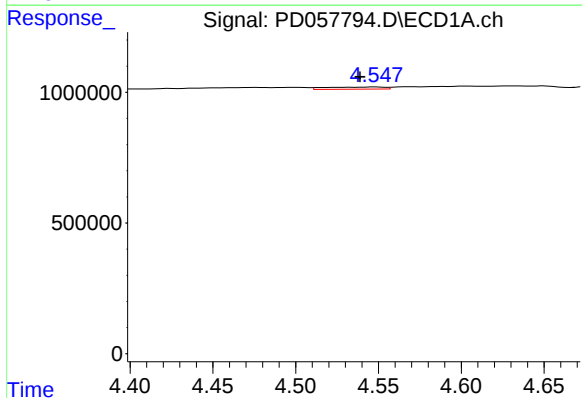


#24 Chlordane-2

R.T.: 4.548 min
Delta R.T.: 0.009 min
Response: 199912
Conc: 6.97 ng/ml

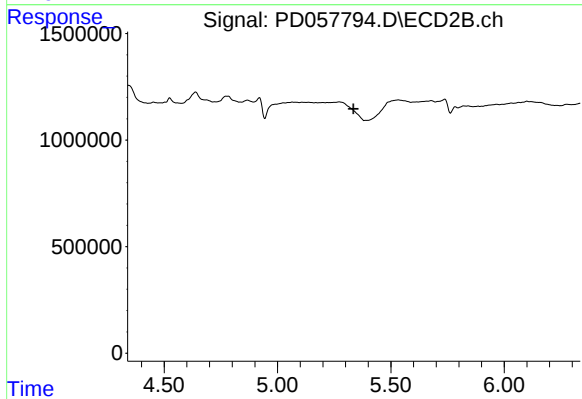

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

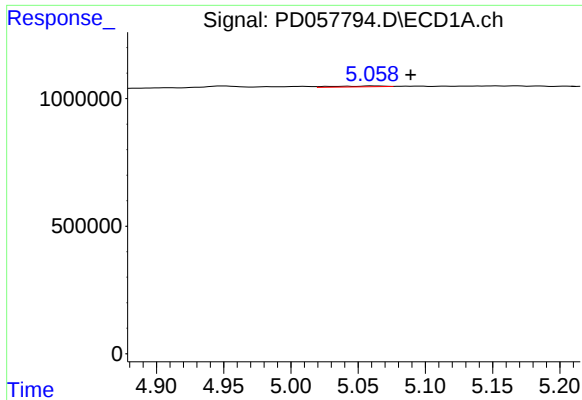

#25 Chlordane-3


R.T.: 5.061 min
Delta R.T.: -0.028 min
Response: 88745
Conc: 1.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

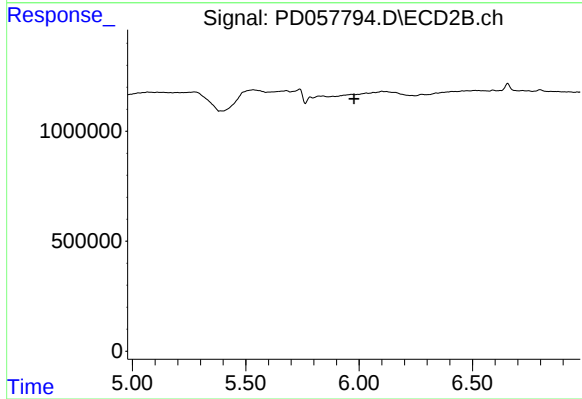


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

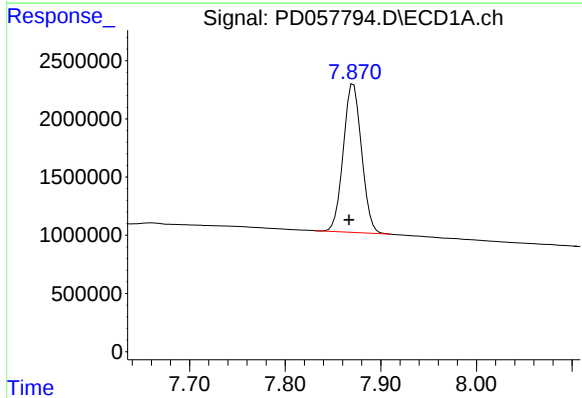

#28 Decachlorobiphenyl

R.T.: 7.871 min
Delta R.T.: 0.005 min
Response: 16962371
Conc: 22.28 ng/ml

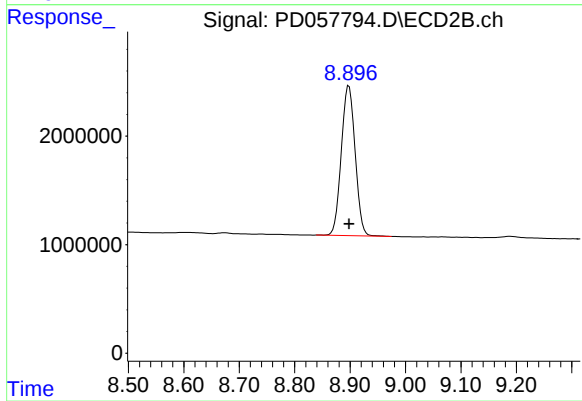

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 23991460
Conc: 27.28 ng/ml