

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
 Data File : PD057785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 15:08
 Operator : AJ\MA
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:03:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 15:53:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.231	3.895	32986009	45532355	46.306	56.948
7) SA Decachlor...	7.875	8.898	40081840	48042434	51.821	53.508
Target Compounds						
2) Toxaphene-1	5.622	6.444	3970068	6432053	462.217	568.808
3) Toxaphene-2	5.998	6.736	6590481	7226308	453.536	558.323
4) Toxaphene-3	6.239	7.024	6512894	15244305	447.983	559.757
5) Toxaphene-4	6.376	7.108	2969788	9519239	482.614	568.936
6) Toxaphene-5	6.657	7.520	2491595	9042756	492.396	554.256

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
Data File : PD057785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 15:08
Operator : AJ\MA
Sample : PTOXCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:03:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 15:53:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

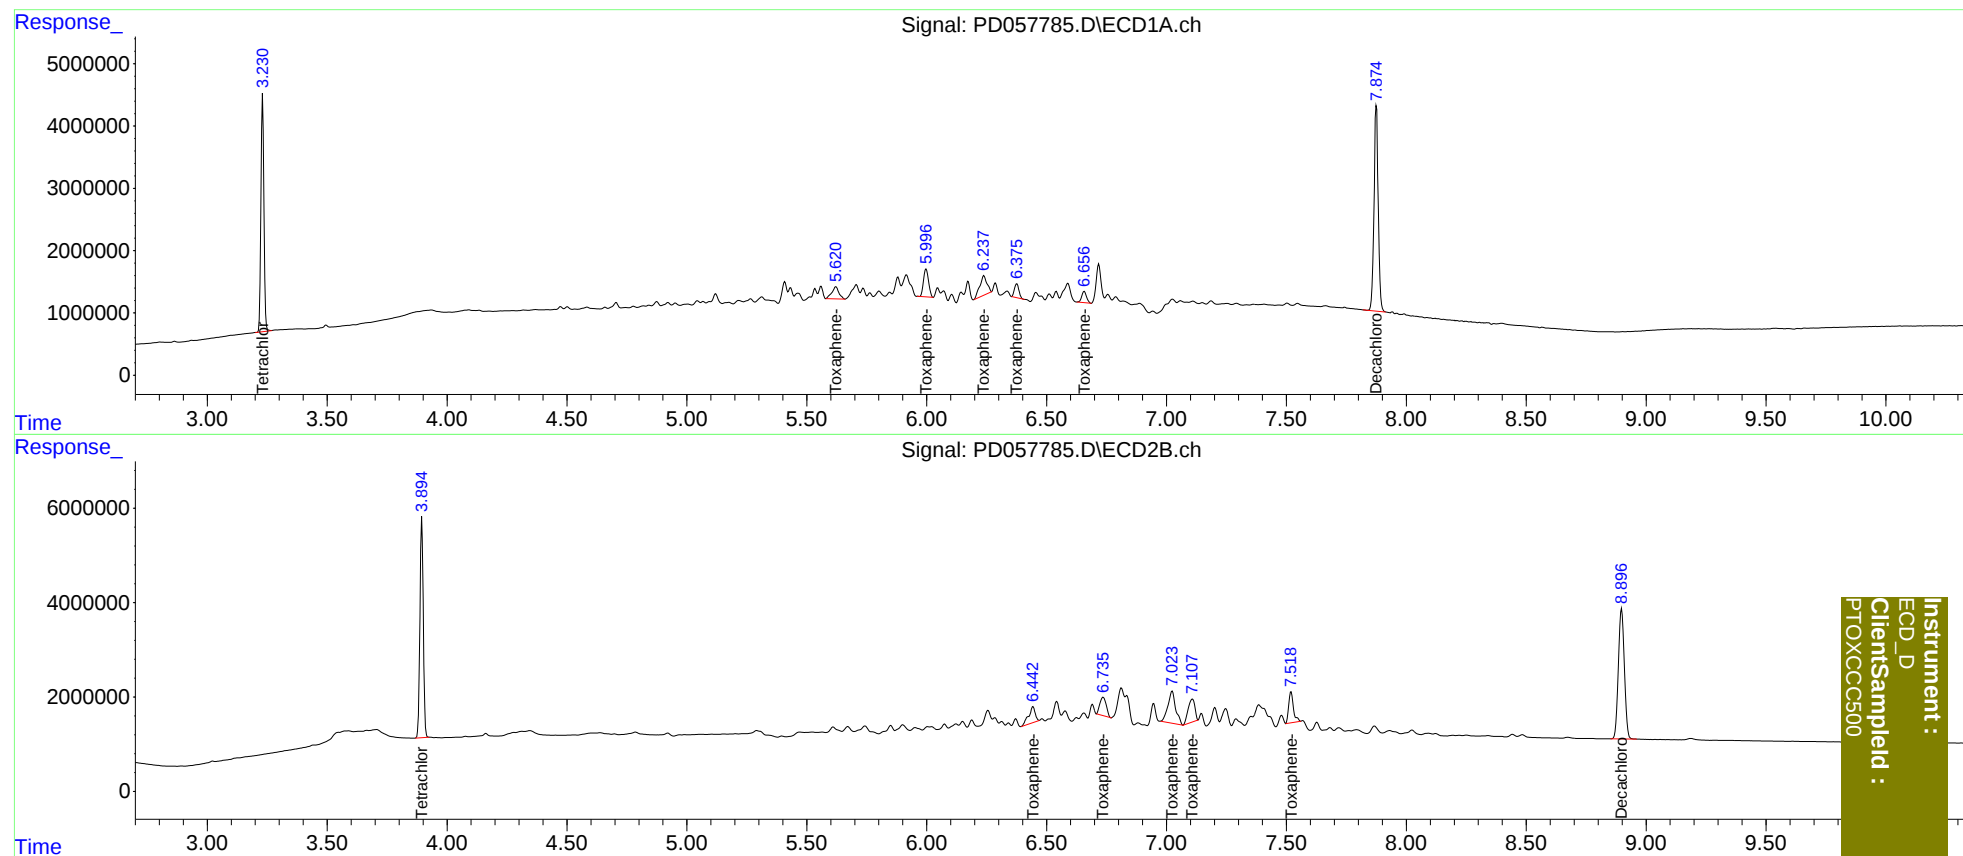

Instrument :
ECD_D
ClientSampled :
PTOXC500