

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
 Data File : PD057793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 18:36
 Operator : AJ\MA
 Sample : L2245-22 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-21A

Manual Integrations
 APPROVED

mohammad
 4/21/2020 8:26:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 07:56:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 15:53:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.229	3.913f	244374	326671	0.343	0.409m
7) SA Decachlor...	7.871	8.917f	1500604	2023003	1.940	2.253
Target Compounds						
2) Toxaphene-1	5.601	6.429f	2128721	1648623	247.837	145.793 #
3) Toxaphene-2	5.990	6.724f	1741732	636262	119.860	49.159 #
4) Toxaphene-3	6.217	7.027	3246796	10848021	223.328	398.330 #
5) Toxaphene-4	6.373	7.128f	3029463	9216456	492.312m	550.840
6) Toxaphene-5	6.651	7.503f	1242515	1250463	245.550	76.644 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
Data File : PD057793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 18:36
Operator : AJ\MA
Sample : L2245-22 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 07:56:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 15:53:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

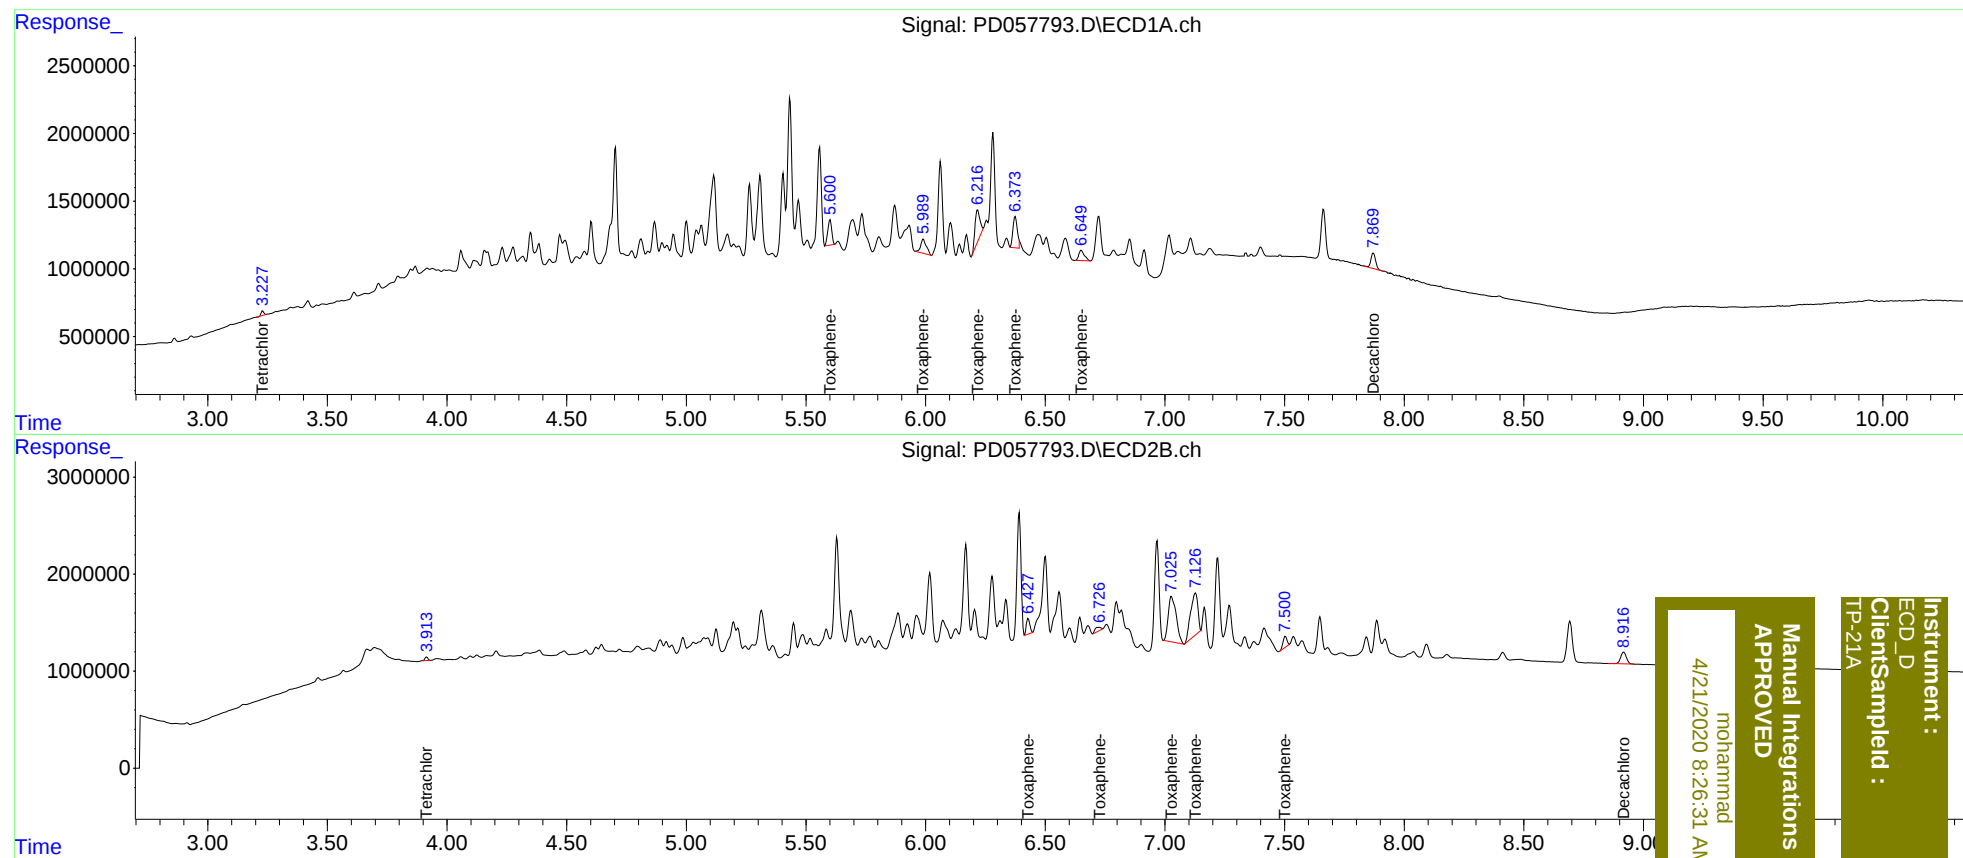

Manual Integrations
APPROVED

4/21/2020 8:26:31 AM
mohammad

Instrument :
ECD_D
ClientSampled :
TP-21A