

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
 Data File : PD057796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 19:19
 Operator : AJ\MA
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

mohammad
 4/21/2020 8:26:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:04:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 27 15:53:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.228	3.896	34673237	46681757	48.675	58.386
7) SA Decachlor...	7.872	8.898	36752812	49165472	47.517	54.759
Target Compounds						
2) Toxaphene-1	5.619	6.444	4443786	6680023	517.370	590.737
3) Toxaphene-2	5.994	6.738	7034607	7278291	484.099	562.339
4) Toxaphene-3	6.237	7.024	7046011	15777430	484.653	579.333
5) Toxaphene-4	6.373	7.108	3195555	9789064	519.303	585.063
6) Toxaphene-5	6.654	7.519	2690639	9326359	531.732	571.639m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041720\
Data File : PD057796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 19:19
Operator : AJ\MA
Sample : PTOXCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:04:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX032720.M
Quant Title : GC Extractables
QLast Update : Fri Mar 27 15:53:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

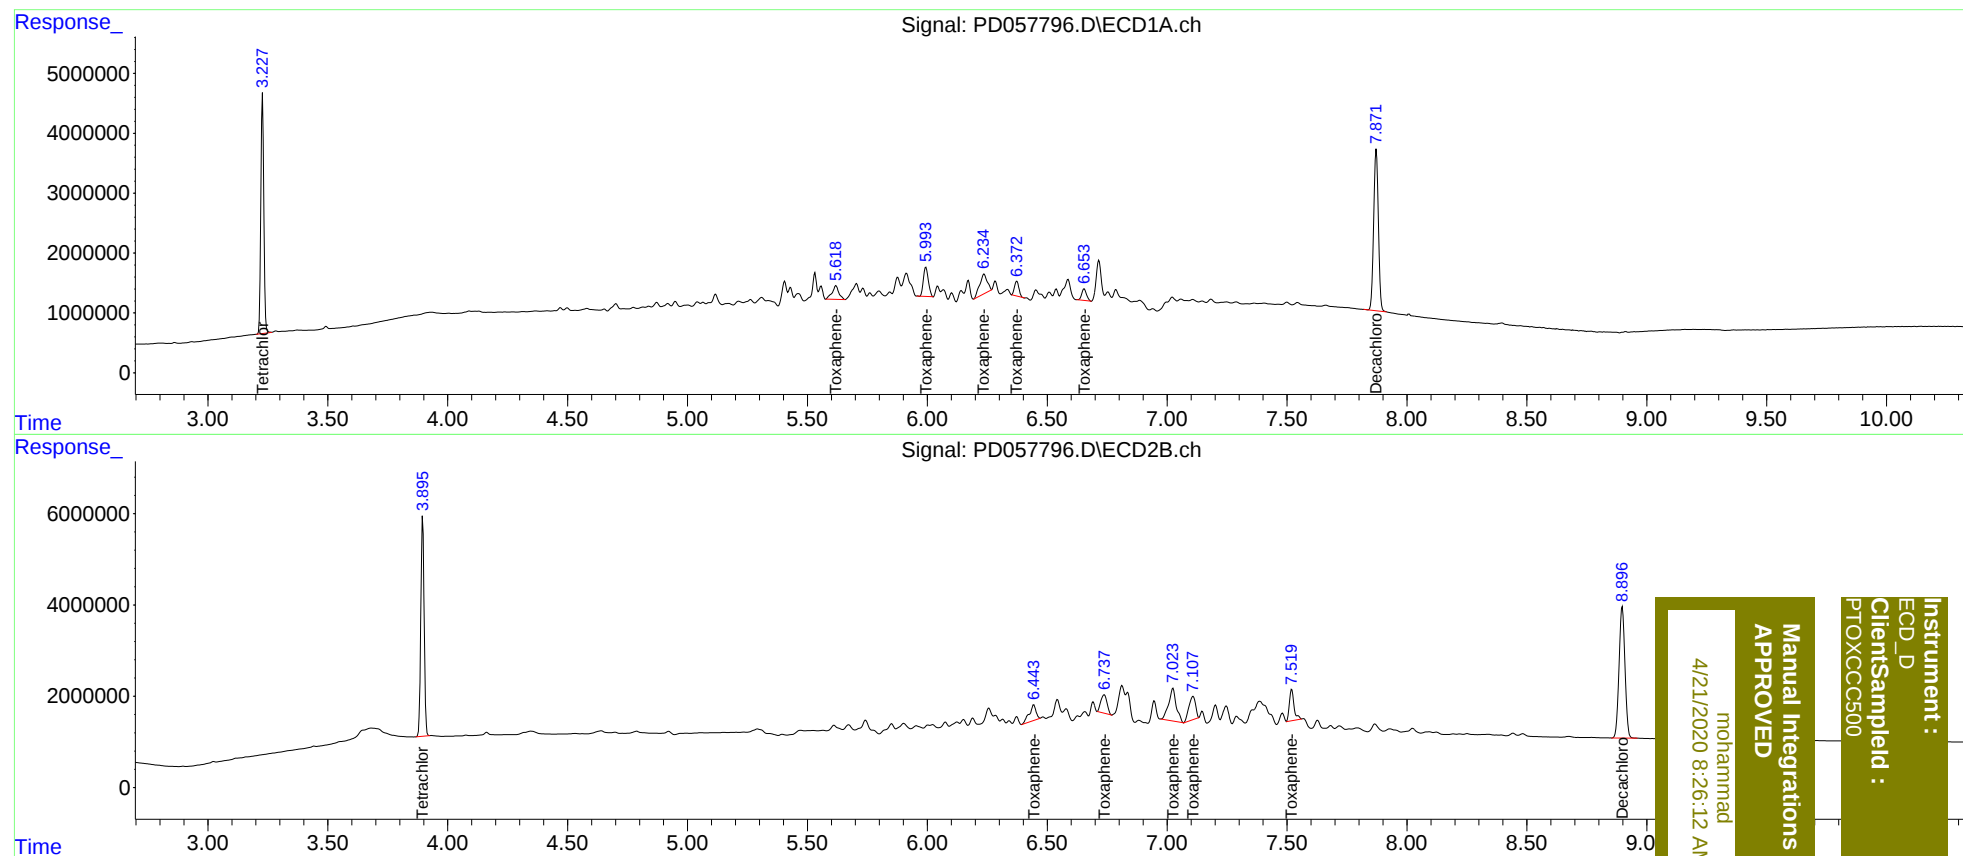

Manual Integrations
APPROVED

mohammad
4/21/2020 8:26:12 AM

Instrument :
ECD_D
Client Sampled :
PTOXCCC500