

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041722\
 Data File : PD069152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 18:26
 Operator : AR\AJ
 Sample : PB144144BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 01:54:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	21849469	216.7E6	17.245	17.954
27)	SA Decachlor...	8.201	9.365	47692523	261.1E6	35.865	37.124
Target Compounds							
3)	MA gamma-BHC...	4.172	0.000	1375320	0	0.760	N.D. #
7)	B delta-BHC	0.000	5.225	0	2078188	N.D.	0.177
8)	B Heptachlo...	0.000	6.070	0	4991341	N.D.	0.448
9)	A Endosulfan I	0.000	6.462	0	291729	N.D.	<MDL
10)	B trans-Chl...	0.000	6.276f	0	1482330	N.D.	0.117
11)	B cis-Chlor...	0.000	6.462f	0	291729	N.D.	<MDL
12)	B 4,4'-DDE	0.000	6.613f	0	1412550	N.D.	0.130
20)	A Methoxychlor	0.000	7.739f	0	3249979	N.D.	0.789
21)	B Endrin ke...	7.155	7.963	210196	353142	0.145	<MDL #
22)	Toxaphene-1	0.000	6.613	0	1412550	N.D.	29.945


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041722\
Data File : PD069152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 18:26
Operator : AR\AJ
Sample : PB144144BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 01:54:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

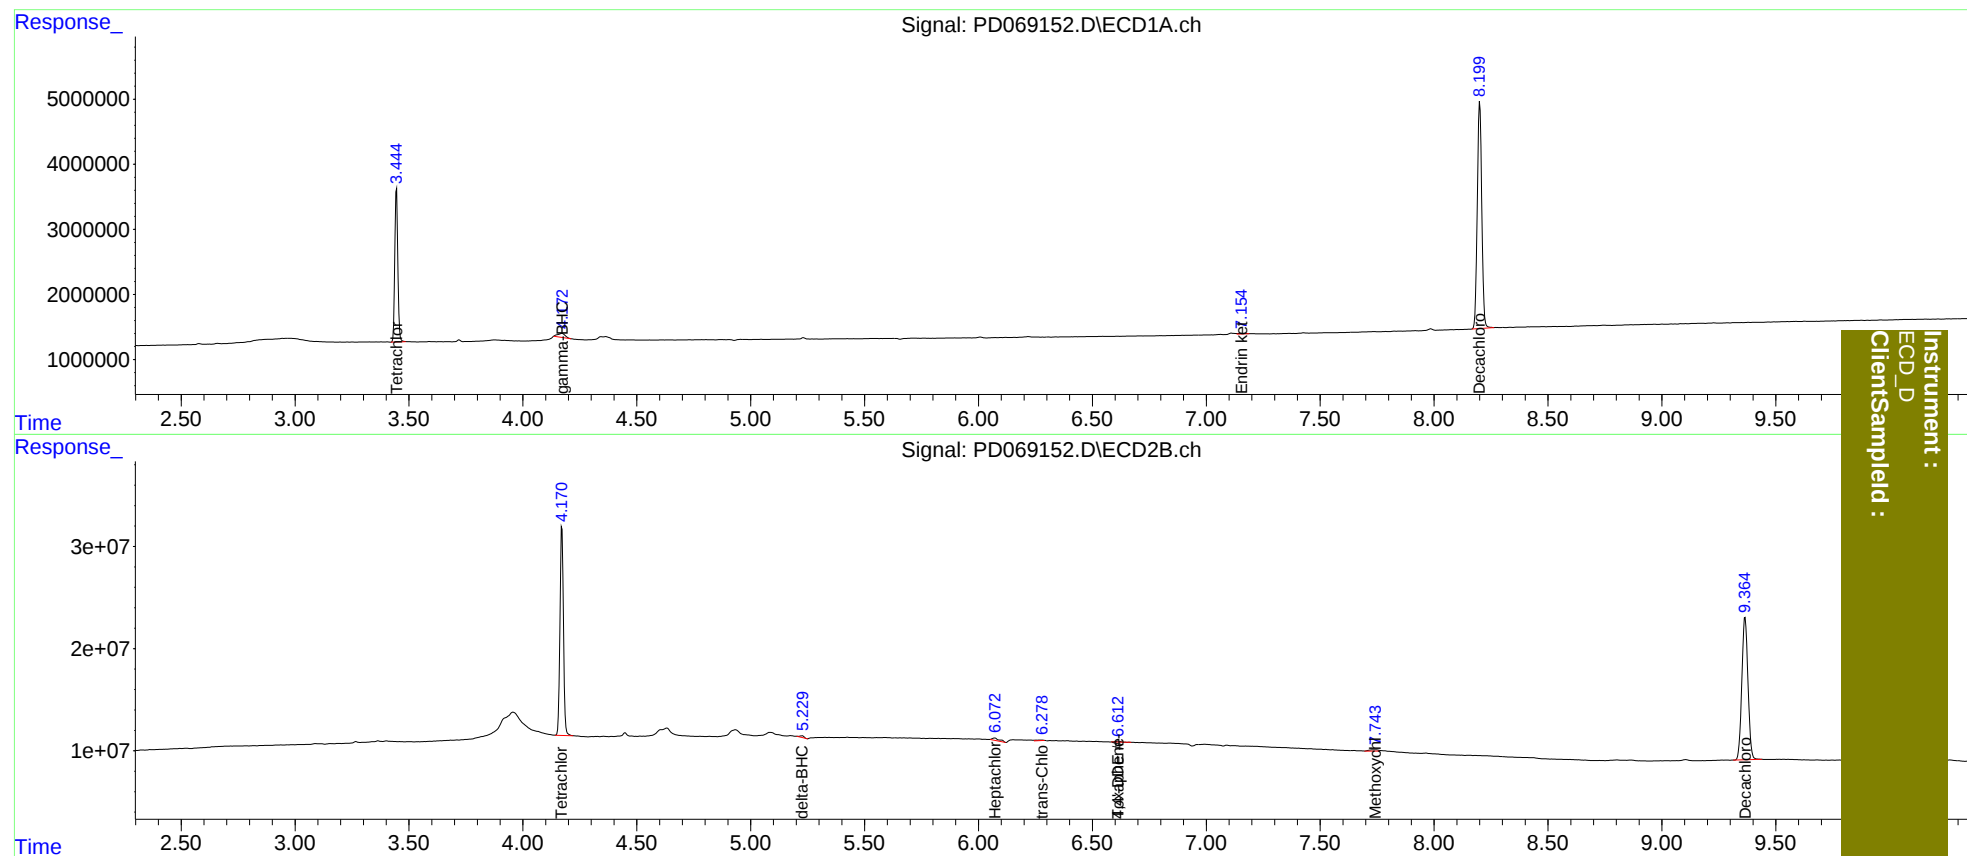


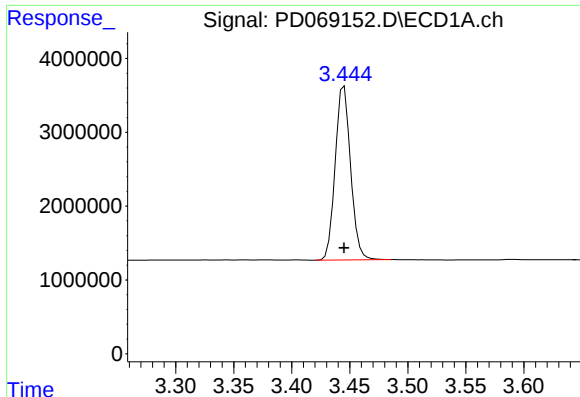

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 21849469
Conc: 17.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

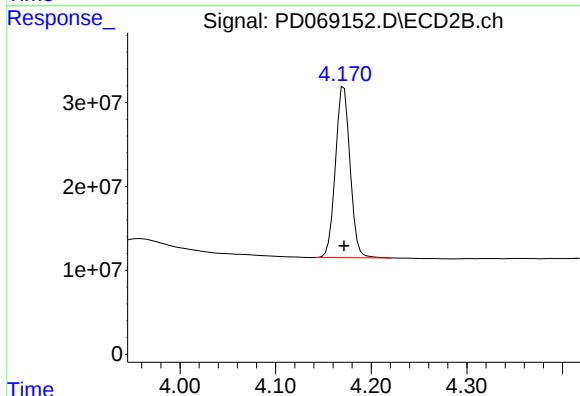


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 216692774
Conc: 17.95 ng/ml

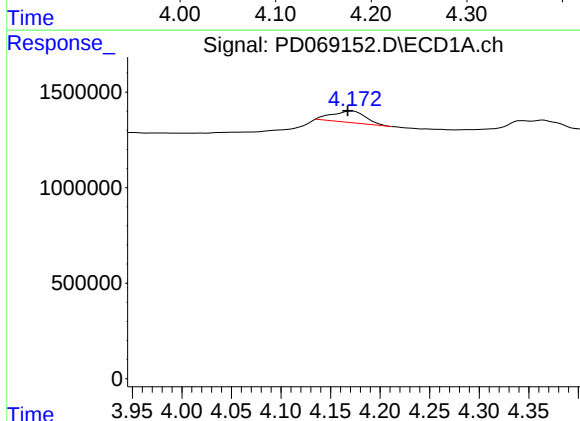


#3 gamma-BHC (Lindane)

R.T.: 4.172 min
Delta R.T.: 0.004 min
Response: 1375320
Conc: 0.76 ng/ml

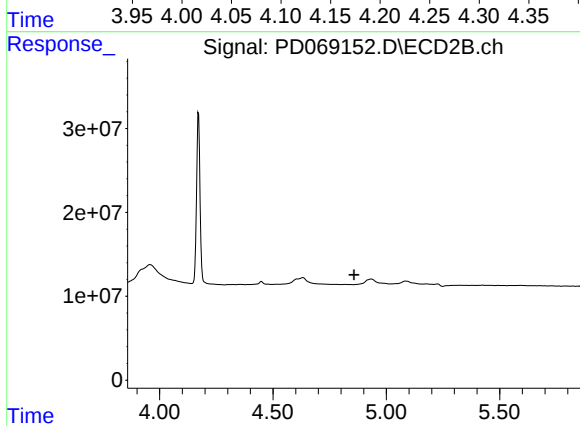

#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.859 min
Response: 0
Conc: N.D.

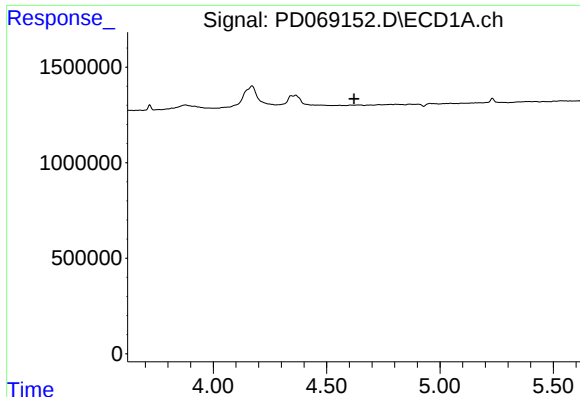

#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.621 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

#7 delta-BHC


R.T.: 5.225 min
Delta R.T.: -0.021 min
Response: 2078188
Conc: 0.18 ng/ml

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.157 min
Response: 0
Conc: N.D.

#8 Heptachlor epoxide


R.T.: 6.070 min
Delta R.T.: -0.016 min
Response: 4991341
Conc: 0.45 ng/ml

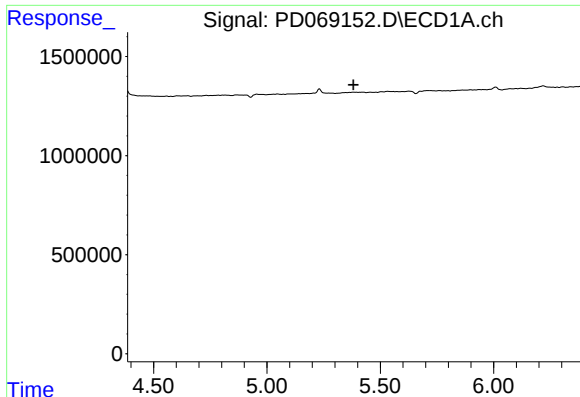

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

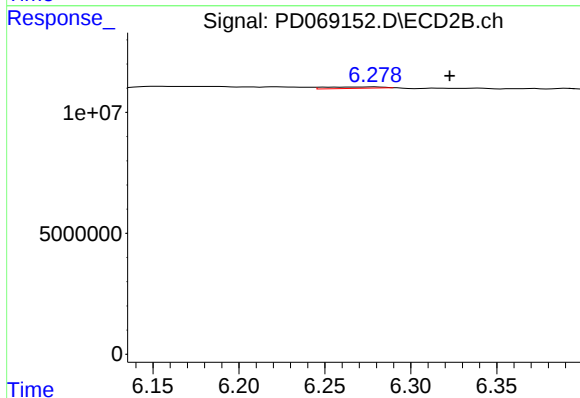


#10 trans-Chlordane

R.T.: 6.276 min
Delta R.T.: -0.047 min
Response: 1482330
Conc: 0.12 ng/ml

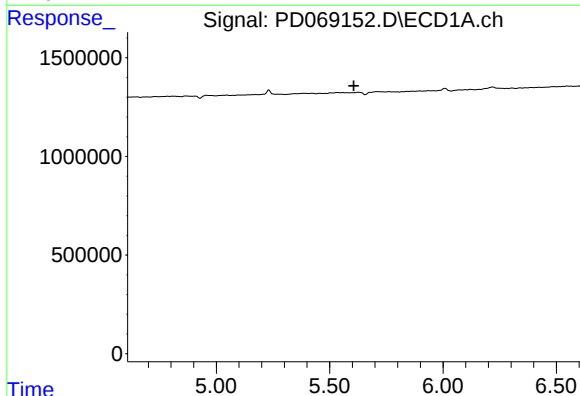


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.606 min
Response: 0
Conc: N.D.

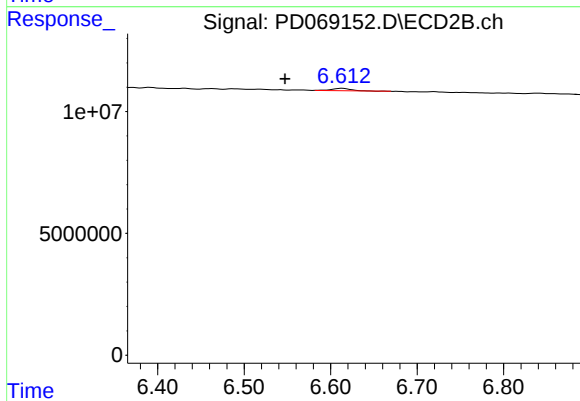

#12 4,4'-DDE


R.T.: 6.613 min
Delta R.T.: 0.066 min
Response: 1412550
Conc: 0.13 ng/ml

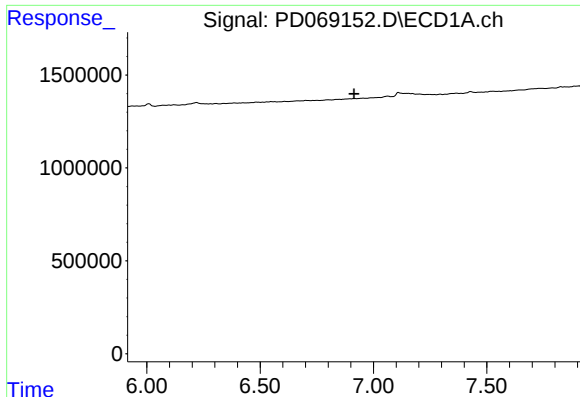

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

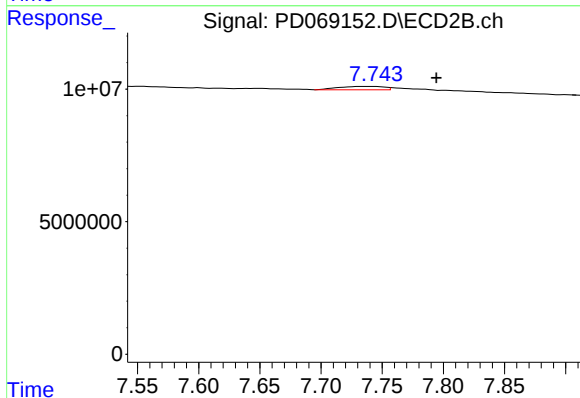


#20 Methoxychlor

R.T.: 7.739 min
Delta R.T.: -0.055 min
Response: 3249979
Conc: 0.79 ng/ml

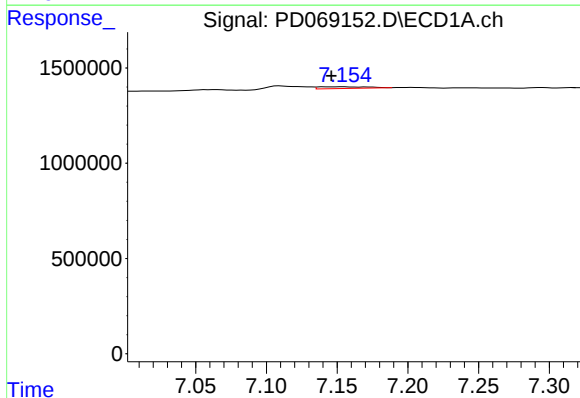


#21 Endrin ketone

R.T.: 7.155 min
Delta R.T.: 0.009 min
Response: 210196
Conc: 0.15 ng/ml

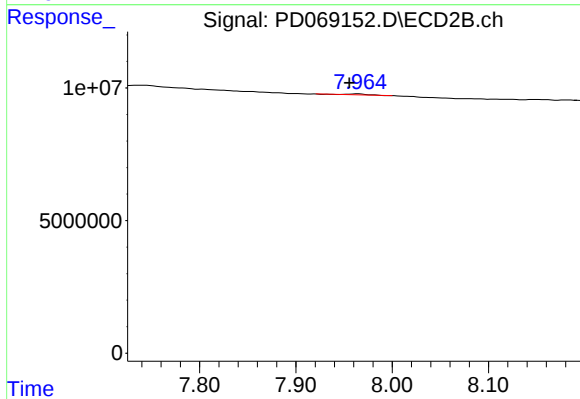

#21 Endrin ketone


R.T.: 7.963 min
Delta R.T.: 0.008 min
Response: 353142
Conc: N.D.

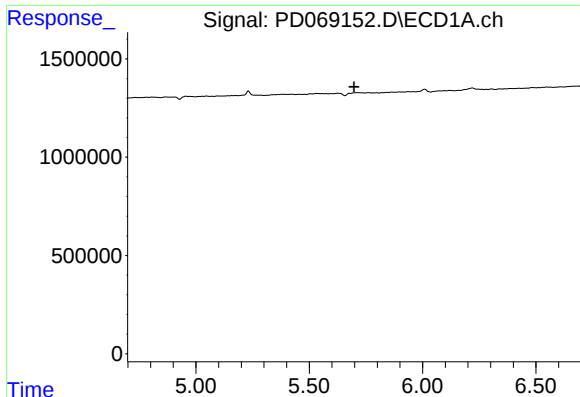

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.697 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

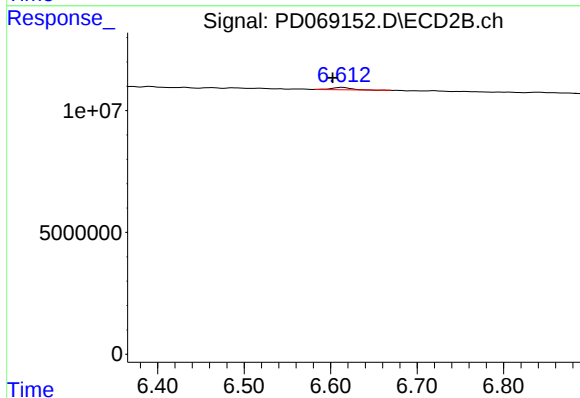


#22 Toxaphene-1

R.T.: 6.613 min
Delta R.T.: 0.011 min
Response: 1412550
Conc: 29.94 ng/ml

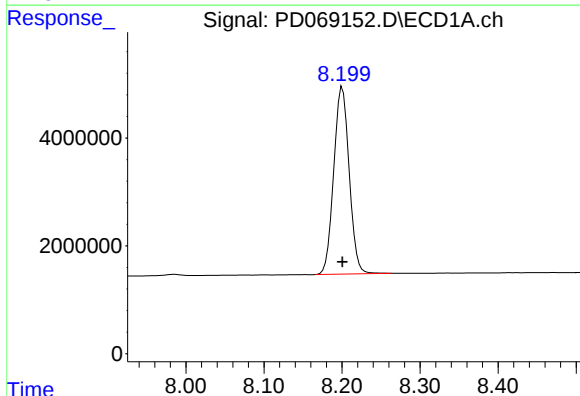

#27 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 47692523
Conc: 35.86 ng/ml

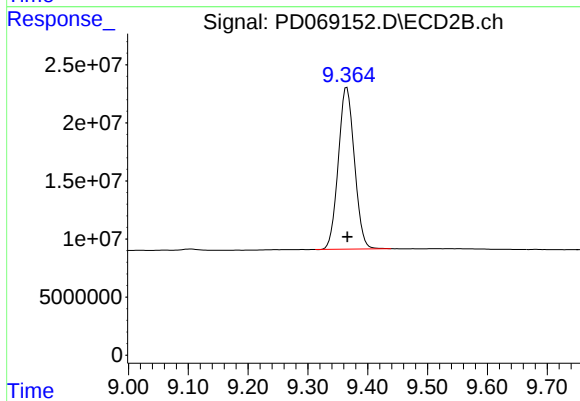

#27 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.000 min
Response: 261060010
Conc: 37.12 ng/ml