

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
 Data File : PD069166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 09:05
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:42:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:40:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.170	22695190	231.4E6	20.444	21.584
28)	SA Decachlor...	8.199	9.362	23944156	137.7E6	19.176	21.036
Target Compounds							
2)	A alpha-BHC	3.883	4.565	15898222	169.5E6	9.743	10.993
3)	MA gamma-BHC...	4.167	4.856	16758513	154.5E6	9.797	10.942
4)	MA Heptachlor	0.000	5.401f	0	103630	N.D.	0.008 #
5)	MB Aldrin	4.711	5.717f	135664	164020	0.093	0.012 #
6)	B beta-BHC	4.417	5.019	7849254	73139734	11.290	11.905
7)	B delta-BHC	0.000	5.220f	0	1325616	N.D.	0.099 #
8)	B Heptachlo...	0.000	6.058f	0	1698454	N.D.	0.144 #
11)	B alpha-Chl...	0.000	6.398	0	1325563	N.D.	0.116 #
12)	B 4,4'-DDE	5.606	6.544	566375	6850684	0.448	0.634 #
13)	MA Dieldrin	0.000	6.704	0	2188903	N.D.	0.196 #
14)	MA Endrin	5.996	6.924	57718515	440.4E6	47.738	48.551
15)	B Endosulfa...	6.272	7.129	814254	31970251	0.704	3.695 #
16)	A 4,4'-DDD	6.123	7.036	3593596	61970540	3.297	7.195 #
17)	MA 4,4'-DDT	6.363	7.339	104.0E6	747.6E6	96.690	86.187
18)	B Endrin al...	6.438	7.254	1631092	17394046	1.767	2.516 #
20)	A Methoxychlor	6.914	7.792	133.7E6	841.1E6	210.396	195.097
21)	B Endrin ke...	7.144	7.953	3721979	25819613	2.643	2.856
23)	Chlordane-1	0.000	5.167f	0	631473	N.D.	1.315 #
26)	Chlordane-4	0.000	6.398	0	1325563	N.D.	0.699 #
27)	Chlordane-5	6.272	0.000	814254	0	18.005	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
Data File : PD069166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 09:05
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:42:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:40:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

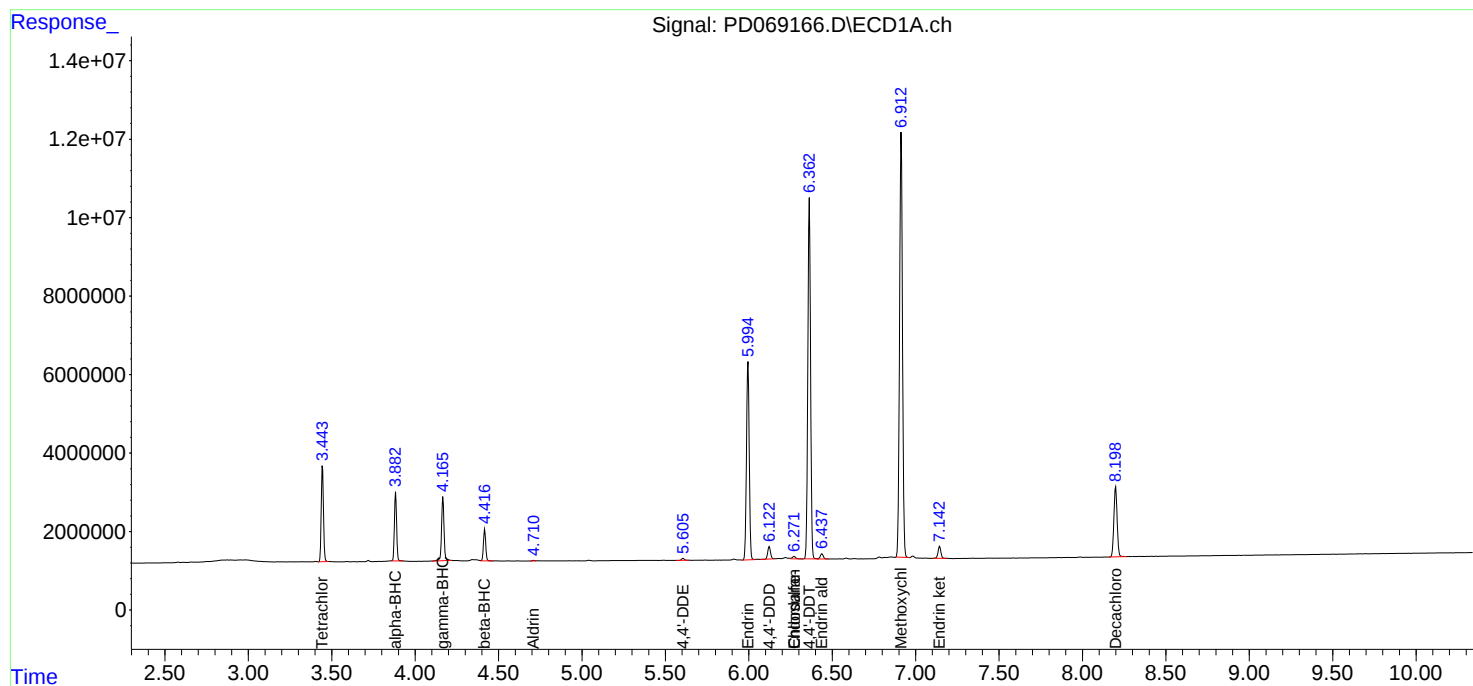


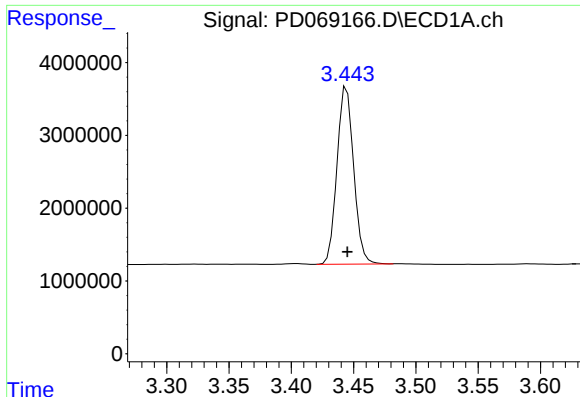

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 22695190
Conc: 20.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

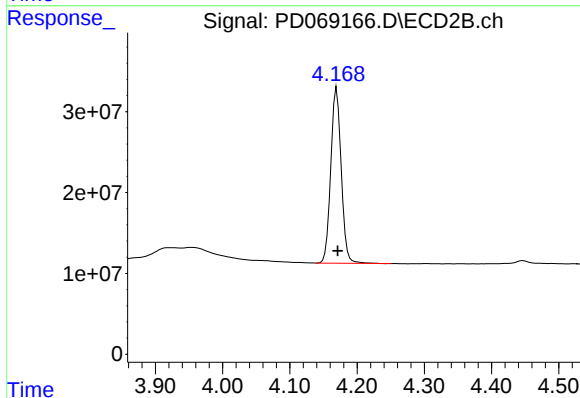


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: -0.002 min
Response: 231419646
Conc: 21.58 ng/ml

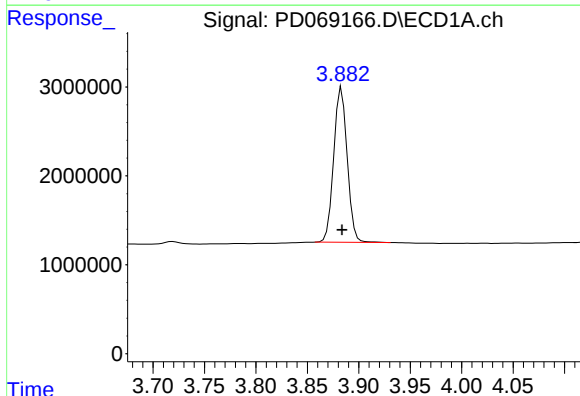


#2 alpha-BHC

R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 15898222
Conc: 9.74 ng/ml

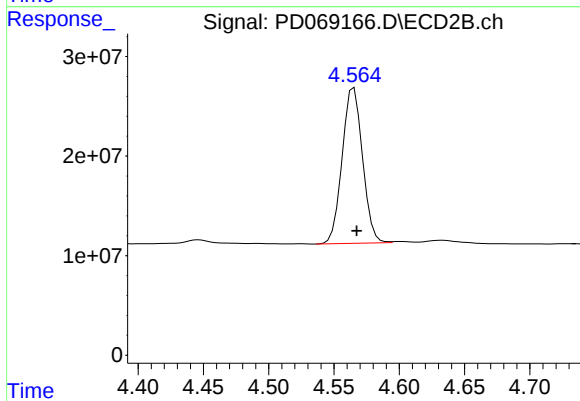

#2 alpha-BHC


R.T.: 4.565 min
Delta R.T.: -0.002 min
Response: 169519952
Conc: 10.99 ng/ml

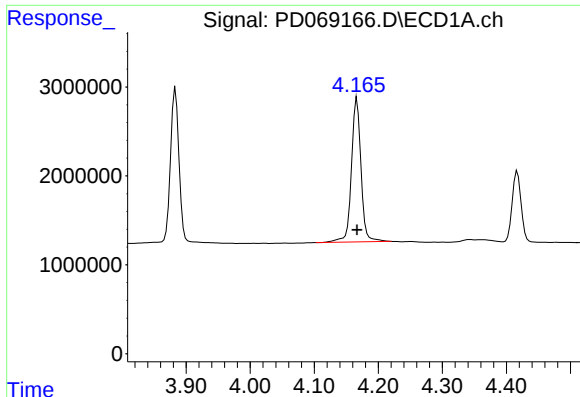

#3 gamma-BHC (Lindane)


R.T.: 4.167 min
Delta R.T.: 0.000 min
Response: 16758513
Conc: 9.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

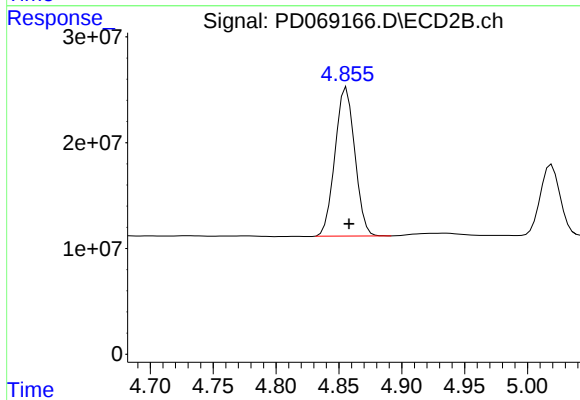


#3 gamma-BHC (Lindane)

R.T.: 4.856 min
Delta R.T.: -0.002 min
Response: 154510479
Conc: 10.94 ng/ml

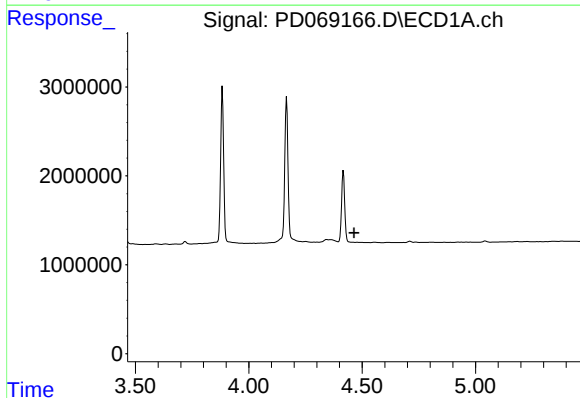


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.465 min
Response: 0
Conc: N.D.

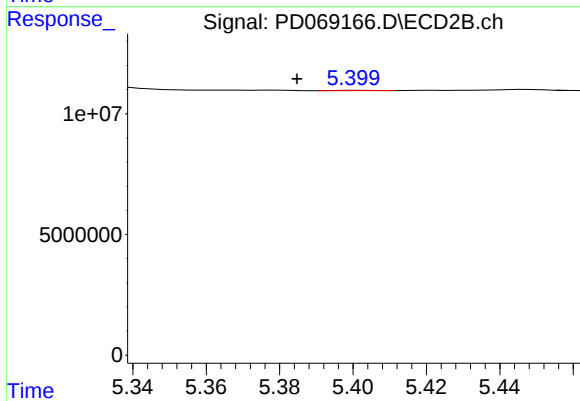

#4 Heptachlor


R.T.: 5.401 min
Delta R.T.: 0.016 min
Response: 103630
Conc: 0.01 ng/ml

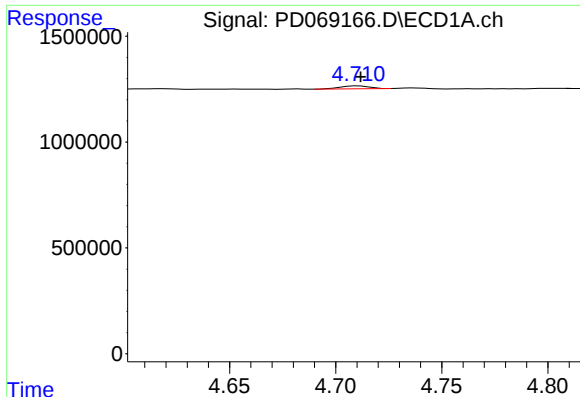

#5 Aldrin


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 135664
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

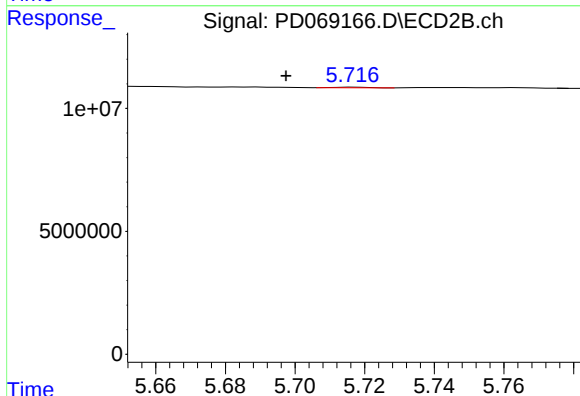


#5 Aldrin

R.T.: 5.717 min
Delta R.T.: 0.020 min
Response: 164020
Conc: 0.01 ng/ml

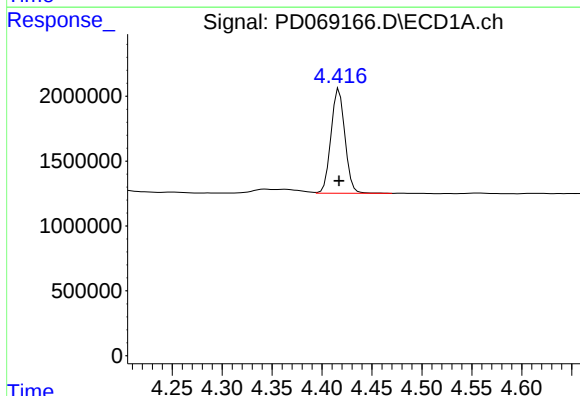


#6 beta-BHC

R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 7849254
Conc: 11.29 ng/ml

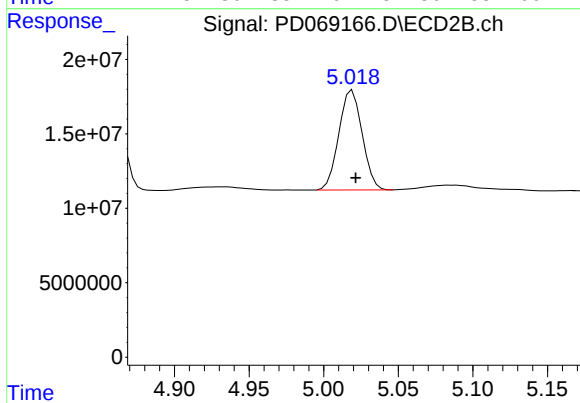

#6 beta-BHC


R.T.: 5.019 min
Delta R.T.: -0.002 min
Response: 73139734
Conc: 11.91 ng/ml

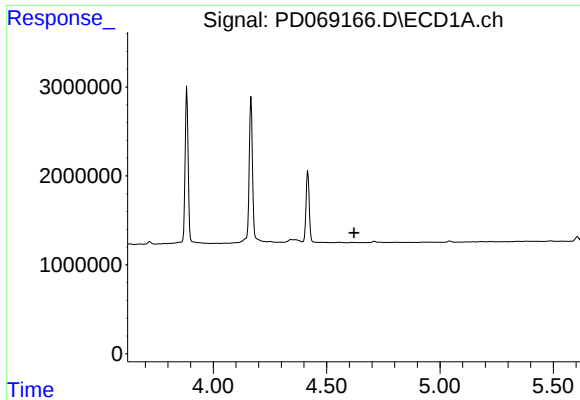

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.621 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

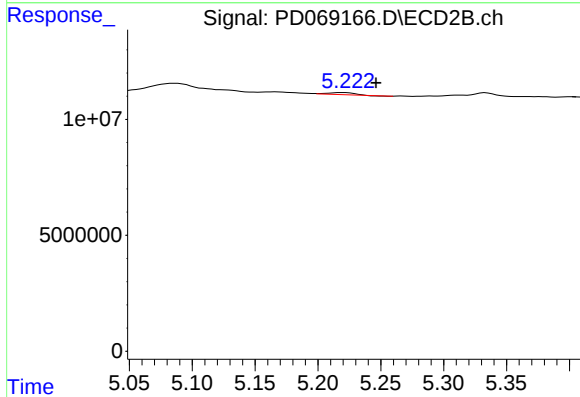


#7 delta-BHC

R.T.: 5.220 min
Delta R.T.: -0.026 min
Response: 1325616
Conc: 0.10 ng/ml

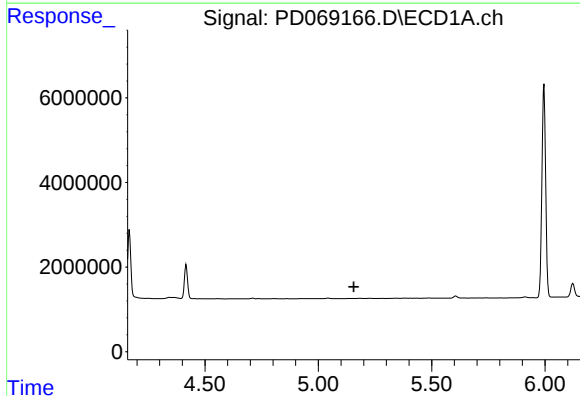


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.156 min
Response: 0
Conc: N.D.

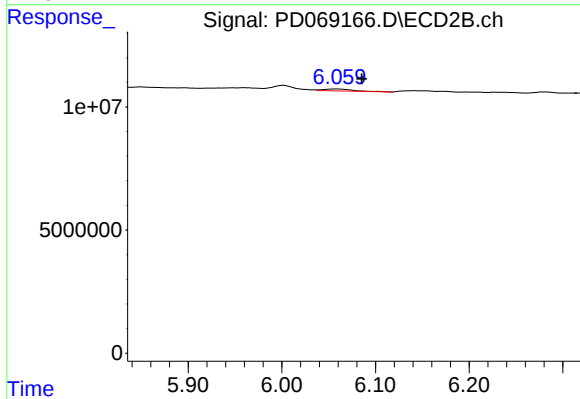

#8 Heptachlor epoxide


R.T.: 6.058 min
Delta R.T.: -0.027 min
Response: 1698454
Conc: 0.14 ng/ml

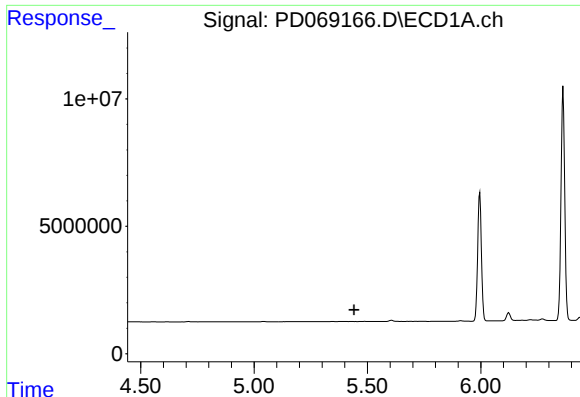

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

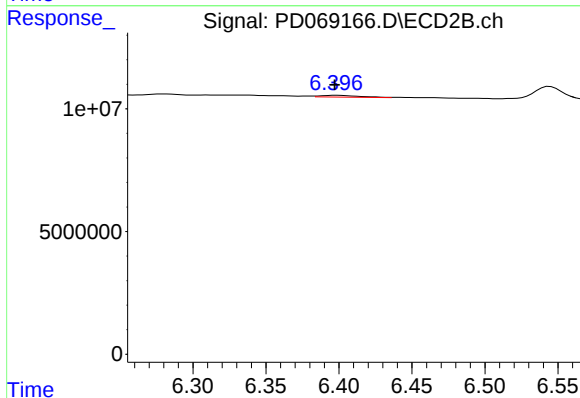


#11 alpha-Chlordane

R.T.: 6.398 min
Delta R.T.: 0.000 min
Response: 1325563
Conc: 0.12 ng/ml

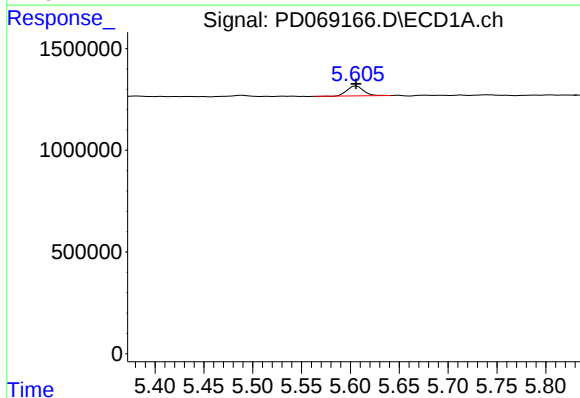


#12 4,4'-DDE

R.T.: 5.606 min
Delta R.T.: 0.000 min
Response: 566375
Conc: 0.45 ng/ml

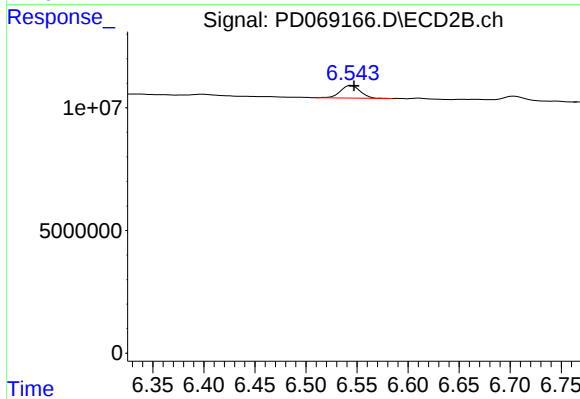

#12 4,4'-DDE


R.T.: 6.544 min
Delta R.T.: -0.003 min
Response: 6850684
Conc: 0.63 ng/ml

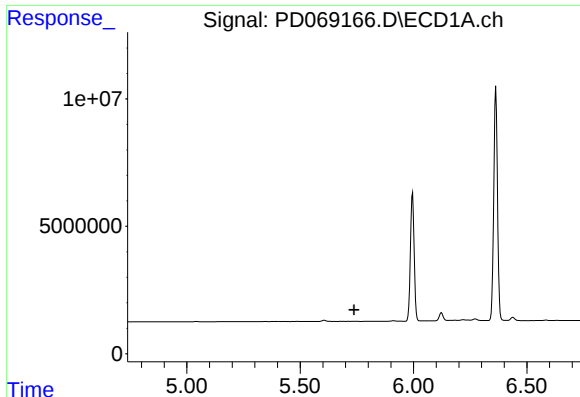

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.738 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

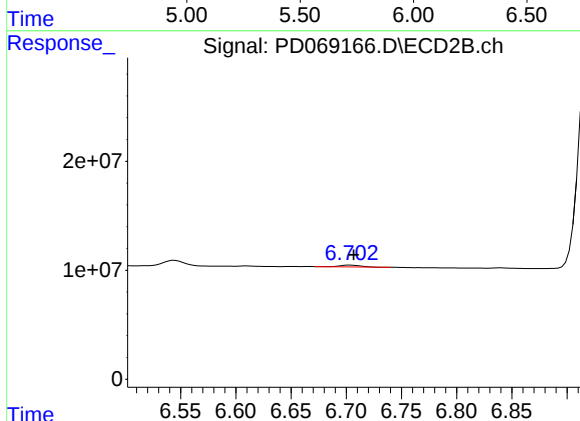


#13 Dieldrin

R.T.: 6.704 min
Delta R.T.: -0.003 min
Response: 2188903
Conc: 0.20 ng/ml

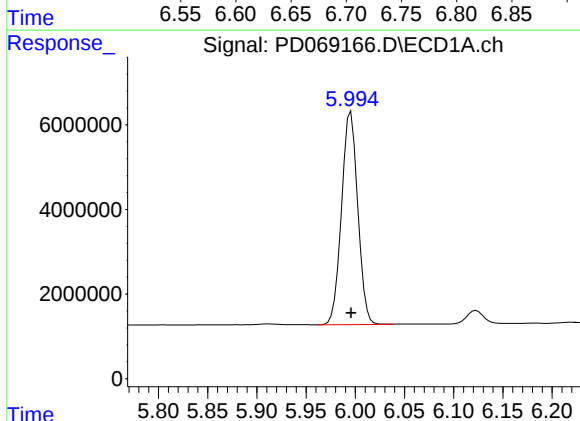


#14 Endrin

R.T.: 5.996 min
Delta R.T.: 0.000 min
Response: 57718515
Conc: 47.74 ng/ml

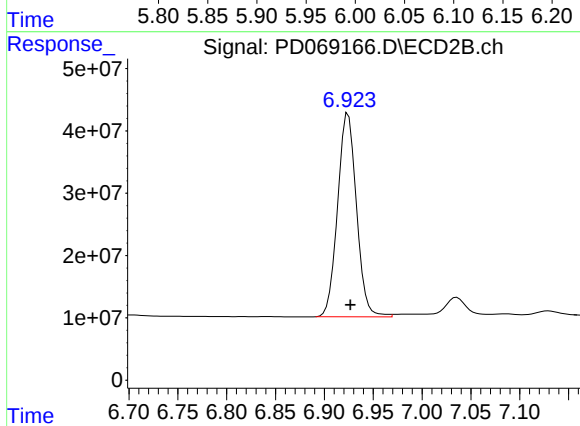

#14 Endrin


R.T.: 6.924 min
Delta R.T.: -0.002 min
Response: 440366691
Conc: 48.55 ng/ml

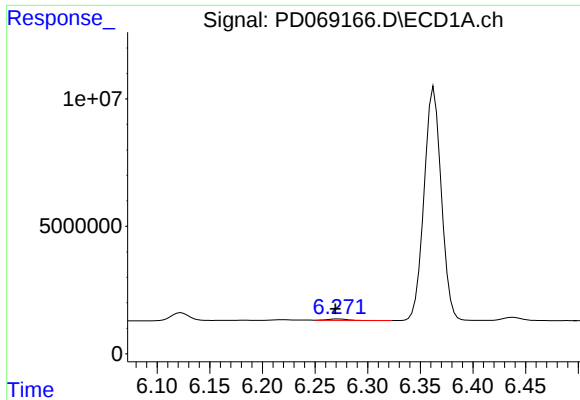

#15 Endosulfan II


R.T.: 6.272 min
Delta R.T.: 0.003 min
Response: 814254
Conc: 0.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

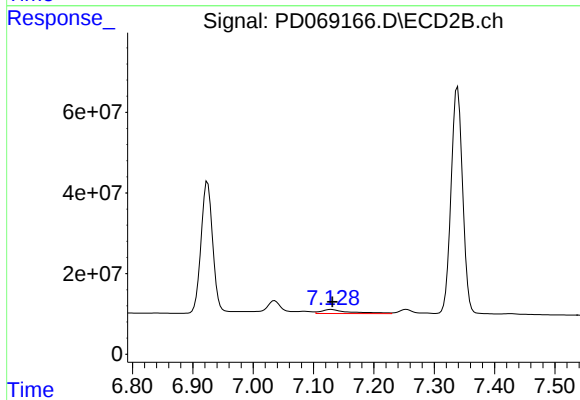


#15 Endosulfan II

R.T.: 7.129 min
Delta R.T.: -0.002 min
Response: 31970251
Conc: 3.70 ng/ml

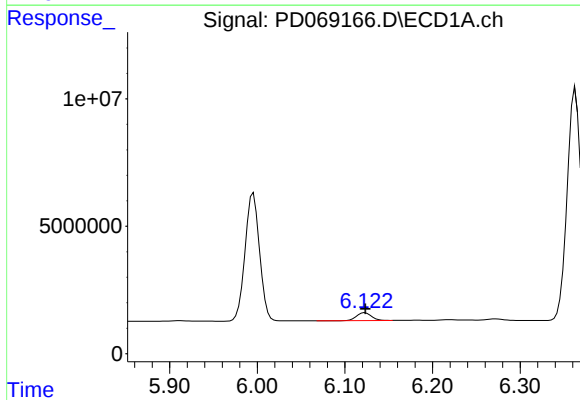


#16 4,4'-DDD

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 3593596
Conc: 3.30 ng/ml

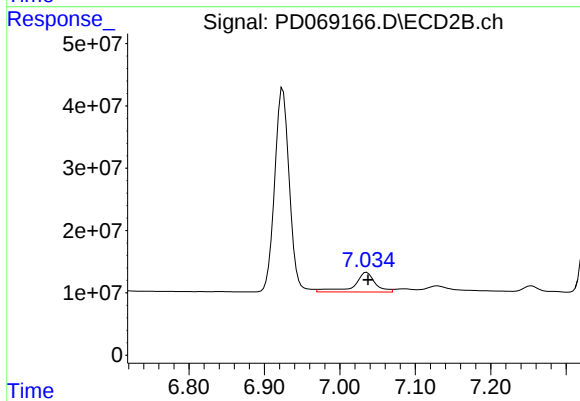

#16 4,4'-DDD


R.T.: 7.036 min
Delta R.T.: -0.002 min
Response: 61970540
Conc: 7.19 ng/ml

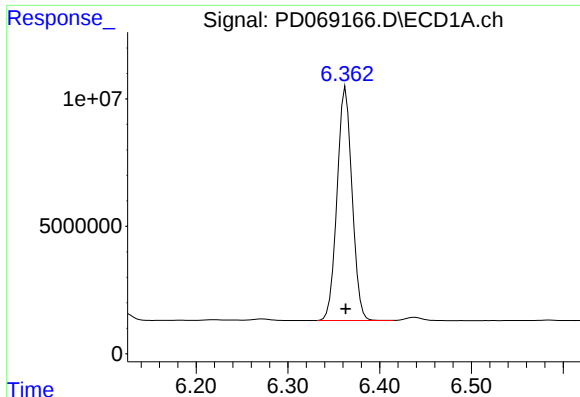

#17 4,4'-DDT


R.T.: 6.363 min
Delta R.T.: 0.000 min
Response: 103958022
Conc: 96.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

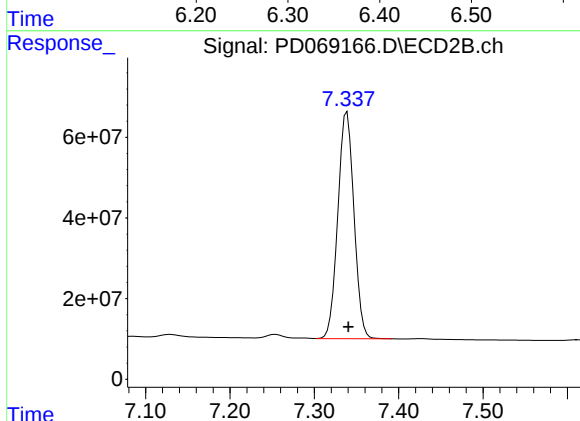


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 747565709
Conc: 86.19 ng/ml

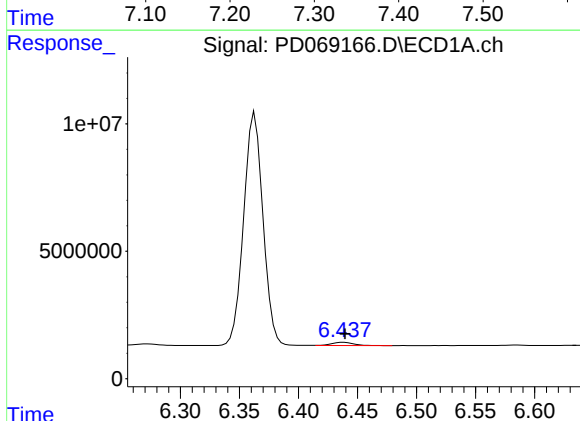


#18 Endrin aldehyde

R.T.: 6.438 min
Delta R.T.: -0.001 min
Response: 1631092
Conc: 1.77 ng/ml

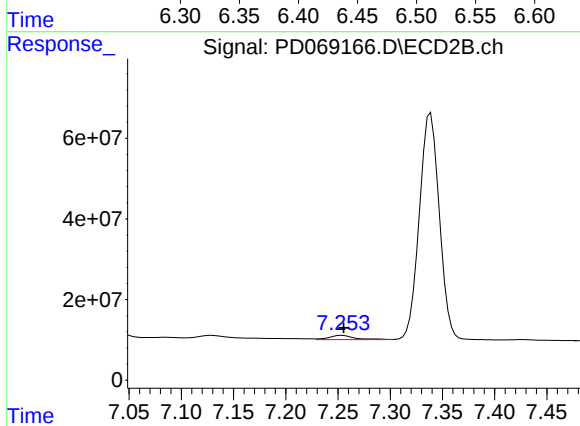

#18 Endrin aldehyde


R.T.: 7.254 min
Delta R.T.: -0.002 min
Response: 17394046
Conc: 2.52 ng/ml

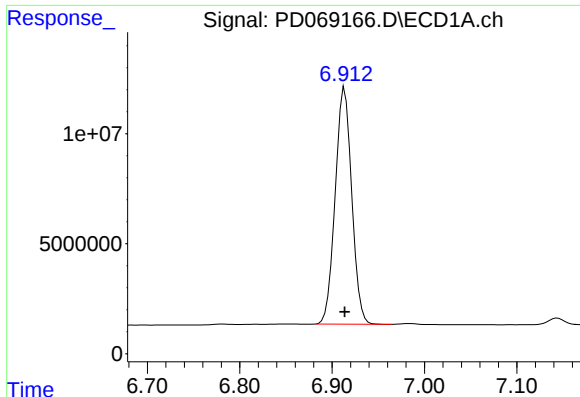

#20 Methoxychlor


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 133654114
Conc: 210.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

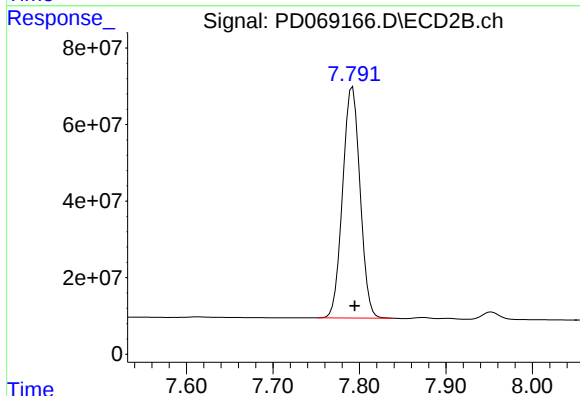


#20 Methoxychlor

R.T.: 7.792 min
Delta R.T.: -0.002 min
Response: 841079601
Conc: 195.10 ng/ml

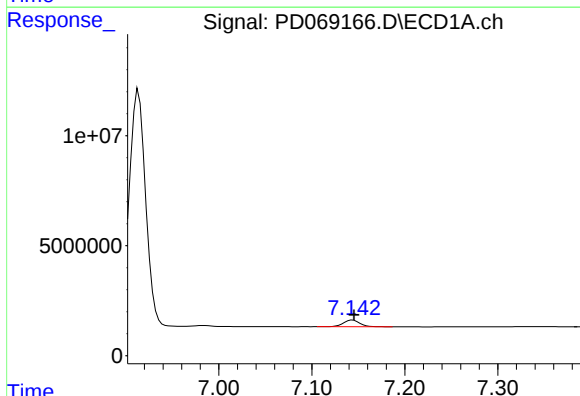


#21 Endrin ketone

R.T.: 7.144 min
Delta R.T.: -0.002 min
Response: 3721979
Conc: 2.64 ng/ml

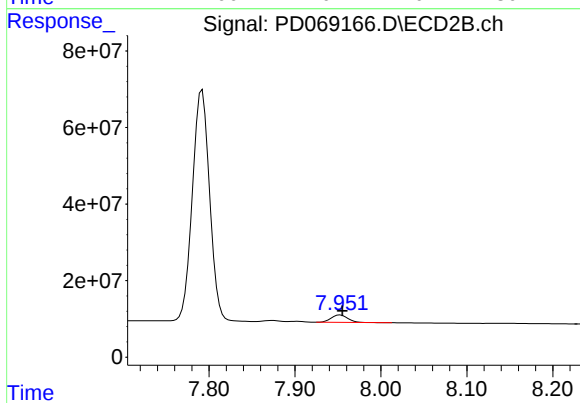

#21 Endrin ketone


R.T.: 7.953 min
Delta R.T.: -0.002 min
Response: 25819613
Conc: 2.86 ng/ml

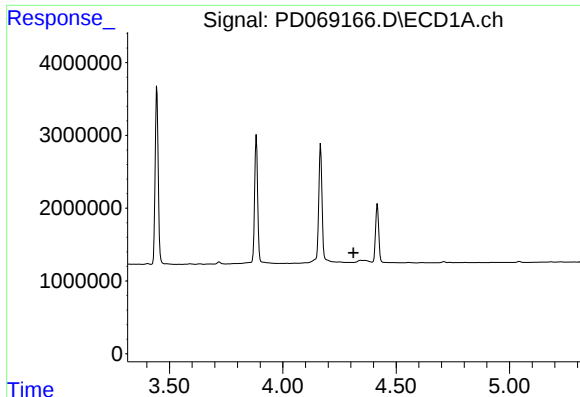

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.312 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

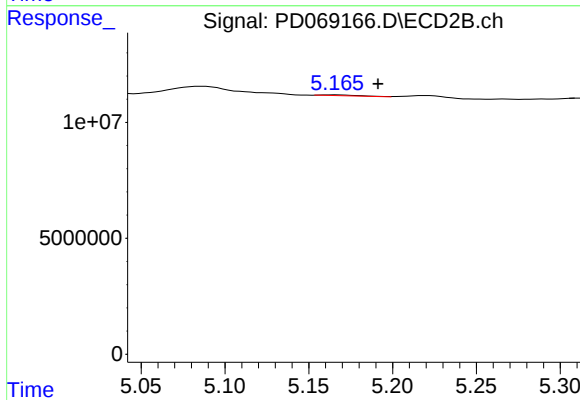


#23 Chlordane-1

R.T.: 5.167 min
Delta R.T.: -0.025 min
Response: 631473
Conc: 1.31 ng/ml

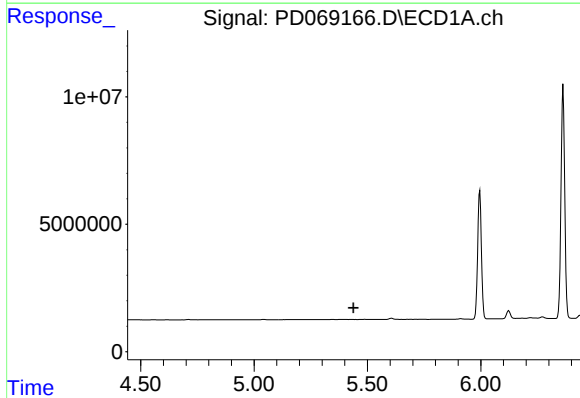


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.439 min
Response: 0
Conc: N.D.

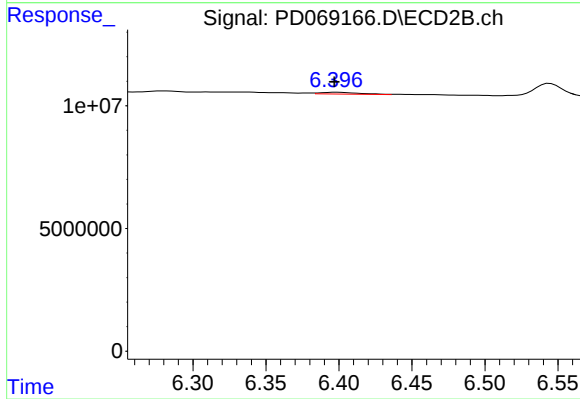

#26 Chlordane-4


R.T.: 6.398 min
Delta R.T.: 0.000 min
Response: 1325563
Conc: 0.70 ng/ml

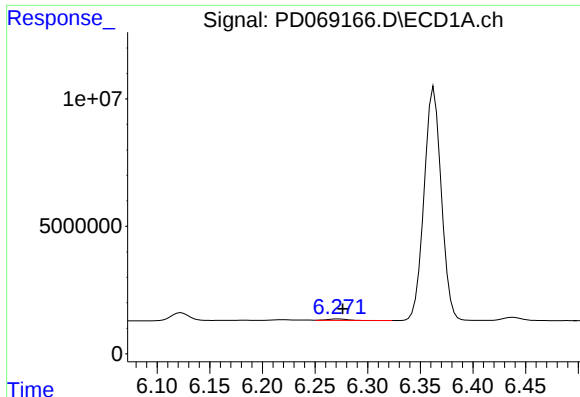

#27 Chlordane-5


R.T.: 6.272 min
Delta R.T.: -0.004 min
Response: 814254
Conc: 18.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

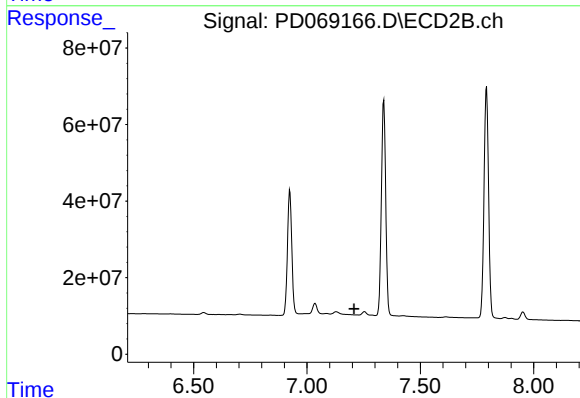


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.208 min
Response: 0
Conc: N.D.

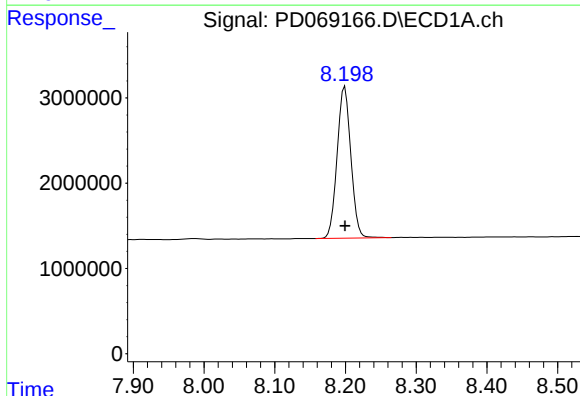

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 23944156
Conc: 19.18 ng/ml

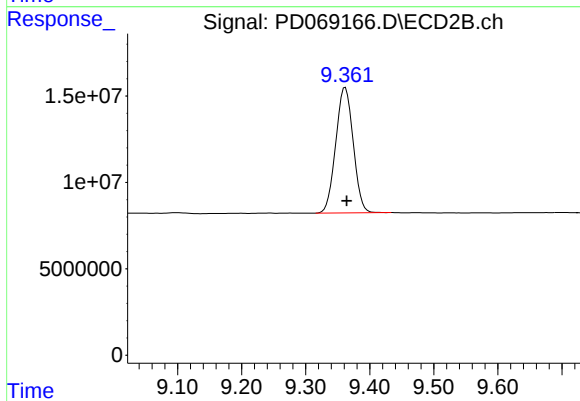

#28 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: -0.002 min
Response: 137656391
Conc: 21.04 ng/ml