

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
 Data File : PD069173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 11:16
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:34:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:32:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.170	65452804	541.8E6	49.780	47.519
28)	SA Decachlor...	8.197	9.361	60520163	330.2E6	49.327	48.192
Target Compounds							
23)	Chlordane-1	4.312	5.192	20680773	228.9E6	499.679	476.669
24)	Chlordane-2	4.813	5.665	24656790	218.3E6	494.533	475.482
25)	Chlordane-3	5.381	6.320	67559072	778.9E6	496.552	478.474
26)	Chlordane-4	5.439	6.397	56577626	914.6E6	494.860	482.373
27)	Chlordane-5	6.276	7.208	22865997	175.5E6	505.617	482.315



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
Data File : PD069173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 11:16
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:34:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:32:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

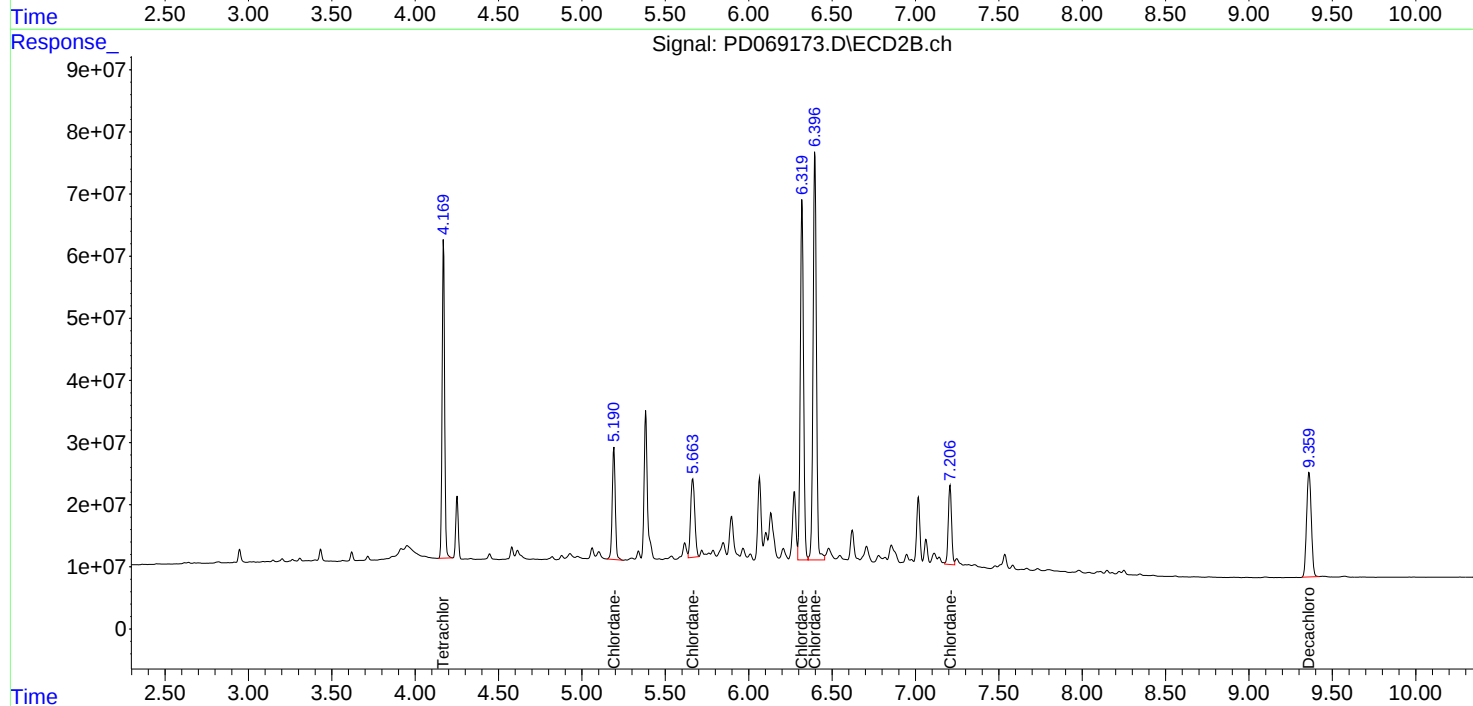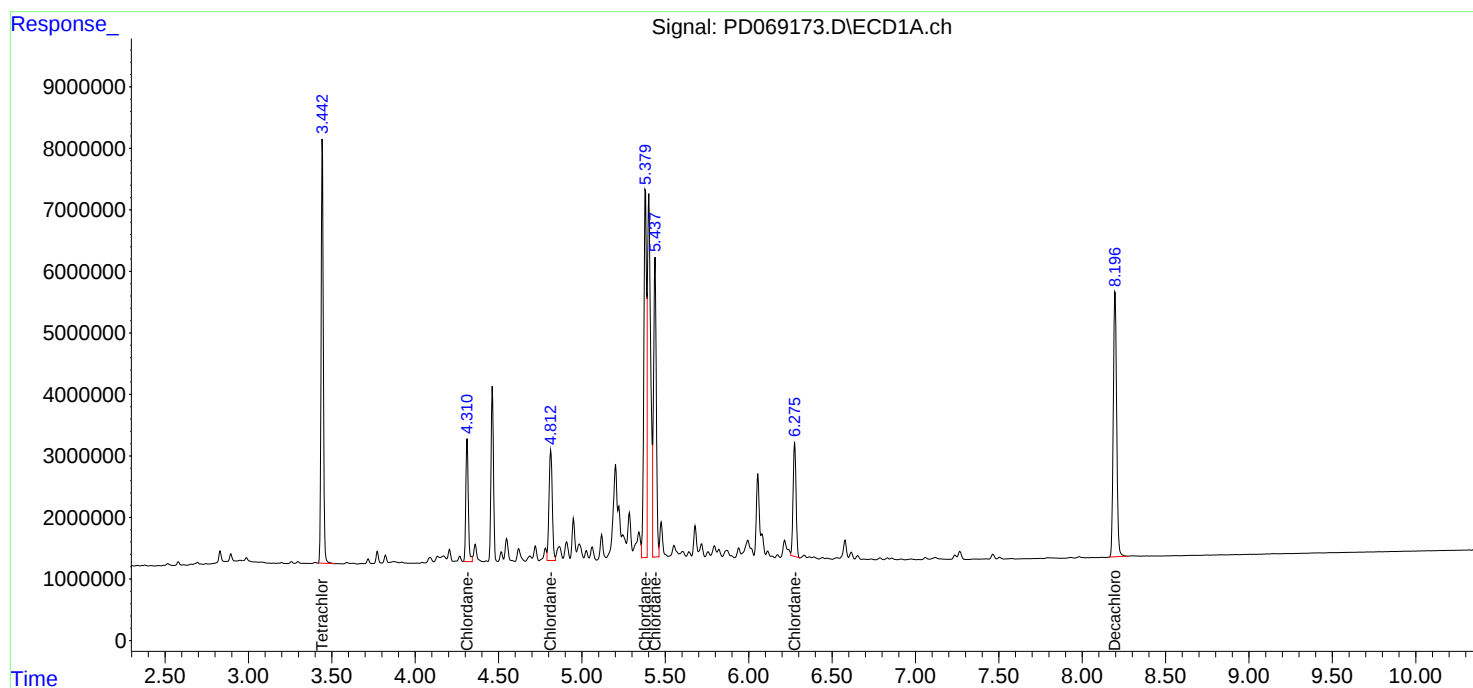


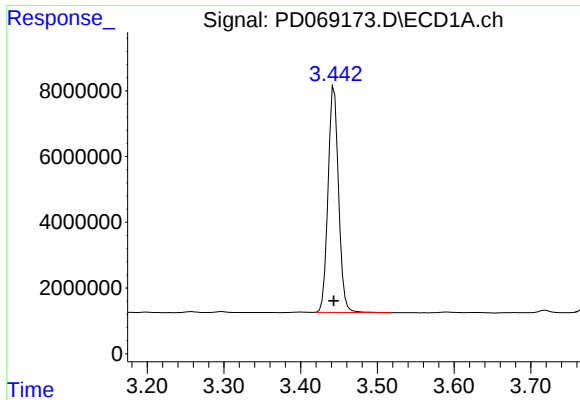

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 65452804
Conc: 49.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

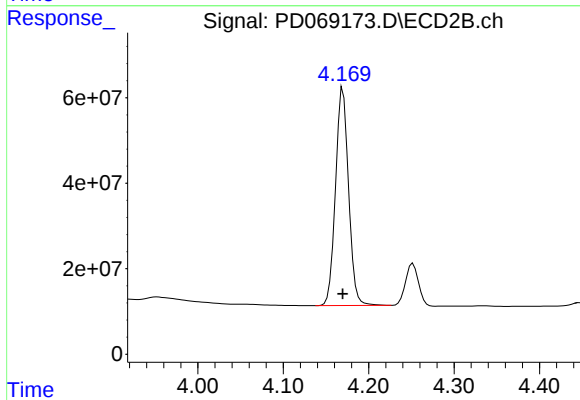


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 541771626
Conc: 47.52 ng/ml

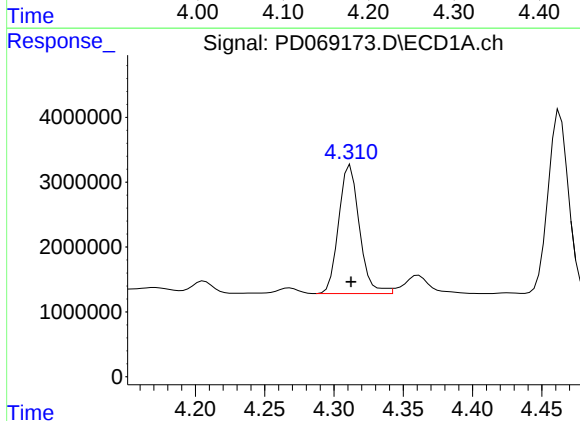


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 20680773
Conc: 499.68 ng/ml

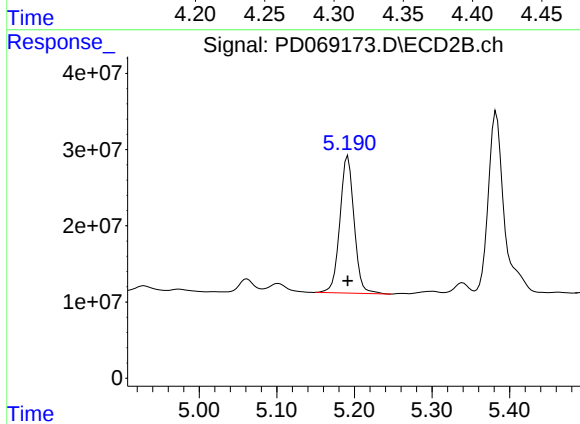

#23 Chlordane-1


R.T.: 5.192 min
Delta R.T.: 0.000 min
Response: 228941588
Conc: 476.67 ng/ml

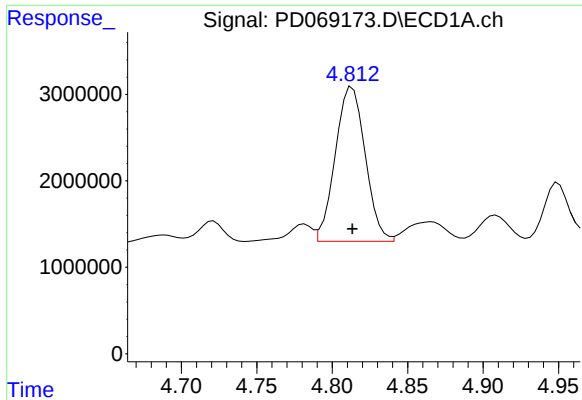

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 24656790
Conc: 494.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

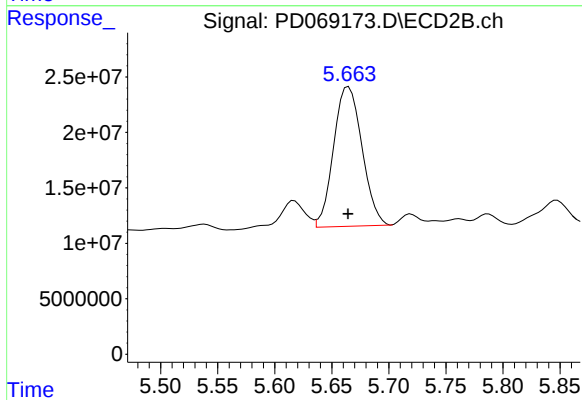


#24 Chlordane-2

R.T.: 5.665 min
Delta R.T.: 0.000 min
Response: 218282899
Conc: 475.48 ng/ml

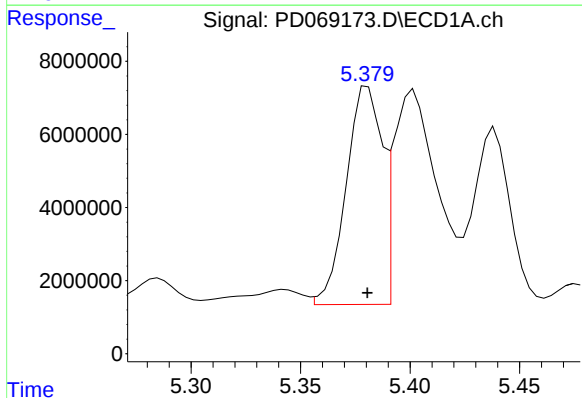


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 67559072
Conc: 496.55 ng/ml

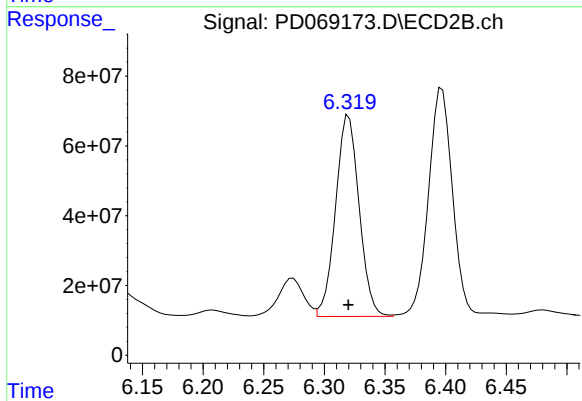

#25 Chlordane-3


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 778923128
Conc: 478.47 ng/ml

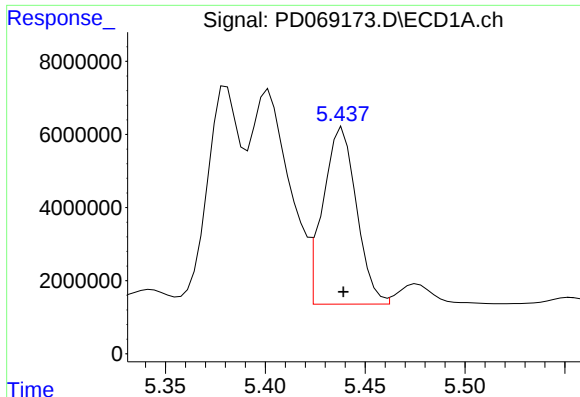

#26 Chlordane-4


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 56577626
Conc: 494.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

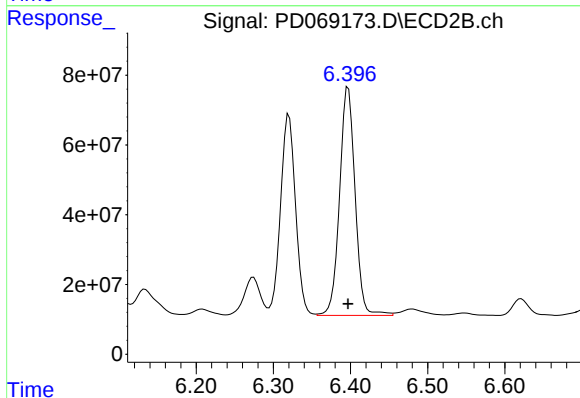


#26 Chlordane-4

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 914566073
Conc: 482.37 ng/ml

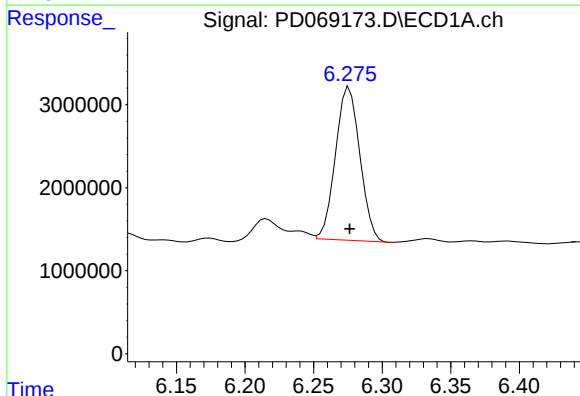


#27 Chlordane-5

R.T.: 6.276 min
Delta R.T.: 0.000 min
Response: 22865997
Conc: 505.62 ng/ml

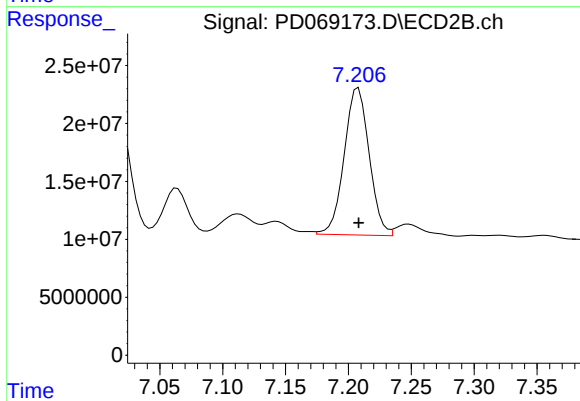

#27 Chlordane-5


R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 175505811
Conc: 482.31 ng/ml

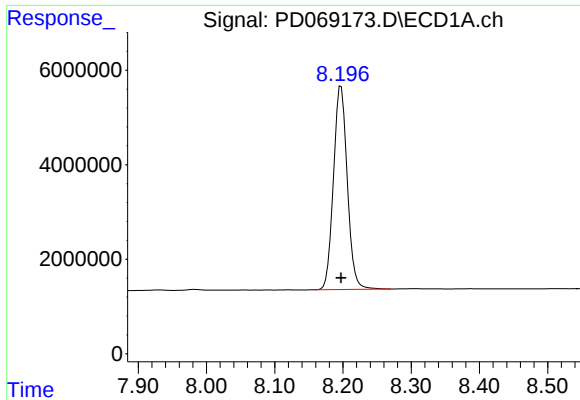

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: 0.000 min
Response: 60520163
Conc: 49.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

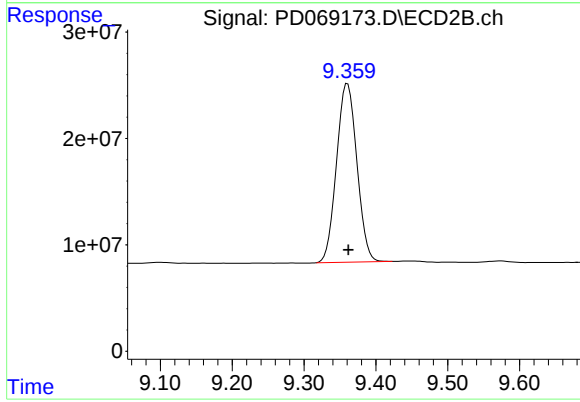

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: -0.001 min
Response: 330221900
Conc: 48.19 ng/ml