

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
 Data File : PD069167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 09:19
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:43:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:40:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.169	26527018	264.4E6	23.896	24.662
28)	SA Decachlor...	8.197	9.361	26834207	155.0E6	21.491	23.683
Target Compounds							
9)	A Endosulfan I	5.492	6.445	14944381	134.7E6	11.580	12.470
10)	B gamma-Chl...	5.380	6.319	16163726	148.8E6	11.628	12.777
12)	B 4,4'-DDE	5.604	6.544	28273702	251.4E6	22.345	23.275
13)	MA Dieldrin	5.736	6.704	30935108	267.2E6	22.926	23.973
19)	B Endosulfa...	6.650	7.477	24937146	186.9E6	20.616	21.899
20)	A Methoxychlor	6.912	7.790	61430993	410.3E6	96.704	95.170
21)	B Endrin ke...	7.143	7.952	30176880	211.6E6	21.432	23.400



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
Data File : PD069167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 09:19
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:43:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:40:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

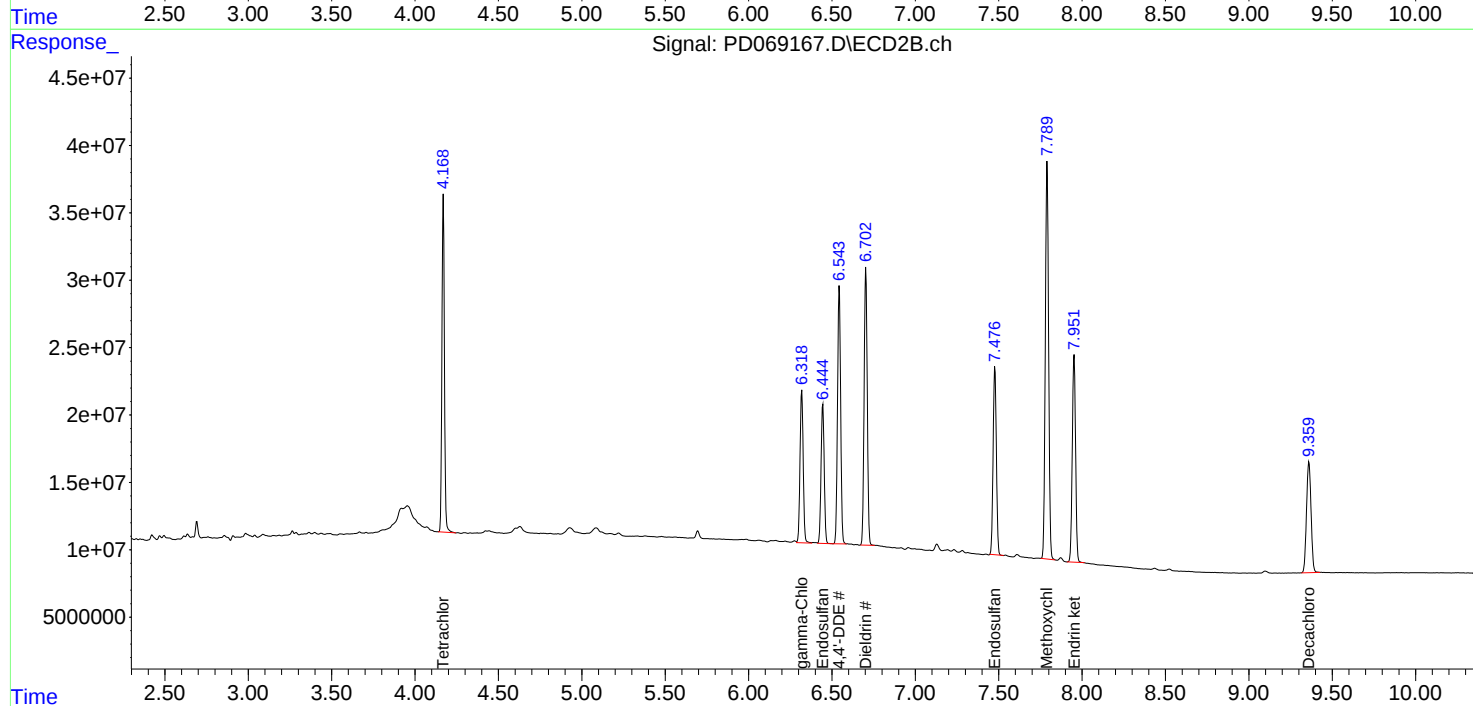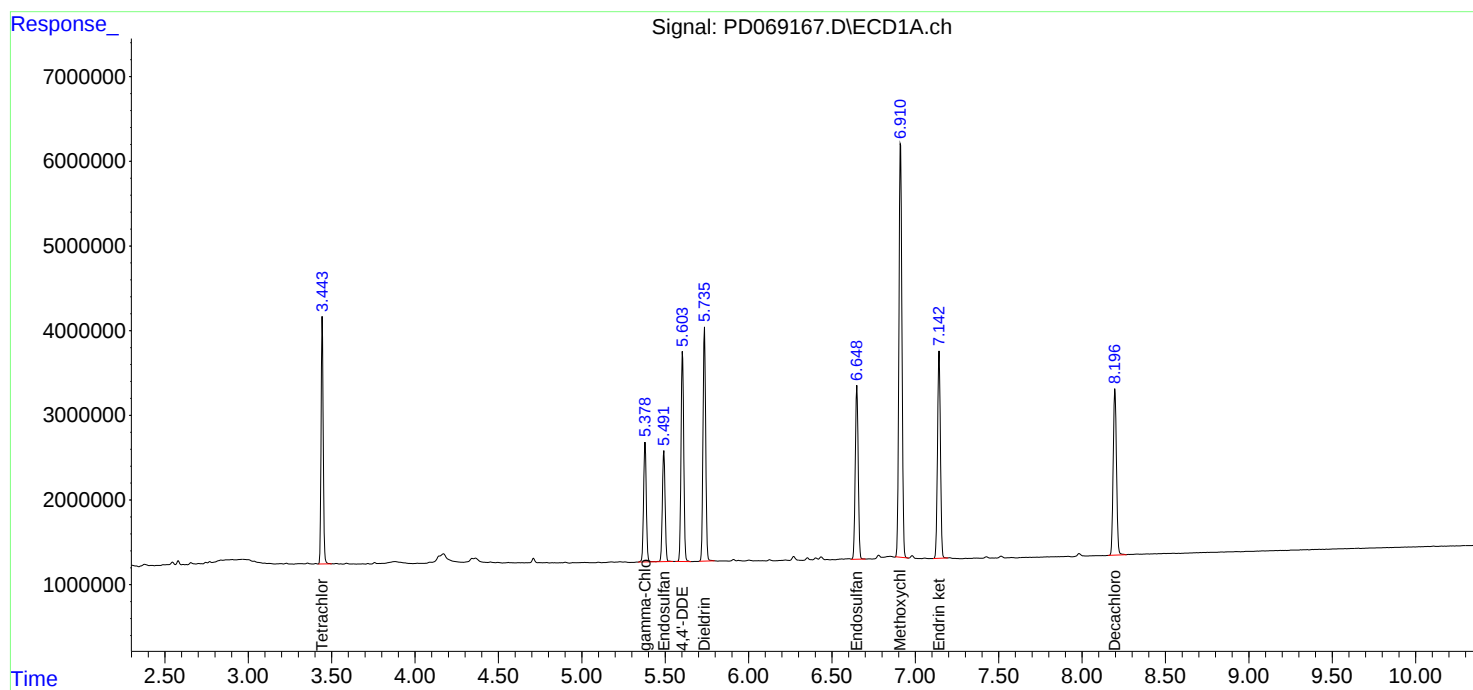


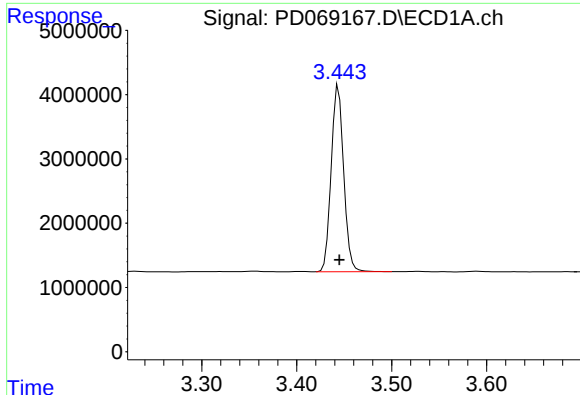

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: -0.001 min
Response: 26527018
Conc: 23.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

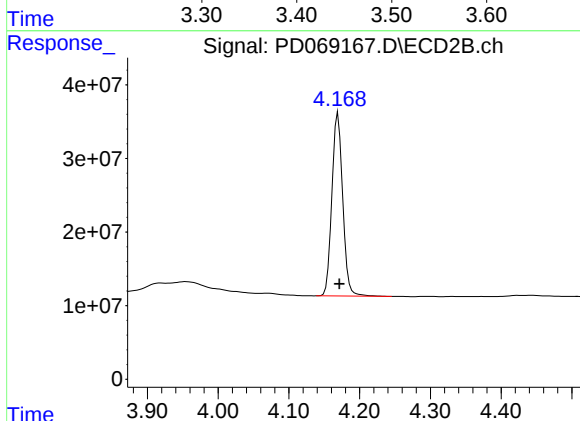


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: -0.002 min
Response: 264417862
Conc: 24.66 ng/ml

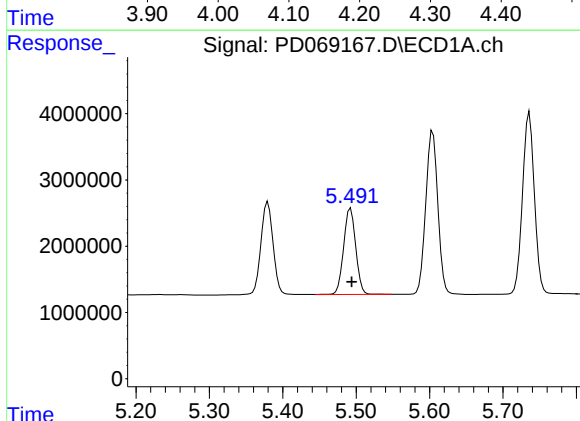


#9 Endosulfan I

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 14944381
Conc: 11.58 ng/ml

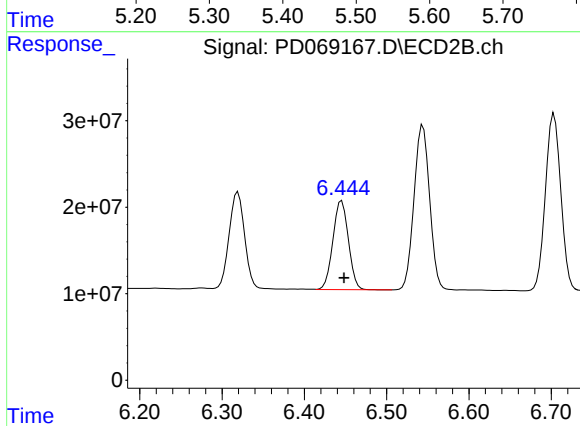

#9 Endosulfan I


R.T.: 6.445 min
Delta R.T.: -0.003 min
Response: 134677500
Conc: 12.47 ng/ml

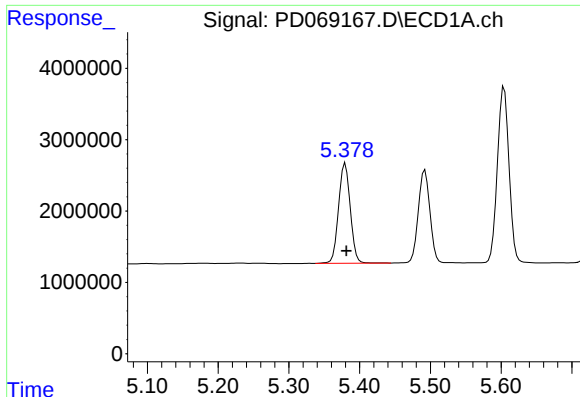

#10 gamma-Chlordane


R.T.: 5.380 min
Delta R.T.: -0.002 min
Response: 16163726
Conc: 11.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

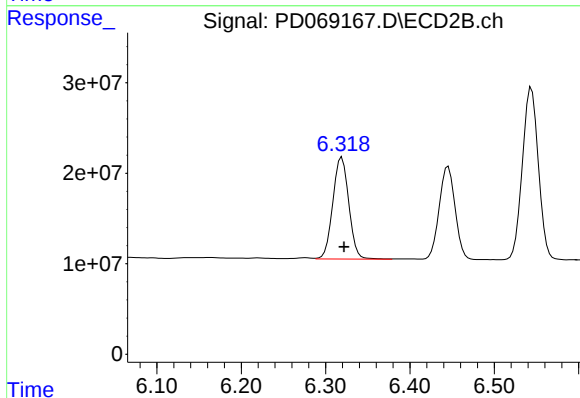


#10 gamma-Chlordane

R.T.: 6.319 min
Delta R.T.: -0.003 min
Response: 148773782
Conc: 12.78 ng/ml

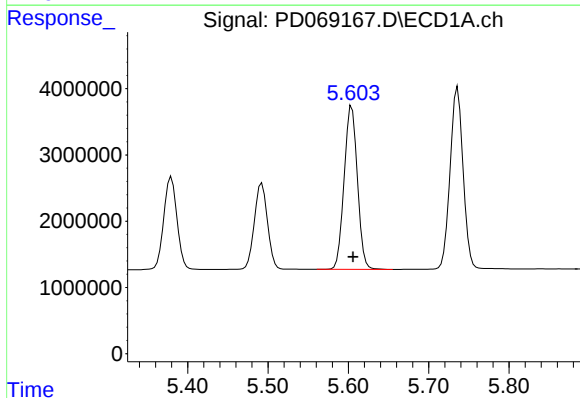


#12 4,4'-DDE

R.T.: 5.604 min
Delta R.T.: -0.002 min
Response: 28273702
Conc: 22.34 ng/ml

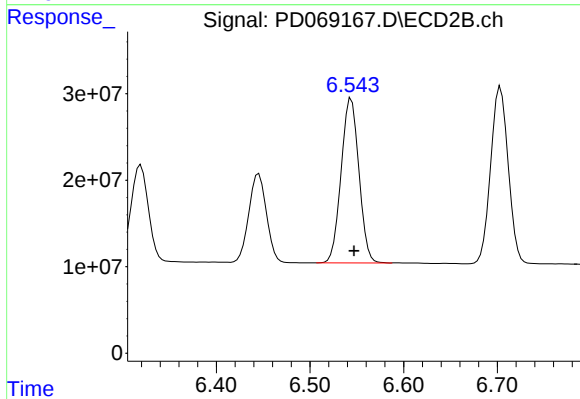

#12 4,4'-DDE


R.T.: 6.544 min
Delta R.T.: -0.003 min
Response: 251427815
Conc: 23.28 ng/ml

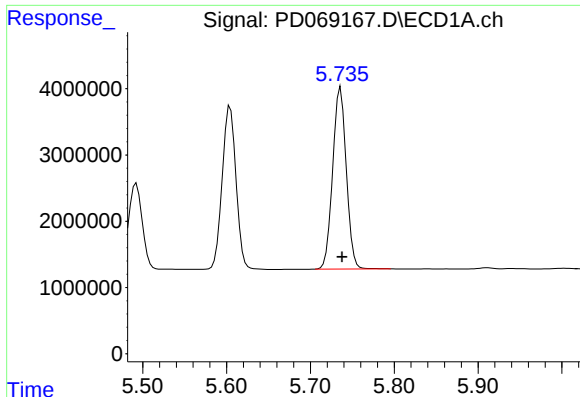

#13 Dieldrin


R.T.: 5.736 min
Delta R.T.: -0.002 min
Response: 30935108
Conc: 22.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

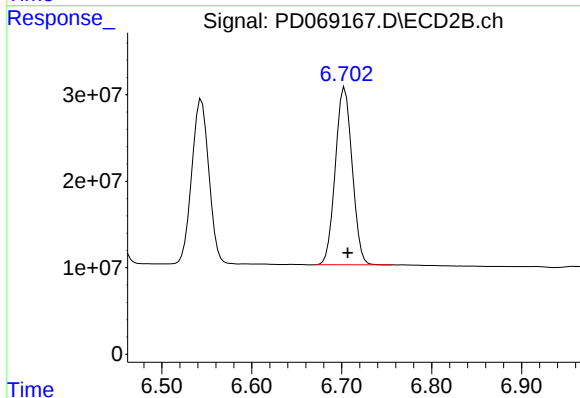


#13 Dieldrin

R.T.: 6.704 min
Delta R.T.: -0.003 min
Response: 267246851
Conc: 23.97 ng/ml

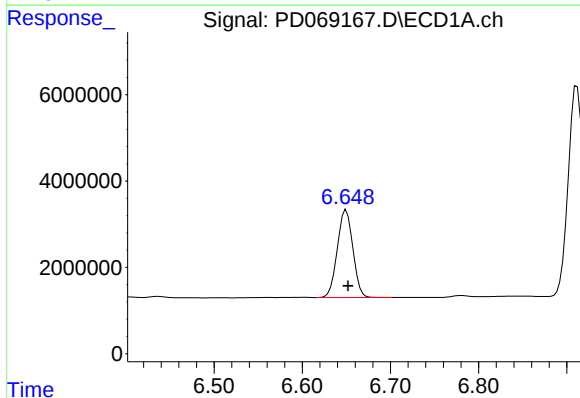


#19 Endosulfan Sulfate

R.T.: 6.650 min
Delta R.T.: -0.002 min
Response: 24937146
Conc: 20.62 ng/ml

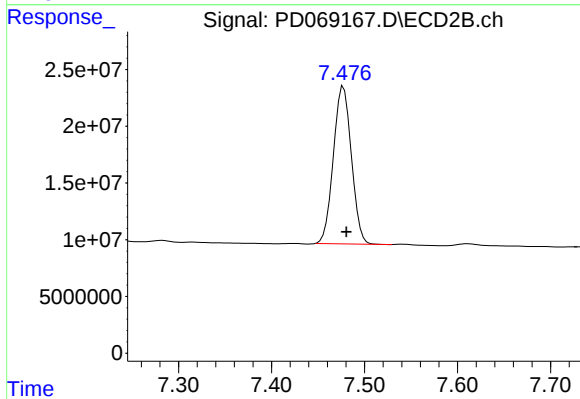

#19 Endosulfan Sulfate


R.T.: 7.477 min
Delta R.T.: -0.003 min
Response: 186940554
Conc: 21.90 ng/ml

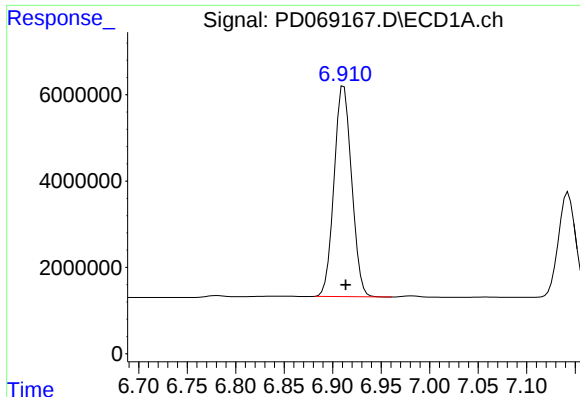

#20 Methoxychlor


R.T.: 6.912 min
Delta R.T.: -0.002 min
Response: 61430993
Conc: 96.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

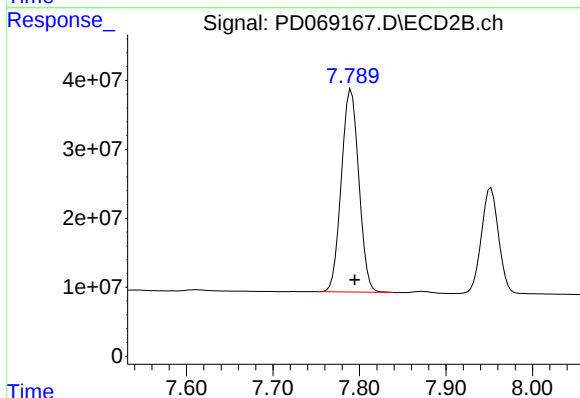


#20 Methoxychlor

R.T.: 7.790 min
Delta R.T.: -0.004 min
Response: 410287628
Conc: 95.17 ng/ml

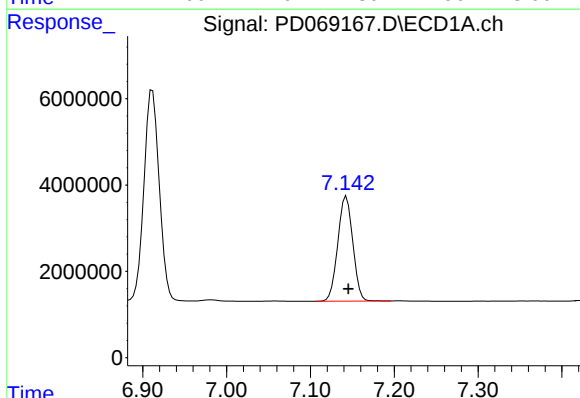


#21 Endrin ketone

R.T.: 7.143 min
Delta R.T.: -0.003 min
Response: 30176880
Conc: 21.43 ng/ml

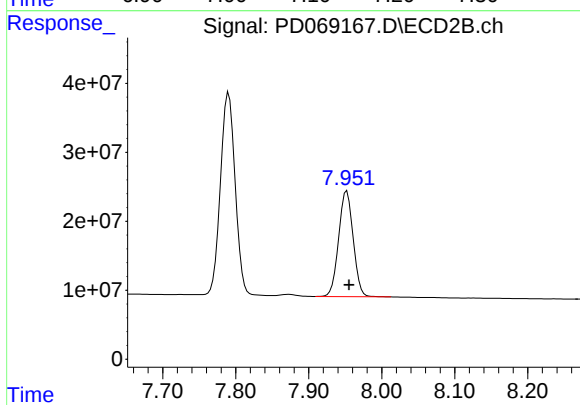

#21 Endrin ketone


R.T.: 7.952 min
Delta R.T.: -0.003 min
Response: 211570541
Conc: 23.40 ng/ml

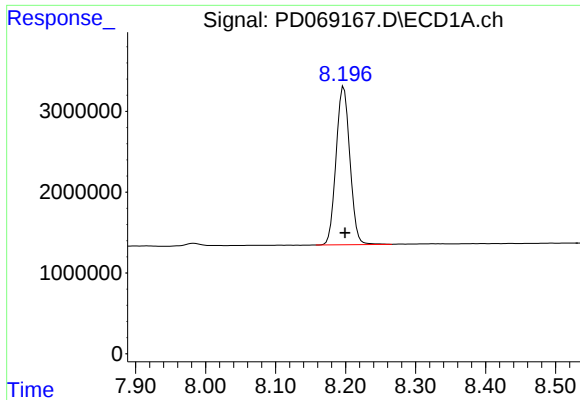

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.002 min
Response: 26834207
Conc: 21.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

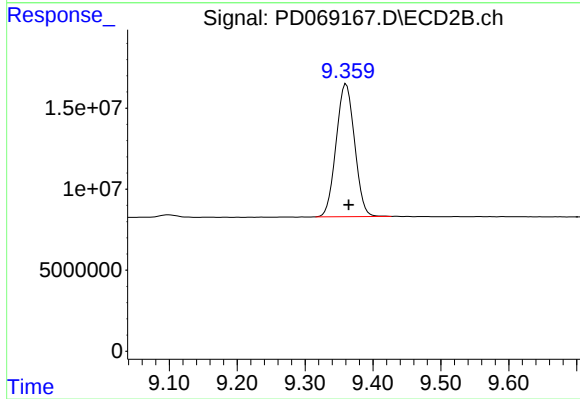

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: -0.003 min
Response: 154979210
Conc: 23.68 ng/ml