

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
 Data File : PD069168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 10:06
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:25:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:25:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.170	131.9E6	1049.1E6	98.992	94.073
28)	SA Decachlor...	8.209	9.365	113.2E6	608.4E6	94.818	91.747
Target Compounds							
23)	Chlordane-1	4.321	5.193	39631729	428.9E6	951.098	916.968
24)	Chlordane-2	4.824	5.666	45512558	401.2E6	917.509	900.733
25)	Chlordane-3	5.391	6.322	135.5E6	1507.7E6	990.752	946.732
26)	Chlordane-4	5.449	6.399	113.1E6	1736.5E6	990.714	942.936
27)	Chlordane-5	6.287	7.211	46311258	329.1E6	997.135	928.746



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
Data File : PD069168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 10:06
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:25:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:25:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

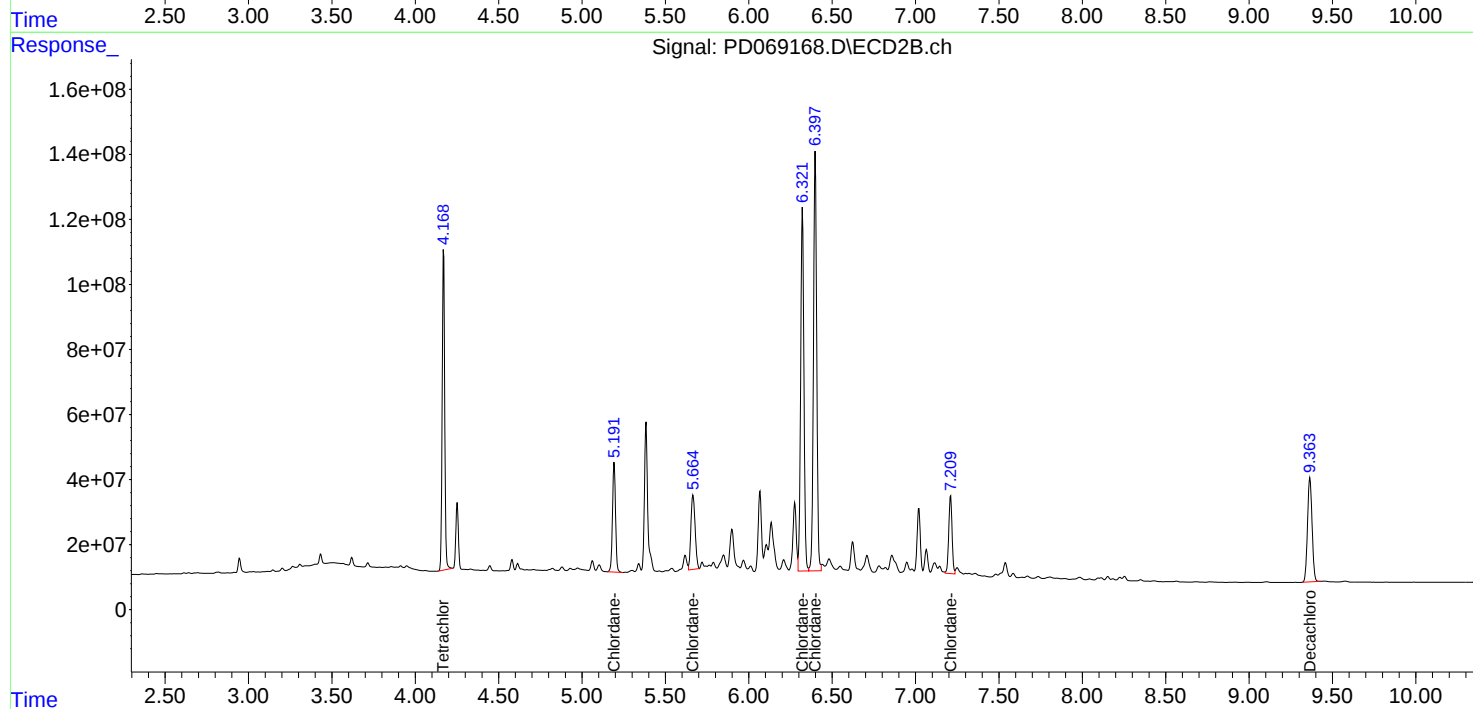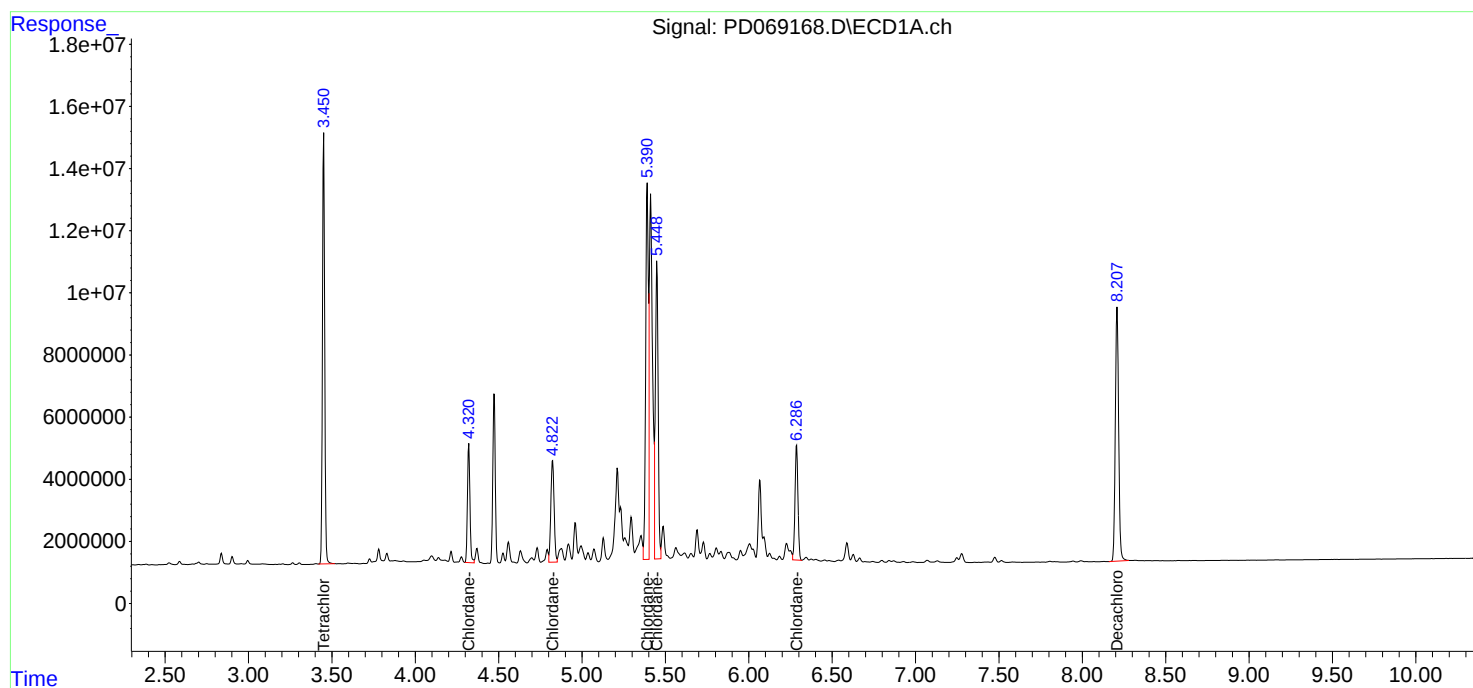


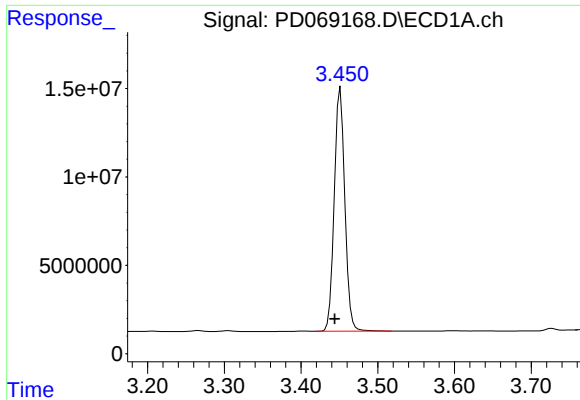

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.007 min
Response: 131876726
Conc: 98.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

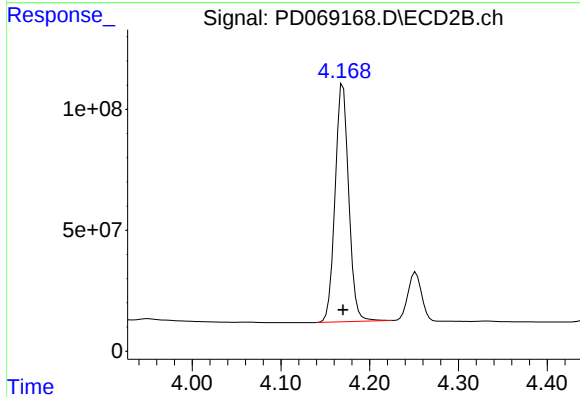


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 1049120848
Conc: 94.07 ng/ml

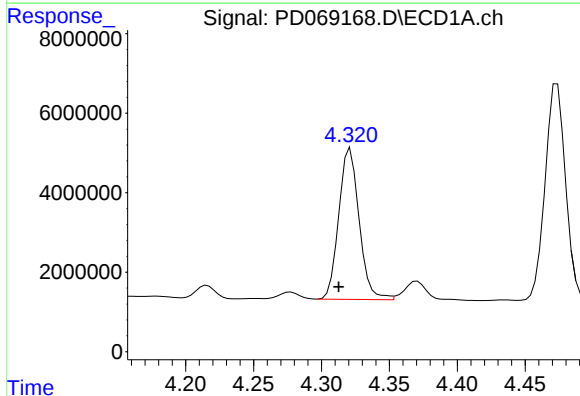


#23 Chlordane-1

R.T.: 4.321 min
Delta R.T.: 0.008 min
Response: 39631729
Conc: 951.10 ng/ml

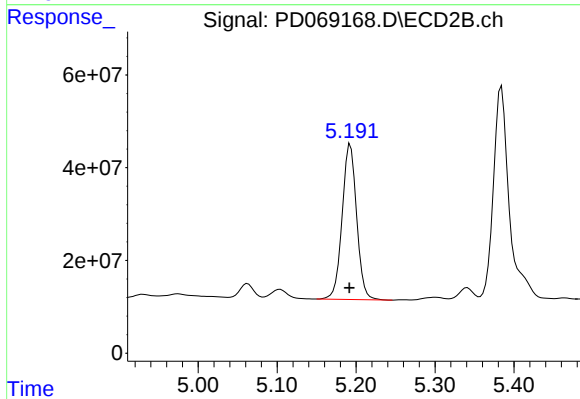

#23 Chlordane-1


R.T.: 5.193 min
Delta R.T.: 0.001 min
Response: 428893093
Conc: 916.97 ng/ml

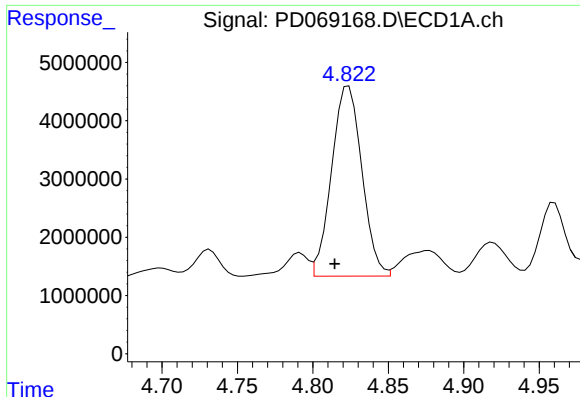

#24 Chlordane-2


R.T.: 4.824 min
Delta R.T.: 0.009 min
Response: 45512558
Conc: 917.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

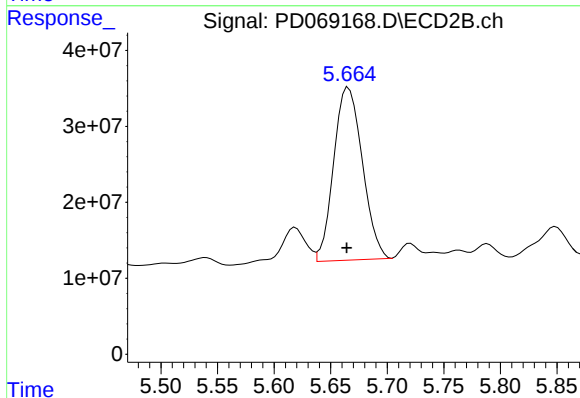


#24 Chlordane-2

R.T.: 5.666 min
Delta R.T.: 0.001 min
Response: 401238052
Conc: 900.73 ng/ml

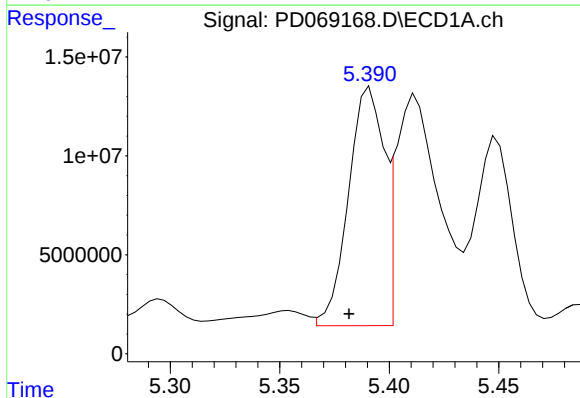


#25 Chlordane-3

R.T.: 5.391 min
Delta R.T.: 0.010 min
Response: 135496579
Conc: 990.75 ng/ml

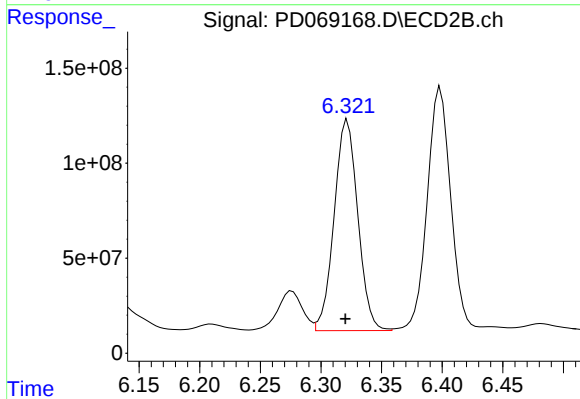

#25 Chlordane-3


R.T.: 6.322 min
Delta R.T.: 0.002 min
Response: 1507689231
Conc: 946.73 ng/ml

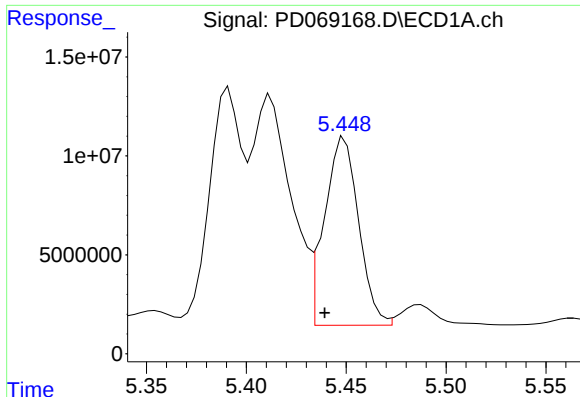

#26 Chlordane-4


R.T.: 5.449 min
Delta R.T.: 0.010 min
Response: 113130923
Conc: 990.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

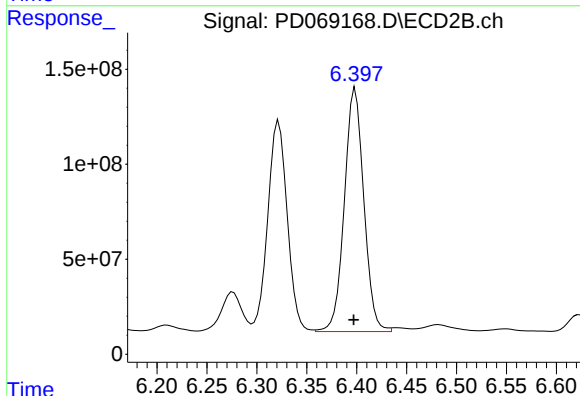


#26 Chlordane-4

R.T.: 6.399 min
Delta R.T.: 0.002 min
Response: 1736484943
Conc: 942.94 ng/ml

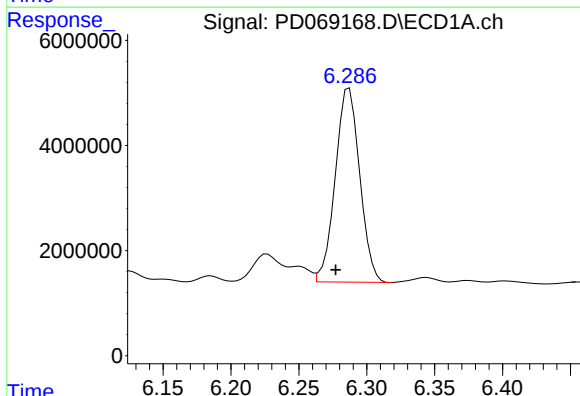


#27 Chlordane-5

R.T.: 6.287 min
Delta R.T.: 0.010 min
Response: 46311258
Conc: 997.14 ng/ml

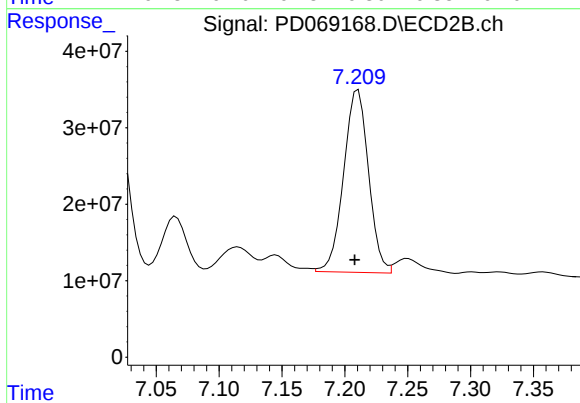

#27 Chlordane-5


R.T.: 7.211 min
Delta R.T.: 0.003 min
Response: 329067147
Conc: 928.75 ng/ml

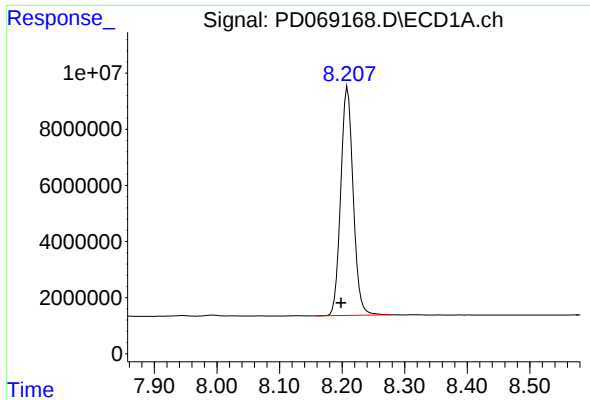

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.011 min
Response: 113159222
Conc: 94.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

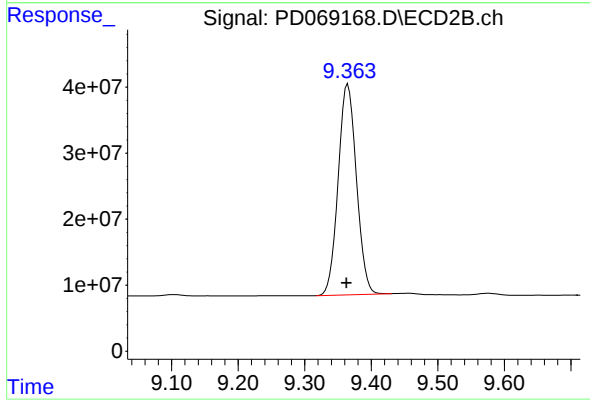

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.002 min
Response: 608425064
Conc: 91.75 ng/ml