

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
 Data File : PD069169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 10:20
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:25:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:25:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.169	99921044	806.5E6	75.005	72.318
28)	SA Decachlor...	8.199	9.363	86981384	473.9E6	72.883	71.463
Target Compounds							
23)	Chlordane-1	4.312	5.191	30429436	333.7E6	730.258	713.349
24)	Chlordane-2	4.814	5.664	35572410	314.4E6	717.121	705.856
25)	Chlordane-3	5.381	6.320	103.4E6	1156.2E6	755.899	726.035
26)	Chlordane-4	5.439	6.397	84473083	1336.4E6	739.751	725.667
27)	Chlordane-5	6.277	7.208	34248447	255.4E6	737.409	720.722



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
Data File : PD069169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 10:20
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:25:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:25:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

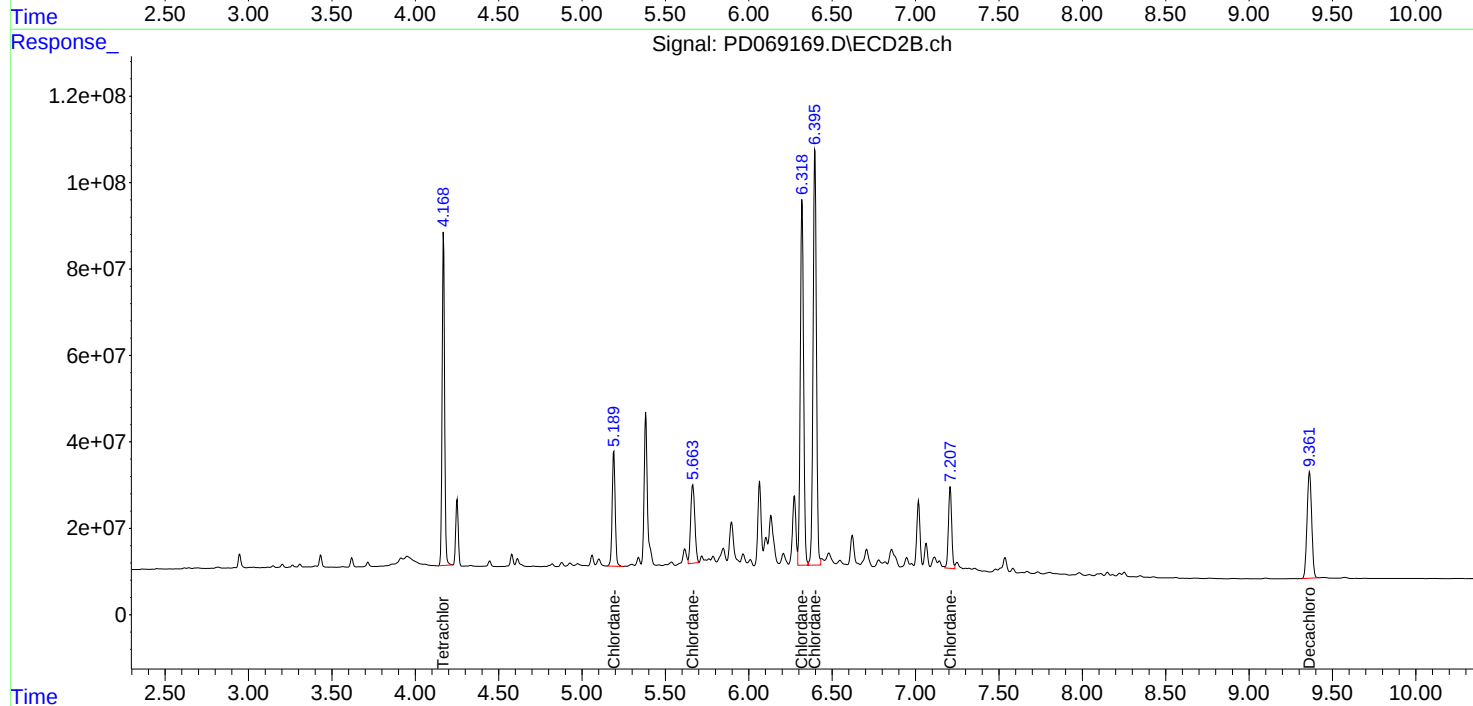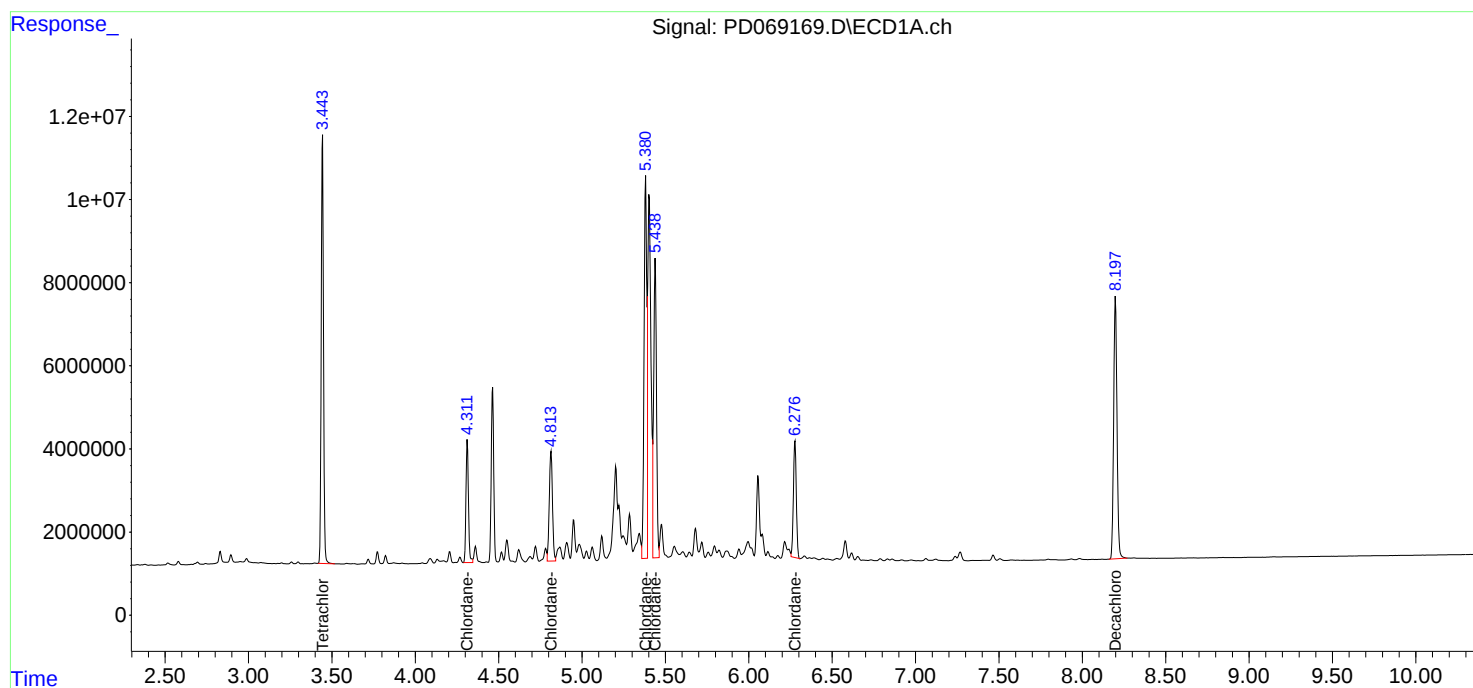


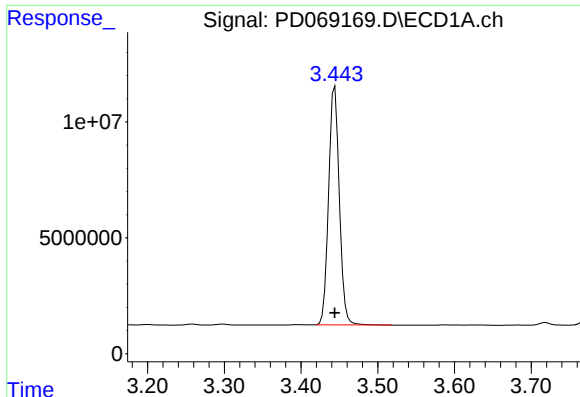

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 99921044
Conc: 75.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

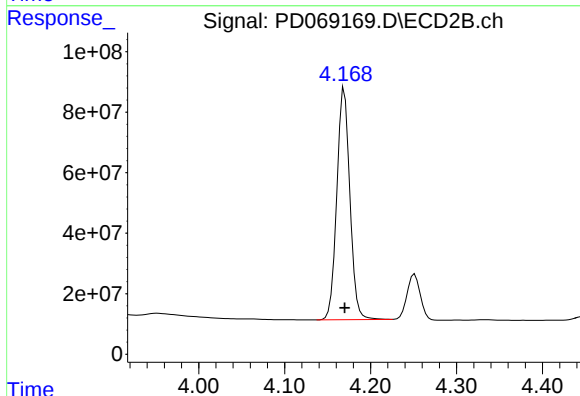


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 806508108
Conc: 72.32 ng/ml

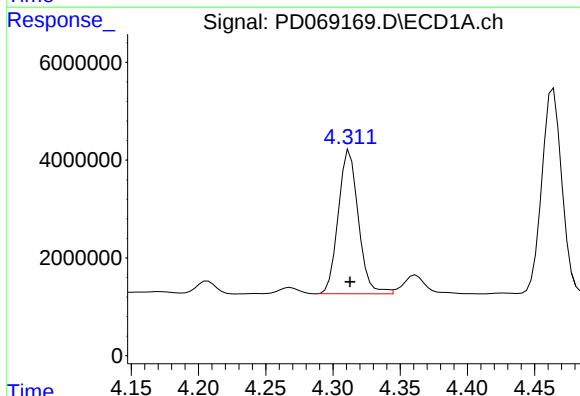


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 30429436
Conc: 730.26 ng/ml

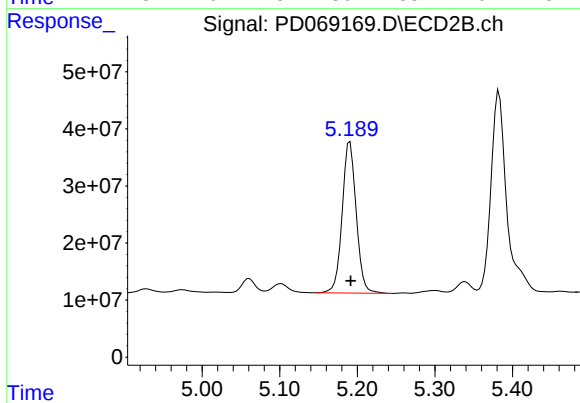

#23 Chlordane-1


R.T.: 5.191 min
Delta R.T.: -0.001 min
Response: 333654396
Conc: 713.35 ng/ml

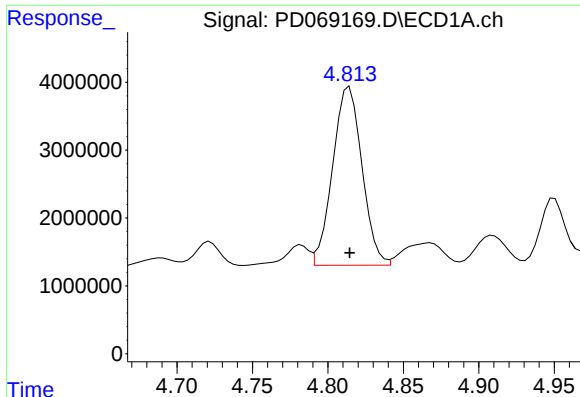

#24 Chlordane-2


R.T.: 4.814 min
Delta R.T.: 0.000 min
Response: 35572410
Conc: 717.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

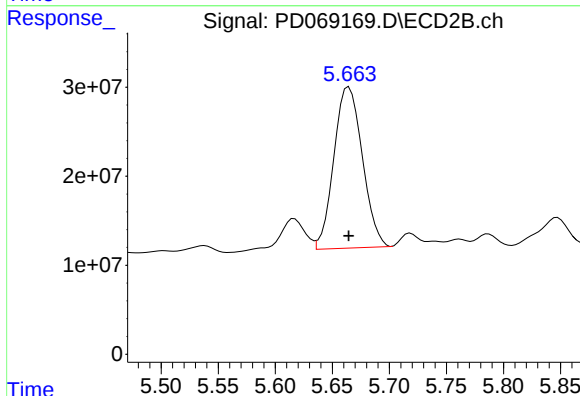


#24 Chlordane-2

R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 314428598
Conc: 705.86 ng/ml

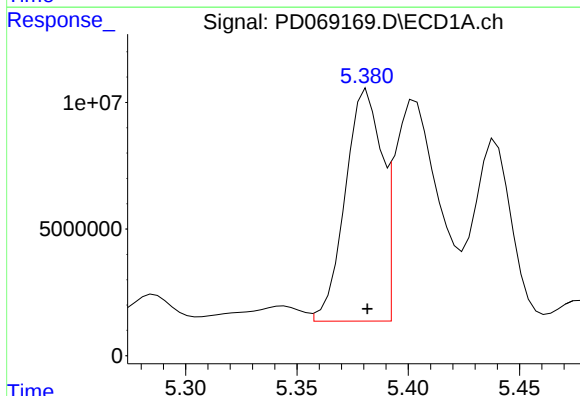


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 103377719
Conc: 755.90 ng/ml

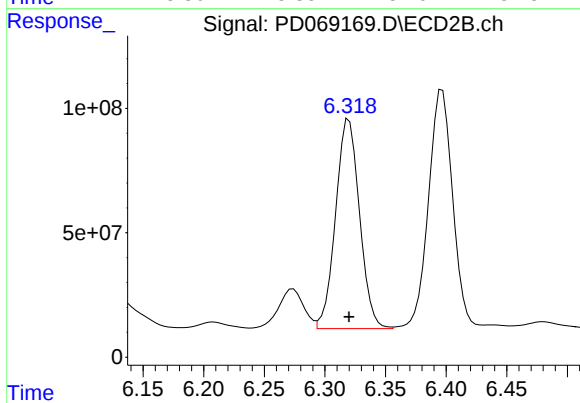

#25 Chlordane-3


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 1156225390
Conc: 726.04 ng/ml

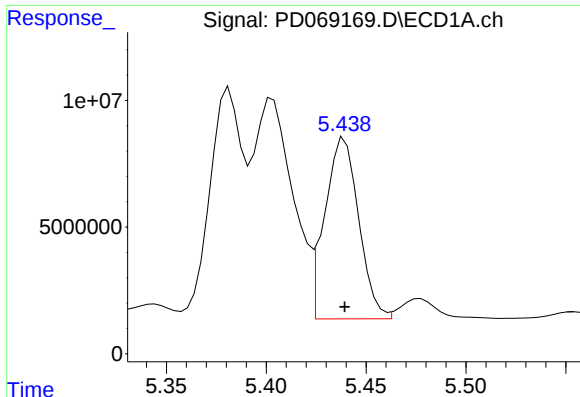

#26 Chlordane-4


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 84473083
Conc: 739.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

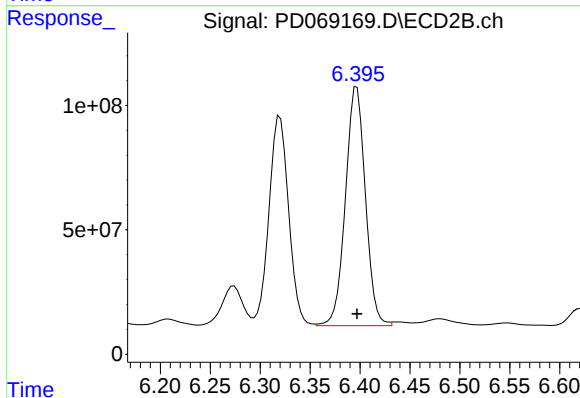


#26 Chlordane-4

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 1336368805
Conc: 725.67 ng/ml

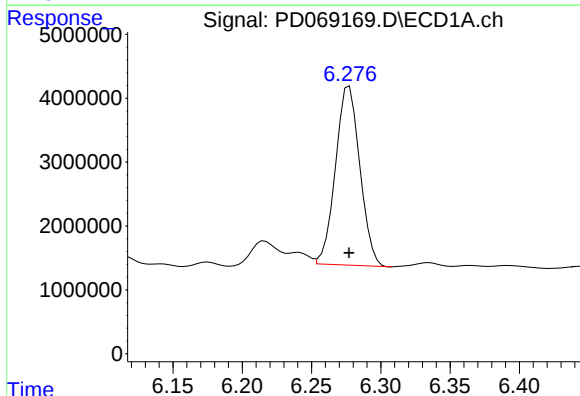


#27 Chlordane-5

R.T.: 6.277 min
Delta R.T.: 0.000 min
Response: 34248447
Conc: 737.41 ng/ml

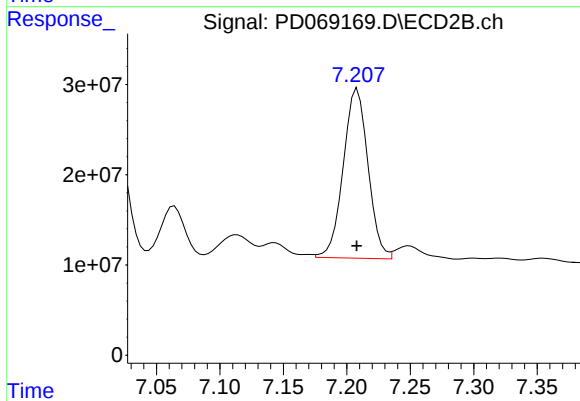

#27 Chlordane-5


R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 255361657
Conc: 720.72 ng/ml

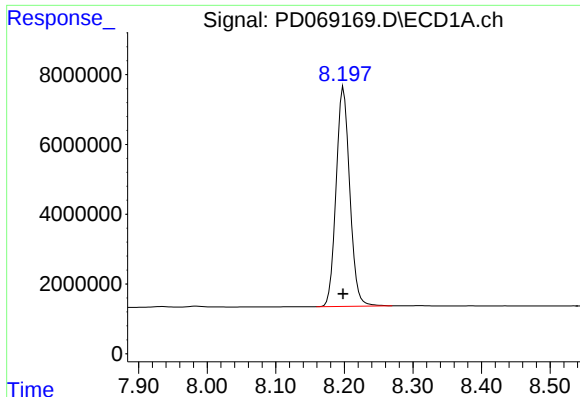

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 86981384
Conc: 72.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

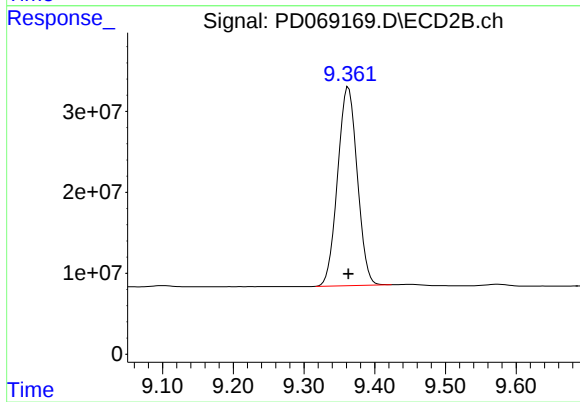

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.000 min
Response: 473915043
Conc: 71.46 ng/ml