

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
 Data File : PD069171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 10:48
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:25:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:25:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.170	33082810	296.3E6	24.833	26.570
28)	SA Decachlor...	8.198	9.362	32190205	182.2E6	26.973	27.473
Target Compounds							
23)	Chlordane-1	4.312	5.191	10642220	125.9E6	255.396	269.084
24)	Chlordane-2	4.814	5.664	13316838	122.4E6	268.460	274.791
25)	Chlordane-3	5.381	6.320	33947801	419.6E6	248.227	263.494
26)	Chlordane-4	5.439	6.397	29078614	488.1E6	254.648	265.019
27)	Chlordane-5	6.276	7.207	11867433	94520463	255.520	266.771


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
Data File : PD069171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 10:48
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:25:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:25:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

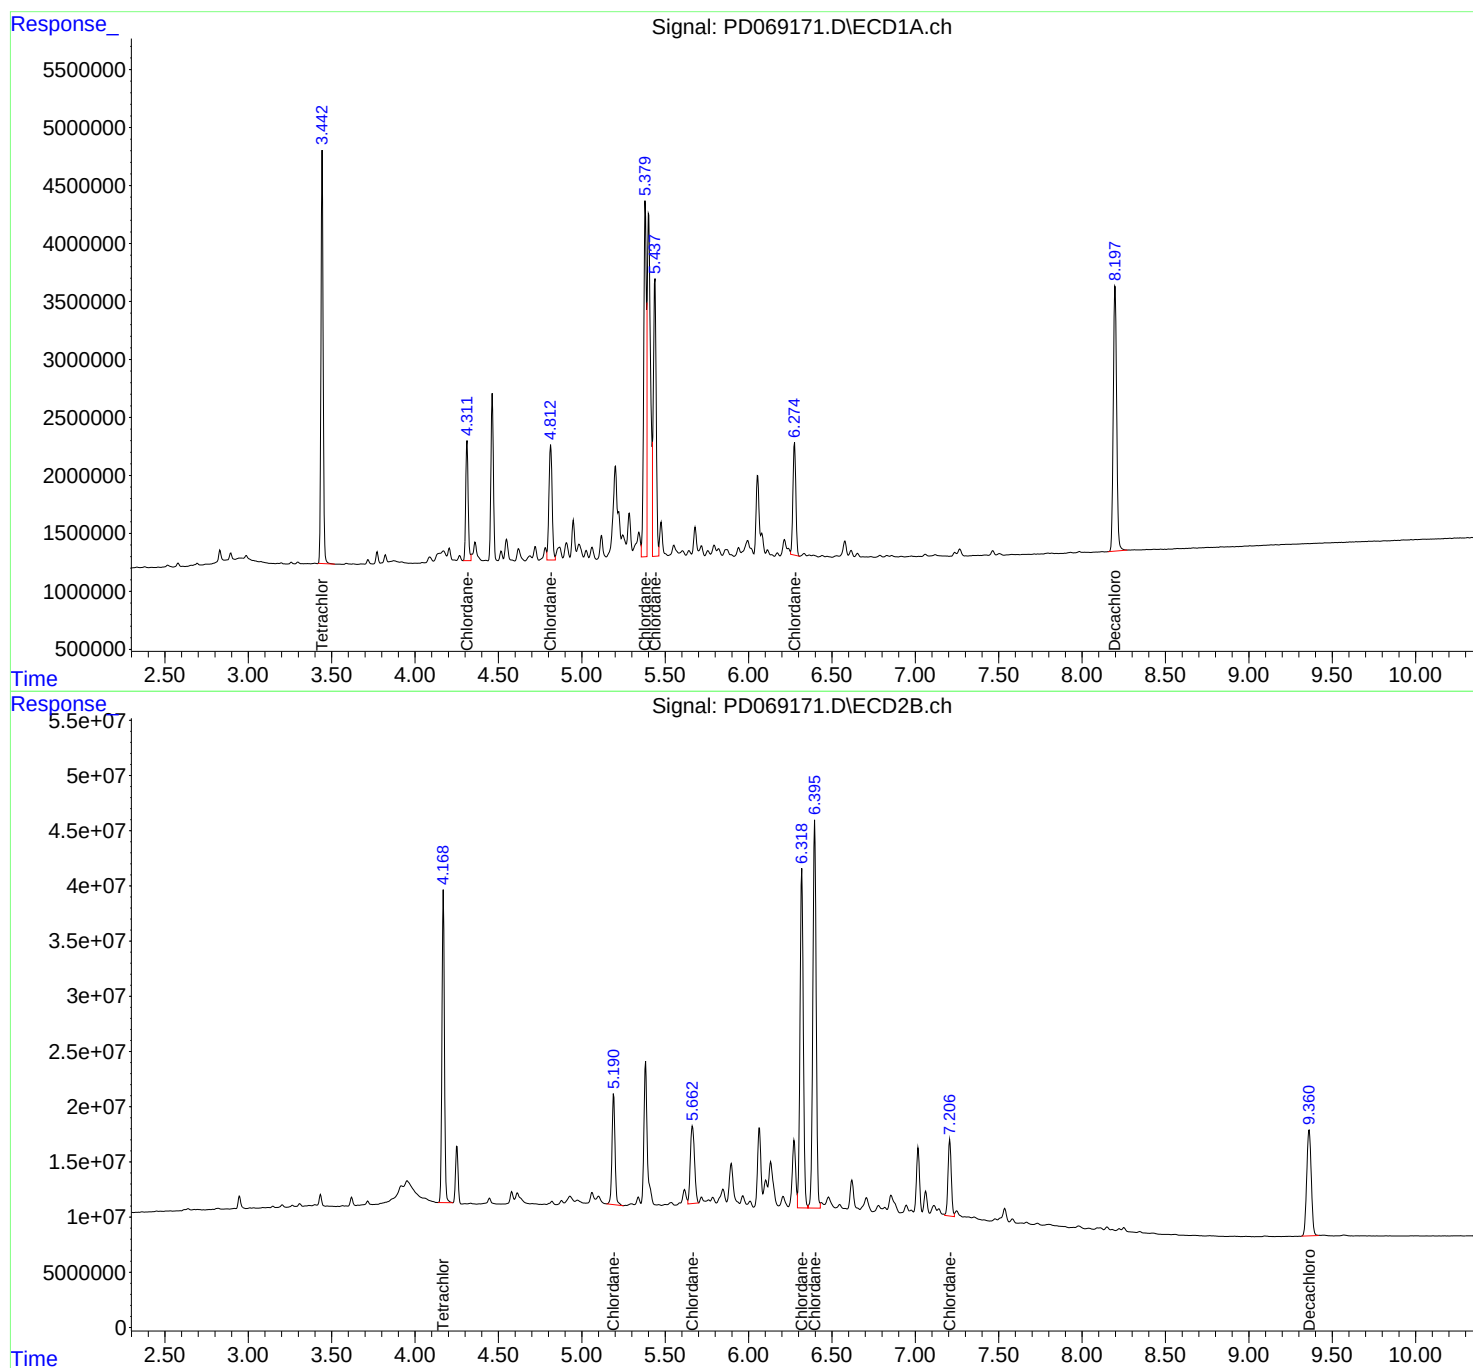


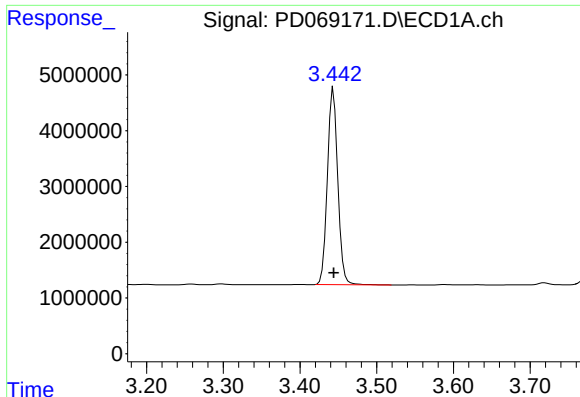

#1 Tetrachloro-m-xylene


R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 33082810
Conc: 24.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

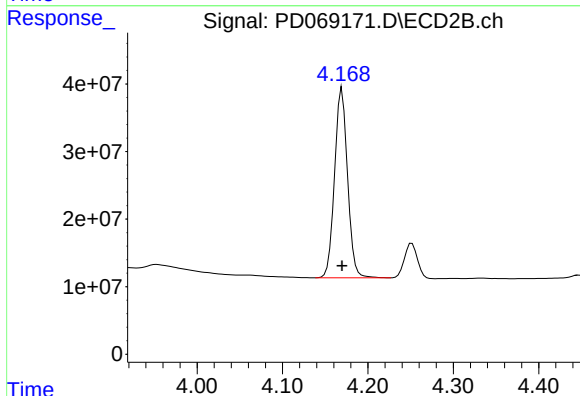


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 296312101
Conc: 26.57 ng/ml

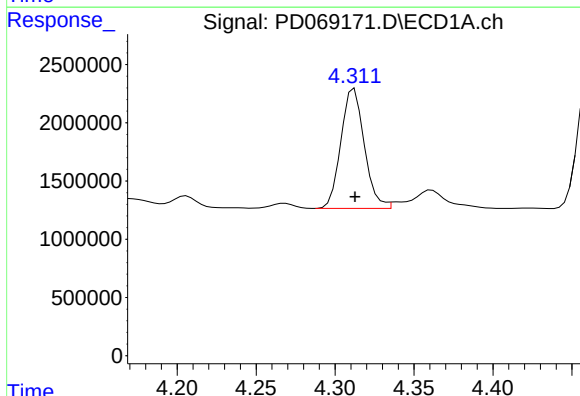


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 10642220
Conc: 255.40 ng/ml

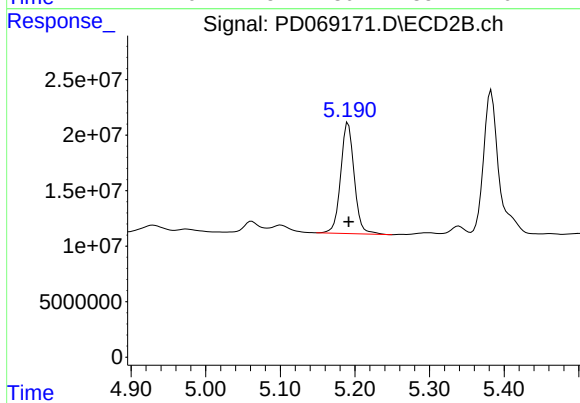

#23 Chlordane-1


R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 125858439
Conc: 269.08 ng/ml

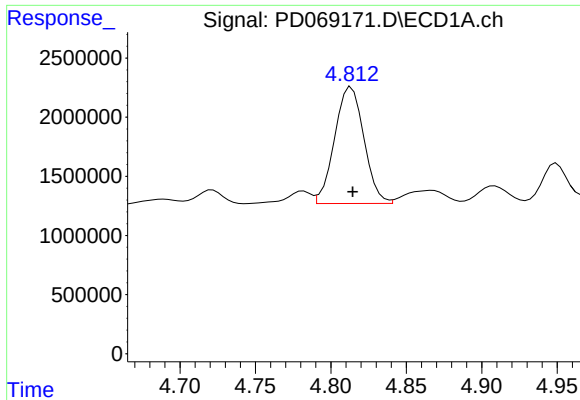

#24 Chlordane-2


R.T.: 4.814 min
Delta R.T.: 0.000 min
Response: 13316838
Conc: 268.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

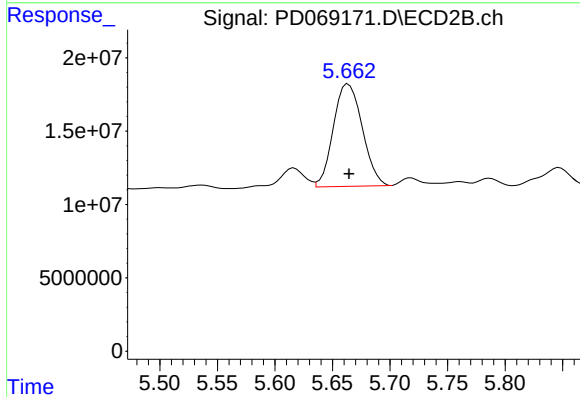


#24 Chlordane-2

R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 122407713
Conc: 274.79 ng/ml

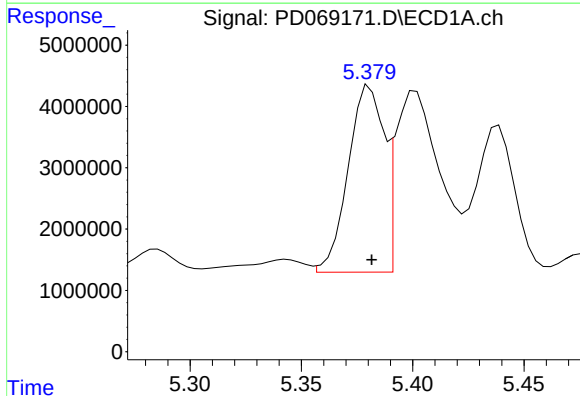


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 33947801
Conc: 248.23 ng/ml

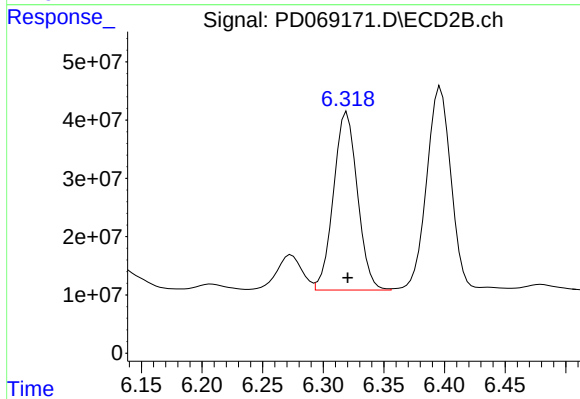

#25 Chlordane-3


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 419618864
Conc: 263.49 ng/ml

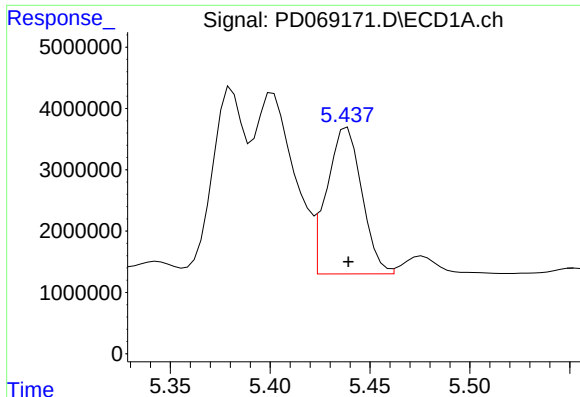

#26 Chlordane-4


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 29078614
Conc: 254.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

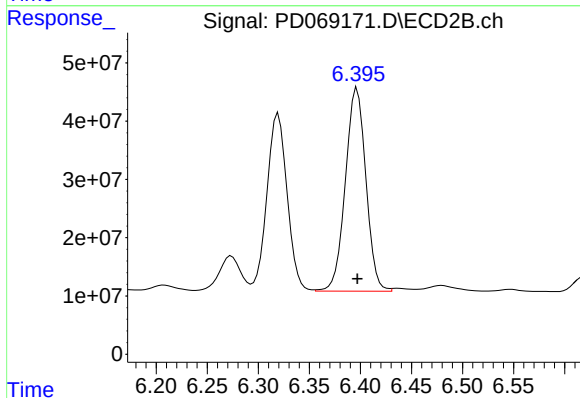


#26 Chlordane-4

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 488051515
Conc: 265.02 ng/ml

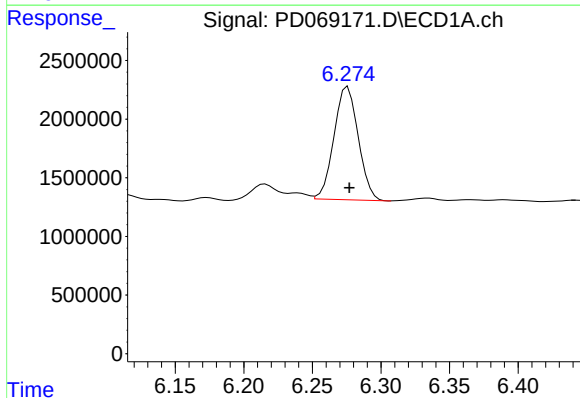


#27 Chlordane-5

R.T.: 6.276 min
Delta R.T.: -0.001 min
Response: 11867433
Conc: 255.52 ng/ml

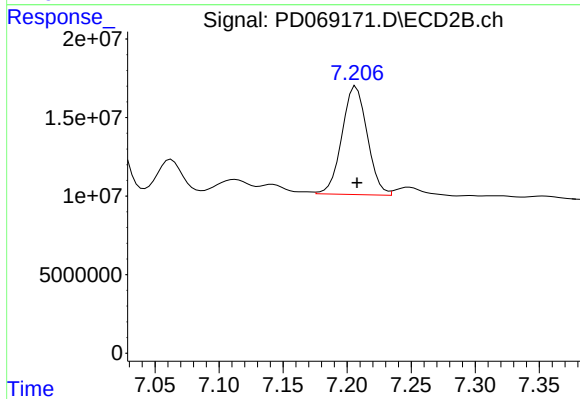

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 94520463
Conc: 266.77 ng/ml

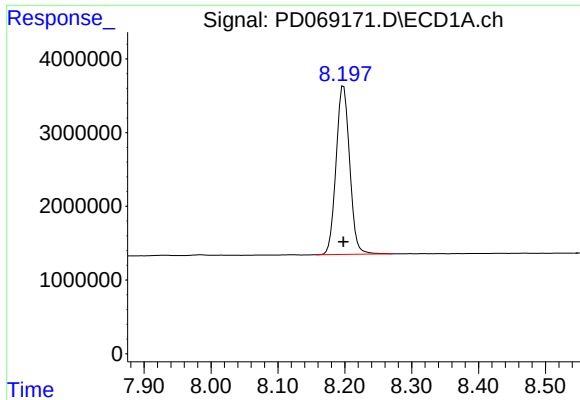

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: 0.000 min
Response: 32190205
Conc: 26.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

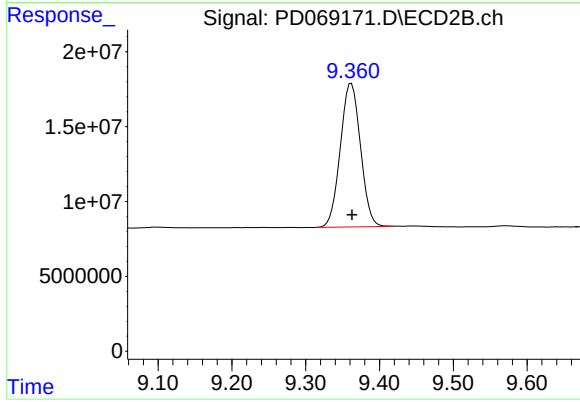

#28 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: 0.000 min
Response: 182188663
Conc: 27.47 ng/ml