

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
 Data File : PD069172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2022 11:02
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:26:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 18 13:25:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.170	6338315	63781262	4.758	5.719
28)	SA Decachlor...	8.197	9.362	6810855	39694278	5.707	5.986
Target Compounds							
23)	Chlordane-1	4.312	5.191	2124894	27827203	50.994	59.494
24)	Chlordane-2	4.813	5.664	2673961	26991108	53.906	60.592
25)	Chlordane-3	5.381	6.320	6719803	90967390	49.135	57.122
26)	Chlordane-4	5.439	6.397	5769250	108.4E6	50.523	58.857
27)	Chlordane-5	6.276	7.208	2011485	20873365	43.310	58.912 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041822\
Data File : PD069172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2022 11:02
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:26:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Mon Apr 18 13:25:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

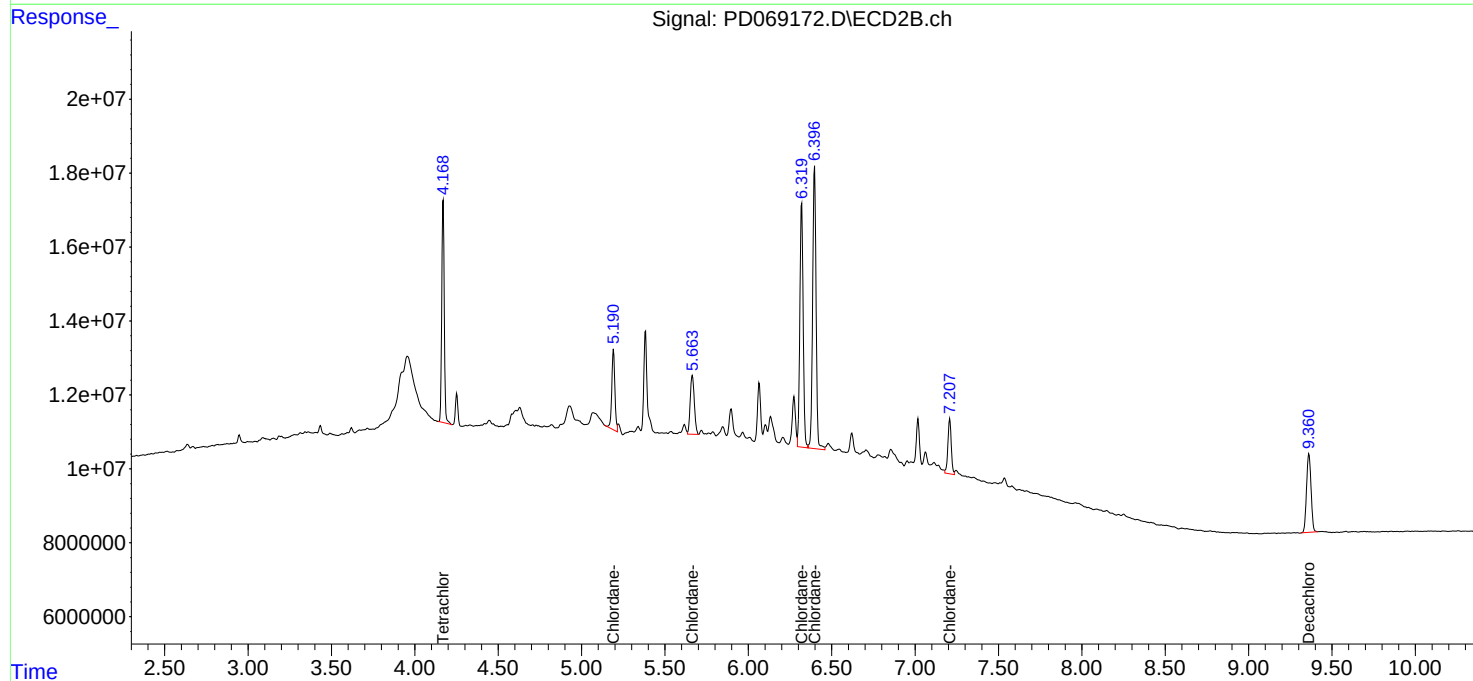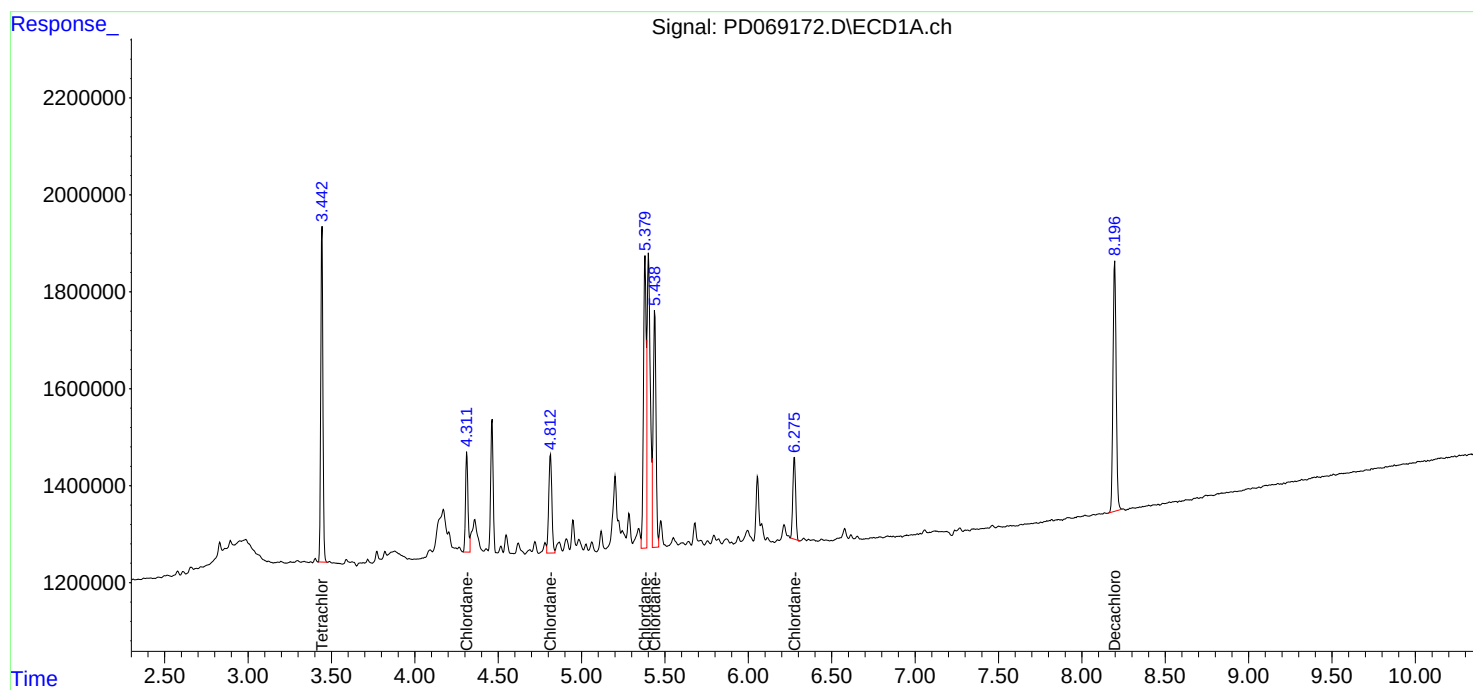


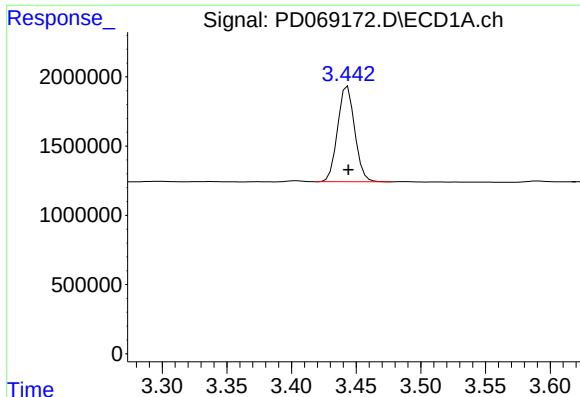

#1 Tetrachloro-m-xylene


R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 6338315
Conc: 4.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

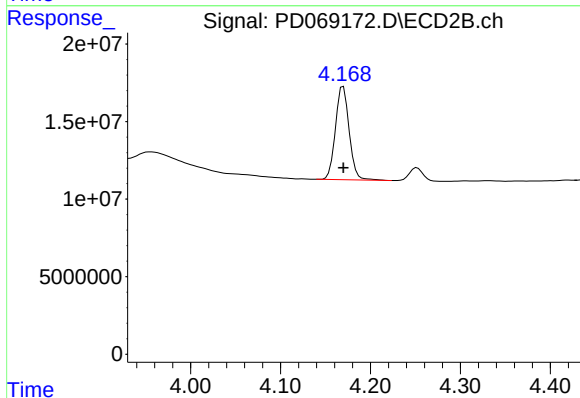


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.000 min
Response: 63781262
Conc: 5.72 ng/ml

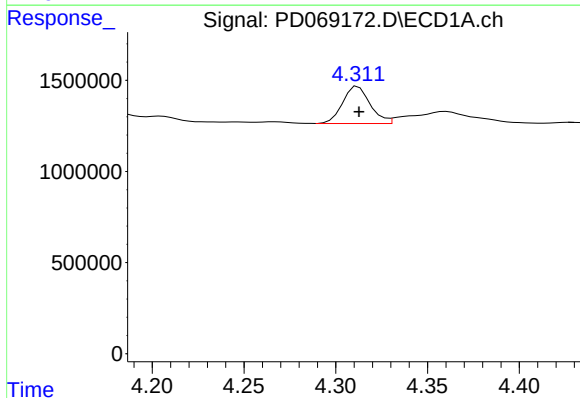


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 2124894
Conc: 50.99 ng/ml

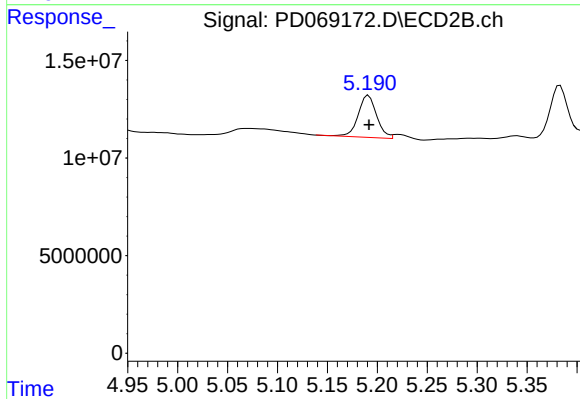

#23 Chlordane-1


R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 27827203
Conc: 59.49 ng/ml

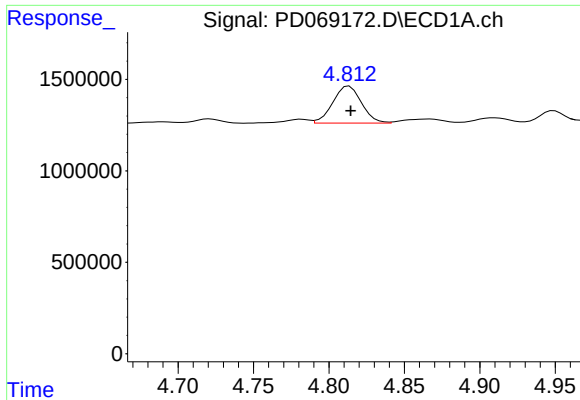

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: -0.001 min
Response: 2673961
Conc: 53.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

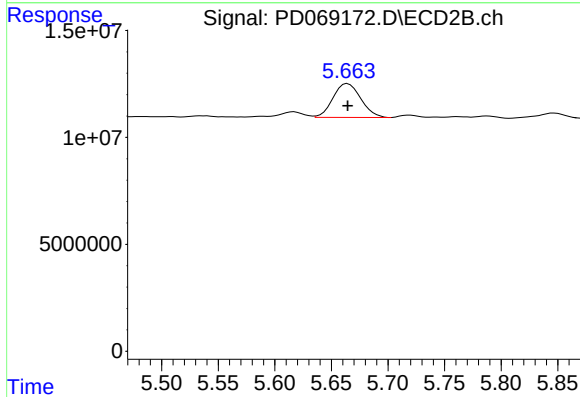


#24 Chlordane-2

R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 26991108
Conc: 60.59 ng/ml

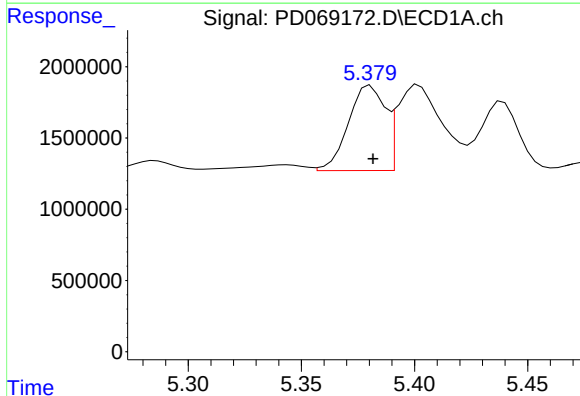


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: -0.001 min
Response: 6719803
Conc: 49.14 ng/ml

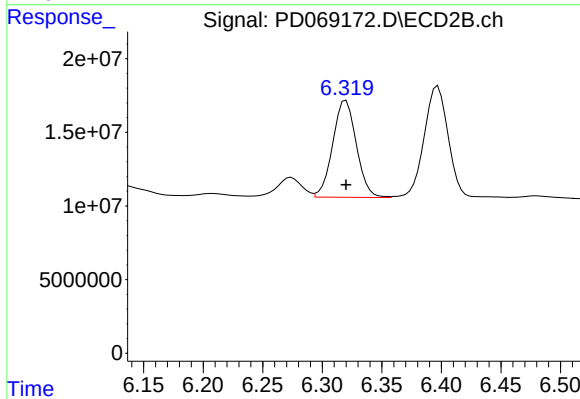

#25 Chlordane-3


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 90967390
Conc: 57.12 ng/ml

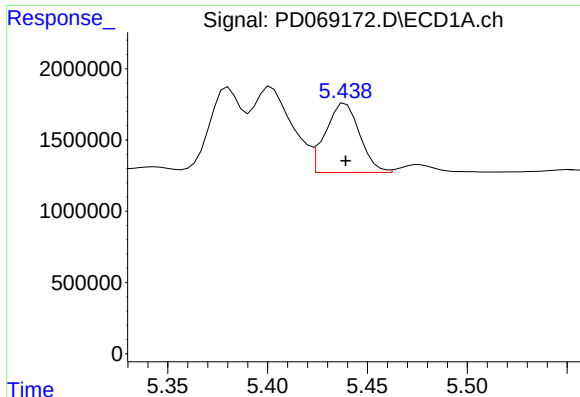

#26 Chlordane-4


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 5769250
Conc: 50.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

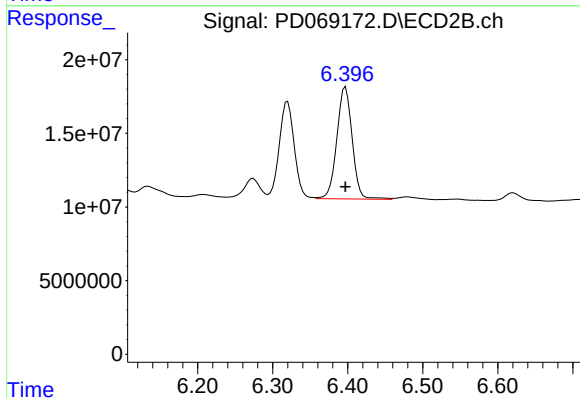


#26 Chlordane-4

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 108388736
Conc: 58.86 ng/ml

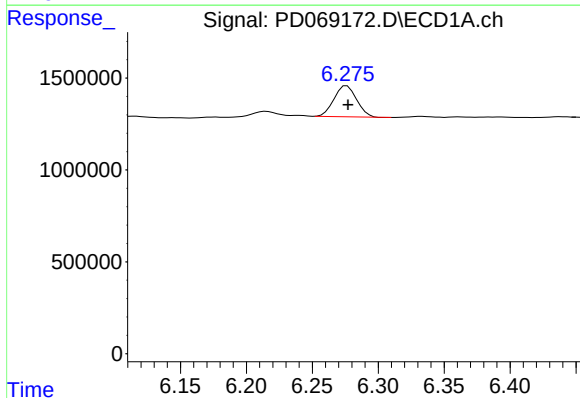


#27 Chlordane-5

R.T.: 6.276 min
Delta R.T.: 0.000 min
Response: 2011485
Conc: 43.31 ng/ml

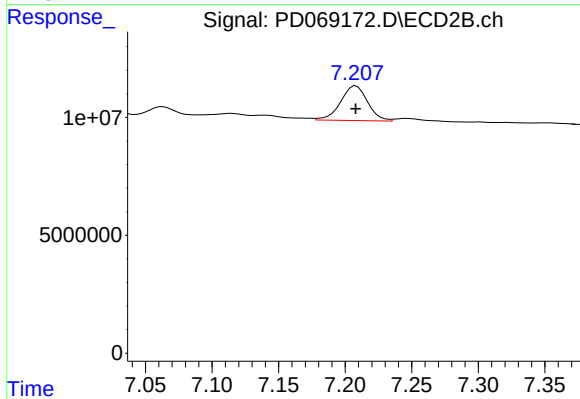

#27 Chlordane-5


R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 20873365
Conc: 58.91 ng/ml

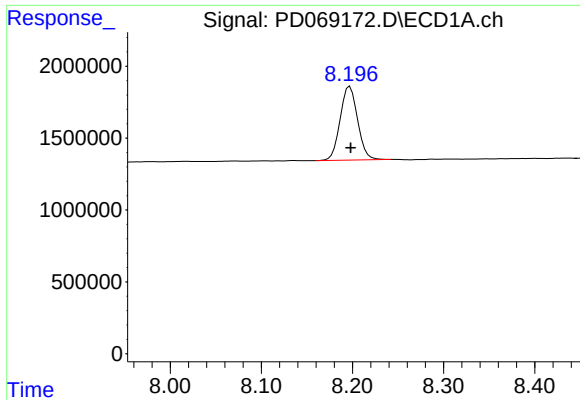

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: 0.000 min
Response: 6810855
Conc: 5.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

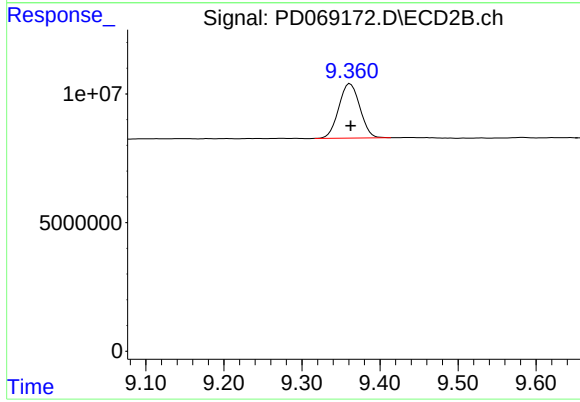

#28 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: -0.001 min
Response: 39694278
Conc: 5.99 ng/ml