

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041823\
 Data File : PD074778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2023 11:55
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:13:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 18 13:11:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.768	52827552	34444888	24.693	24.354
28)	SA Decachlor...	9.095	7.921	70639730	31449508	26.642	26.187
Target Compounds							
23)	Chlordane-1	4.715	3.769	28307855	12343157	253.988	250.007
24)	Chlordane-2	5.245	4.346	33552240	15357527	261.861	264.482
25)	Chlordane-3	5.959	4.977	120.5E6	41371984	240.273	244.564
26)	Chlordane-4	6.042	5.041	148.8E6	40106011	243.399	246.705
27)	Chlordane-5	6.893	5.938	26819446	15308084	250.840	249.495



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041823\
Data File : PD074778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2023 11:55
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:13:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
Quant Title : GC Extractables
QLast Update : Tue Apr 18 13:11:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

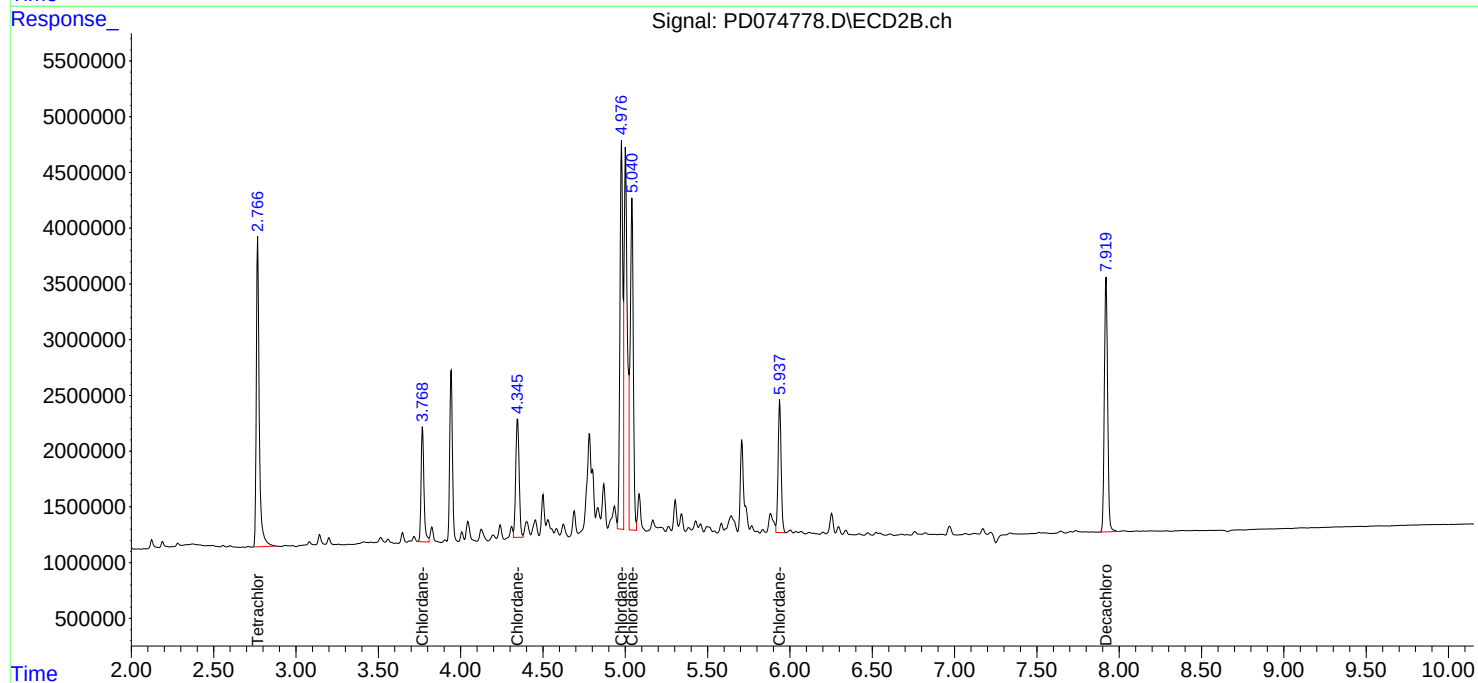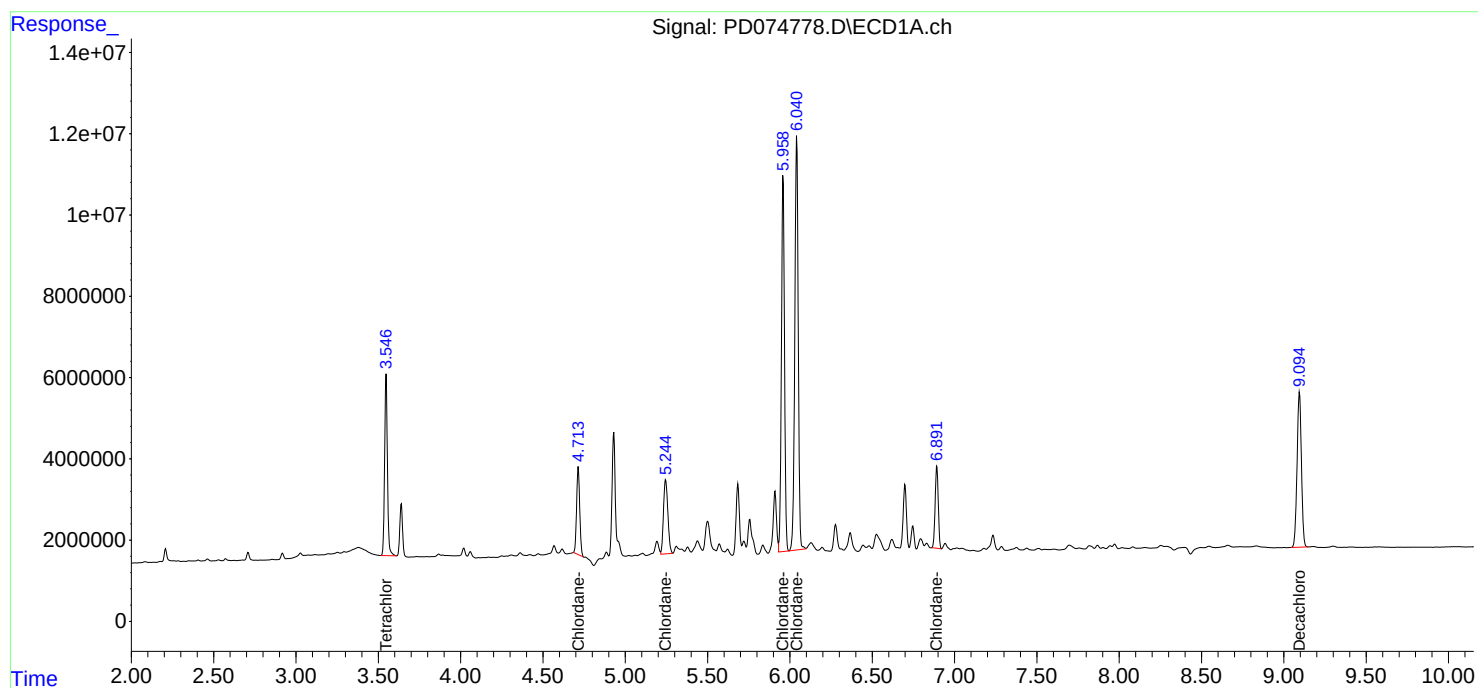


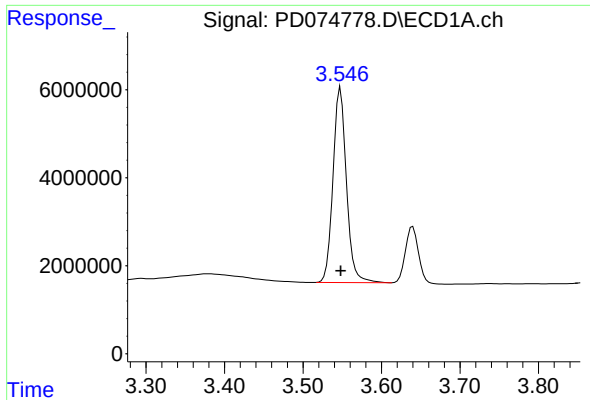

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 52827552
Conc: 24.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

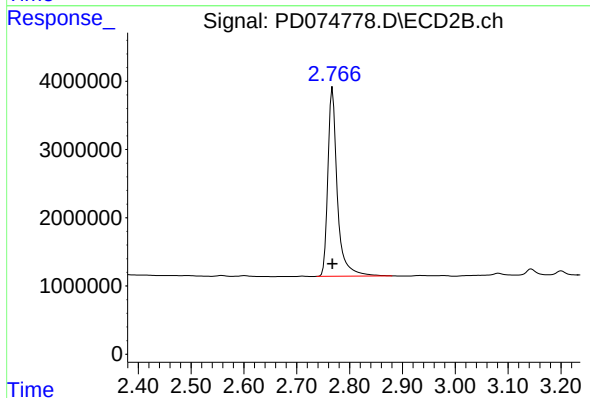


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 34444888
Conc: 24.35 ng/ml

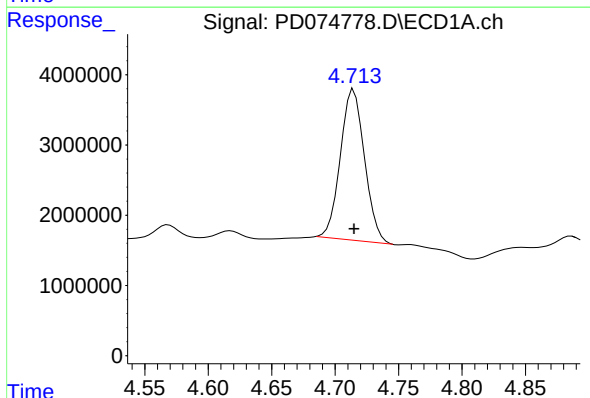


#23 Chlordane-1

R.T.: 4.715 min
Delta R.T.: 0.000 min
Response: 28307855
Conc: 253.99 ng/ml

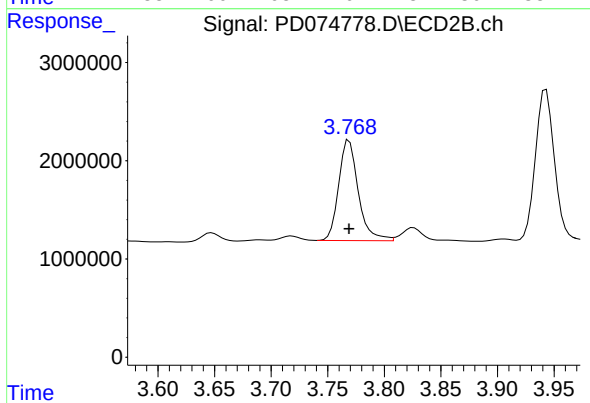

#23 Chlordane-1


R.T.: 3.769 min
Delta R.T.: 0.000 min
Response: 12343157
Conc: 250.01 ng/ml

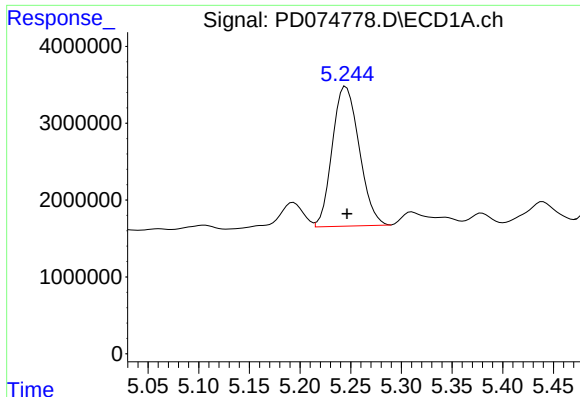

#24 Chlordane-2


R.T.: 5.245 min
Delta R.T.: 0.000 min
Response: 33552240
Conc: 261.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

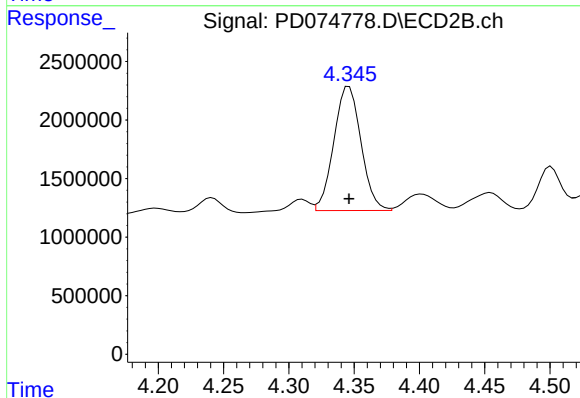


#24 Chlordane-2

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 15357527
Conc: 264.48 ng/ml

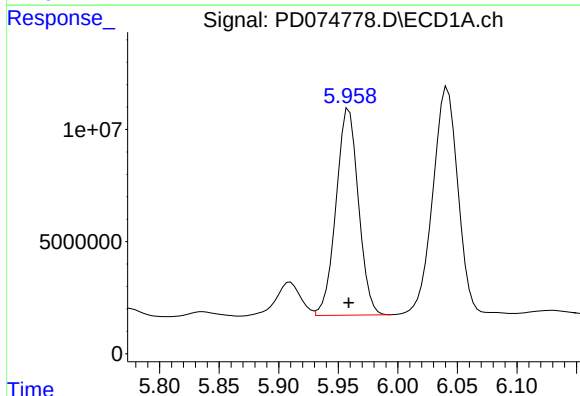


#25 Chlordane-3

R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 120507094
Conc: 240.27 ng/ml

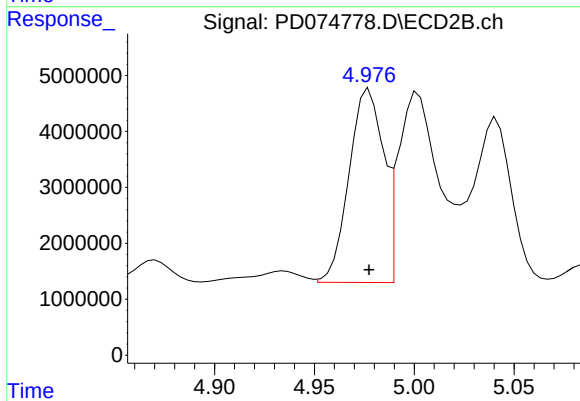

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 41371984
Conc: 244.56 ng/ml

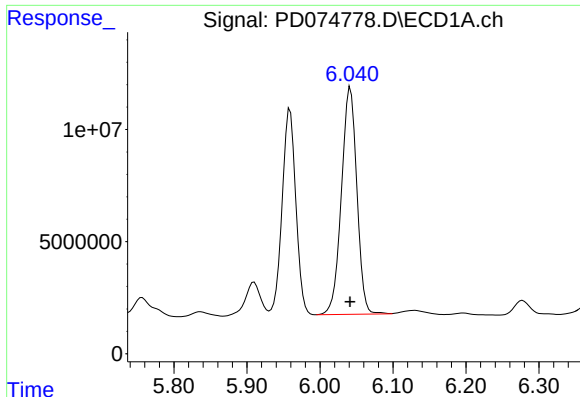

#26 Chlordane-4


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 148831467
Conc: 243.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

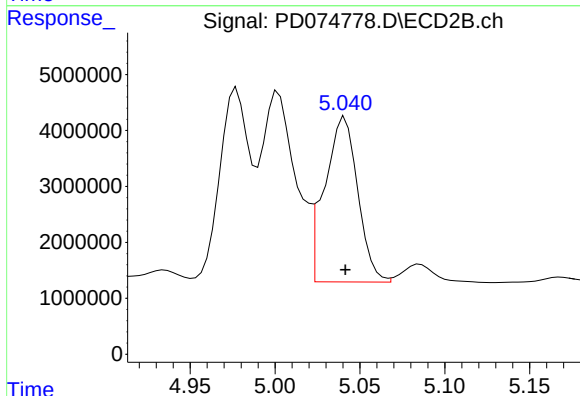


#26 Chlordane-4

R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 40106011
Conc: 246.71 ng/ml

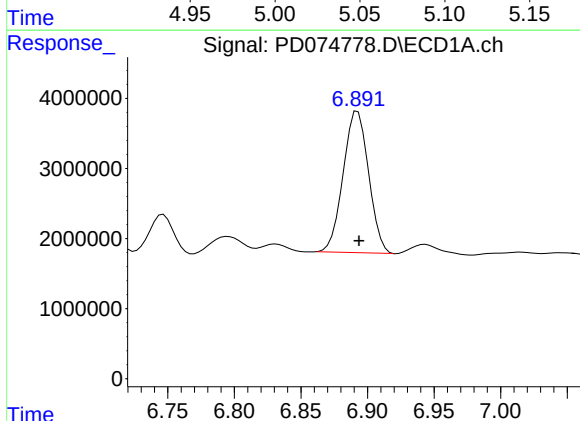


#27 Chlordane-5

R.T.: 6.893 min
Delta R.T.: -0.001 min
Response: 26819446
Conc: 250.84 ng/ml

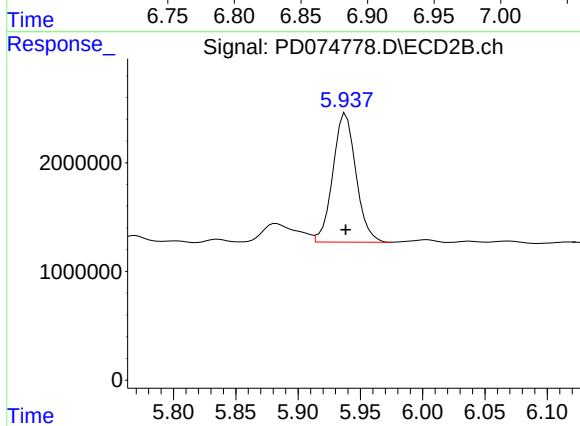

#27 Chlordane-5


R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 15308084
Conc: 249.50 ng/ml

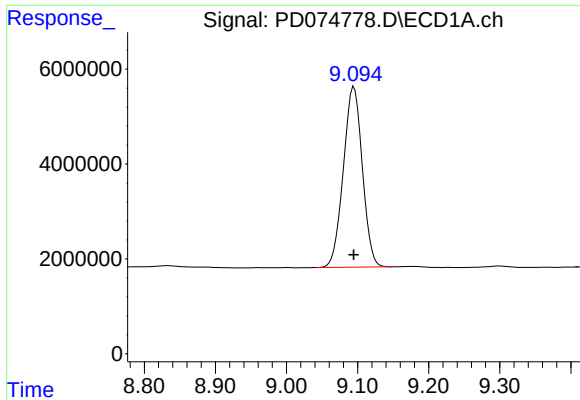

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 70639730
Conc: 26.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

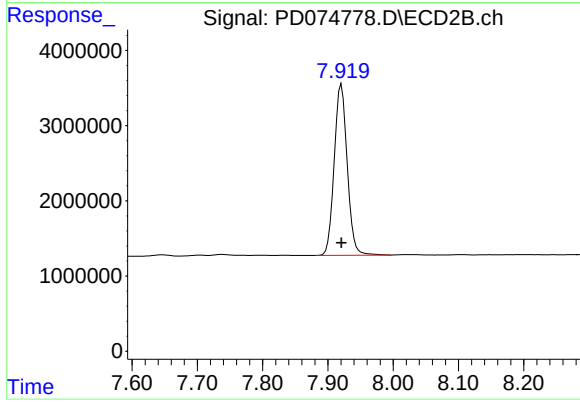

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: 0.000 min
Response: 31449508
Conc: 26.19 ng/ml