

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041823\
 Data File : PD074769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2023 09:54
 Operator : AR\AJ
 Sample : RESCH
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 16:11:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 18 13:17:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.768	49929990	27678343	20.933	21.233
28)	SA Decachlor...	9.095	7.921	62903108	27825849	20.714	20.861
Target Compounds							
9)	A Endosulfan I	6.087	5.097	31885220	16267435	9.772m	10.144
10)	B gamma-Chl...	5.956	4.977	33544394	18082541	9.673m	10.443
12)	B 4,4'-DDE	6.209	5.231	61995159	31189478	19.337	19.887
13)	MA Dieldrin	6.364	5.362	67845664	34299500	19.890	20.429
19)	B Endosulfa...	7.178	6.334	52645032	25216069	18.226	18.247
20)	A Methoxychlor	7.519	6.615	151.4E6	69965416	92.994	92.828
21)	B Endrin ke...	7.665	6.842	65120965	32961903	19.994	20.170



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041823\
Data File : PD074769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2023 09:54
Operator : AR\AJ
Sample : RESCH
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 16:11:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
Quant Title : GC Extractables
QLast Update : Tue Apr 18 13:17:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

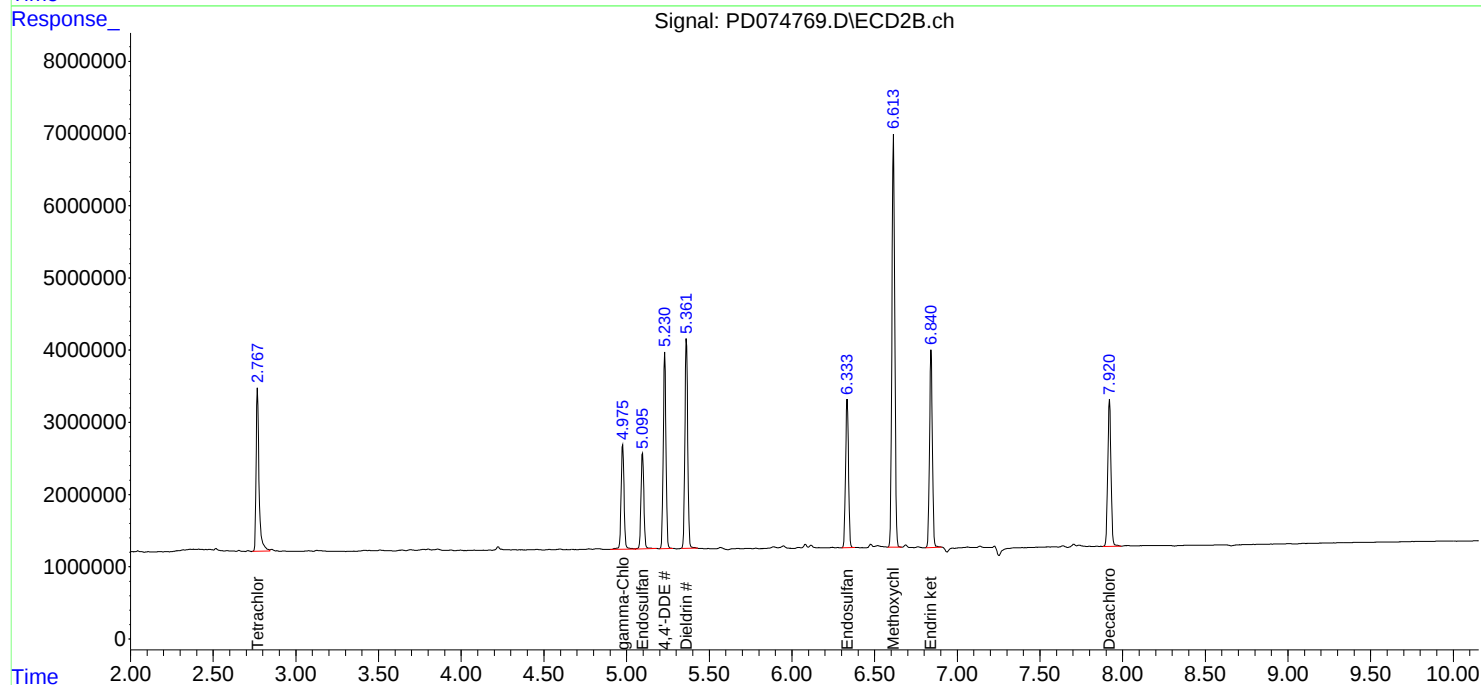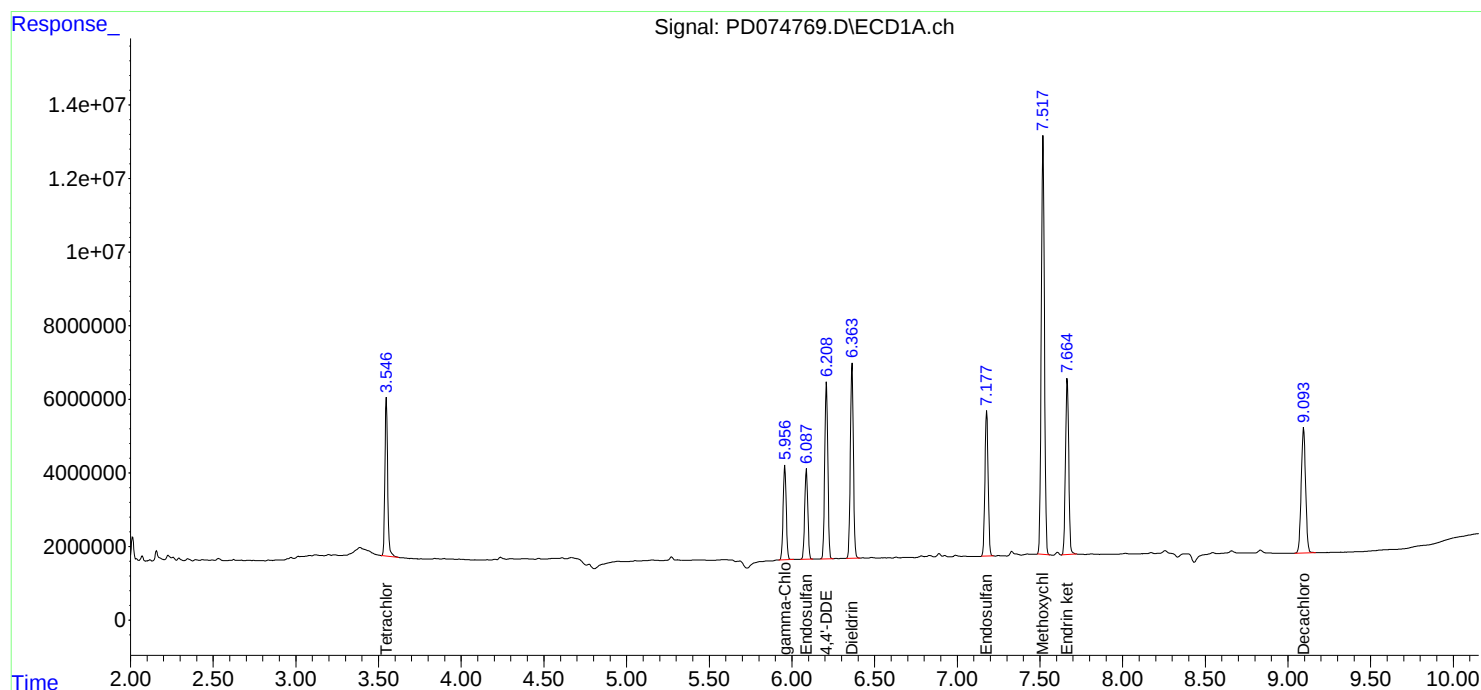


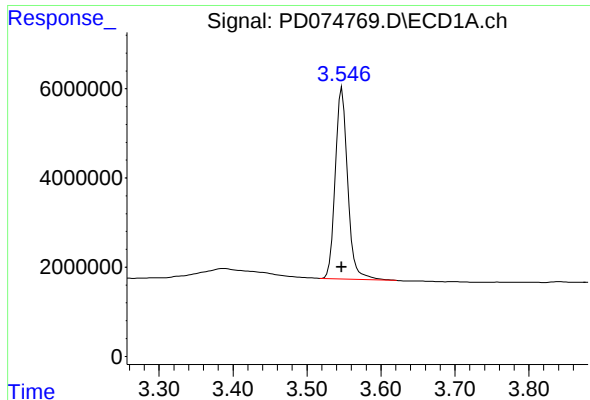

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 49929990
Conc: 20.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCH

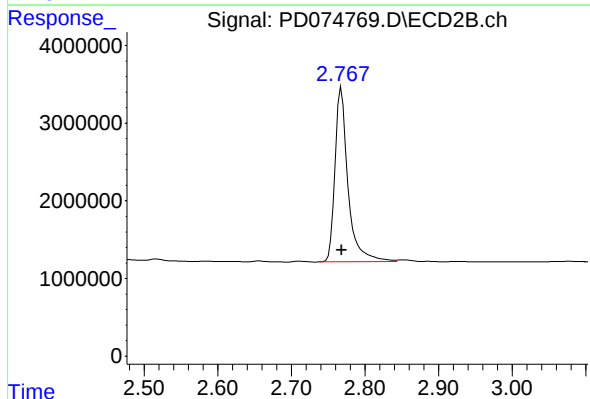


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 27678343
Conc: 21.23 ng/ml

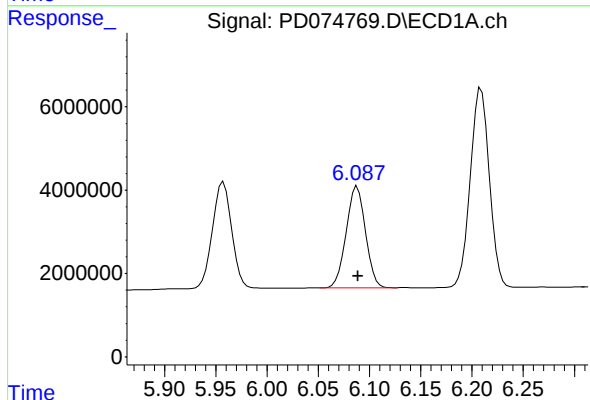


#9 Endosulfan I

R.T.: 6.087 min
Delta R.T.: -0.002 min
Response: 31885220
Conc: 9.77 ng/ml m

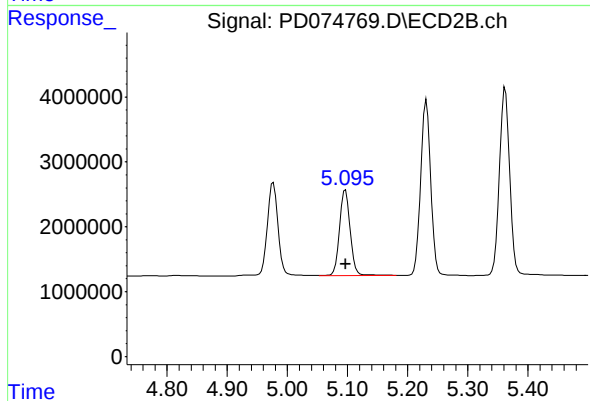

#9 Endosulfan I


R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 16267435
Conc: 10.14 ng/ml

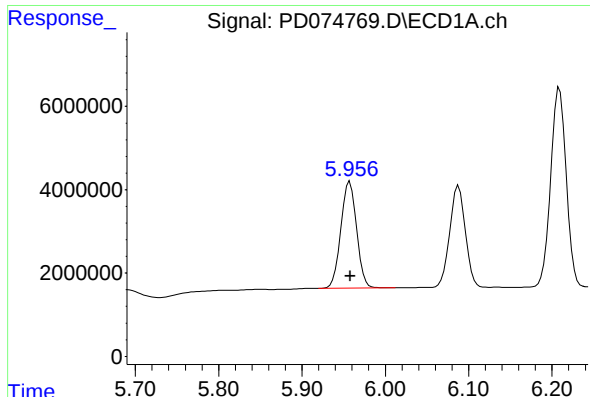

#10 gamma-Chlordane


R.T.: 5.956 min
Delta R.T.: -0.002 min
Response: 33544394
Conc: 9.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCH

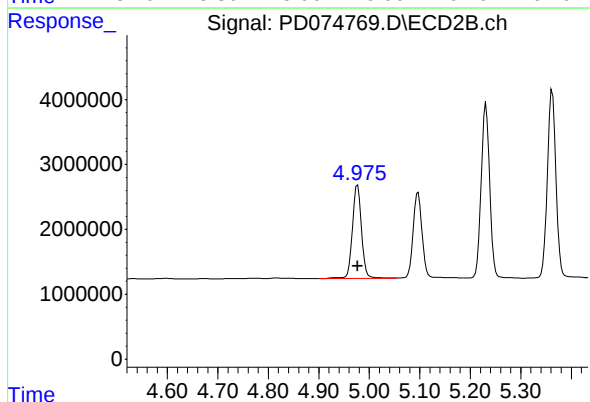


#10 gamma-Chlordane

R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 18082541
Conc: 10.44 ng/ml

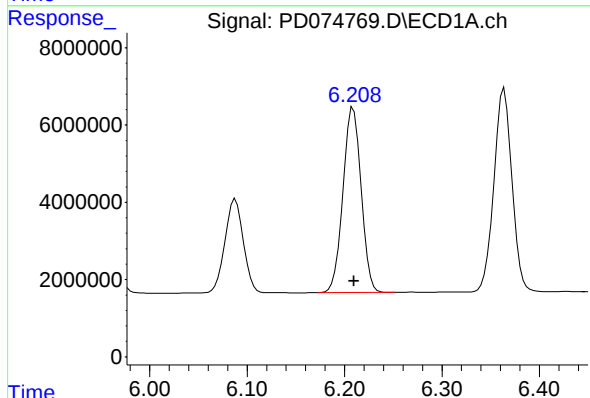


#12 4,4'-DDE

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 61995159
Conc: 19.34 ng/ml

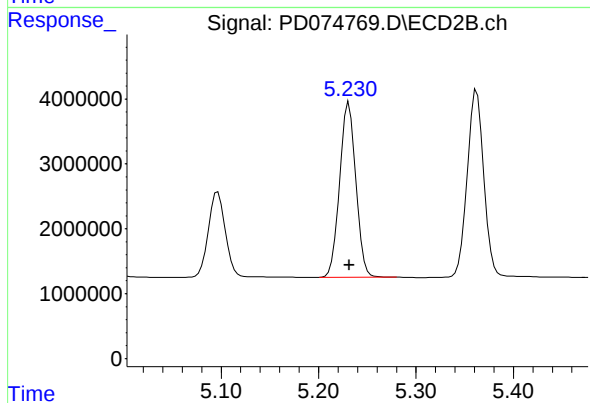

#12 4,4'-DDE


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 31189478
Conc: 19.89 ng/ml

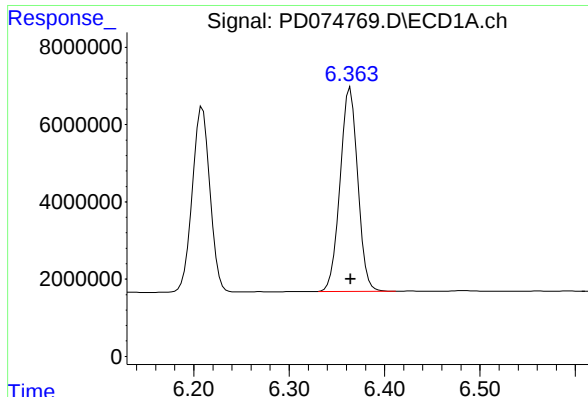

#13 Dieldrin


R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 67845664
Conc: 19.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCH

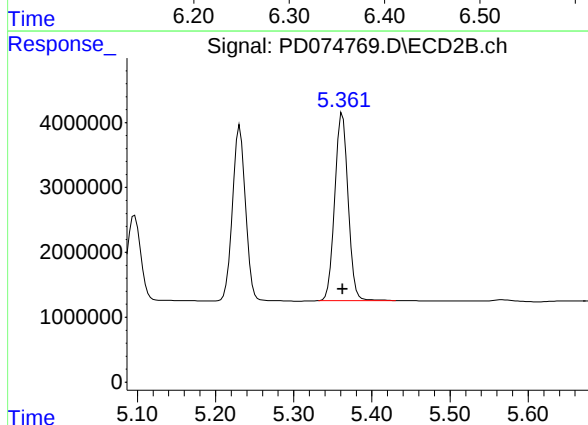


#13 Dieldrin

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 34299500
Conc: 20.43 ng/ml

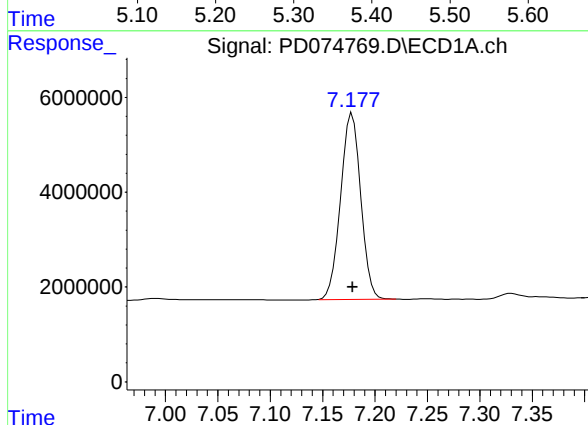


#19 Endosulfan Sulfate

R.T.: 7.178 min
Delta R.T.: 0.000 min
Response: 52645032
Conc: 18.23 ng/ml

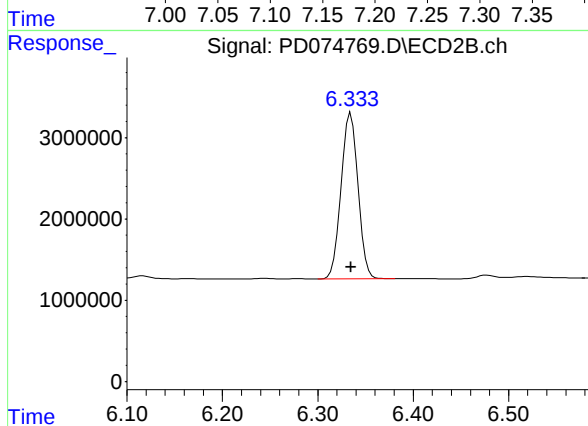

#19 Endosulfan Sulfate


R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 25216069
Conc: 18.25 ng/ml

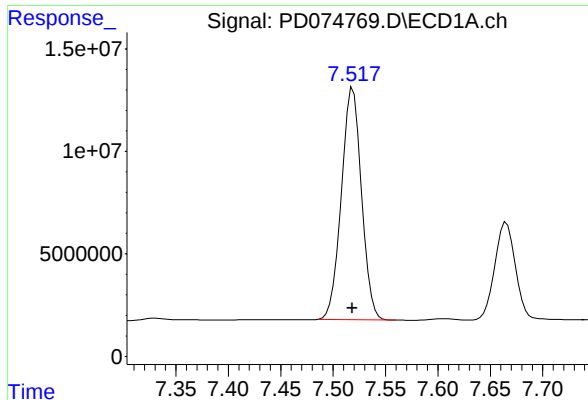

#20 Methoxychlor


R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 151439785
Conc: 92.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCH

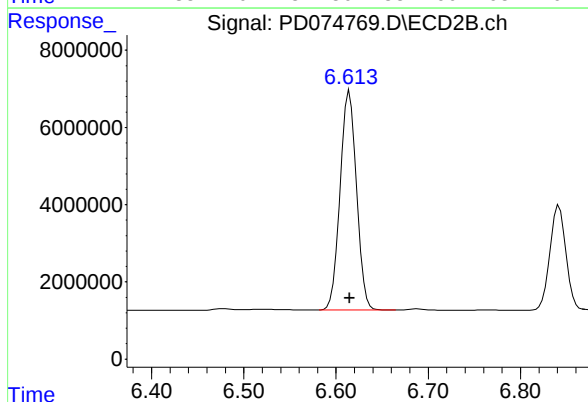


#20 Methoxychlor

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 69965416
Conc: 92.83 ng/ml

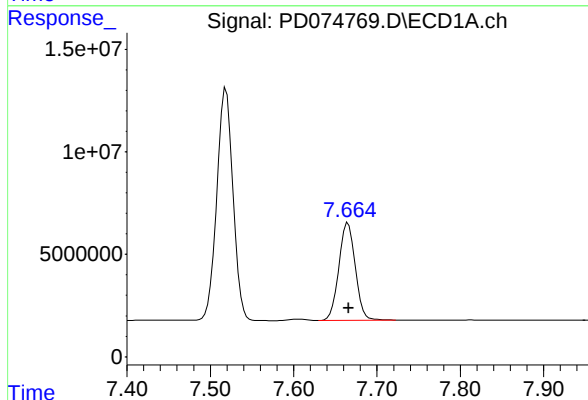


#21 Endrin ketone

R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 65120965
Conc: 19.99 ng/ml

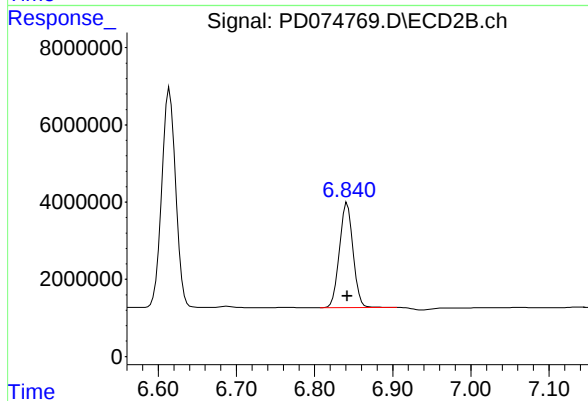

#21 Endrin ketone


R.T.: 6.842 min
Delta R.T.: 0.000 min
Response: 32961903
Conc: 20.17 ng/ml

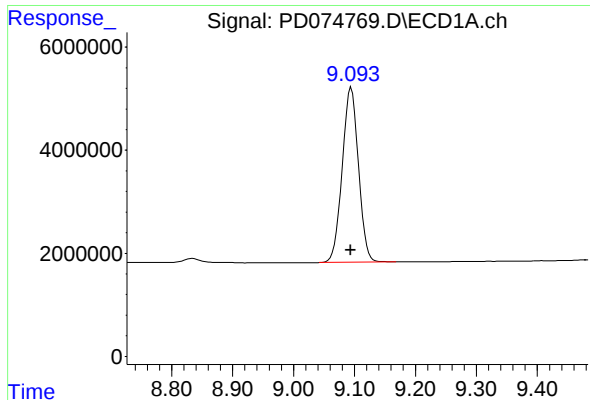

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 62903108
Conc: 20.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCH

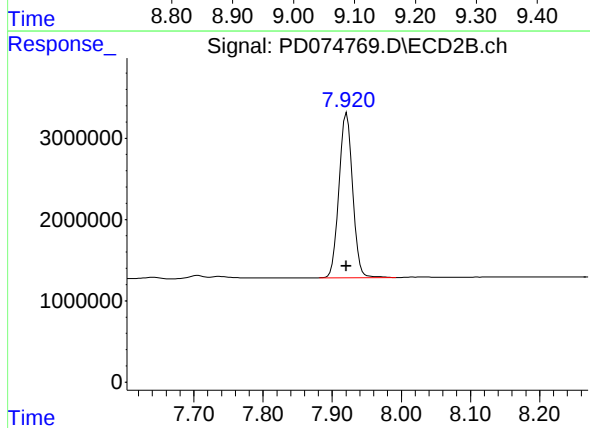

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: 0.000 min
Response: 27825849
Conc: 20.86 ng/ml