

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041823\
 Data File : PD074777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2023 11:41
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:12:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 18 13:11:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.768	107.0E6	70716848	50.000	50.000
28) SA Decachlor...	9.095	7.921	132.6E6	60047627	50.000	50.000
Target Compounds						
23) Chlordane-1	4.715	3.769	55726720	24685587	500.000	500.000
24) Chlordane-2	5.246	4.346	64064985	29033243	500.000	500.000
25) Chlordane-3	5.959	4.977	250.8E6	84583021	500.000	500.000
26) Chlordane-4	6.041	5.041	305.7E6	81283274	500.000	500.000
27) Chlordane-5	6.894	5.938	53459321	30678109	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041823\
Data File : PD074777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2023 11:41
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:12:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
Quant Title : GC Extractables
QLast Update : Tue Apr 18 13:11:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

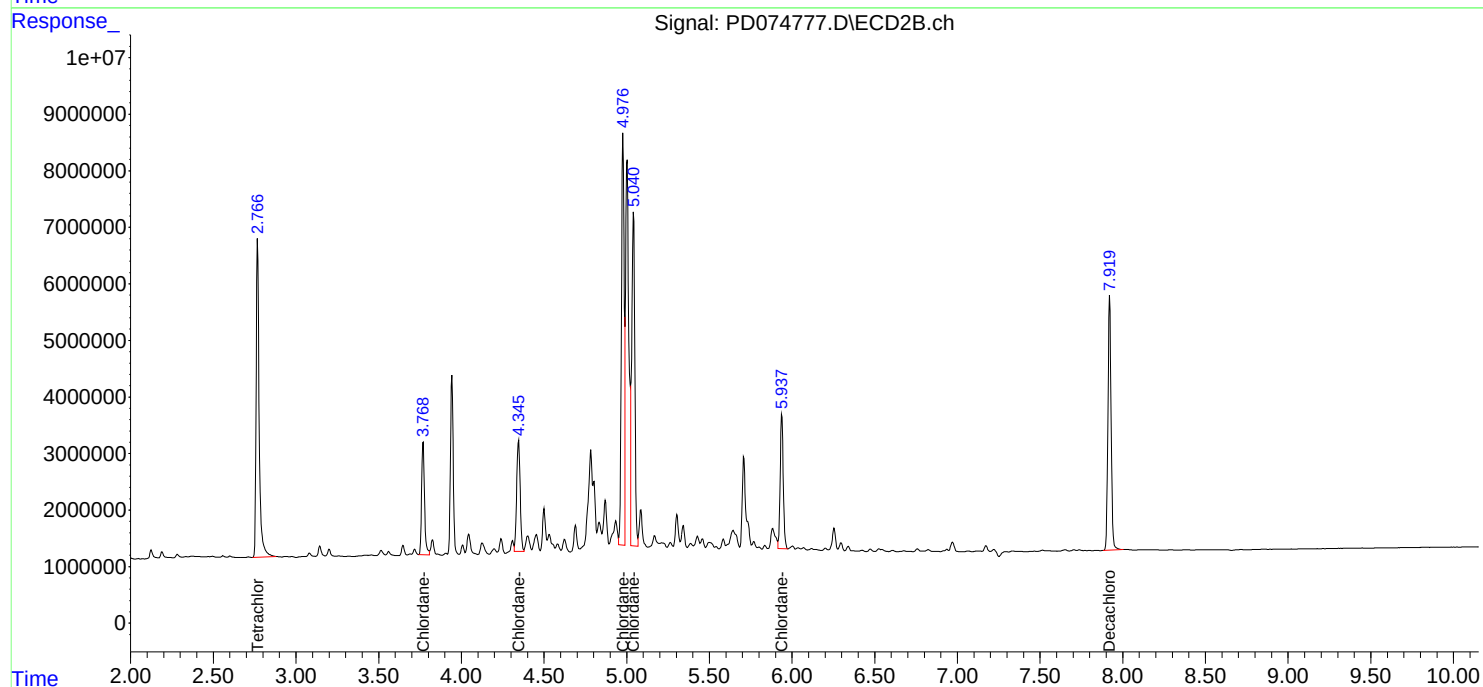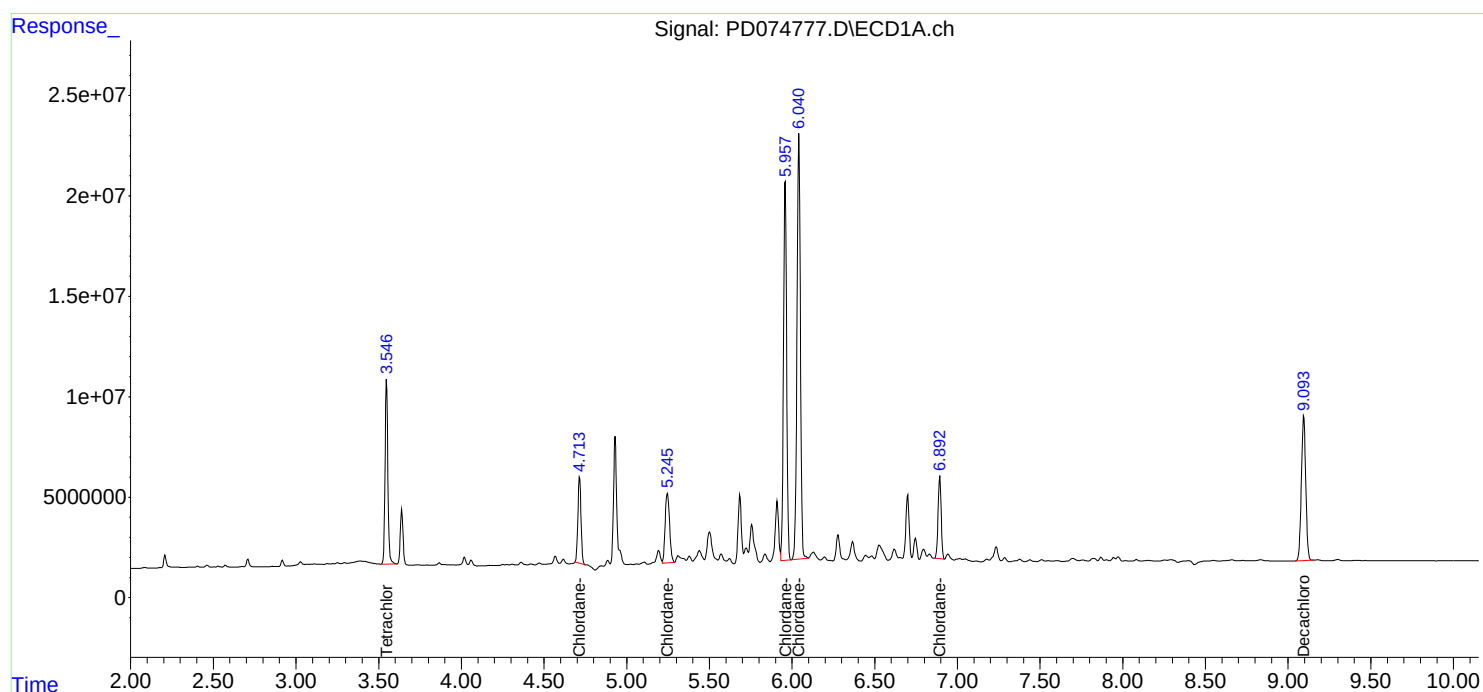


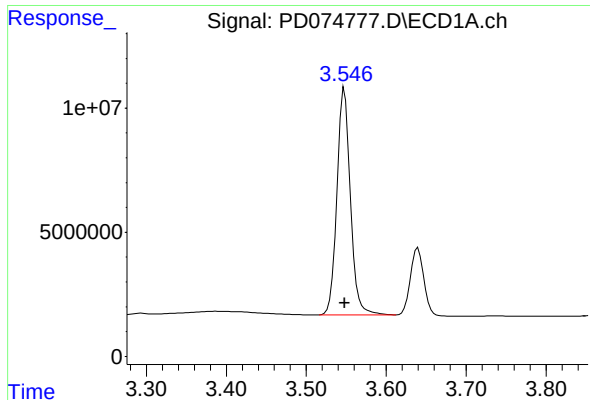

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 106969120
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

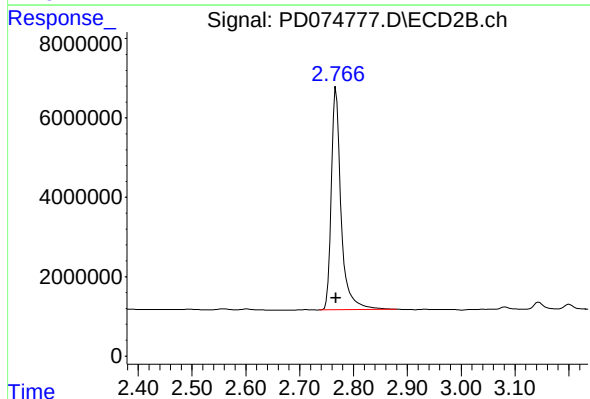


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 70716848
Conc: 50.00 ng/ml

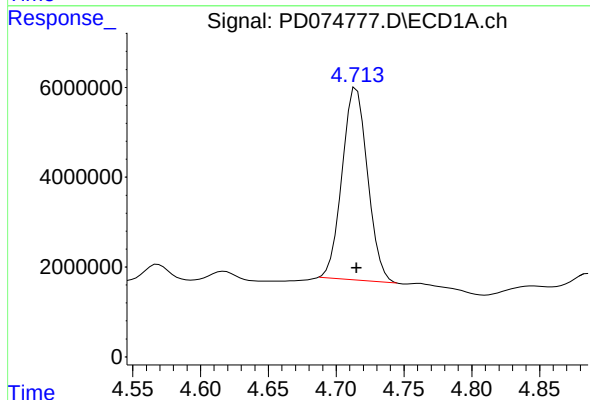


#23 Chlordane-1

R.T.: 4.715 min
Delta R.T.: 0.000 min
Response: 55726720
Conc: 500.00 ng/ml

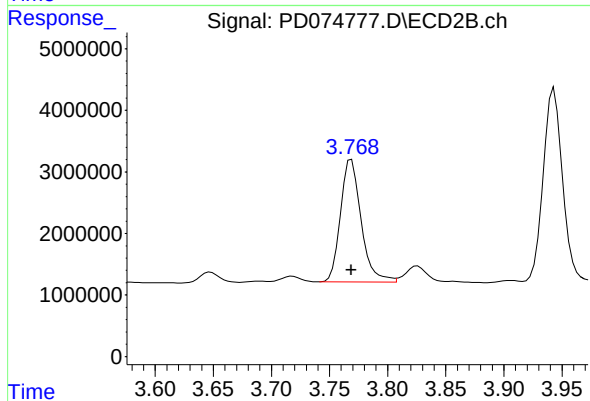

#23 Chlordane-1


R.T.: 3.769 min
Delta R.T.: 0.000 min
Response: 24685587
Conc: 500.00 ng/ml

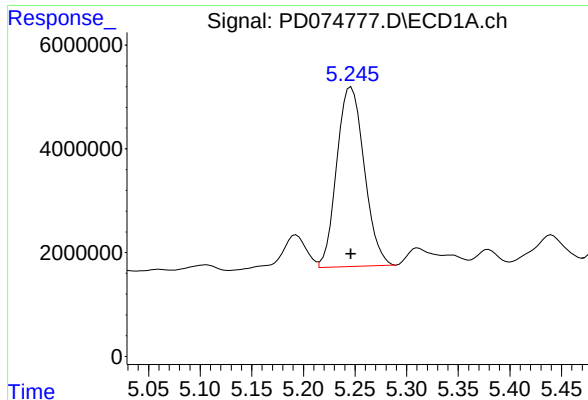

#24 Chlordane-2


R.T.: 5.246 min
Delta R.T.: 0.000 min
Response: 64064985
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

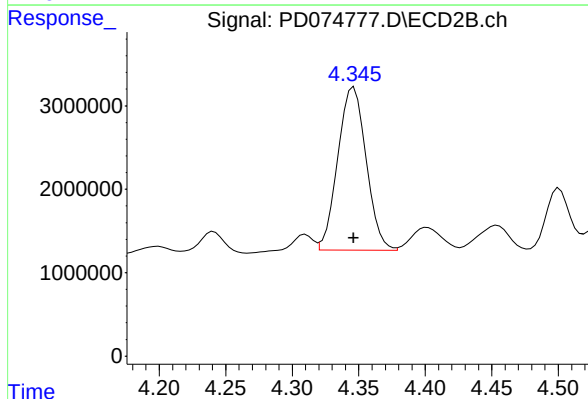


#24 Chlordane-2

R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 29033243
Conc: 500.00 ng/ml

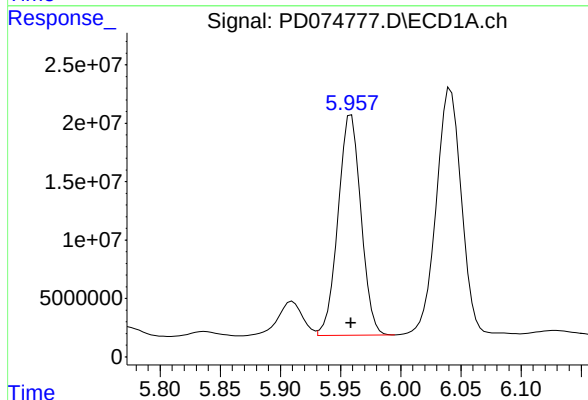


#25 Chlordane-3

R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 250771579
Conc: 500.00 ng/ml

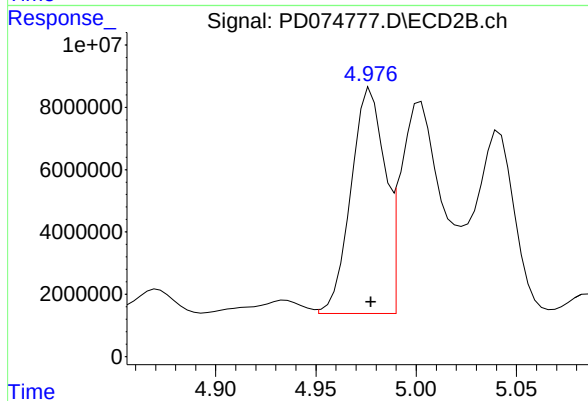

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 84583021
Conc: 500.00 ng/ml

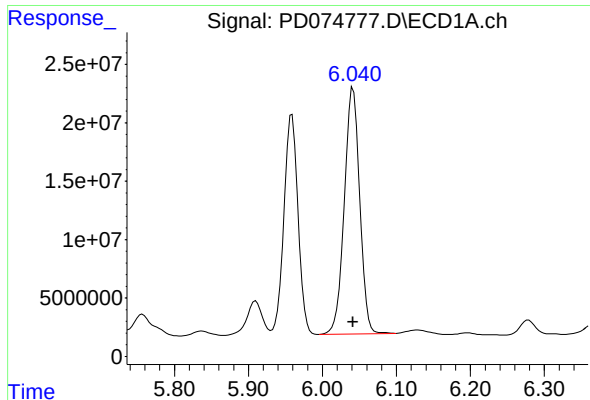

#26 Chlordane-4


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 305735517
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

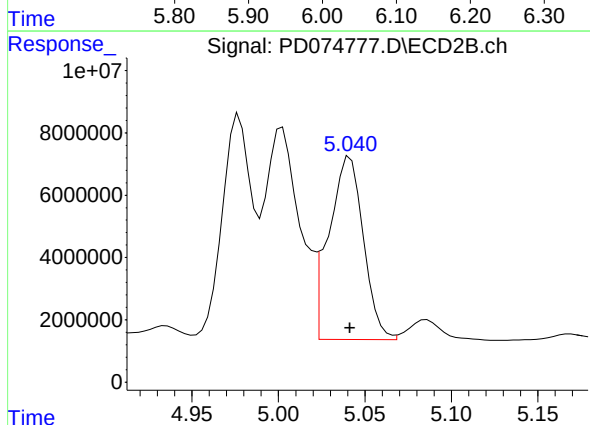


#26 Chlordane-4

R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 81283274
Conc: 500.00 ng/ml

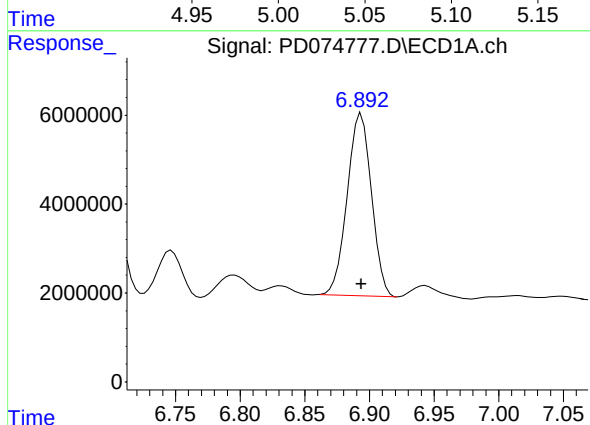


#27 Chlordane-5

R.T.: 6.894 min
Delta R.T.: 0.000 min
Response: 53459321
Conc: 500.00 ng/ml

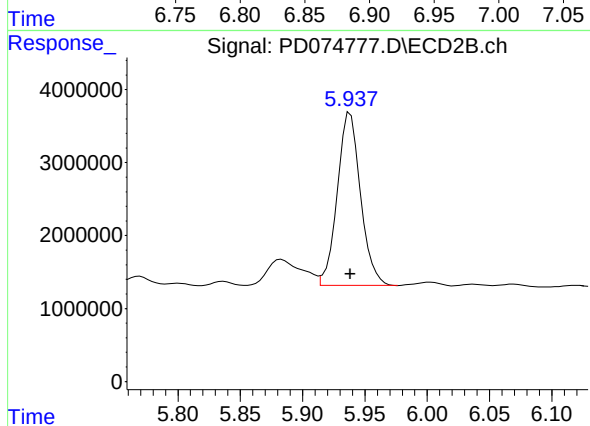

#27 Chlordane-5


R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 30678109
Conc: 500.00 ng/ml

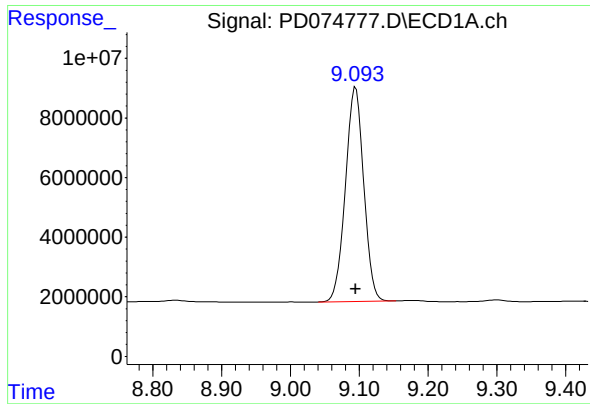

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 132574050
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

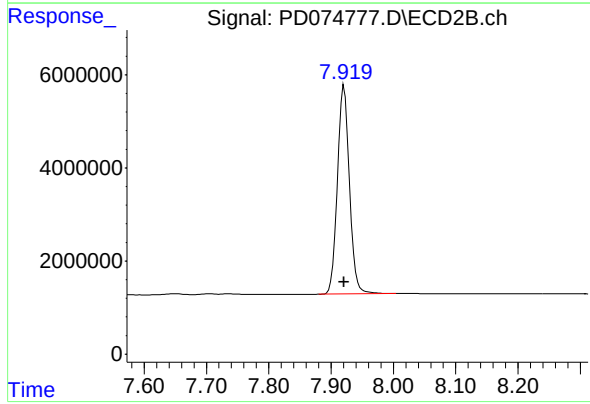

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: 0.000 min
Response: 60047627
Conc: 50.00 ng/ml