

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041825\
 Data File : PD088130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2025 15:18
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 05:48:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 19 05:47:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.883	141.7E6	1256.0E6	73.617	72.537
28) SA Decachlor...	9.075	8.077	221.1E6	1249.0E6	71.508	71.107
Target Compounds						
23) Chlordane-1	4.717	3.909	121.3E6	550.7E6	748.609	717.554
24) Chlordane-2	5.243	4.490	116.5E6	552.8E6	724.476	705.952
25) Chlordane-3	5.948	5.129	504.2E6	1726.8E6	756.864	720.458
26) Chlordane-4	6.034	5.194	599.5E6	1453.8E6	752.089	715.523
27) Chlordane-5	6.872	6.094	98919330	665.5E6	743.468	714.416



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041825\
Data File : PD088130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2025 15:18
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 05:48:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
Quant Title : GC Extractables
QLast Update : Sat Apr 19 05:47:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

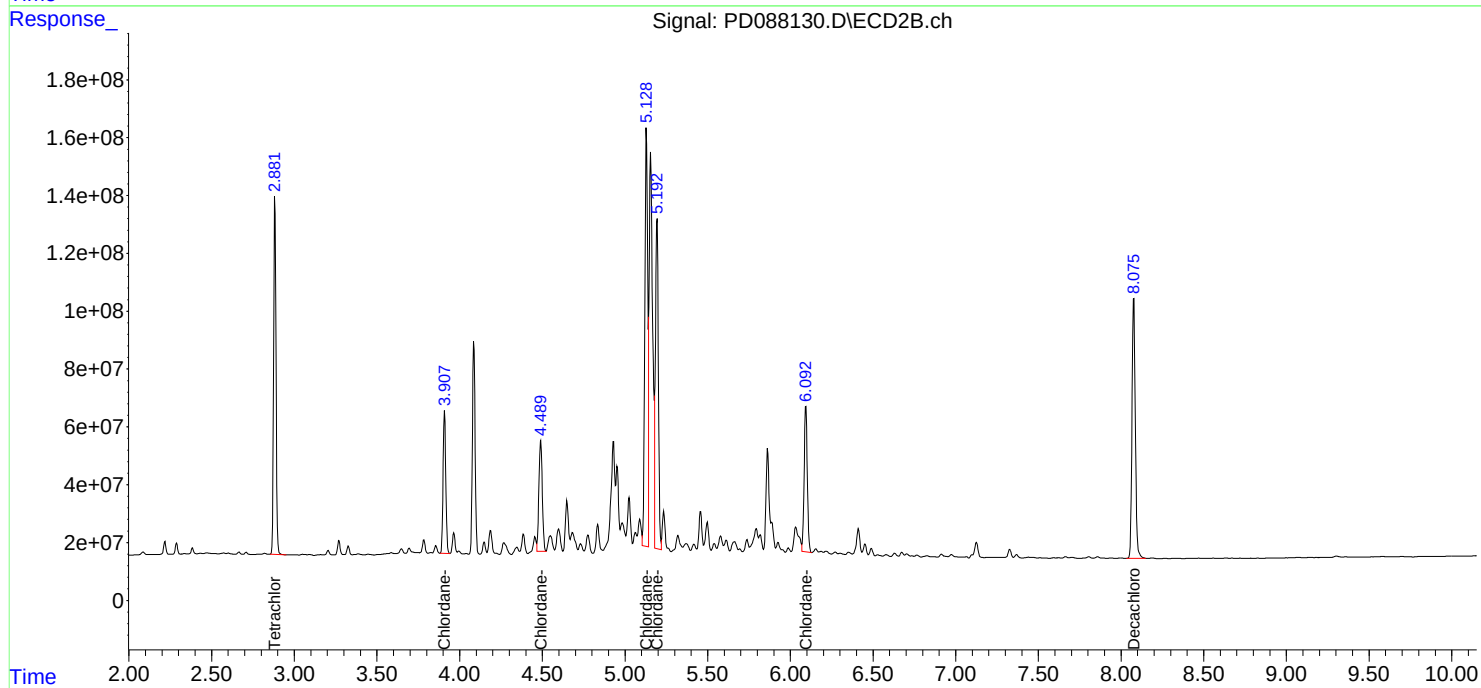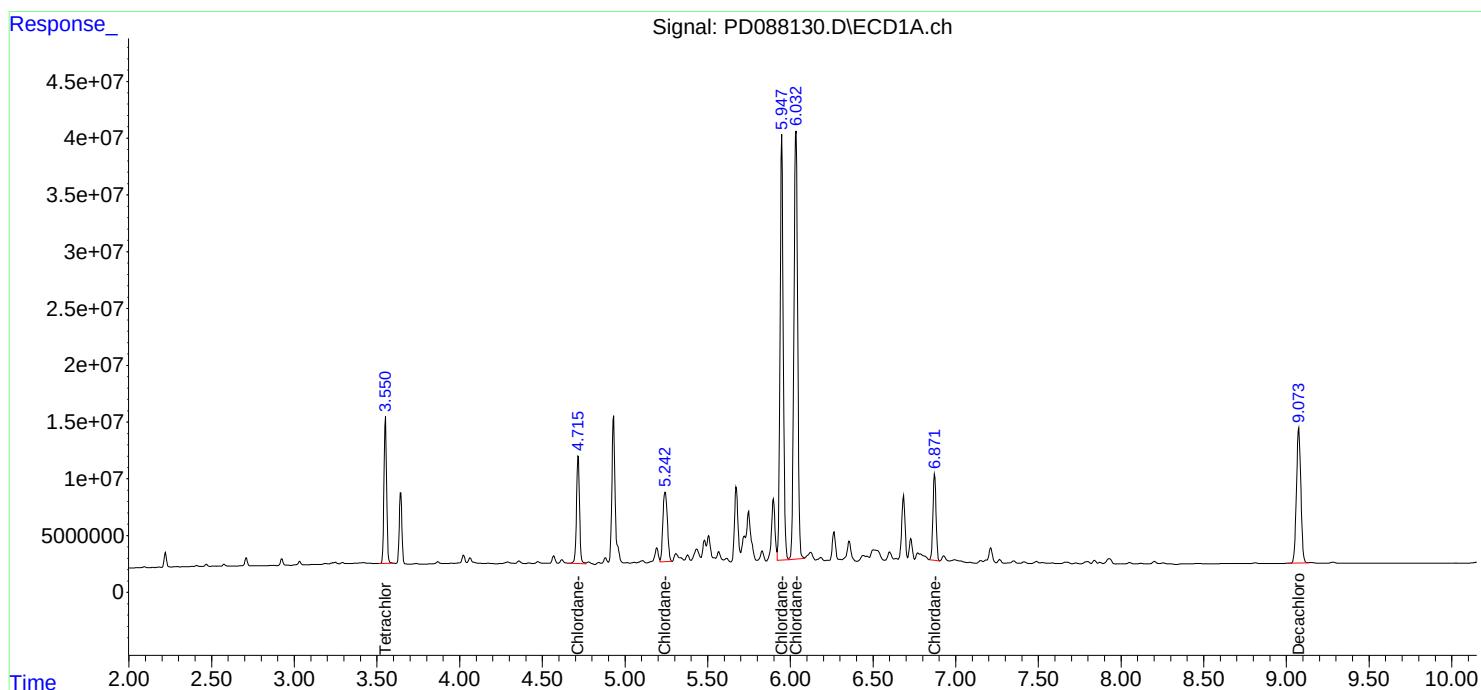


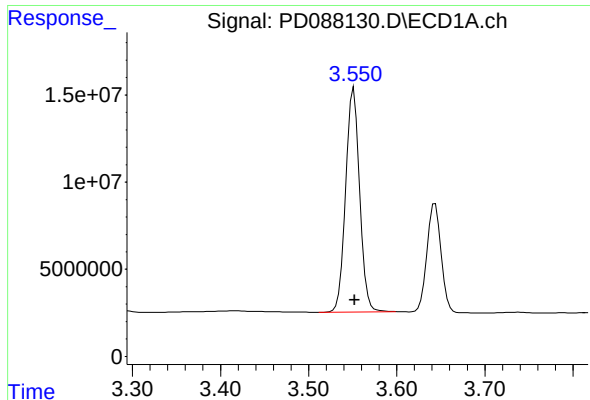

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 141690173
Conc: 73.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

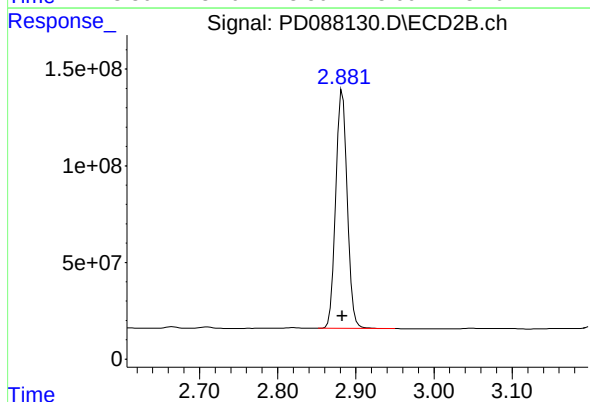


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 1256045108
Conc: 72.54 ng/ml

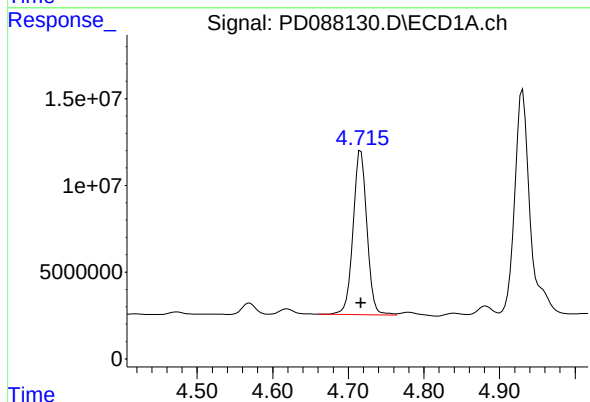


#23 Chlordane-1

R.T.: 4.717 min
Delta R.T.: 0.000 min
Response: 121270832
Conc: 748.61 ng/ml

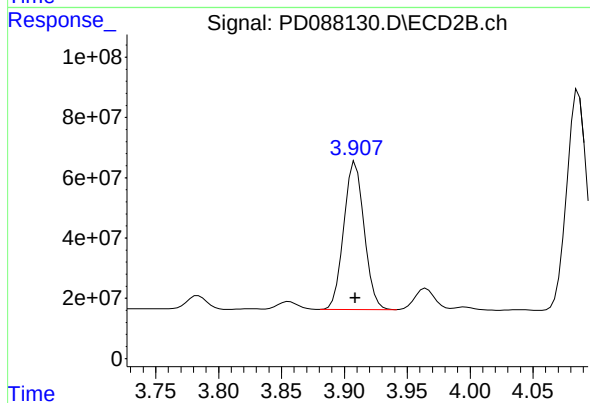

#23 Chlordane-1


R.T.: 3.909 min
Delta R.T.: 0.000 min
Response: 550742598
Conc: 717.55 ng/ml

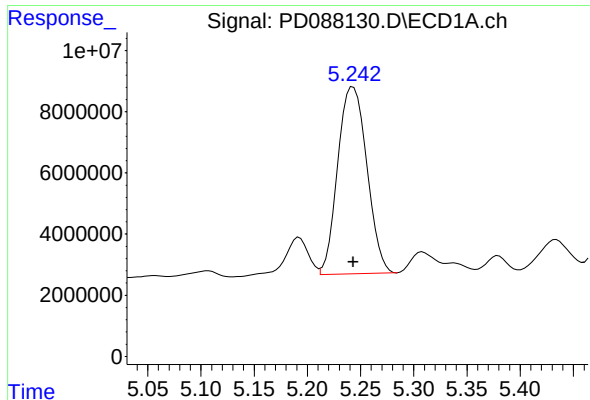

#24 Chlordane-2


R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 116481245
Conc: 724.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

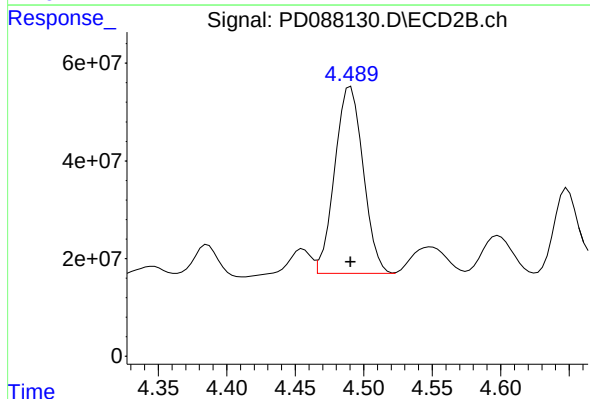


#24 Chlordane-2

R.T.: 4.490 min
Delta R.T.: 0.000 min
Response: 552818390
Conc: 705.95 ng/ml

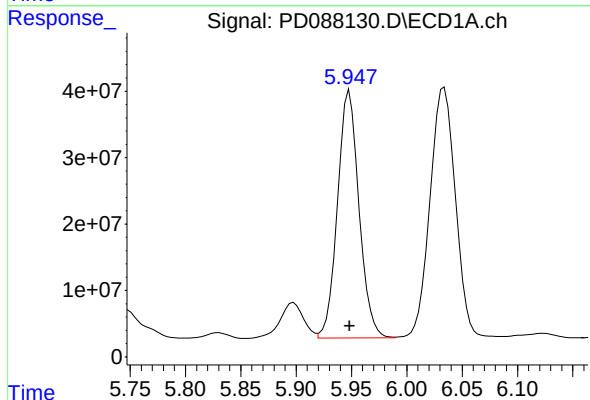


#25 Chlordane-3

R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 504211347
Conc: 756.86 ng/ml

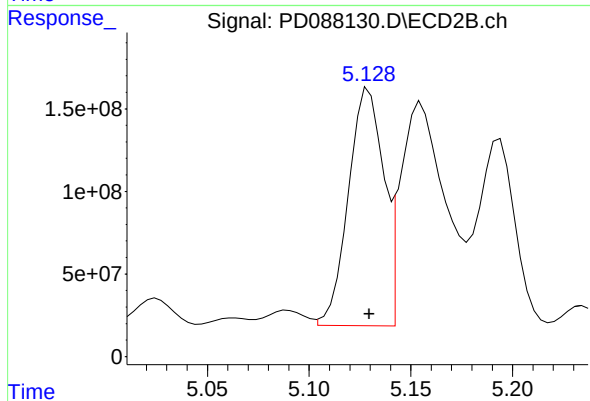

#25 Chlordane-3


R.T.: 5.129 min
Delta R.T.: 0.000 min
Response: 1726815007
Conc: 720.46 ng/ml

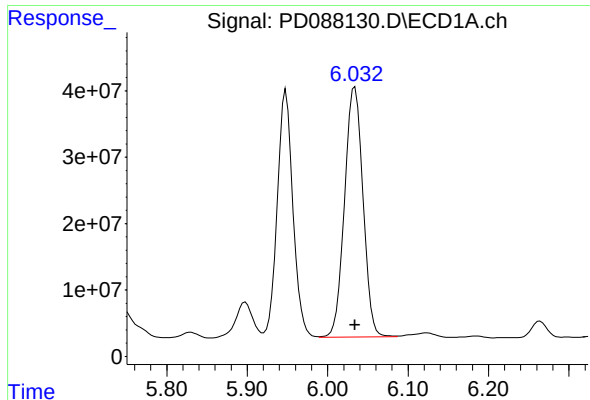

#26 Chlordane-4


R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 599490653
Conc: 752.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

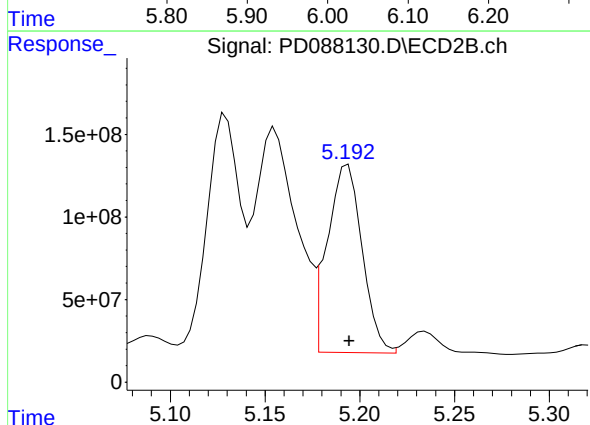


#26 Chlordane-4

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 1453758132
Conc: 715.52 ng/ml

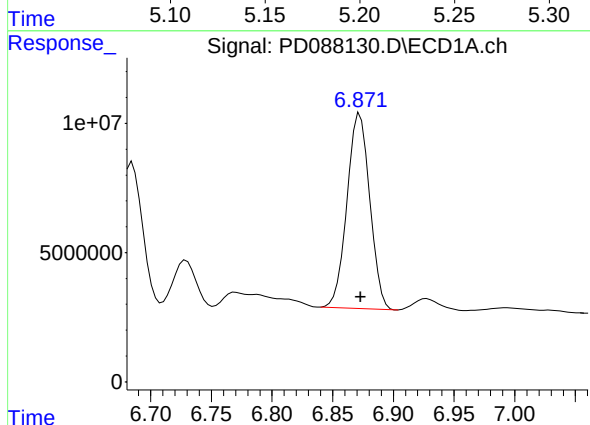


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 98919330
Conc: 743.47 ng/ml

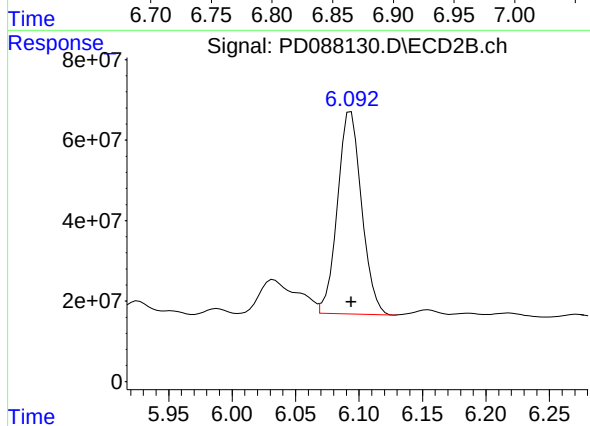

#27 Chlordane-5


R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 665514943
Conc: 714.42 ng/ml

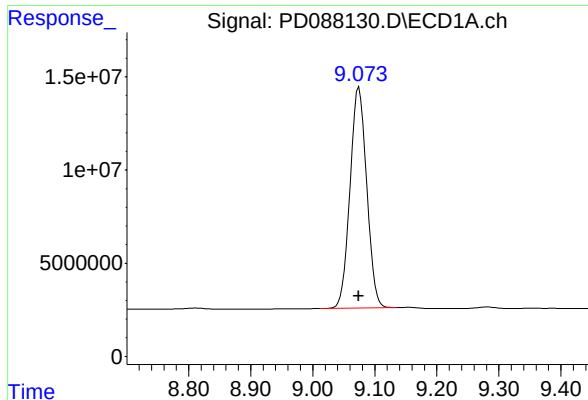

#28 Decachlorobiphenyl

R.T.: 9.075 min
Delta R.T.: 0.000 min
Response: 221094455
Conc: 71.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

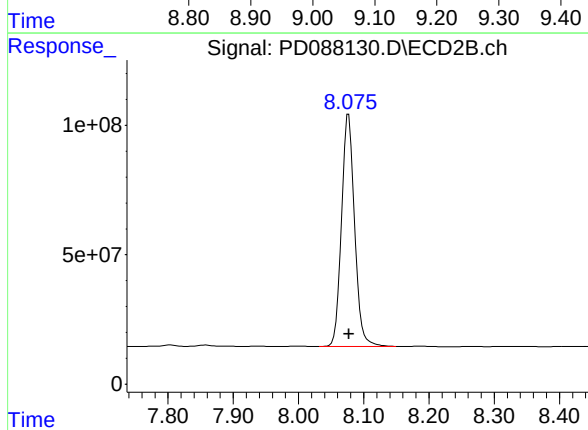

#28 Decachlorobiphenyl

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 1249049226
Conc: 71.11 ng/ml