

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041919\
 Data File : PD052986.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Apr 2019 14:45
 Operator : AJ\SJ
 Sample : PIBLK46
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK47

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:53:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.043	30737342	639.5E6	20.188	20.208
27)	SA Decachlor...	7.814	9.162	56089556	677.7E6	39.781	47.002
Target Compounds							
6)	B beta-BHC	0.000	4.934f	0 18605188	N.D.	0.951	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041919\
Data File : PD052986.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Apr 2019 14:45
Operator : AJ\SJ
Sample : PIBLK46
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK47

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:53:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

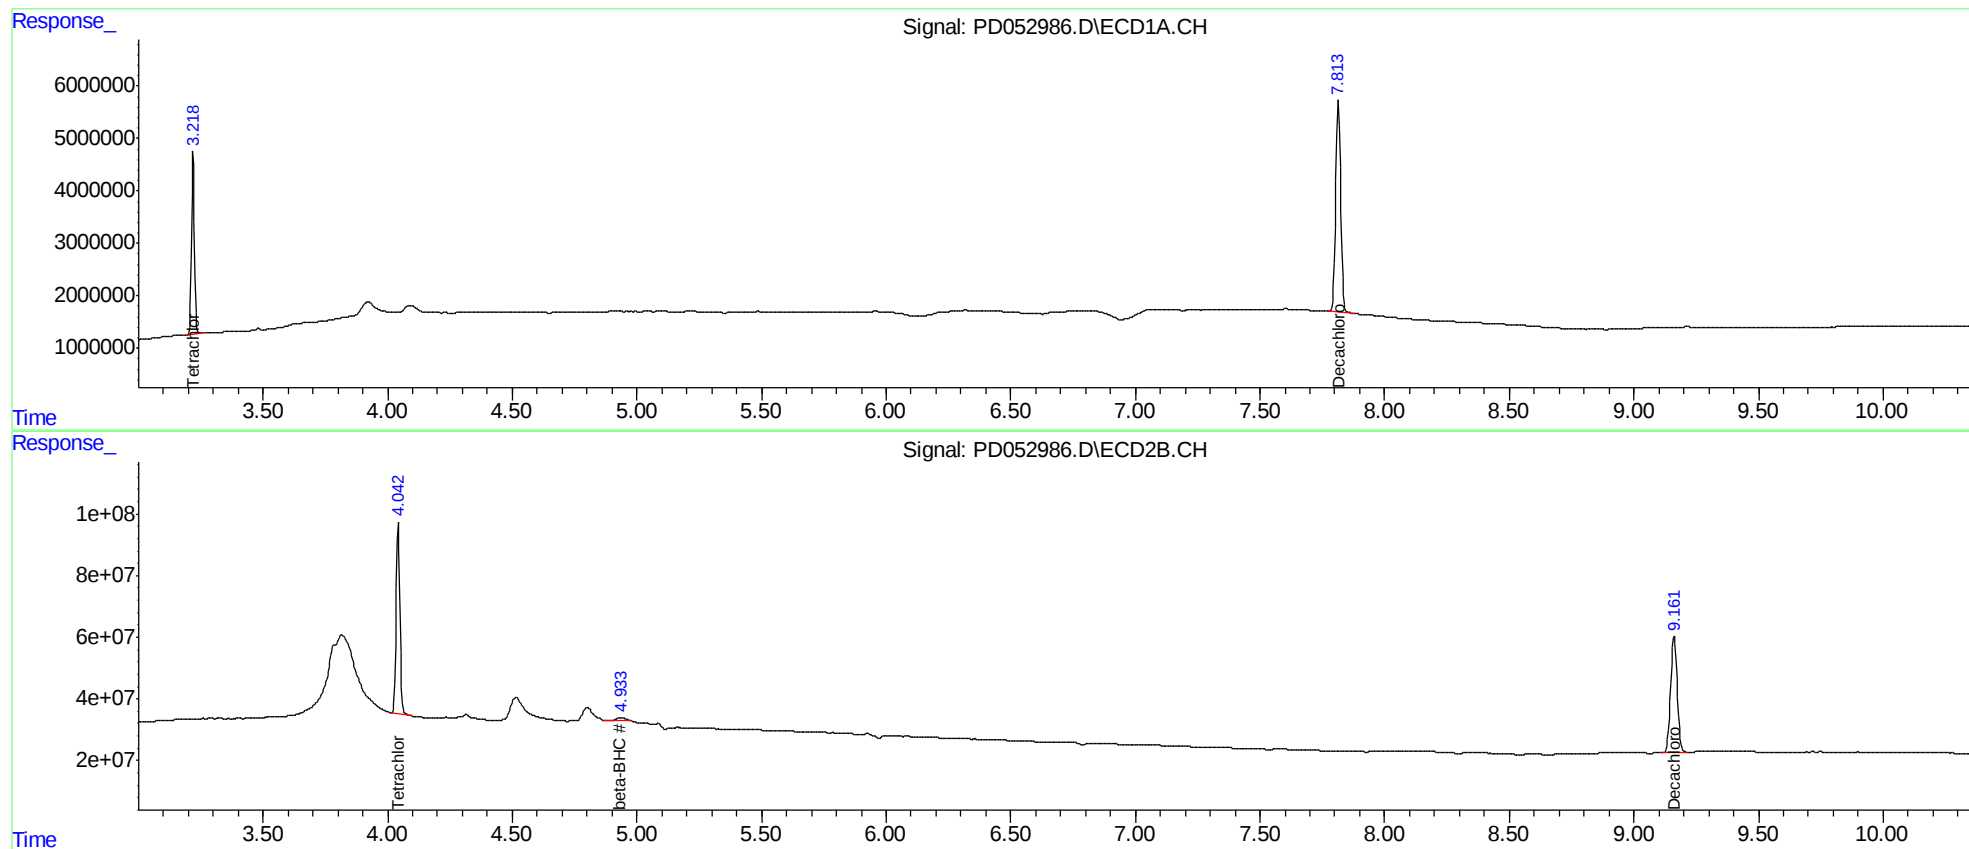


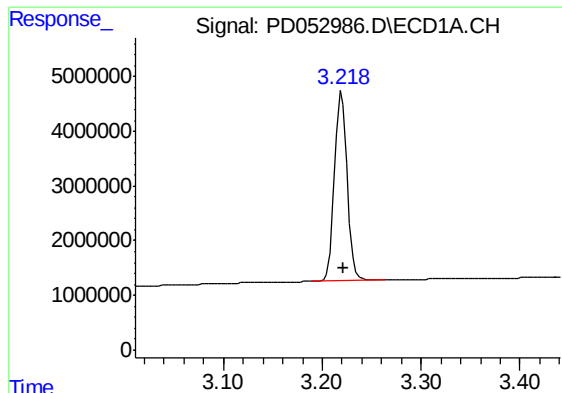

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: -0.001 min
Response: 30737342
Conc: 20.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK47

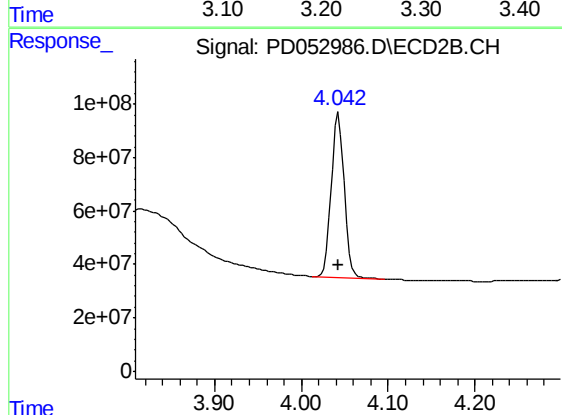


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 639486894
Conc: 20.21 ng/ml

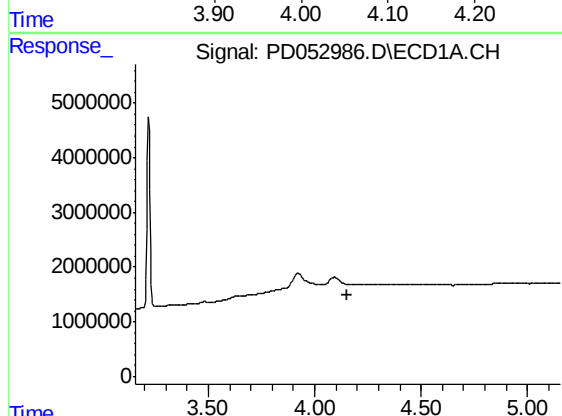


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

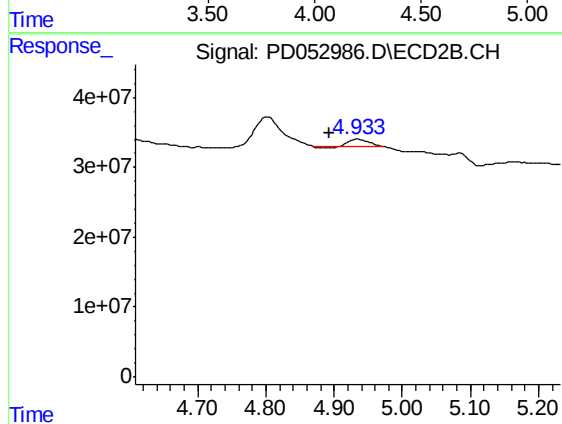

#6 beta-BHC


R.T.: 4.934 min
Delta R.T.: 0.041 min
Response: 18605188
Conc: 0.95 ng/ml

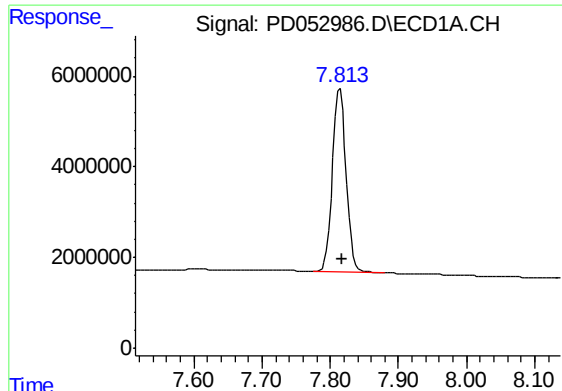

#27 Decachlorobiphenyl

R.T.: 7.814 min
Delta R.T.: -0.003 min
Response: 56089556
Conc: 39.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK47

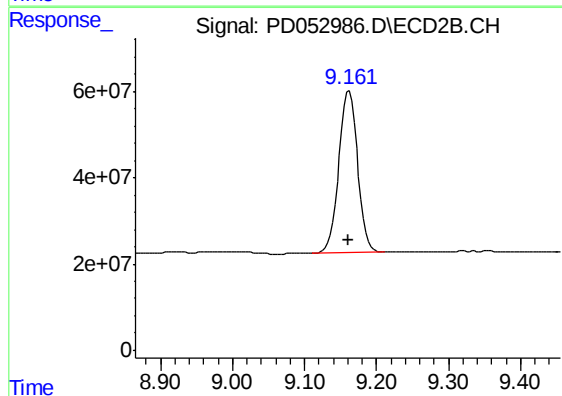

#27 Decachlorobiphenyl

R.T.: 9.162 min
Delta R.T.: 0.000 min
Response: 677706266
Conc: 47.00 ng/ml