

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041922\
 Data File : PD069193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 14:17
 Operator : AR\AJ
 Sample : N2374-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFD9

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/22/2022
 Supervised By : Yogesh Patel 04/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:07:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.445	4.172	16537154	149.6E6	13.053	12.393
2) SA Decachlor...	8.201	9.364	34555108	199.6E6	25.985	28.381m
Target Compounds						
11) B cis-Chlor...	5.440	6.399	4677884	62453007	3.134m	5.014m#
12) B 4,4'-DDE	5.606	6.546	3166143	17636224	2.360m	1.621m#
16) A 4,4'-DDD	6.127	7.037	8269388	114.4E6	6.783m	12.216m#
17) MA 4,4'-DDT	6.364	7.345	6223172	38079025	5.073	4.230

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041922\
Data File : PD069193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 14:17
Operator : AR\AJ
Sample : N2374-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:07:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

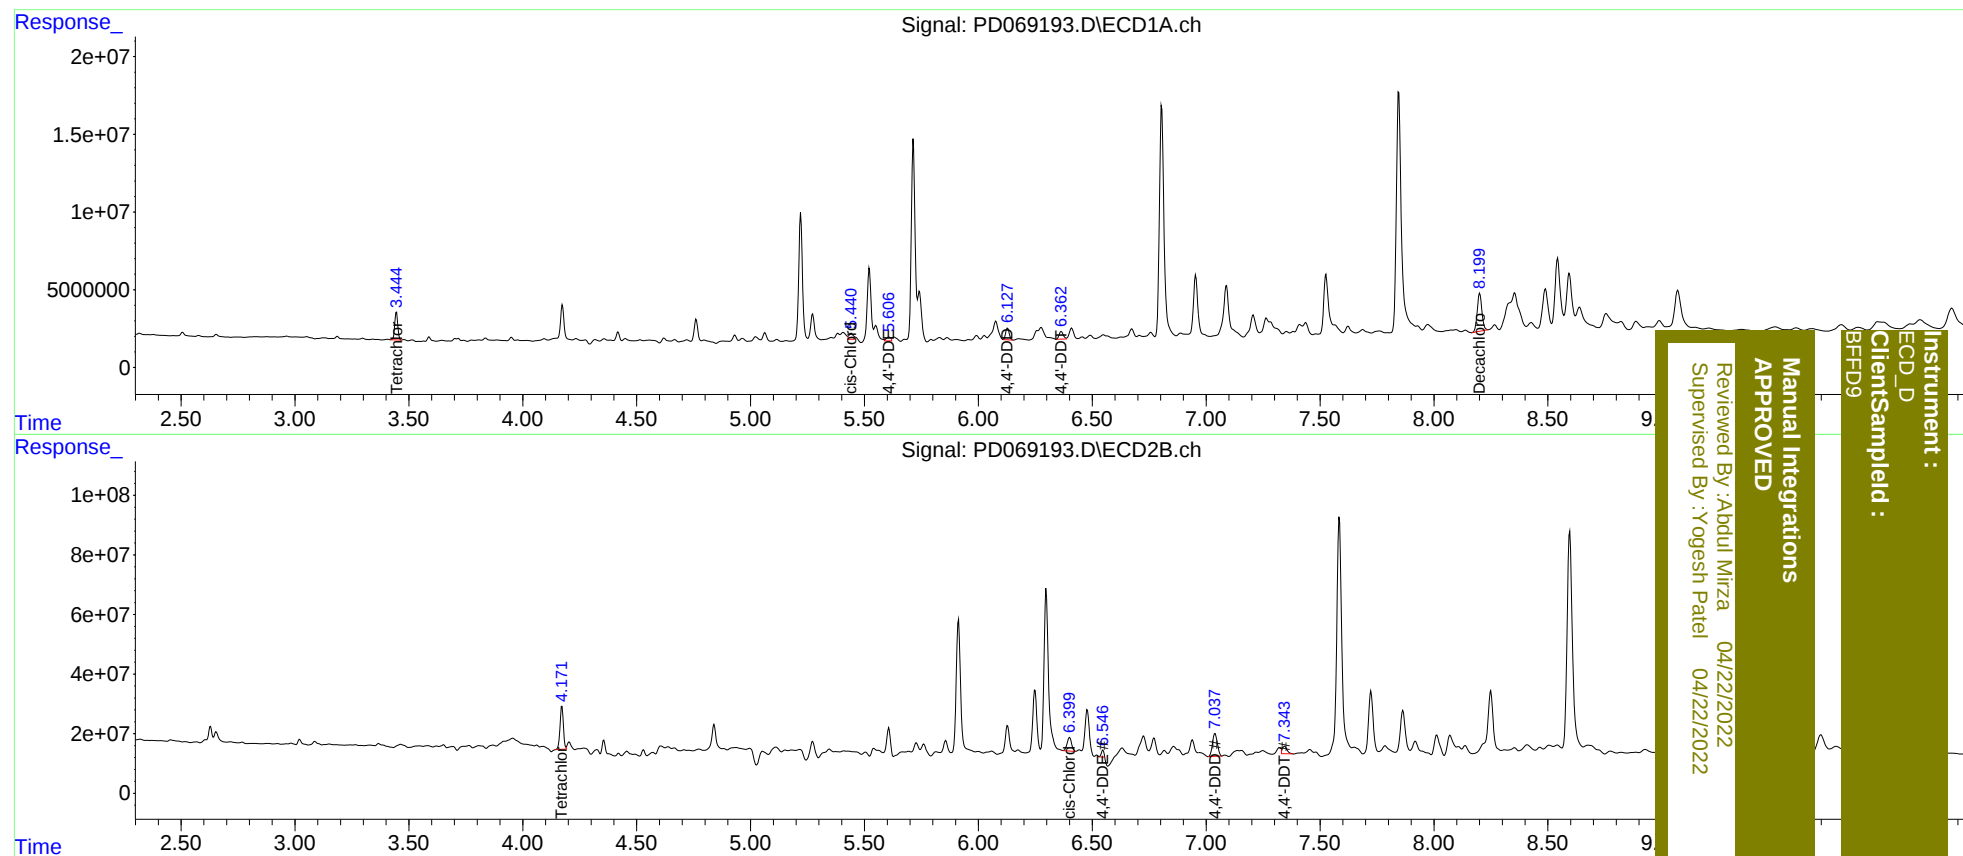

Reviewed By: Abdul Miza 04/22/2022
Supervised By: Yogesh Patel 04/22/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BFFD9