

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041922\
 Data File : PD069195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 14:45
 Operator : AR\AJ
 Sample : N2374-06MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFD9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/22/2022
 Supervised By : Yogesh Patel 04/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:07:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	17206239	173.6E6	13.581	14.384
27)	SA Decachlor...	8.201	9.365	35357674	205.6E6	26.589	29.242m
Target Compounds							
2)	A alpha-BHC	3.884	4.566	75864539	581.0E6	42.442	35.344m
3)	MA gamma-BHC...	4.168	4.857	95592068	623.8E6	52.848	40.037m
4)	MA Heptachlor	4.465	5.386	73034737	556.7E6	43.016	36.776
5)	MB Aldrin	4.712	5.699	75157790	546.2E6	47.180	38.263
6)	B beta-BHC	4.418	5.020	39723569	123.5E6	51.285	18.404 #
7)	B delta-BHC	4.621	5.247	38552834	173.6E6	24.153	14.790m#
8)	B Heptachlo...	5.157	6.087	63268714	407.1E6	42.980	36.538
9)	A Endosulfan I	5.497	6.450	43859470	431.1E6	30.056	36.299
10)	B trans-Chl...	5.383	6.322	81900041	464.1E6	54.630	36.582m#
11)	B cis-Chlor...	5.442	6.398	75798676	487.7E6	50.781	39.161
12)	B 4,4'-DDE	5.607	6.548	123.7E6	767.1E6	92.211	70.508
13)	MA Dieldrin	5.739	6.708	168.2E6	923.8E6	108.063	76.589 #
14)	MA Endrin	5.997	6.929	118.2E6	714.6E6	84.474	73.479
15)	B Endosulfa...	6.271	7.134	115.2E6	739.1E6	89.387	77.117
16)	A 4,4'-DDD	6.124	7.040	96145373	745.5E6	78.859	79.612
17)	MA 4,4'-DDT	6.365	7.343	102.5E6	751.5E6	83.558	83.478
18)	B Endrin al...	6.441	7.258	72828044	573.6E6	73.369	80.284
19)	B Endosulfa...	6.653	7.483	107.7E6	577.3E6	85.989	65.790
20)	A Methoxychlor	6.915	7.796	270.9E6	1593.6E6	399.167	386.700
21)	B Endrin ke...	7.147	7.958	113.0E6	668.5E6	78.208	72.411

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041922\
Data File : PD069195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 14:45
Operator : AR\AJ
Sample : N2374-06MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:07:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

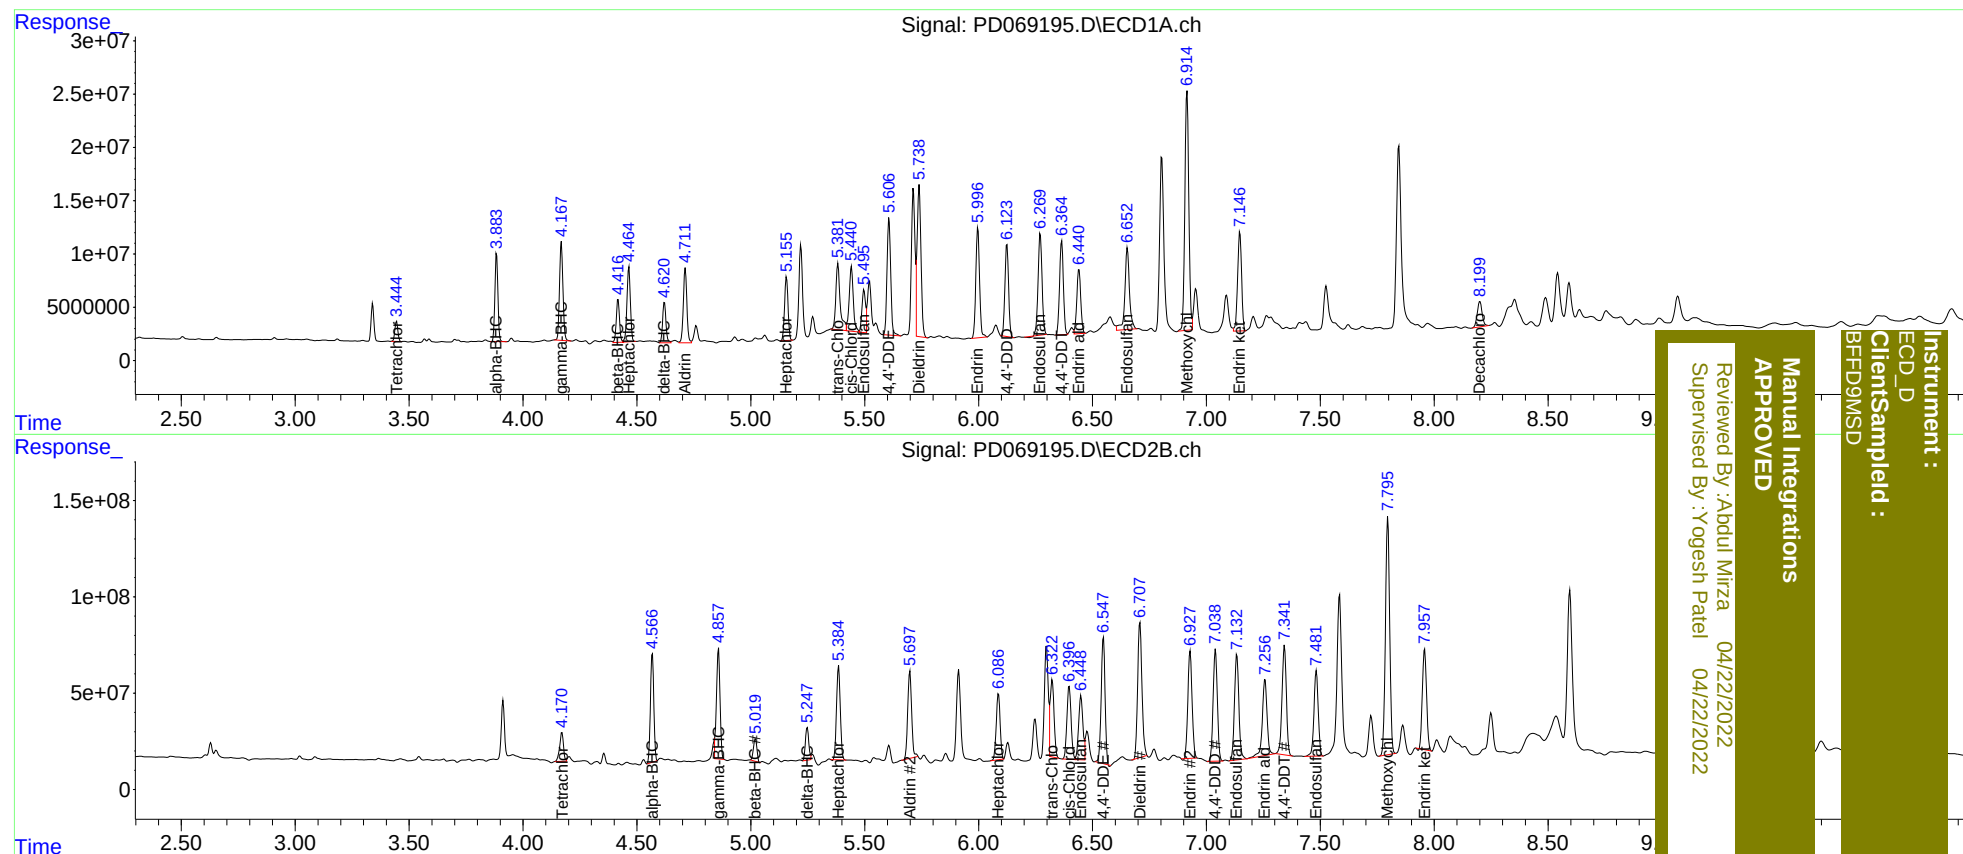

Instrument :
ECD_D
ClientSampled :
BFFD9MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/22/2022
Supervised By :Yogesh Patel 04/22/2022