

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041922\
 Data File : PD069199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 15:41
 Operator : AR\AJ
 Sample : N2374-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFF4

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/22/2022
 Supervised By : Yogesh Patel 04/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:08:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.445	4.172	13552109	127.4E6	10.696	10.557
2) SA Decachlor...	8.202	9.367	20728100	92783152	15.588	13.194m
Target Compounds						
12) B 4,4'-DDE	5.606	6.546	1628106	7494216	1.214m	0.689m#
16) A 4,4'-DDD	6.123	7.039	2426826	28617290	1.990m	3.056 #
17) MA 4,4'-DDT	6.362	7.343	1368004	4376778	1.115m	0.486m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041922\
Data File : PD069199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 15:41
Operator : AR\AJ
Sample : N2374-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:08:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

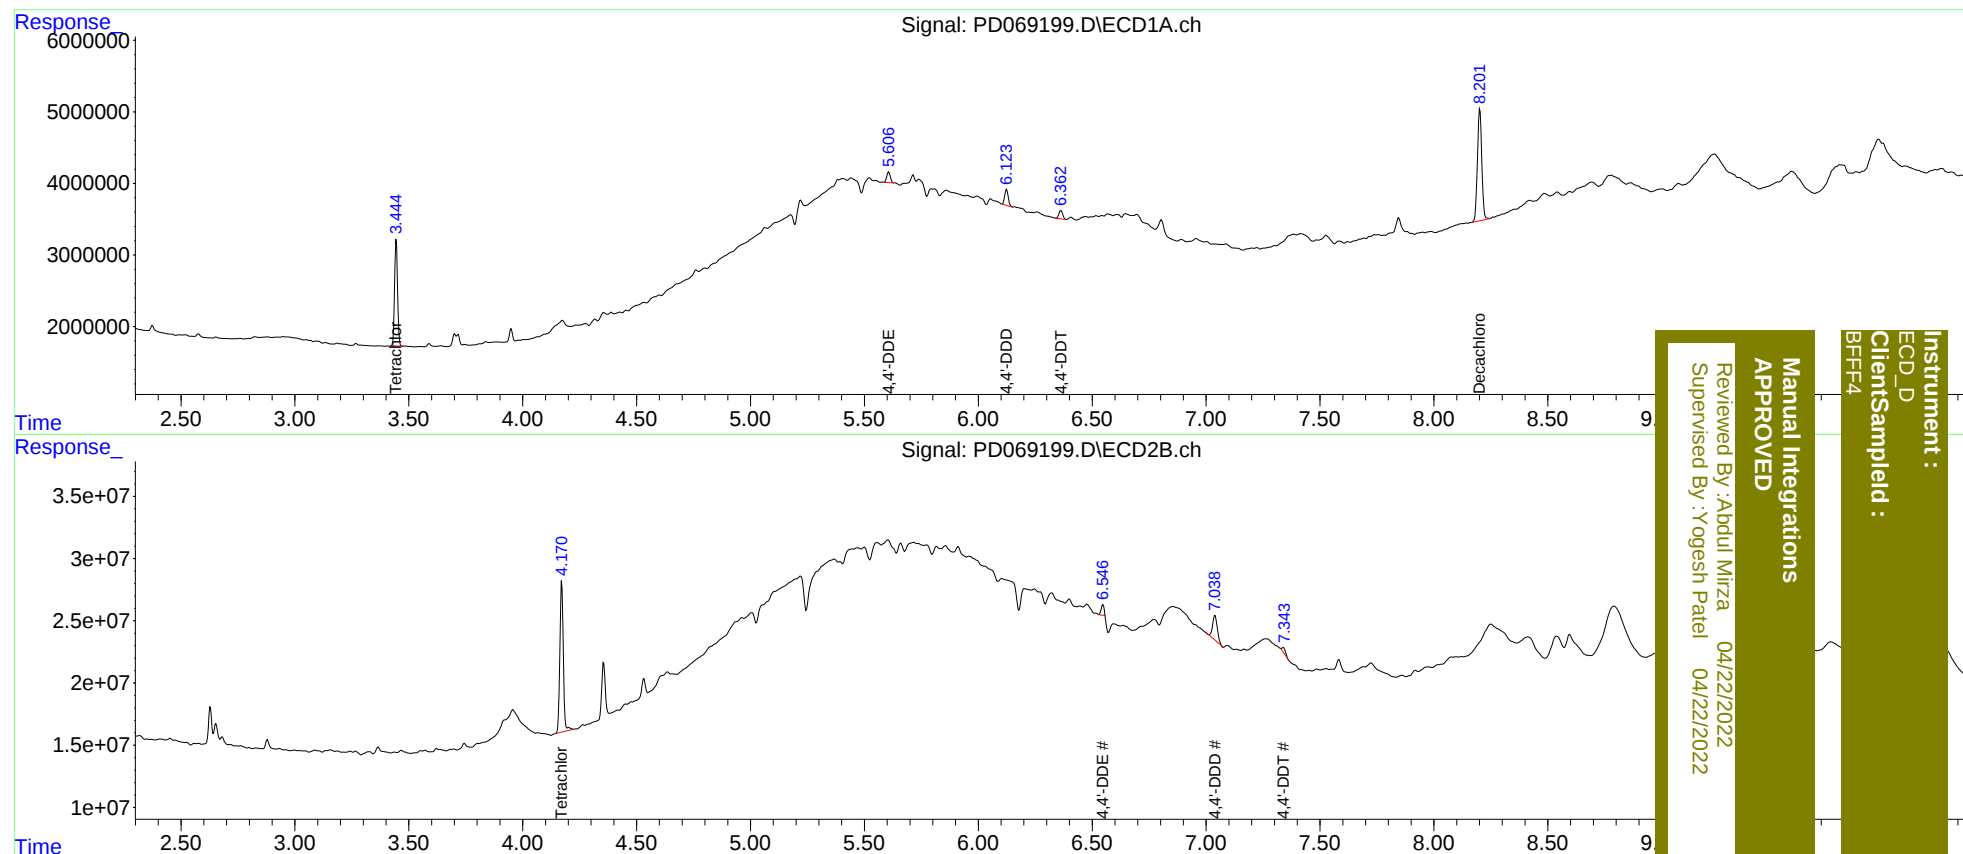

Manual Integrations
APPROVED
Reviewed By : Abdul Miza 04/22/2022
Supervised By : Yogesh Patel 04/22/2022

Instrument :
ECD_D
ClientSampled :
BFFF4