

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041922\
 Data File : PD069194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 14:31
 Operator : AR\AJ
 Sample : N2374-05MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFD9MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/22/2022
 Supervised By : Yogesh Patel 04/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:07:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	17877694	182.6E6	14.111	15.132
27)	SA Decachlor...	8.200	9.363	36491811	209.4E6	27.442	29.775m
Target Compounds							
2)	A alpha-BHC	3.884	4.566	78358702	608.6E6	43.838	37.023m
3)	MA gamma-BHC...	4.169	4.857	98581676	664.1E6	54.501	42.625m
4)	MA Heptachlor	4.465	5.386	75493851	590.9E6	44.465	39.034
5)	MB Aldrin	4.713	5.698	77353880	585.2E6	48.559	40.996
6)	B beta-BHC	4.418	5.020	41014513	134.9E6	52.951	20.117 #
7)	B delta-BHC	4.622	5.247	40217102	184.8E6	25.195	15.739m#
8)	B Heptachlo...	5.157	6.087	65535195	427.2E6	44.520	38.348
9)	A Endosulfan I	5.496	6.449	46221861	460.6E6	31.675	38.777
10)	B trans-Chl...	5.383	6.321	81144861	380.6E6	54.126	30.001m#
11)	B cis-Chlor...	5.442	6.398	78054958	519.0E6	52.293	41.674
12)	B 4,4'-DDE	5.607	6.548	128.9E6	812.2E6	96.118	74.652
13)	MA Dieldrin	5.739	6.708	174.0E6	991.3E6	111.785	82.185 #
14)	MA Endrin	5.997	6.928	123.0E6	763.4E6	87.880	78.491
15)	B Endosulfa...	6.271	7.133	120.9E6	784.7E6	93.841	81.870
16)	A 4,4'-DDD	6.125	7.039	98876279	795.3E6	81.099	84.933
17)	MA 4,4'-DDT	6.365	7.342	108.4E6	815.2E6	88.368	90.560
18)	B Endrin al...	6.441	7.257	76922978	584.7E6	77.495	81.832
19)	B Endosulfa...	6.653	7.482	107.9E6	625.1E6	86.100	71.240
20)	A Methoxychlor	6.916	7.796	280.1E6	1687.1E6	412.728	409.389
21)	B Endrin ke...	7.147	7.956	118.8E6	728.6E6	82.250	78.921m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041922\
Data File : PD069194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 14:31
Operator : AR\AJ
Sample : N2374-05MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:07:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

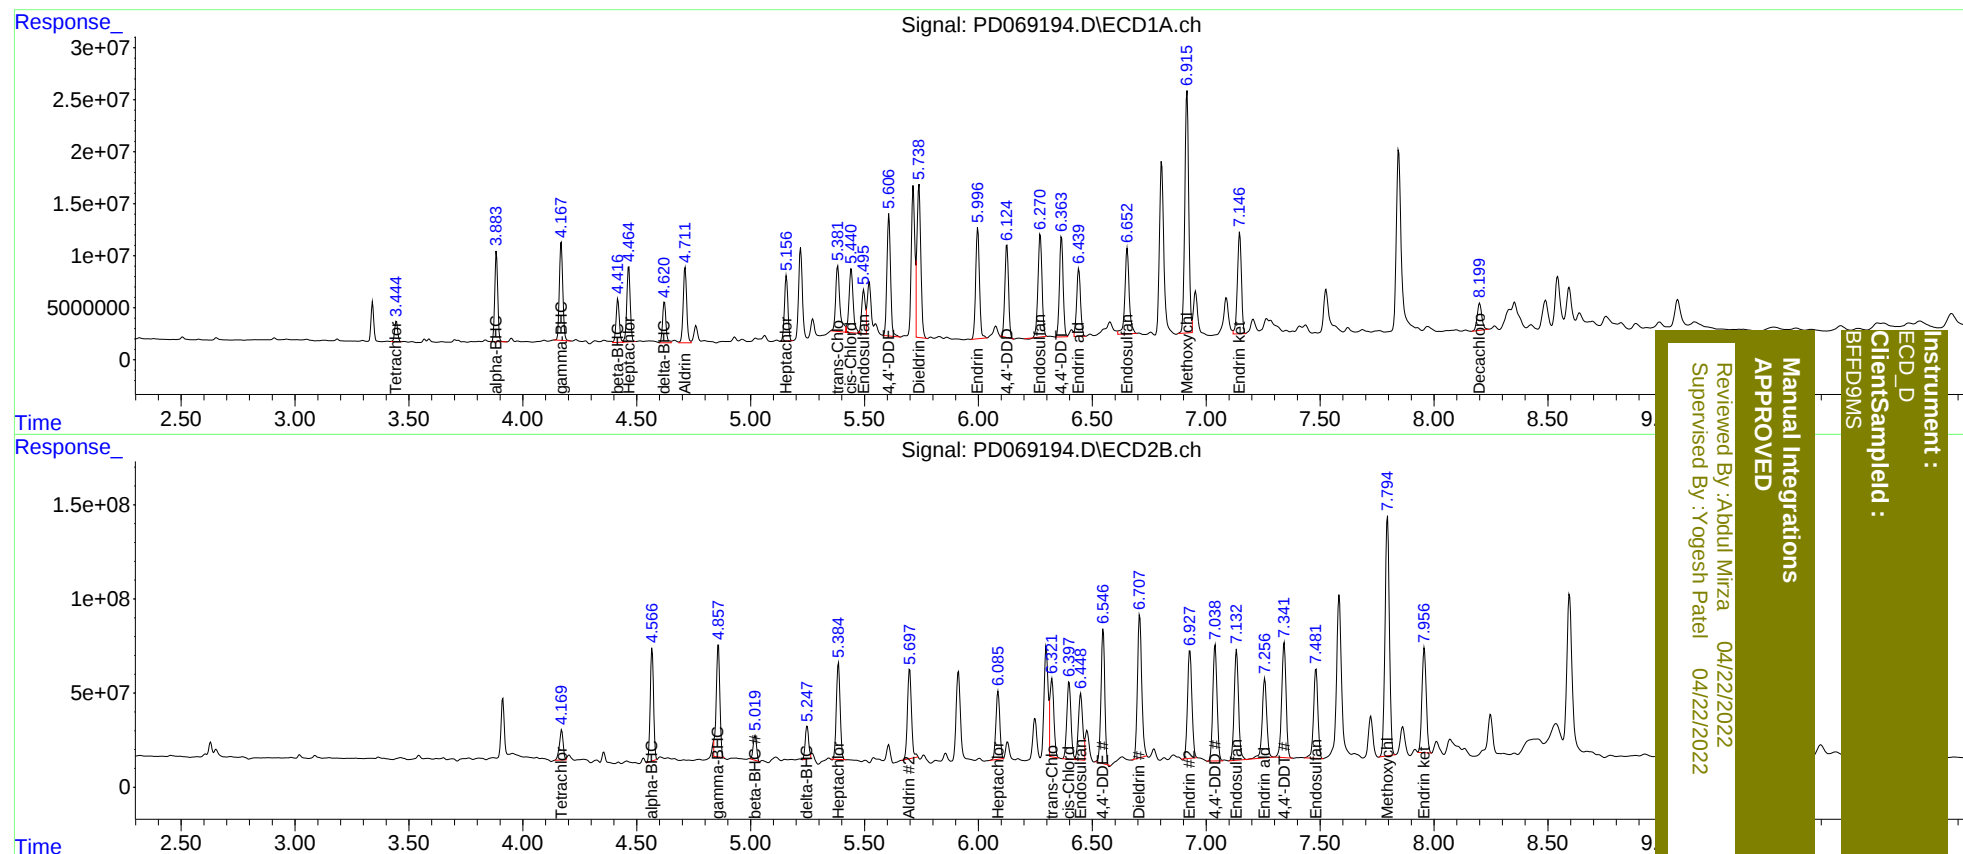

Instrument :
ECD_D
ClientSampled :
BFFD9MS

Manual Integrations
APPROVED

Reviewed By :Abdul Miza 04/22/2022
Supervised By :Yogesh Patel 04/22/2022