

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042021\
 Data File : PD062212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 11:45
 Operator : AR\AJ
 Sample : M2031-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG538

Manual Integrations
 APPROVED

Ankita
 4/26/2021 4:00:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 23:45:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 05:02:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.484	3.979	19476092	245.2E6	19.897	24.568m
2) SA Decachlor...	8.256	9.040	48612205	354.9E6	36.253	38.550
Target Compounds						
2) A alpha-BHC	3.910	4.374	5093315	65290995	3.582m	3.951m
4) MA Heptachlor	4.499	5.146	737793	61963682	0.521	4.212m#
7) B delta-BHC	4.650	5.034	5145617	25106762	3.746m	1.639m#
8) B Heptachlo...	5.191	5.866	1078731	91989584	0.819m	6.853m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042021\
Data File : PD062212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 11:45
Operator : AR\AJ
Sample : M2031-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 23:45:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 05:02:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

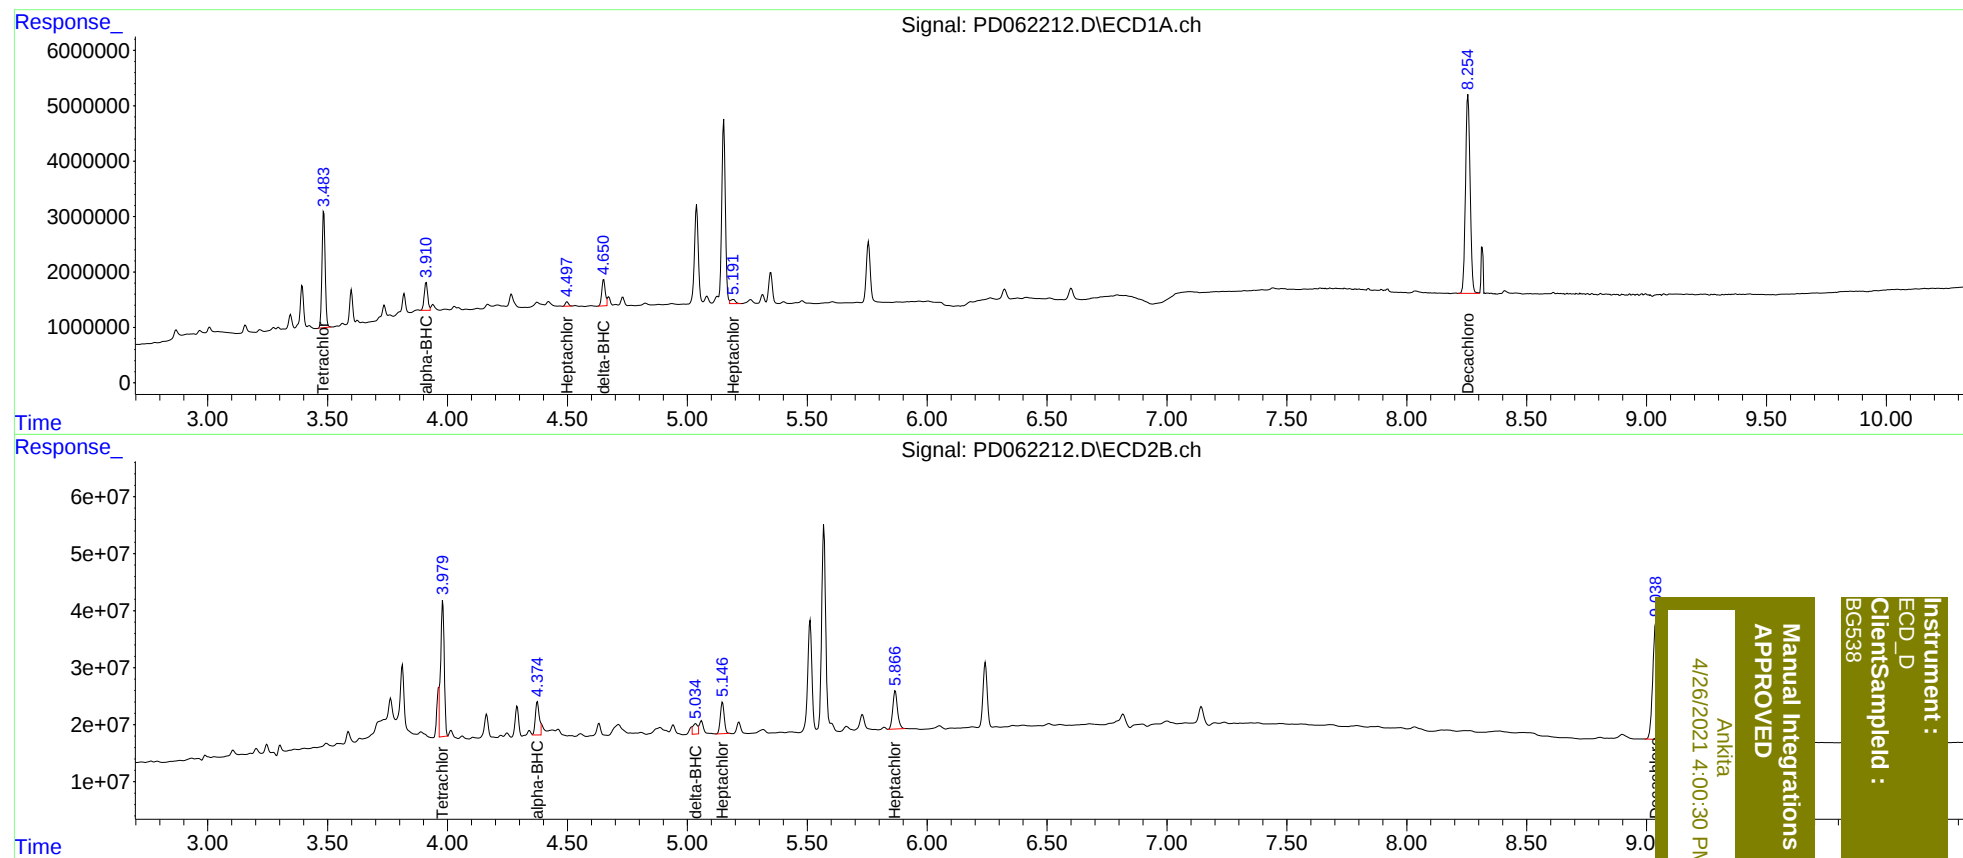

Instrument :
ECD_D
ClientSample :
BG538

Manual Integrations
APPROVED

Ankita
4/26/2021 4:00:30 PM