

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042021\
 Data File : PD062223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 14:19
 Operator : AR\AJ
 Sample : INDA328
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3028

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 02:17:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 05:02:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	18871356	226.7E6	19.279	22.716
27)	SA Decachlor...	8.255	9.040	56131791	417.8E6	41.861	45.387
Target Compounds							
2)	A alpha-BHC	3.924	4.369	27648492	363.7E6	19.444	22.011
3)	MA gamma-BHC...	4.209	4.654	26564879	336.9E6	19.078	22.652
4)	MA Heptachlor	4.512	5.162	28639537	336.0E6	20.217	22.837
9)	A Endosulfan I	5.546	6.209	26357807	280.5E6	20.829	22.730
13)	MA Dieldrin	5.790	6.466	58439525	604.4E6	41.722	45.775
14)	MA Endrin	6.049	6.684	49028923	495.0E6	42.022	46.781
16)	A 4,4'-DDD	6.172	6.805	48326327	500.6E6	44.270	47.720
17)	MA 4,4'-DDT	6.414	7.104	39883612	409.2E6	37.423	41.186
20)	A Methoxychlor	6.960	7.562	117.4E6	1006.7E6	195.959	217.448

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042021\
Data File : PD062223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 14:19
Operator : AR\AJ
Sample : INDA328
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 02:17:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 05:02:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

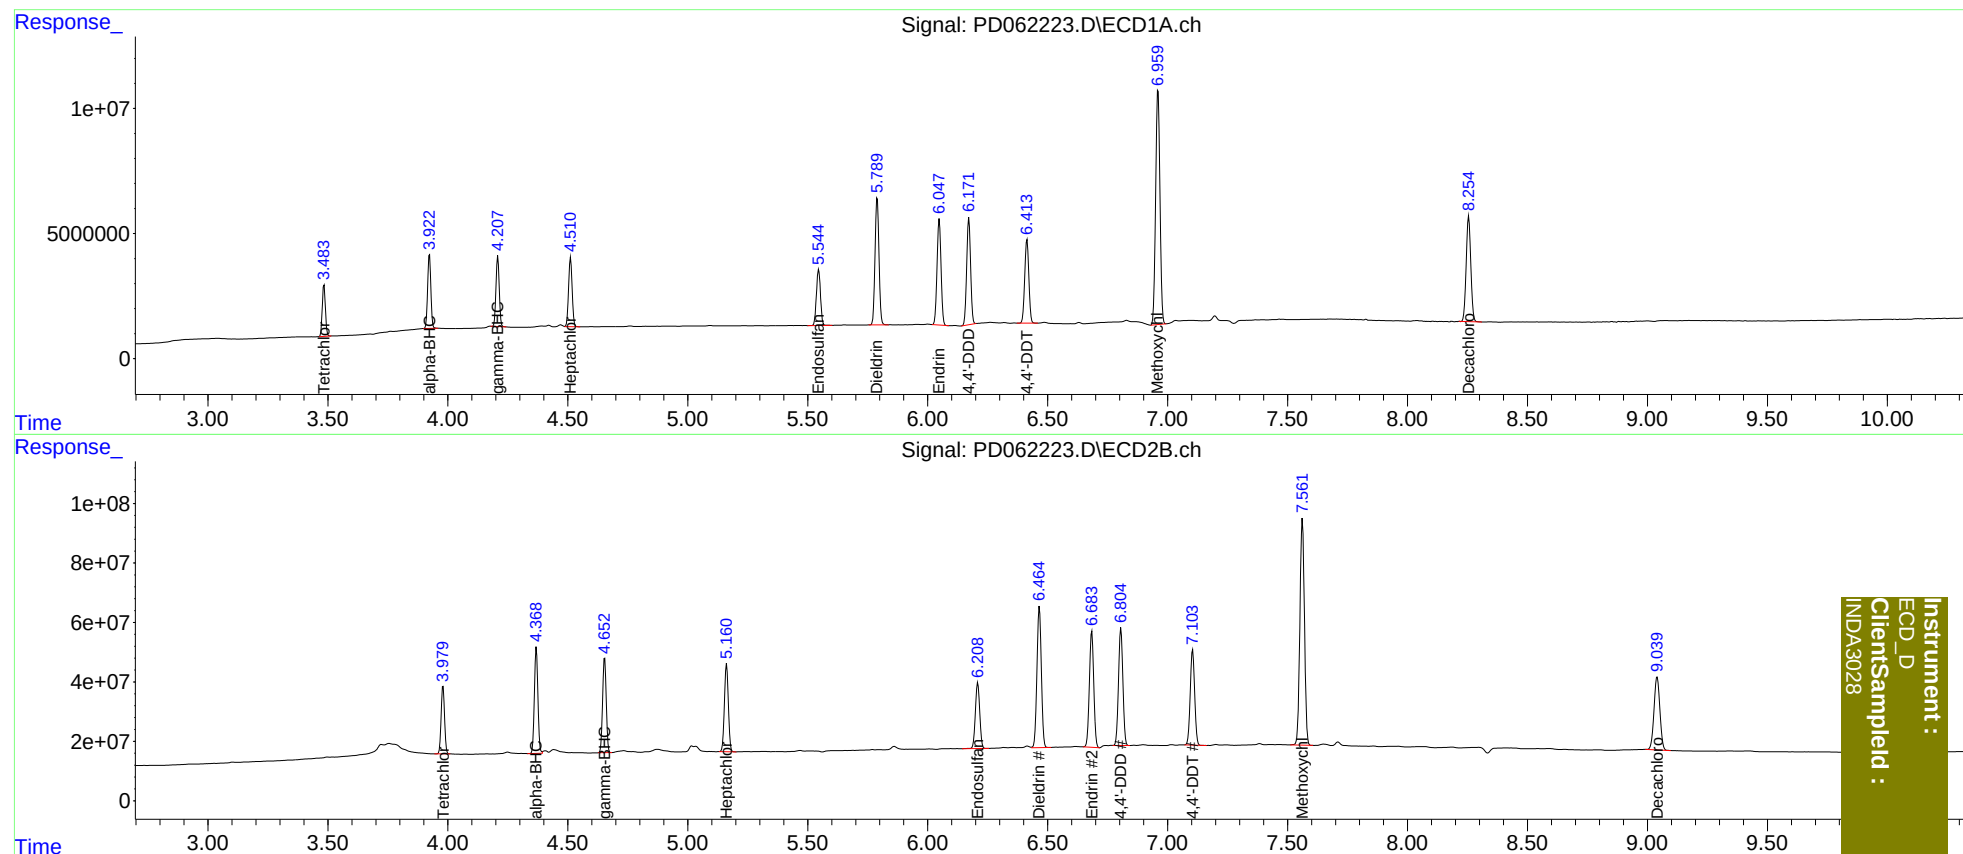

Instrument :
ECD_D
ClientSampled :
INDA3028