

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042022\
 Data File : PD069215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 18:38
 Operator : AR\AJ
 Sample : N2373-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFE7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/22/2022
 Supervised By : mohammad ahmed 04/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 02:43:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.443	4.169	13334716	104.9E6	10.525m	8.693m
2) SA Decachlor...	8.197	9.360	20907948	76881165	15.723	10.933m#
Target Compounds						
12) B 4,4'-DDE	5.603	6.544	5334834	65158031	3.977m	5.989m#
16) A 4,4'-DDD	6.124	7.033	5367447	56107680	4.402m	5.934m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042022\
Data File : PD069215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 18:38
Operator : AR\AJ
Sample : N2373-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 02:43:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

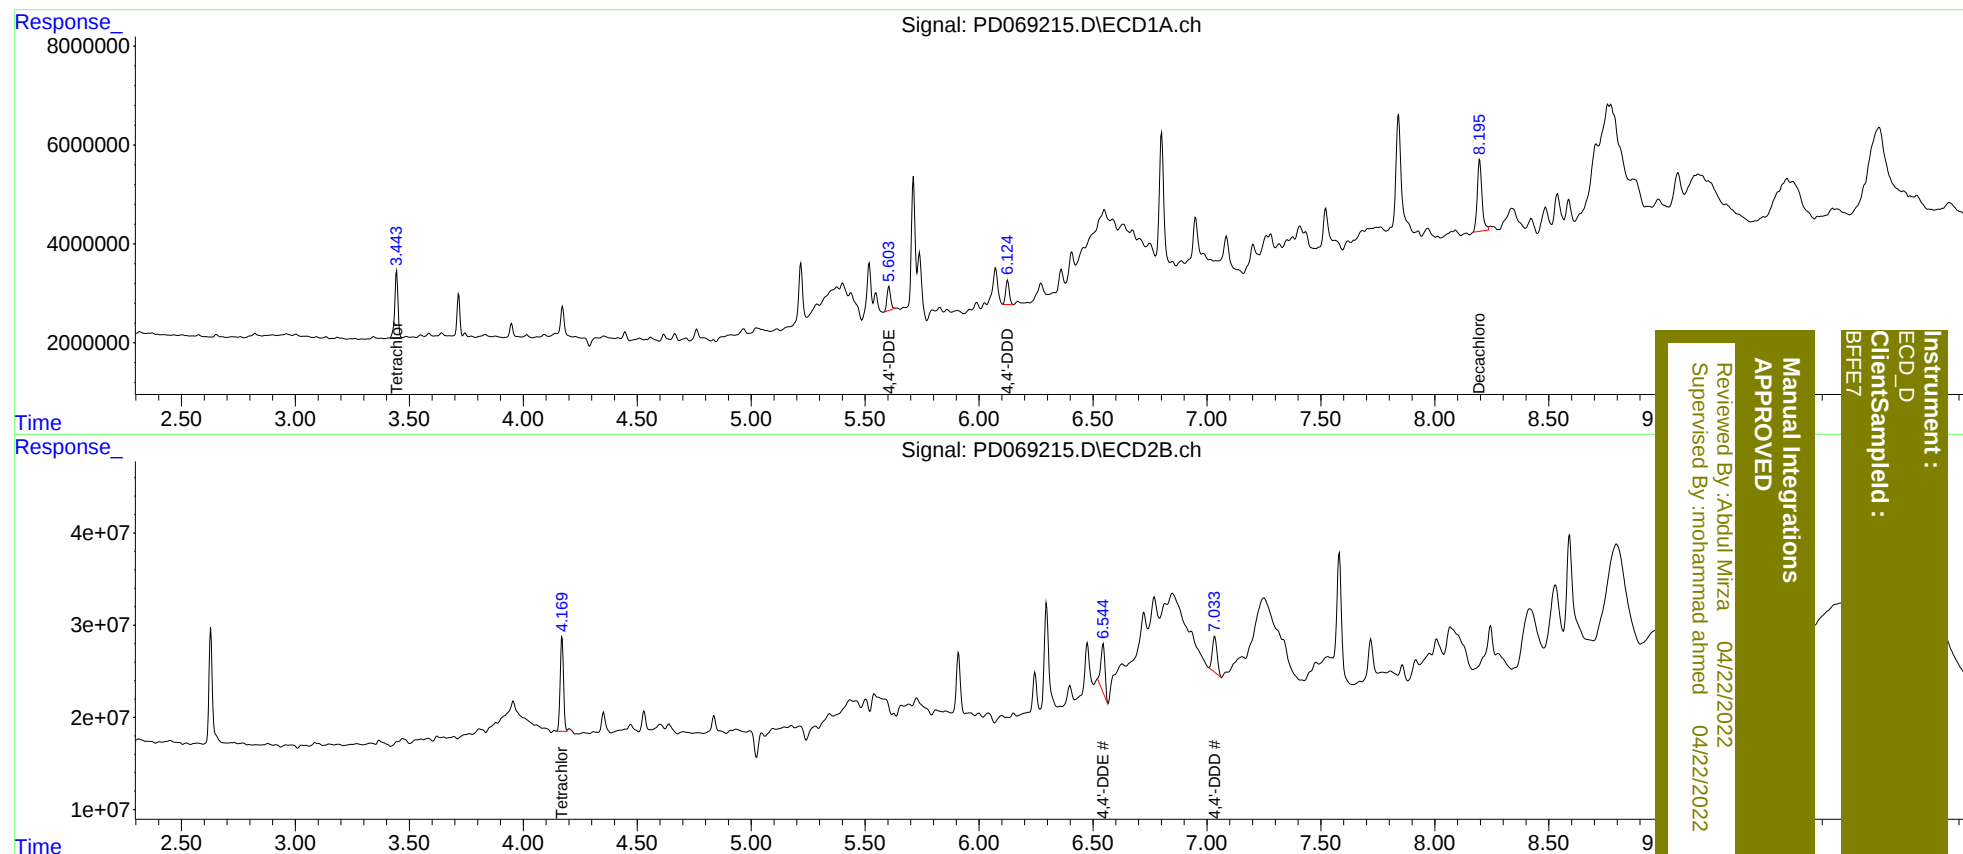

Reviewed By: Abdul Miza 04/22/2022
Supervised By: mohammad ahmed 04/22/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BFE7