

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042022\
 Data File : PD069216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 18:52
 Operator : AR\AJ
 Sample : N2373-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFF0

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/22/2022
 Supervised By :mohammad ahmed 04/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 02:43:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.443	4.170	17012137	138.5E6	13.427m	11.475
2) SA Decachlor...	8.197	9.359	26661941	116.8E6	20.050	16.606m
Target Compounds						
12) B 4,4'-DDE	5.603	6.543	1747660	31941431	1.303m	2.936m#
16) A 4,4'-DDD	6.125	7.033	4160187	36806456	3.412m	3.892m
17) MA 4,4'-DDT	6.362	7.340	3209250	10299036	2.616	1.144m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042022\
Data File : PD069216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 18:52
Operator : AR\AJ
Sample : N2373-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 02:43:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

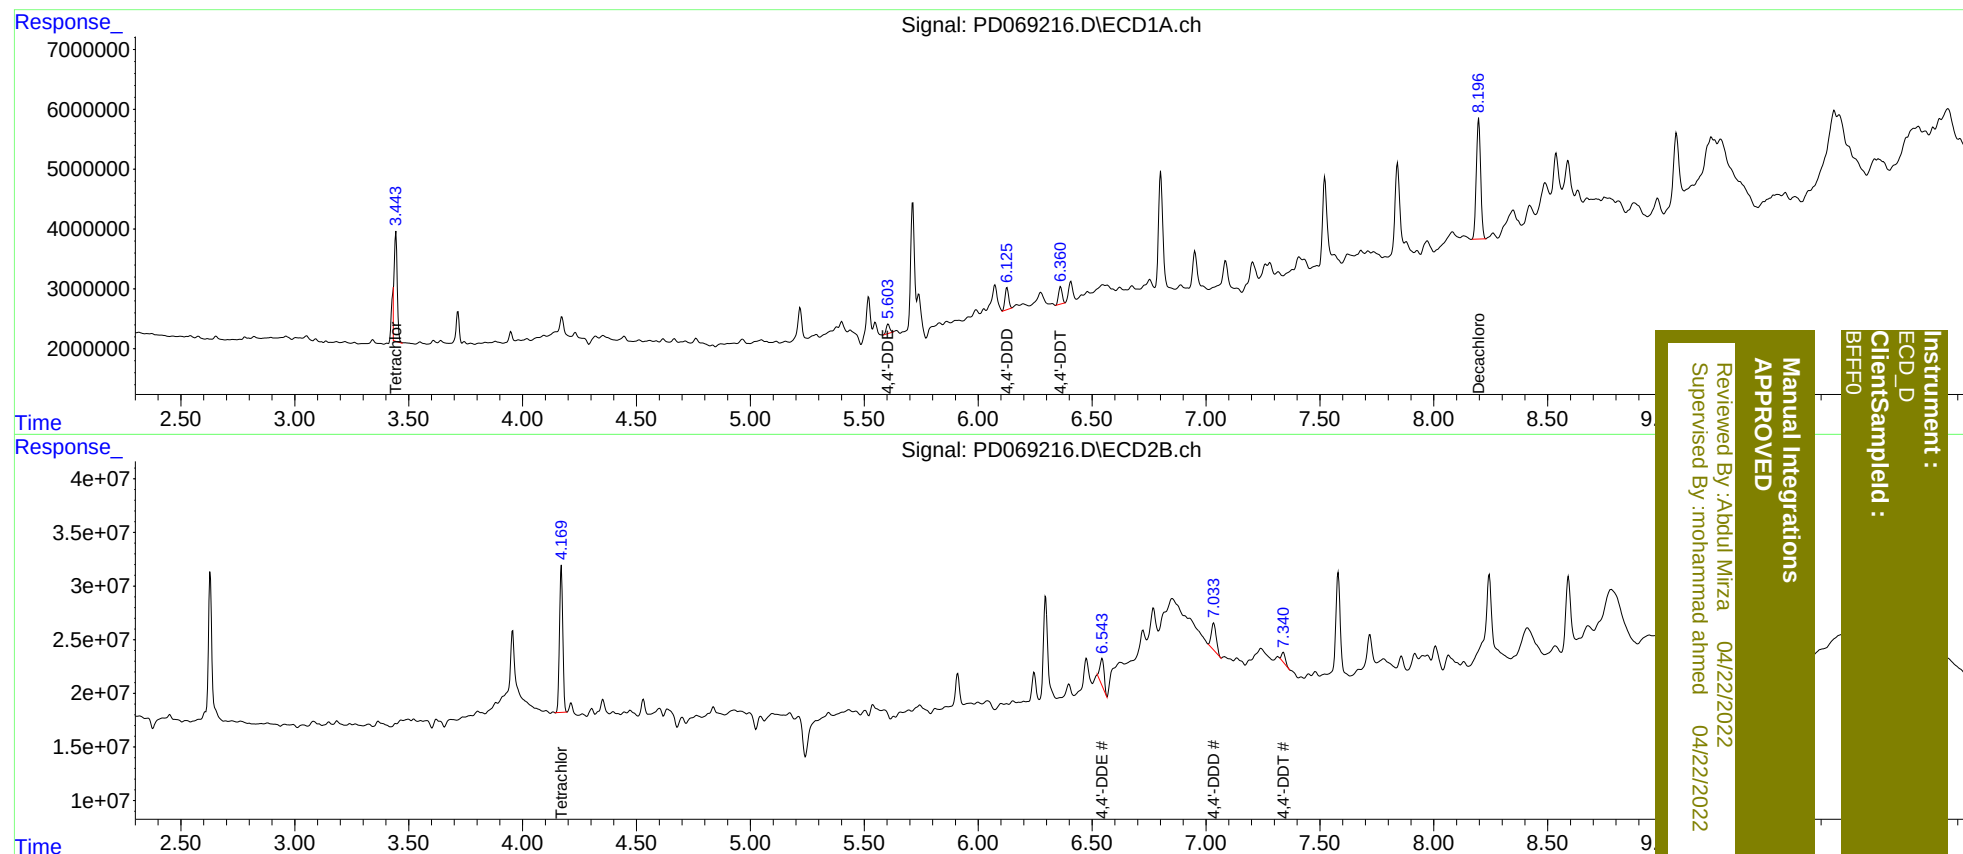

Reviewed By: Abdul Mirza 04/22/2022
Supervised By: mohammad ahmed 04/22/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BFFF0