

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042024\
 Data File : PD082534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2024 17:20
 Operator : AR\AJ
 Sample : P2170-05MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZZZ9MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/22/2024
 Supervised By :Ankita Jodhani 04/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 21:21:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 02:08:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.775	20712543	43772325	13.659	12.696
27)	SA Decachlor...	9.118	7.907	20611163	40651750	10.540	12.493
Target Compounds							
2)	A alpha-BHC	4.022	3.275	106.3E6	241.2E6	41.396	44.927
3)	MA gamma-BHC...	4.355	3.604	109.4E6	236.2E6	43.991m	47.098
4)	MA Heptachlor	4.947	3.943	110.1E6	234.7E6	43.582m	50.163
5)	MB Aldrin	5.292	4.223	102.0E6	222.5E6	43.821	48.396
6)	B beta-BHC	4.552	3.900	42716070	93734576	40.742	45.087
7)	B delta-BHC	4.801	4.130	57747255	126.2E6	23.917	25.851
8)	B Heptachlo...	5.719	4.724	96880774	201.9E6	44.634	47.708
9)	A Endosulfan I	6.107	5.095	95445961	171.6E6	44.173	44.685
10)	B trans-Chl...	5.977	4.974	97745754	220.3E6	47.600	54.719
11)	B cis-Chlor...	6.057	5.038	104.7E6	220.8E6	49.519	53.430
12)	B 4,4'-DDE	6.228	5.226	208.9E6	470.7E6	101.491	121.497
13)	MA Dieldrin	6.384	5.358	199.5E6	426.8E6	90.557	101.295
14)	MA Endrin	6.614	5.633	171.2E6	381.9E6	93.385	105.264
15)	B Endosulfa...	6.834	5.927	164.6E6	355.1E6	86.668	102.579
16)	A 4,4'-DDD	6.747	5.780	148.1E6	315.7E6	93.993	102.492
17)	MA 4,4'-DDT	7.062	6.031	164.9E6	358.0E6	100.827	109.069
18)	B Endrin al...	6.964	6.106	121.9E6	261.4E6	89.829	98.803
19)	B Endosulfa...	7.199	6.328	138.9E6	298.9E6	82.351	89.490
20)	A Methoxychlor	7.539	6.606	378.1E6	742.6E6	429.236	443.408
21)	B Endrin ke...	7.686	6.834	165.1E6	360.0E6	91.888	95.735

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042024\
Data File : PD082534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2024 17:20
Operator : AR\AJ
Sample : P2170-05MS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 21:21:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 02:08:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

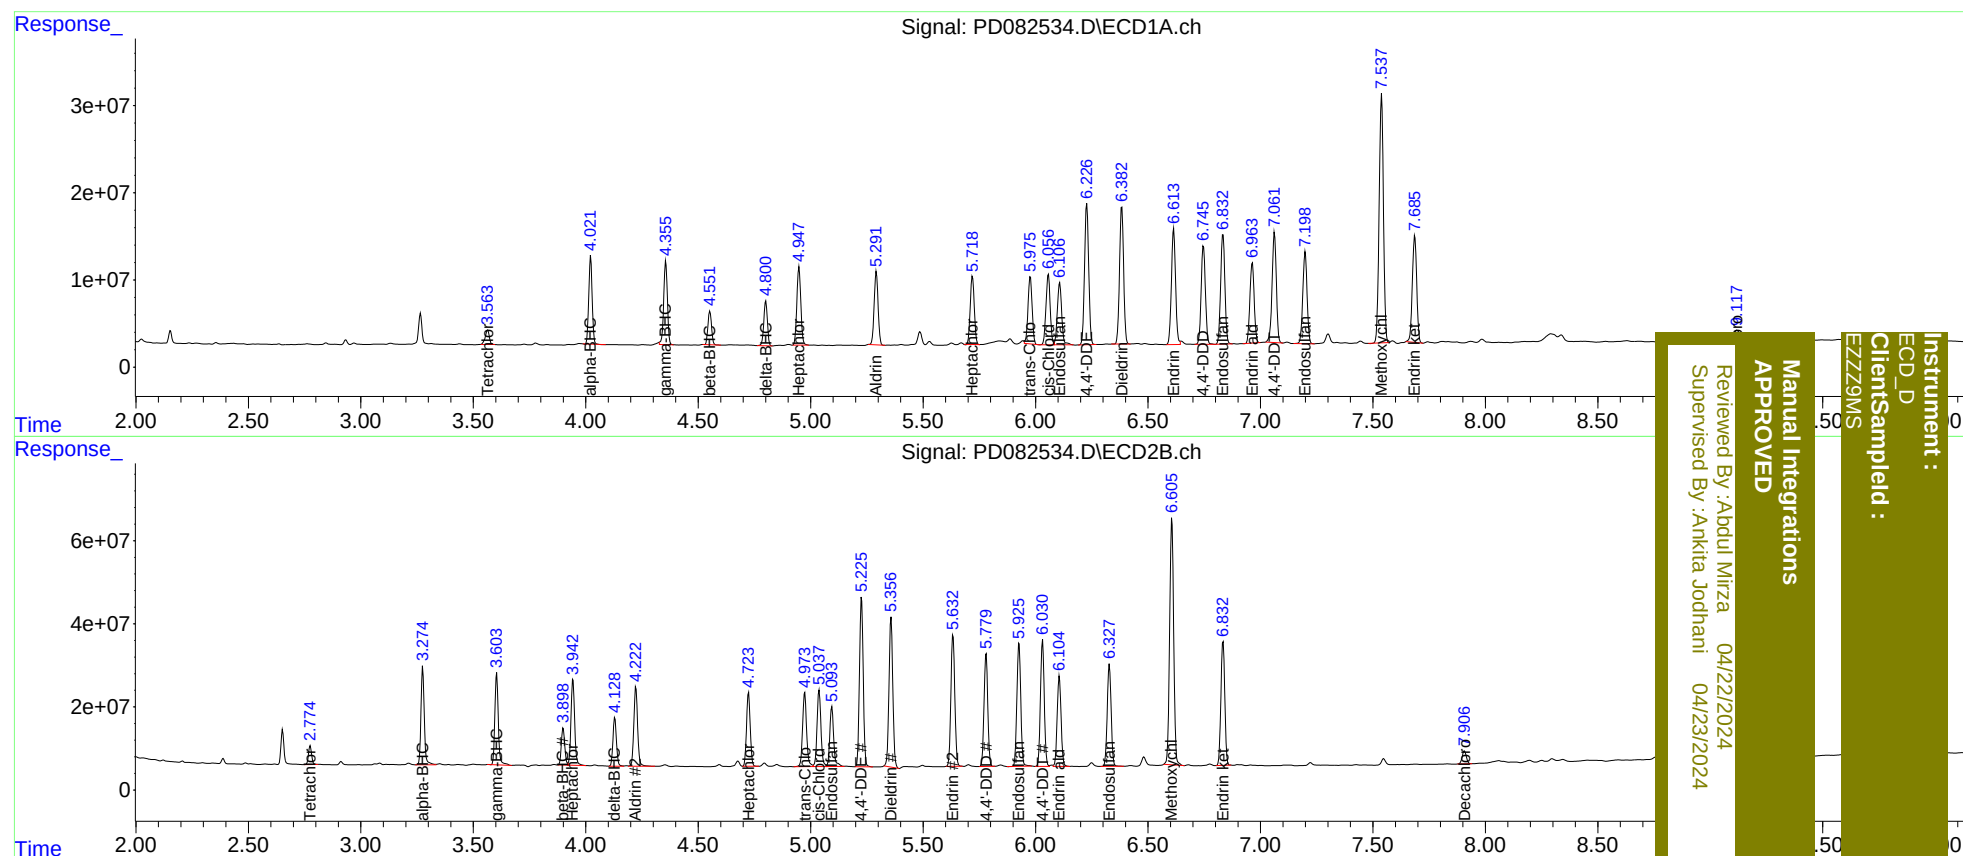

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/22/2024
Supervised By: Ankita Jodhani 04/23/2024

Instrument :
ECD_D
Client Sampled :
EZZZ9MS