

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
 Data File : PD074811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 11:14
 Operator : AR\AJ
 Sample : 02390-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SPC-3WC-23-04-17

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2023
 Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 21:35:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 18 13:17:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.767	19745380	11339273	8.278	8.699
28) SA Decachlor...	9.087	7.917	21354812	8264371	7.032	6.196
Target Compounds						
16) A 4,4'-DDD	6.724	5.784	172.2E6	57783798	64.989m	43.830 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
Data File : PD074811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 11:14
Operator : AR\AJ
Sample : 02390-11
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SPC-3WC-23-04-17


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 21:35:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
Quant Title : GC Extractables
QLast Update : Tue Apr 18 13:17:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

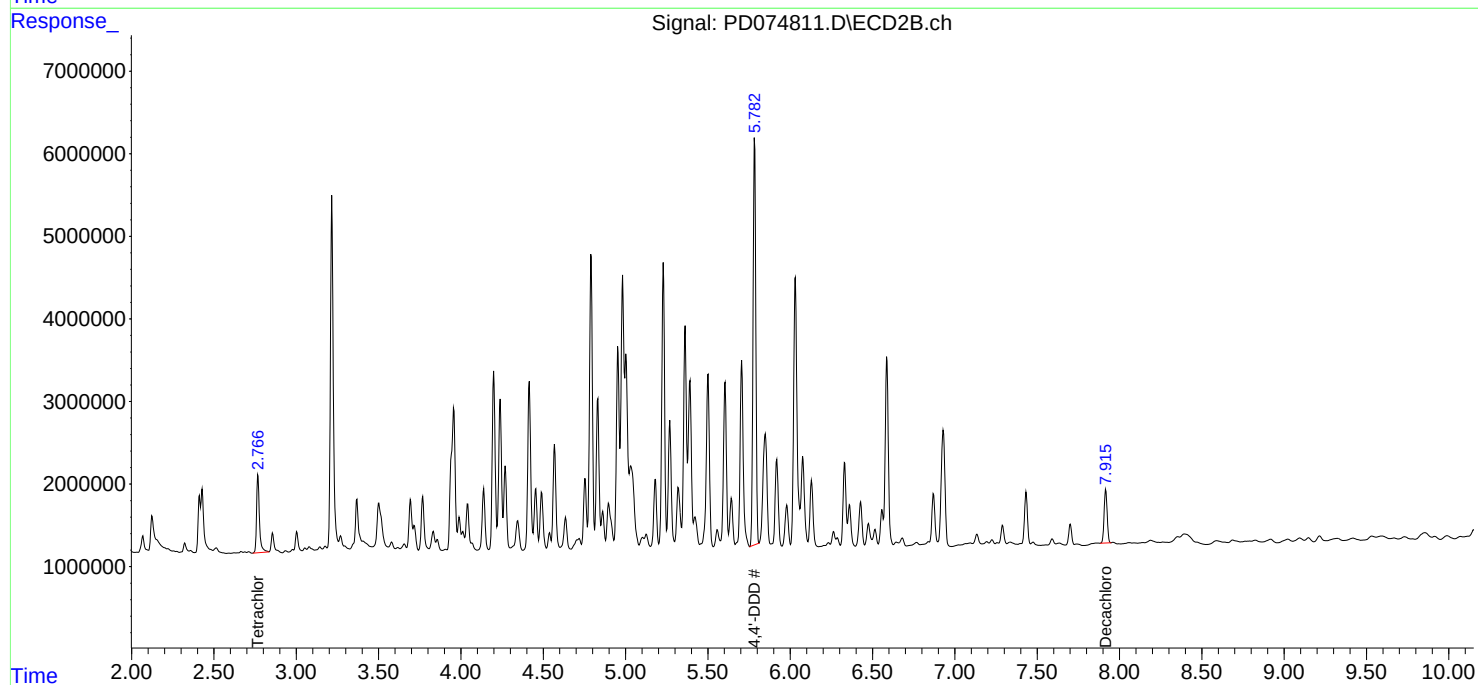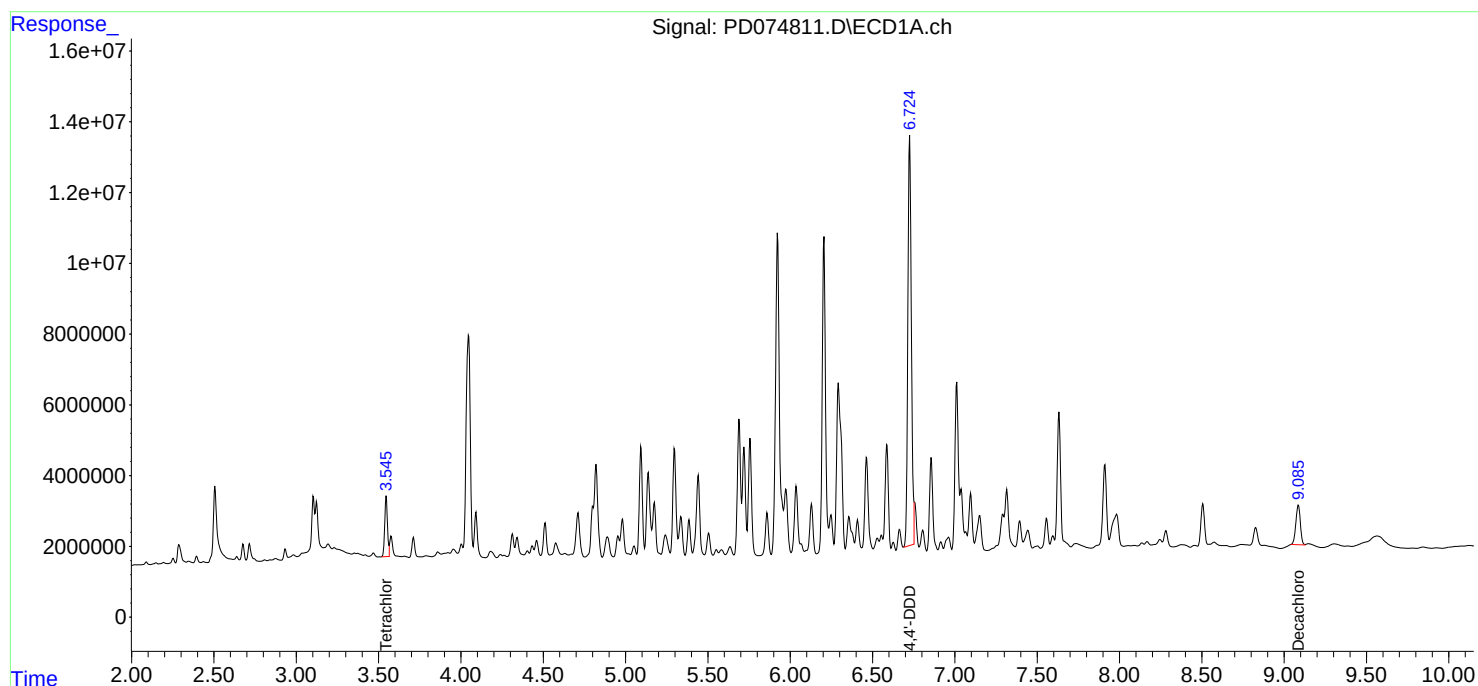

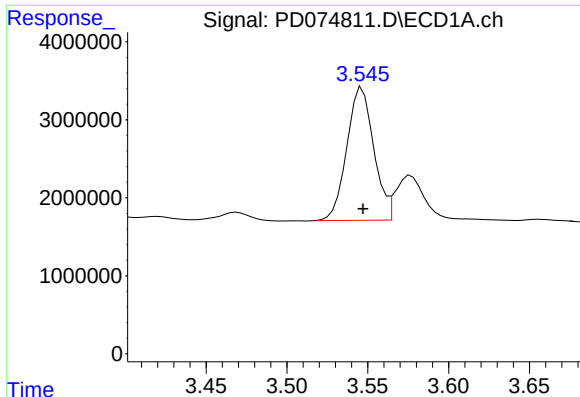


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 19745380
Conc: 8.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
SPC-3WC-23-04-17


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

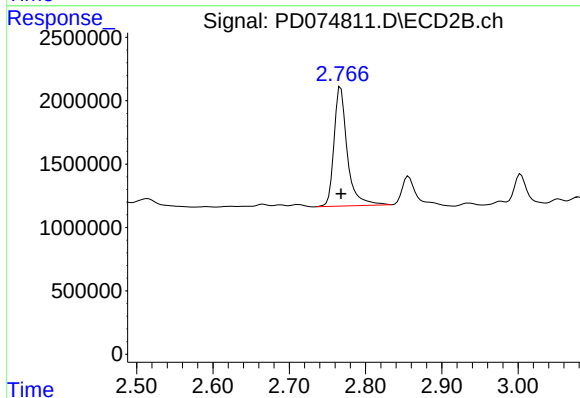


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 11339273
Conc: 8.70 ng/ml

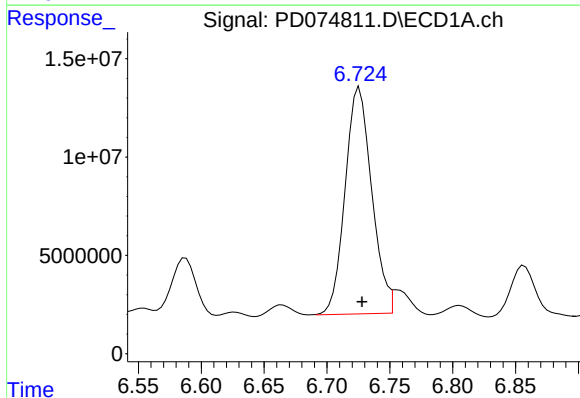


#16 4,4'-DDD

R.T.: 6.724 min
Delta R.T.: -0.003 min
Response: 172204485
Conc: 64.99 ng/ml m

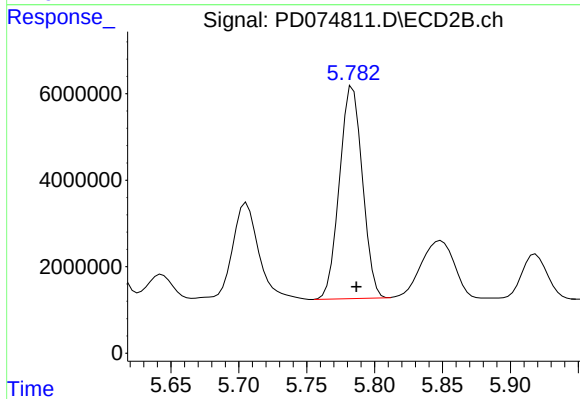

#16 4,4'-DDD

R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 57783798
Conc: 43.83 ng/ml

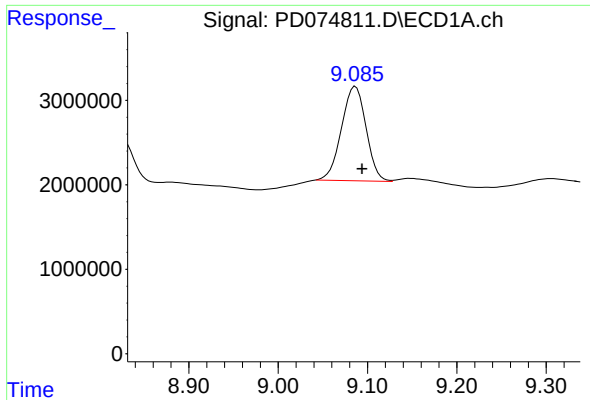


#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: -0.007 min
Response: 21354812
Conc: 7.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
SPC-3WC-23-04-17

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

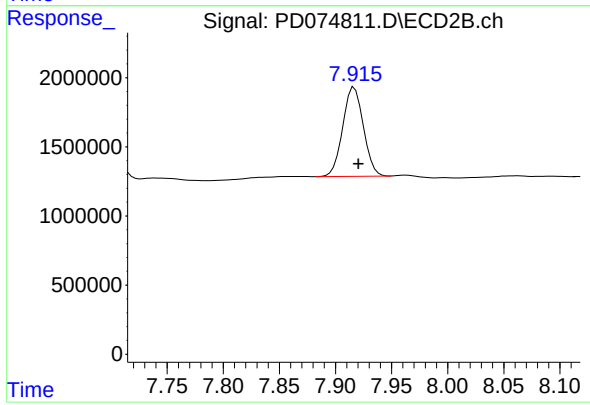

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: -0.004 min
Response: 8264371
Conc: 6.20 ng/ml