

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
 Data File : PD074818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 13:00
 Operator : AR\AJ
 Sample : 02389-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SPB-5WC-23-04-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 21:41:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 18 13:17:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.768	24295995	10821282	10.186	8.301
28)	SA Decachlor...	9.089	7.917	26166549	14829206	8.617	11.118 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
Data File : PD074818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 13:00
Operator : AR\AJ
Sample : 02389-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SPB-5WC-23-04-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 21:41:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
Quant Title : GC Extractables
QLast Update : Tue Apr 18 13:17:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

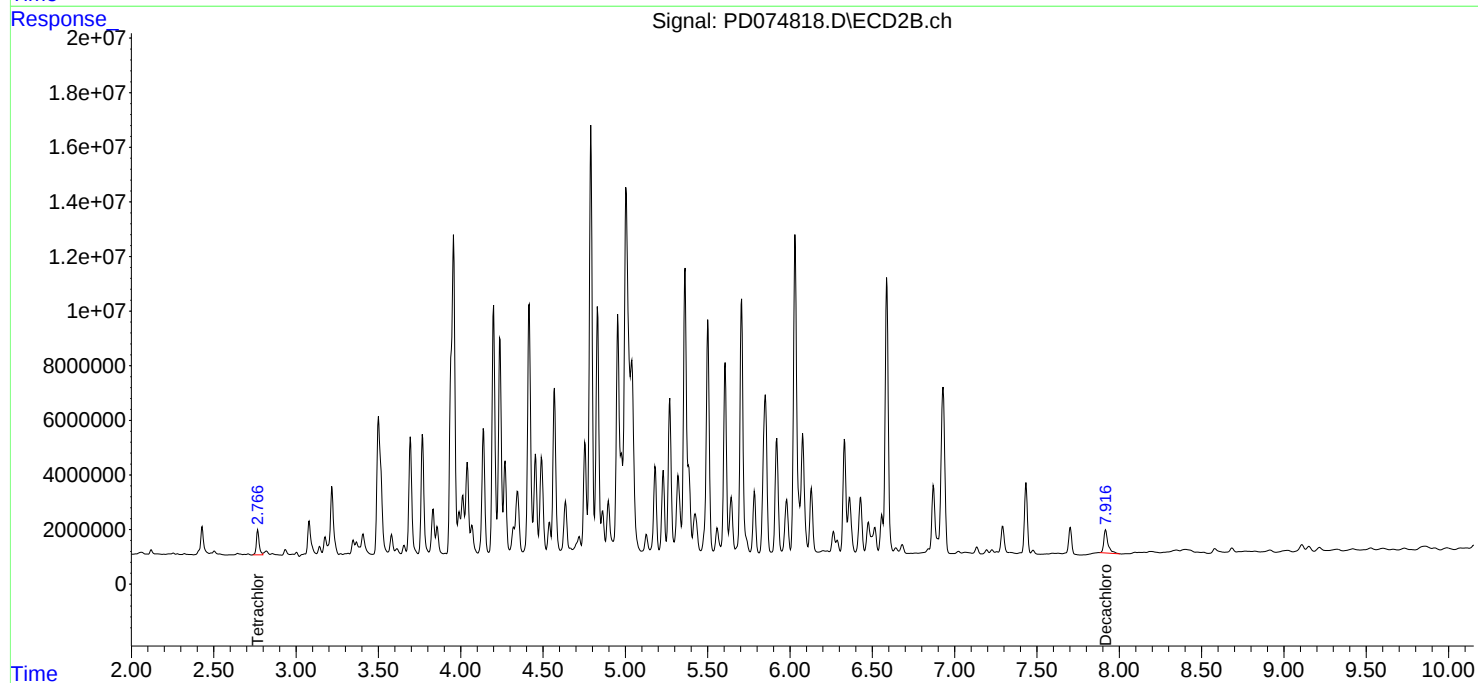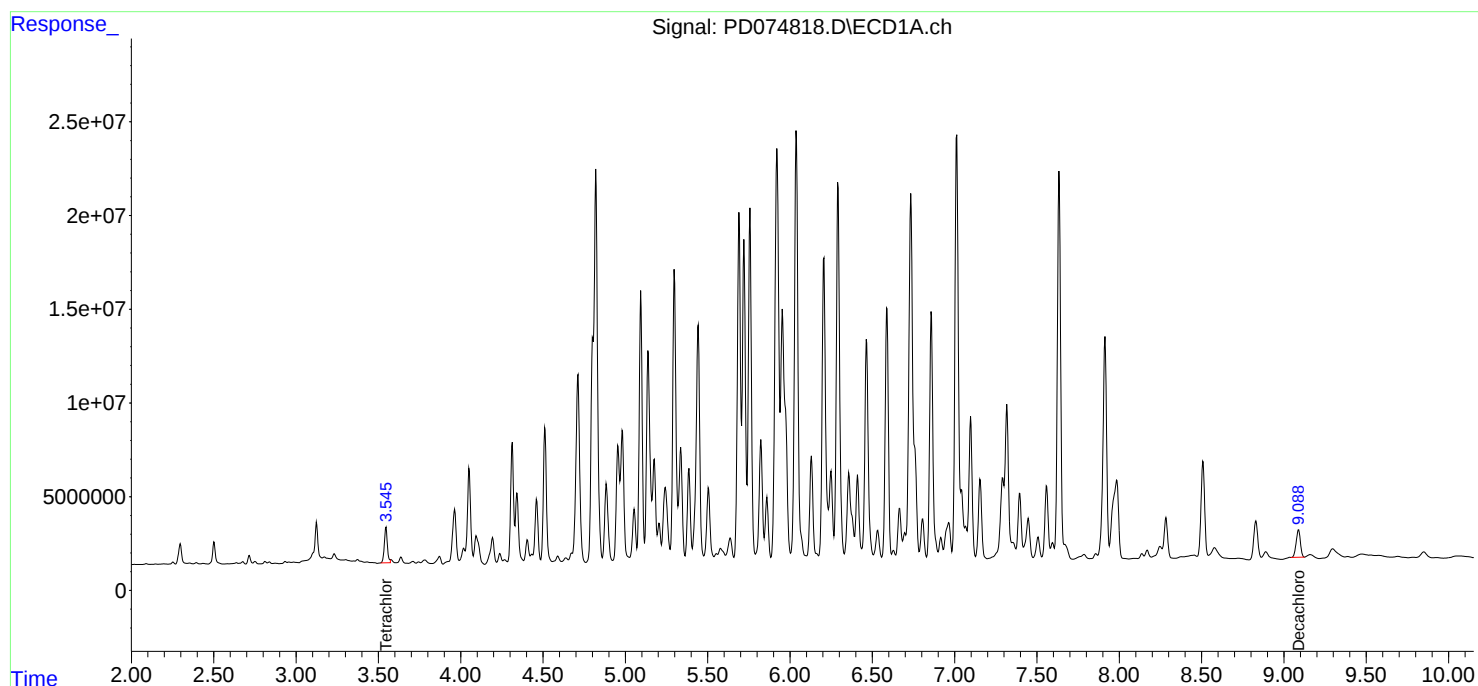


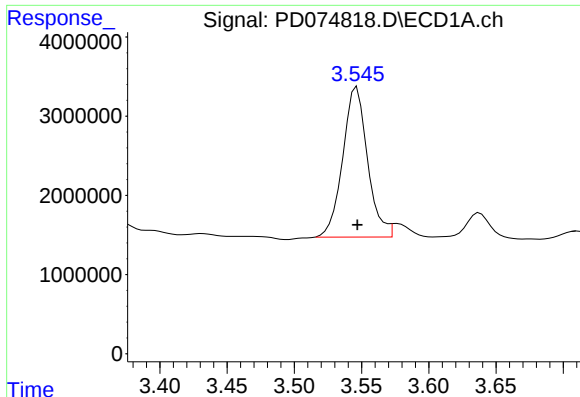

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 24295995
Conc: 10.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
SPB-5WC-23-04-17

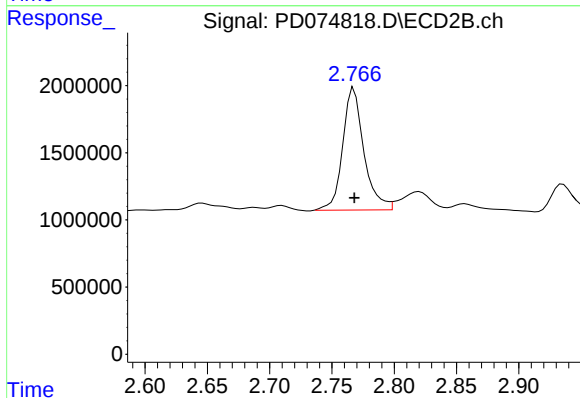


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 10821282
Conc: 8.30 ng/ml

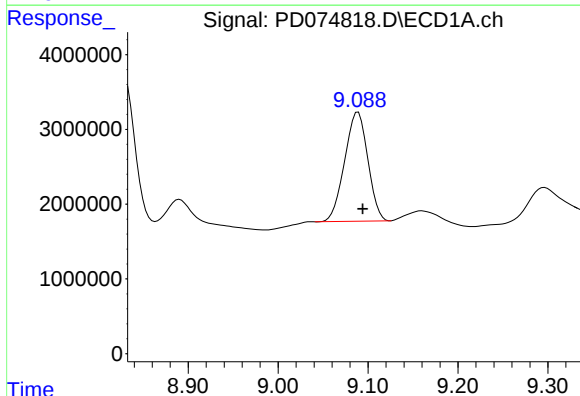

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: -0.005 min
Response: 26166549
Conc: 8.62 ng/ml

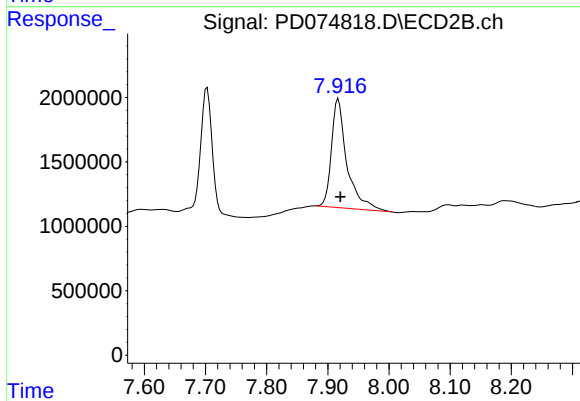

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: -0.003 min
Response: 14829206
Conc: 11.12 ng/ml