

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
 Data File : PD074834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 17:19
 Operator : AR\AJ
 Sample : 02386-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SPA-2WC-23-04

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 04/21/2023
 Supervised By :Ankita Jodhani 04/21/2023

04/21/2023
 Supervised By :Ankita
 Jodhani

04/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 21:53:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 18 13:17:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.769	35299649	26410441	14.799m	20.260 #
28) SA Decachlor...	9.088	7.918	39775687	16434934	13.098	12.321
Target Compounds						
13) MA Dieldrin	6.361	5.362	12819977	9477300	3.758	5.645 #
16) A 4,4'-DDD	6.724	5.785	93116822	38120815	35.142	28.915

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
Data File : PD074834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 17:19
Operator : AR\AJ
Sample : 02386-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SPA-2WC-23-04

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023


04/21/2023
Supervised By :Ankita
Jodhani

04/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 21:53:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
Quant Title : GC Extractables
QLast Update : Tue Apr 18 13:17:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

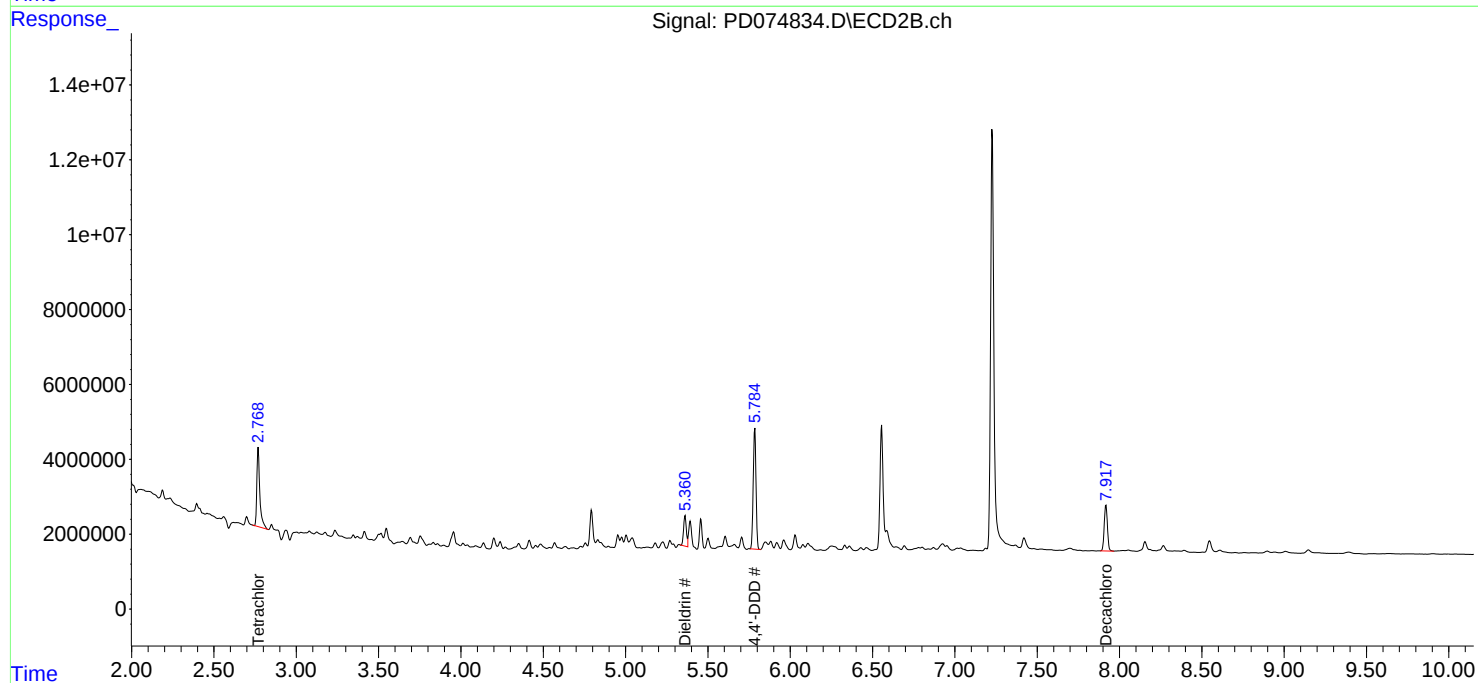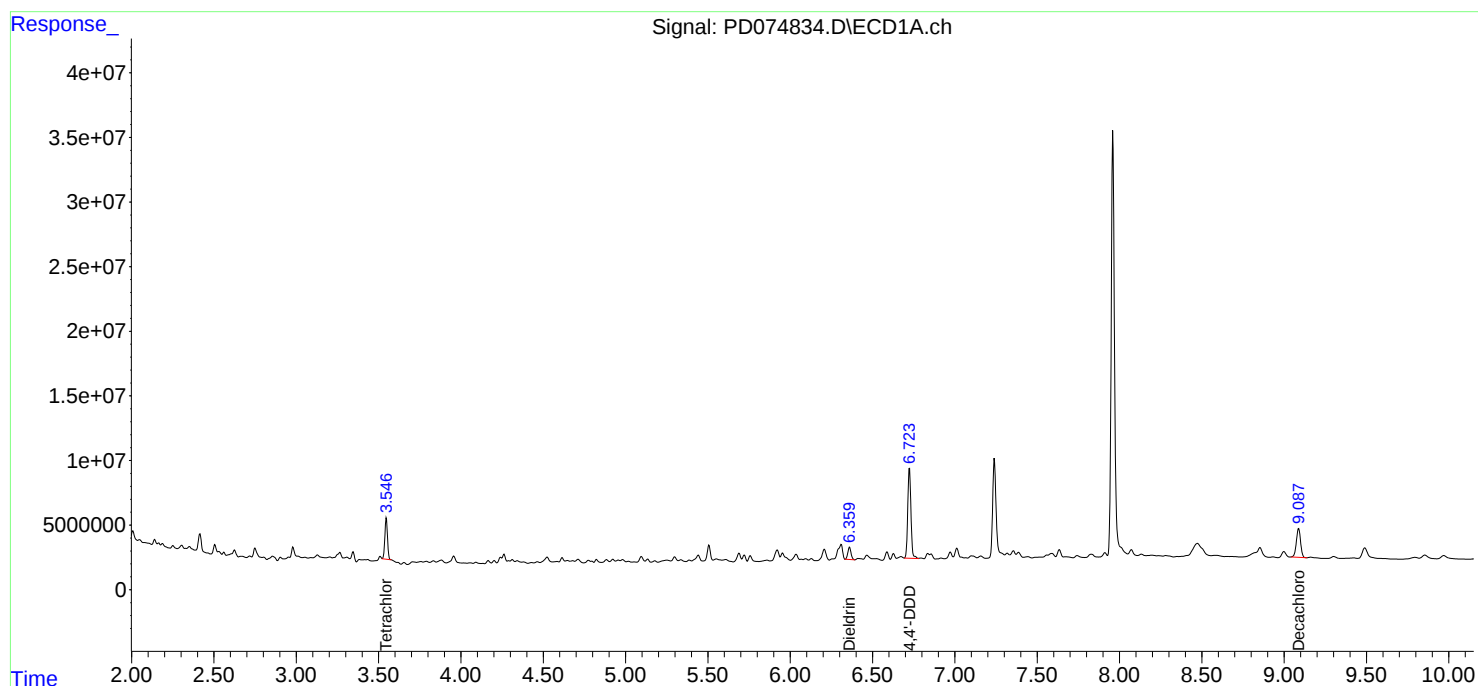

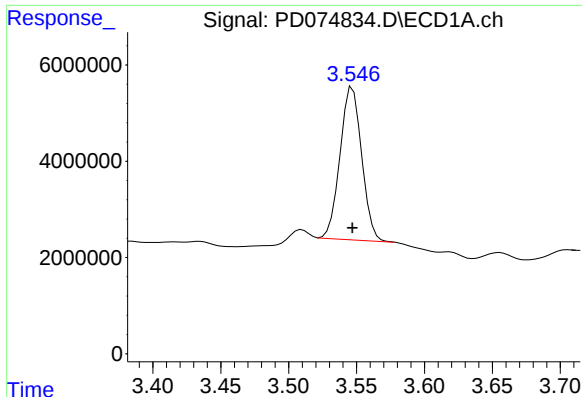

#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.001 min
Response: 35299649
Conc: 14.80 ng/ml


Instrument :
ECD_D
ClientSampleId :
SPA-2WC-23-04

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023


04/21/2023
Supervised By :Ankita
Jodhani

04/21/2023

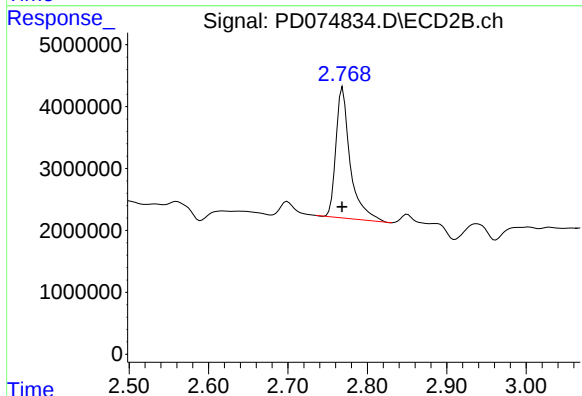


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: 0.000 min
Response: 26410441
Conc: 20.26 ng/ml

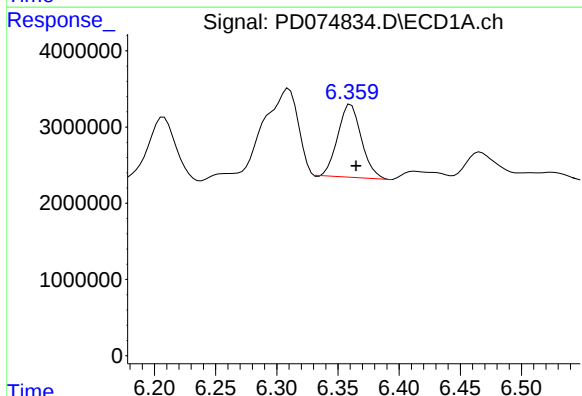


#13 Dieldrin

R.T.: 6.361 min
Delta R.T.: -0.004 min
Response: 12819977
Conc: 3.76 ng/ml

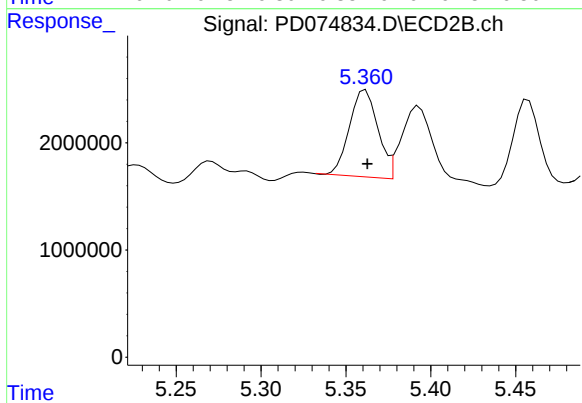

#13 Dieldrin

R.T.: 5.362 min
Delta R.T.: -0.001 min
Response: 9477300
Conc: 5.64 ng/ml

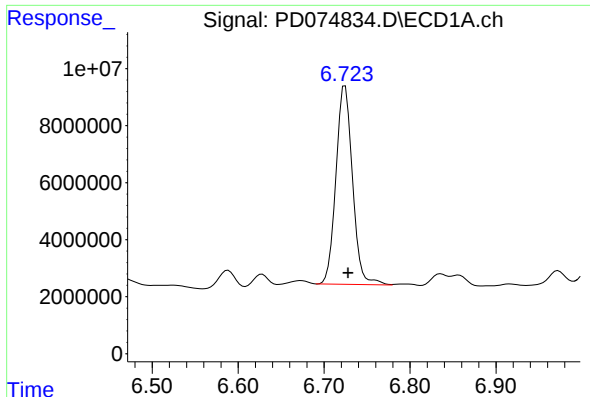

#16 4,4'-DDD

R.T.: 6.724 min
Delta R.T.: -0.003 min
Response: 93116822
Conc: 35.14 ng/ml


Instrument :
ECD_D
ClientSampleId :
SPA-2WC-23-04

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023


04/21/2023
Supervised By :Ankita
Jodhani

04/21/2023

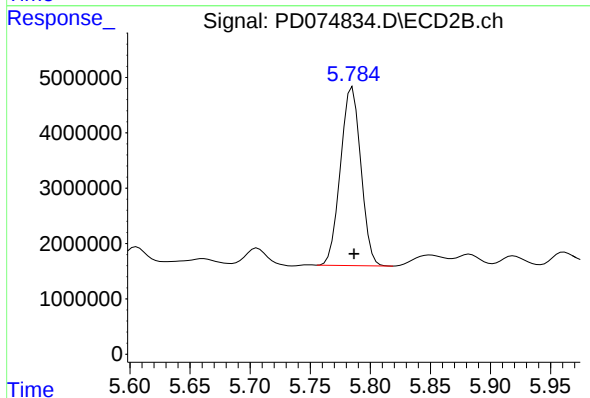


#16 4,4'-DDD

R.T.: 5.785 min
Delta R.T.: -0.001 min
Response: 38120815
Conc: 28.91 ng/ml

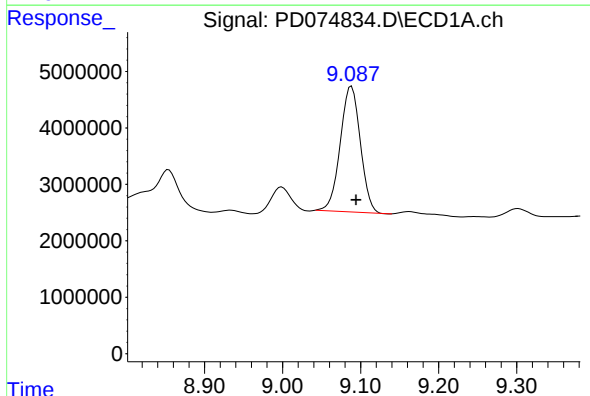

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: -0.006 min
Response: 39775687
Conc: 13.10 ng/ml

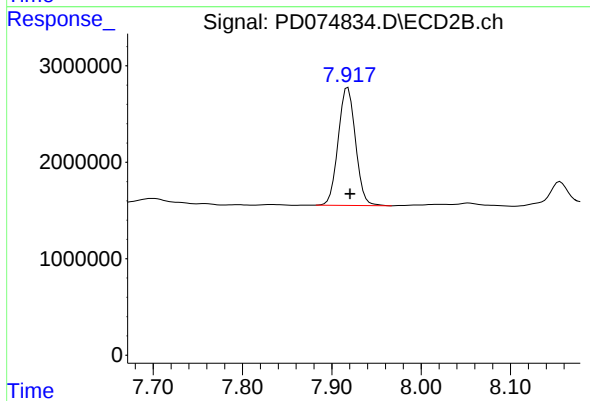

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: -0.002 min
Response: 16434934
Conc: 12.32 ng/ml