

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
 Data File : PD074848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 21:50
 Operator : AR\AJ
 Sample : 02390-04
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SPC-1WC-23-04-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:52:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 18 13:17:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.768	47152562	22437289	19.769	17.212
28)	SA Decachlor...	9.086	7.917	47835932	19755259	15.752	14.811
Target Compounds							
16)	A 4,4'-DDD	6.724	5.784	2187979	730370	0.826	0.554 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
Data File : PD074848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 21:50
Operator : AR\AJ
Sample : 02390-04
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SPC-1WC-23-04-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:52:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
Quant Title : GC Extractables
QLast Update : Tue Apr 18 13:17:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

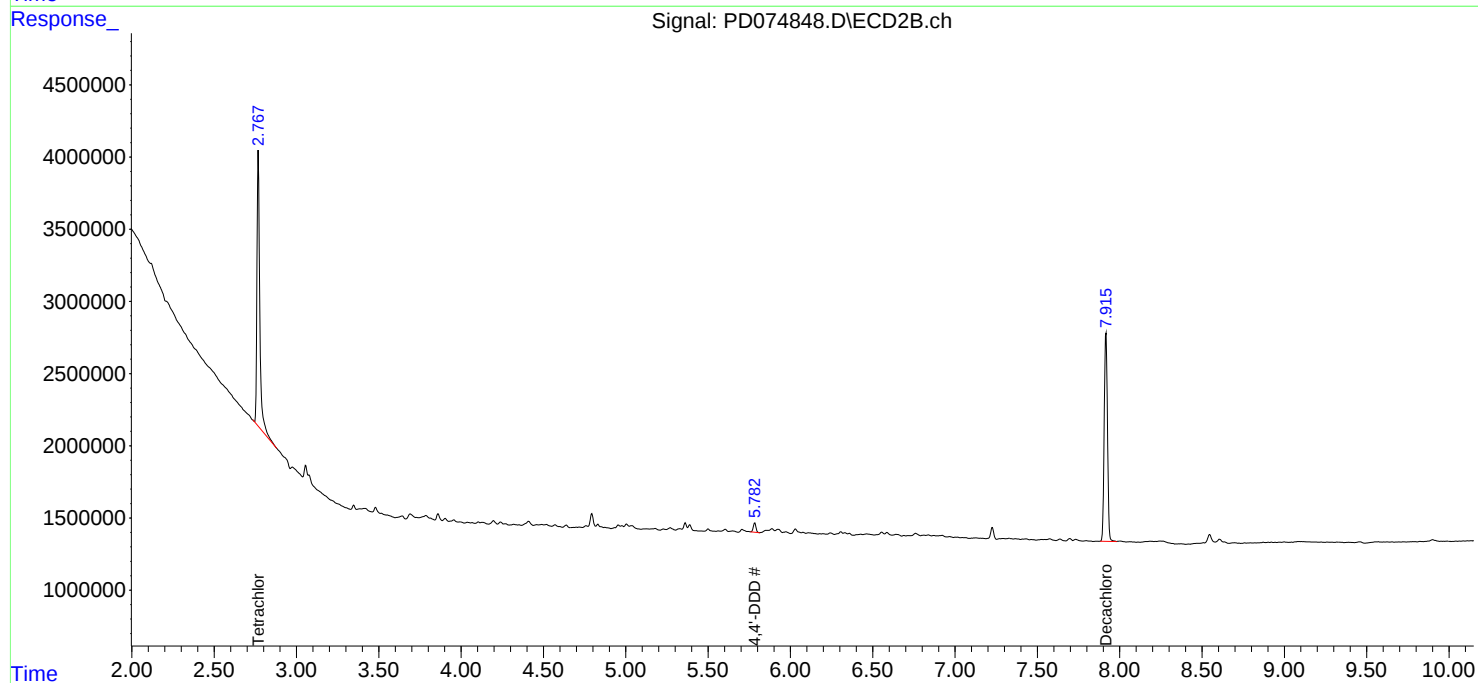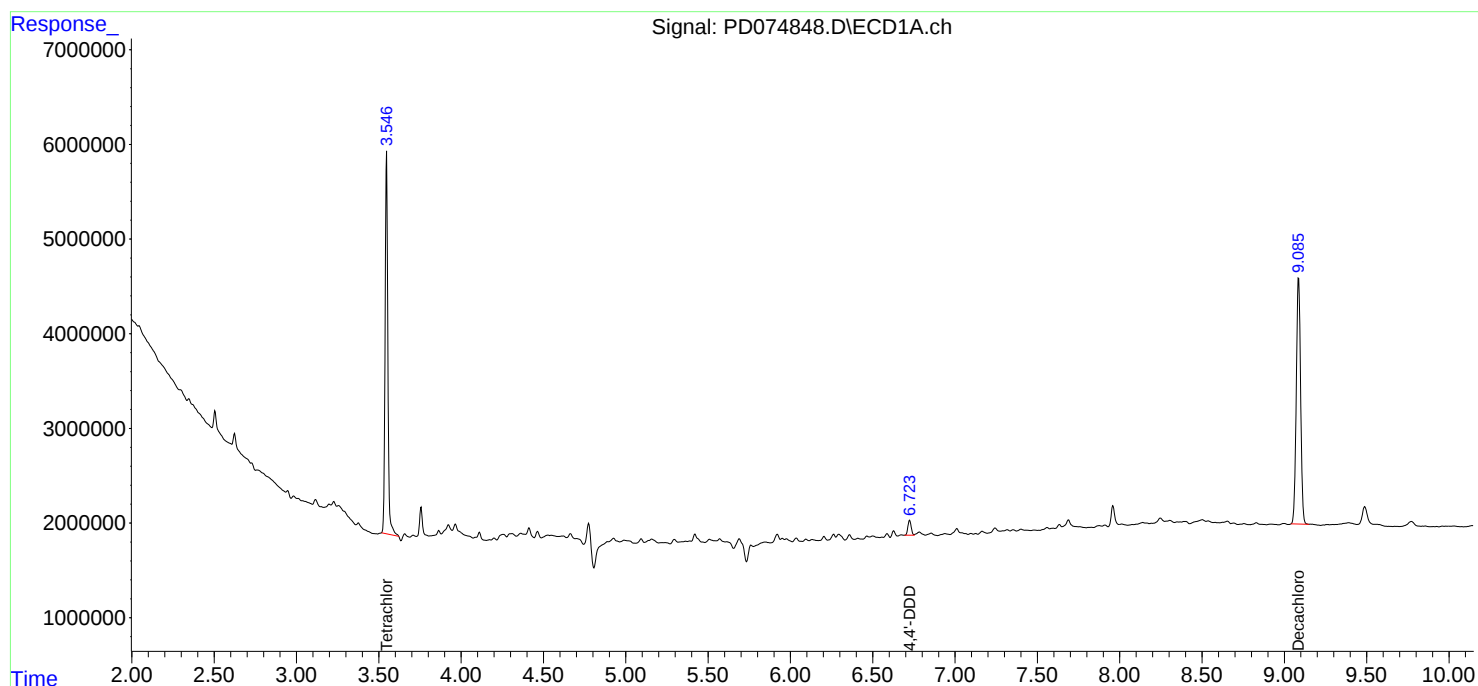


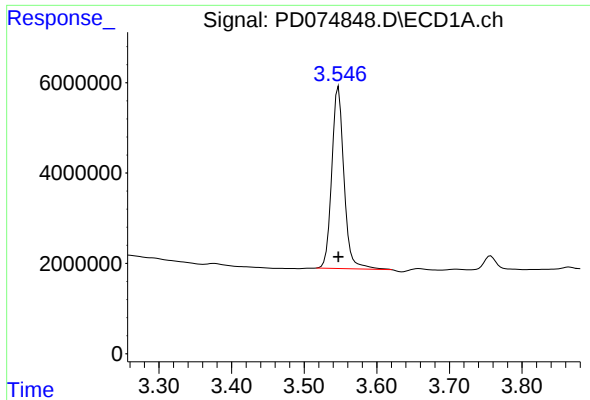

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 47152562
Conc: 19.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
SPC-1WC-23-04-17

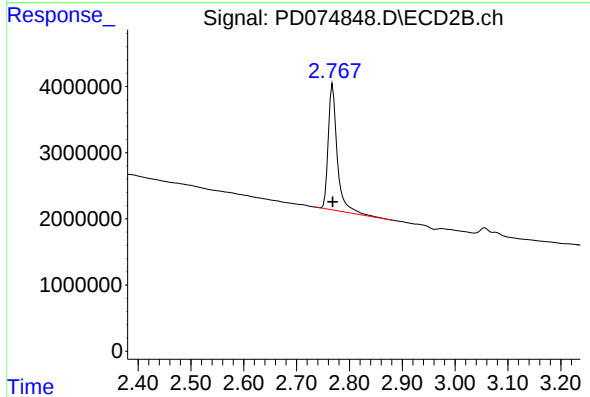


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 22437289
Conc: 17.21 ng/ml

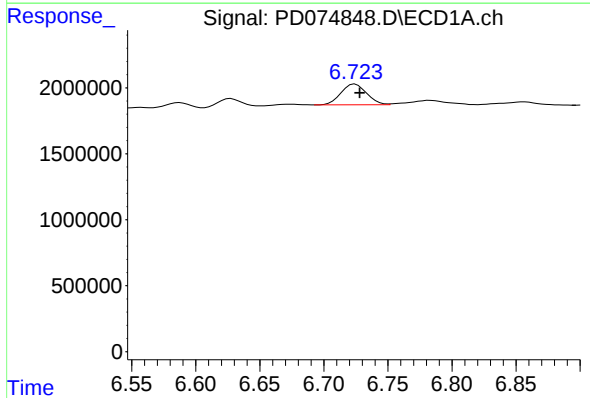


#16 4,4'-DDD

R.T.: 6.724 min
Delta R.T.: -0.003 min
Response: 2187979
Conc: 0.83 ng/ml

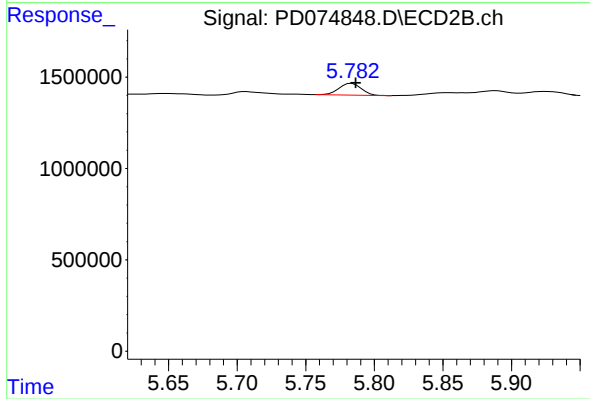

#16 4,4'-DDD


R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 730370
Conc: 0.55 ng/ml

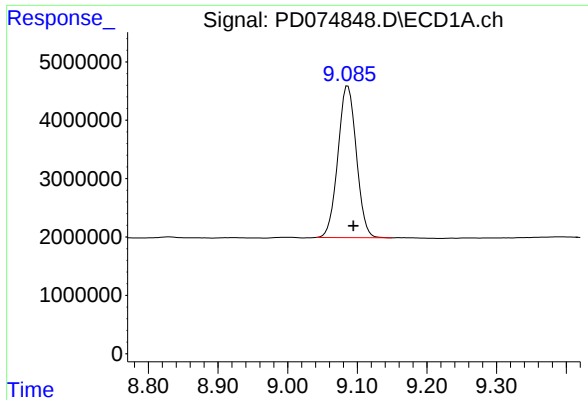

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: -0.008 min
Response: 47835932
Conc: 15.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
SPC-1WC-23-04-17

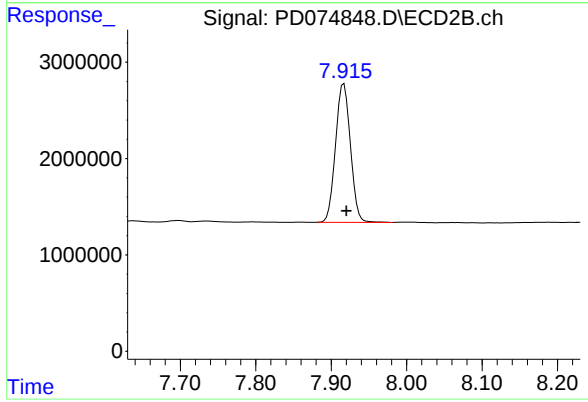

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: -0.004 min
Response: 19755259
Conc: 14.81 ng/ml