

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
 Data File : PD074850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 22:17
 Operator : AR\AJ
 Sample : 02390-12
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SPC-3WC-23-04-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:52:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 18 13:17:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.768	51624717	26816889	21.644	20.572
28)	SA Decachlor...	9.088	7.917	49955857	20606268	16.450	15.449
Target Compounds							
16)	A 4,4'-DDD	6.724	5.784	23653581	10989563	8.927	8.336



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042123\
Data File : PD074850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 22:17
Operator : AR\AJ
Sample : 02390-12
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SPC-3WC-23-04-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:52:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041823.M
Quant Title : GC Extractables
QLast Update : Tue Apr 18 13:17:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

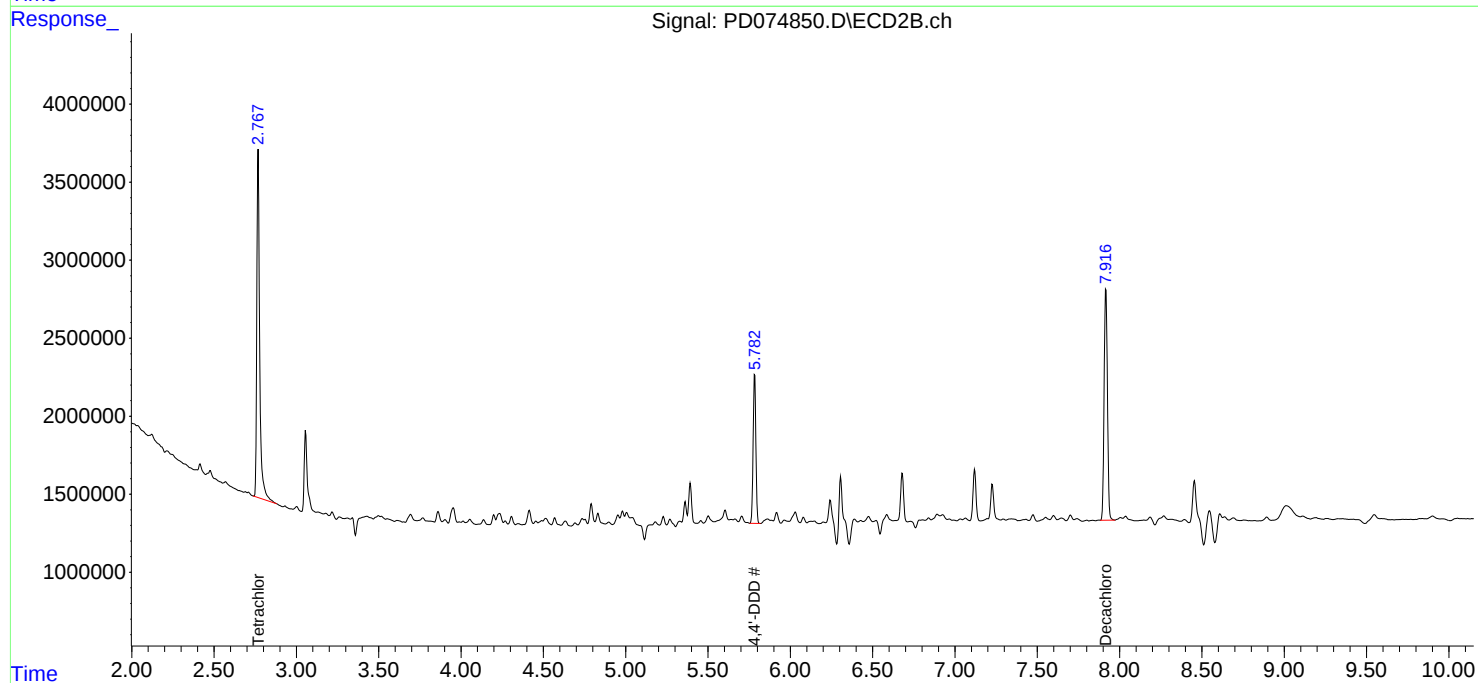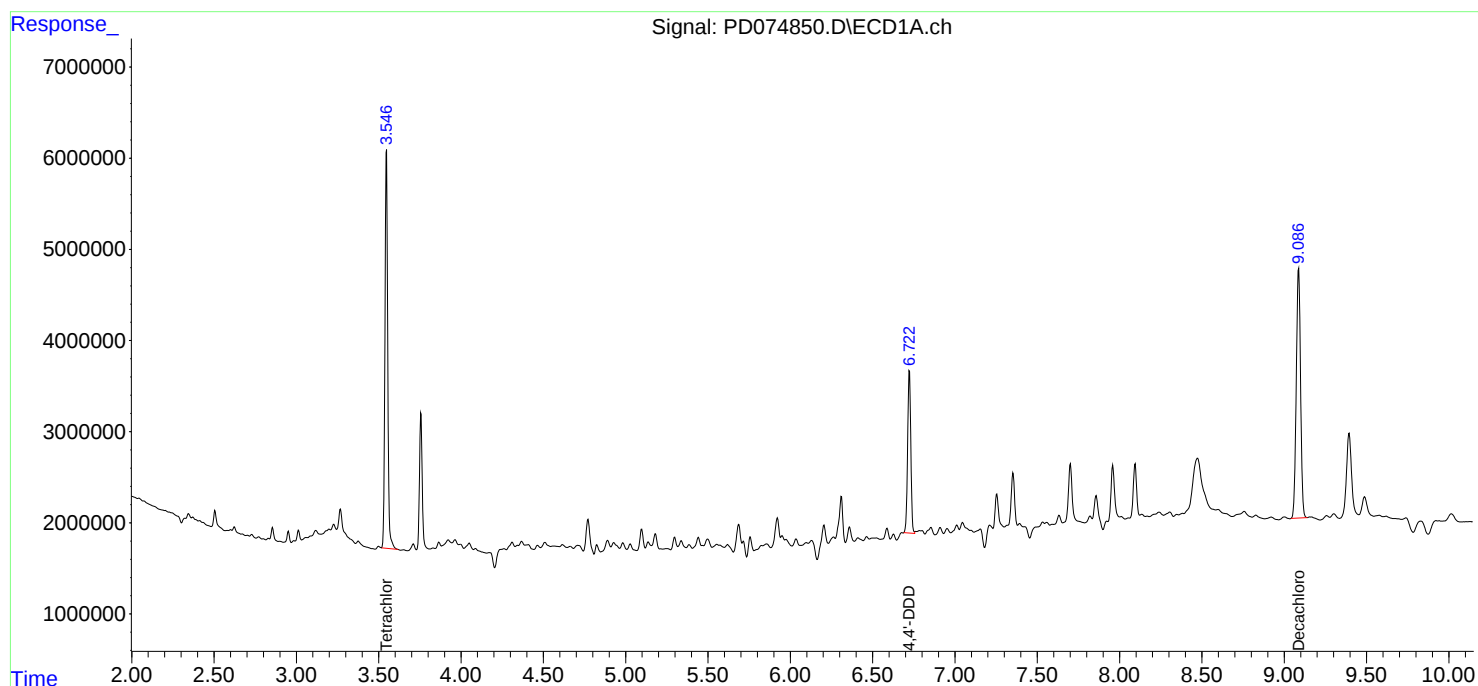


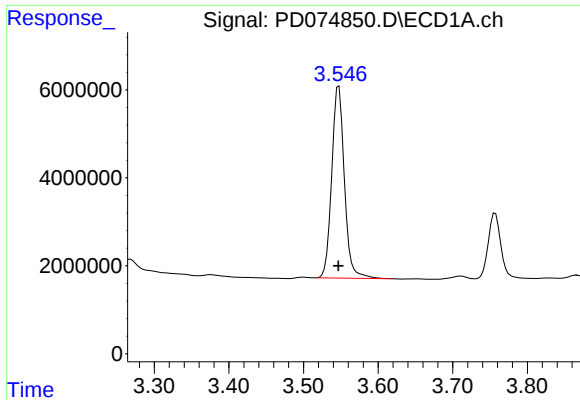

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 51624717
Conc: 21.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
SPC-3WC-23-04-17

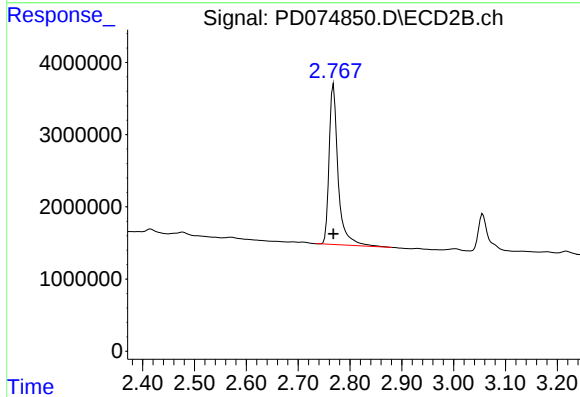


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 26816889
Conc: 20.57 ng/ml

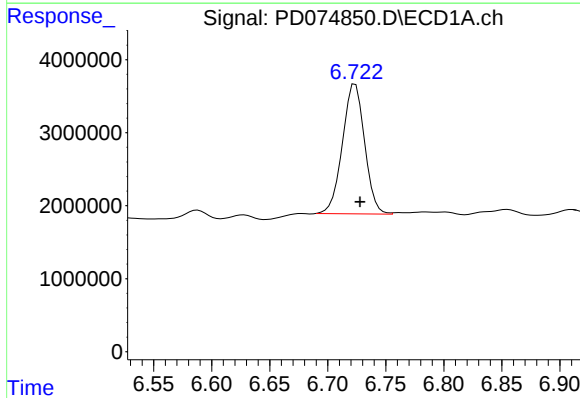


#16 4,4'-DDD

R.T.: 6.724 min
Delta R.T.: -0.004 min
Response: 23653581
Conc: 8.93 ng/ml

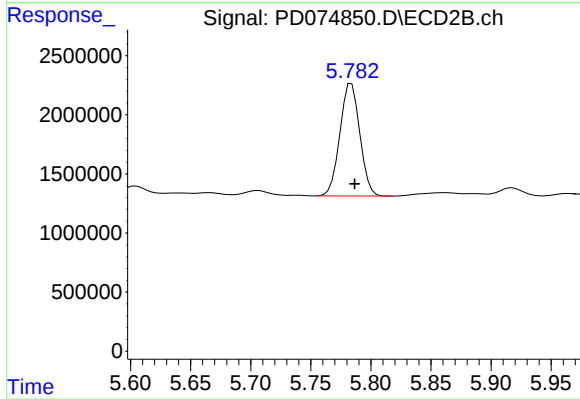

#16 4,4'-DDD


R.T.: 5.784 min
Delta R.T.: -0.003 min
Response: 10989563
Conc: 8.34 ng/ml

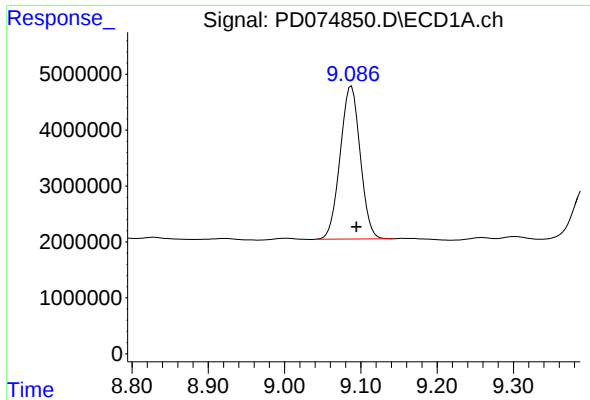

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: -0.006 min
Response: 49955857
Conc: 16.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
SPC-3WC-23-04-17

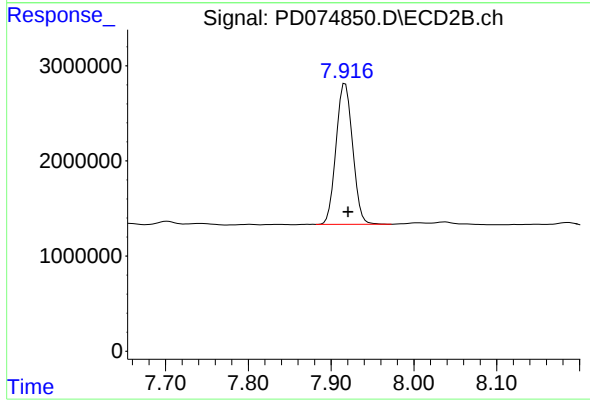

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: -0.003 min
Response: 20606268
Conc: 15.45 ng/ml