

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
 Data File : PD052989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2019 8:05
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:26:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.181f	0	2557275	N.D.	0.164 #
Target Compounds							
4)	MA Heptachlor	0.000	5.243	0	1117568	N.D.	0.028 #
9)	A Endosulfan I	5.150f	6.265f	597895	2113734	0.335	0.072 #
10)	B gamma-Chl...	5.072	0.000	1131774	0	0.580	N.D. #
11)	B alpha-Chl...	5.099f	6.265f	640308	2113734	0.332	0.067 #
14)	MA Endrin	5.660	0.000	993112	0	0.539	N.D. #
16)	A 4,4'-DDD	5.800	0.000	54451	0	0.036	N.D. #
17)	MA 4,4'-DDT	6.012	7.164f	1018457	37385996	0.708	2.006 #
18)	B Endrin al...	0.000	7.081f	0	51301331	N.D.	2.492 #
21)	B Endrin ke...	0.000	7.796	0	44059519	N.D.	2.150 #
25)	Chlordane-3	5.072	0.000	1131774	0	5.118	N.D. #
26)	Chlordane-4	5.099f	6.265f	640308	2113734	3.019	0.416 #
27)	Chlordane-5	0.000	7.039	0	8947877	N.D.	9.698 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
Data File : PD052989.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2019 8:05
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:26:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

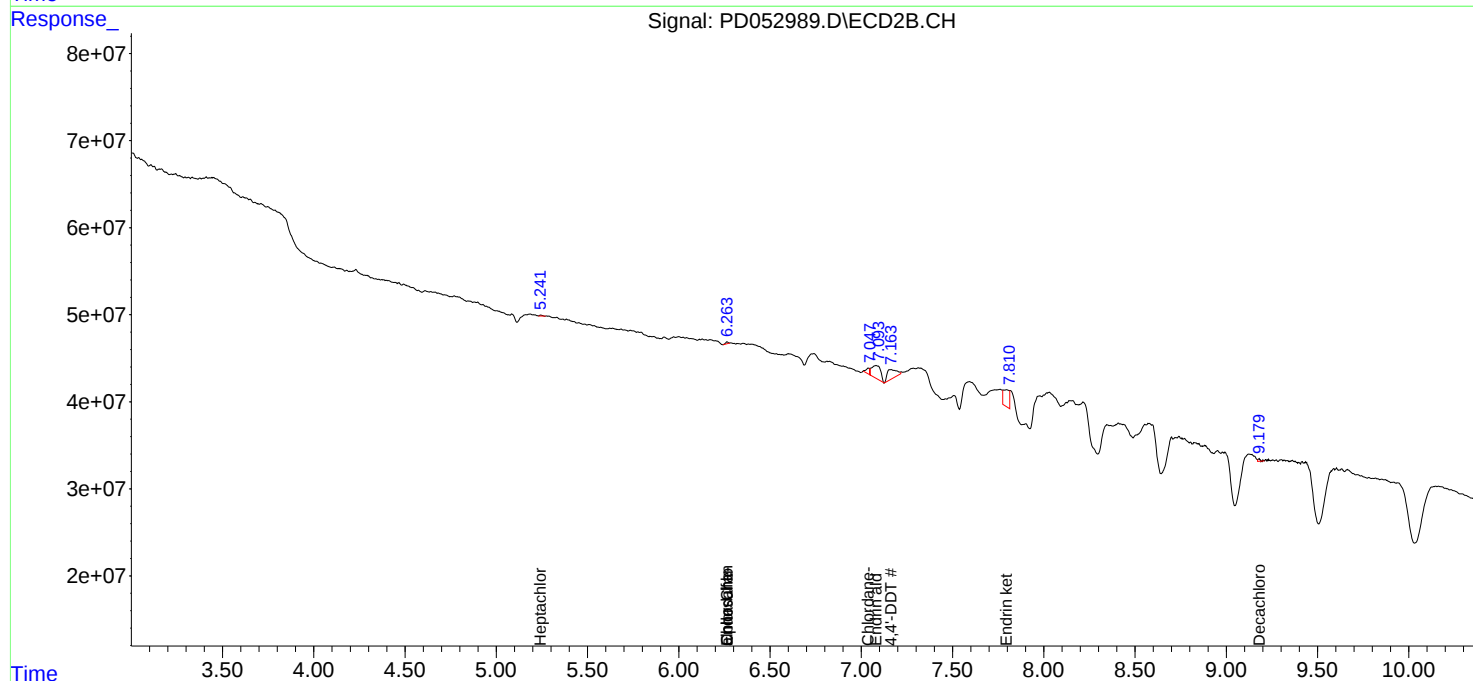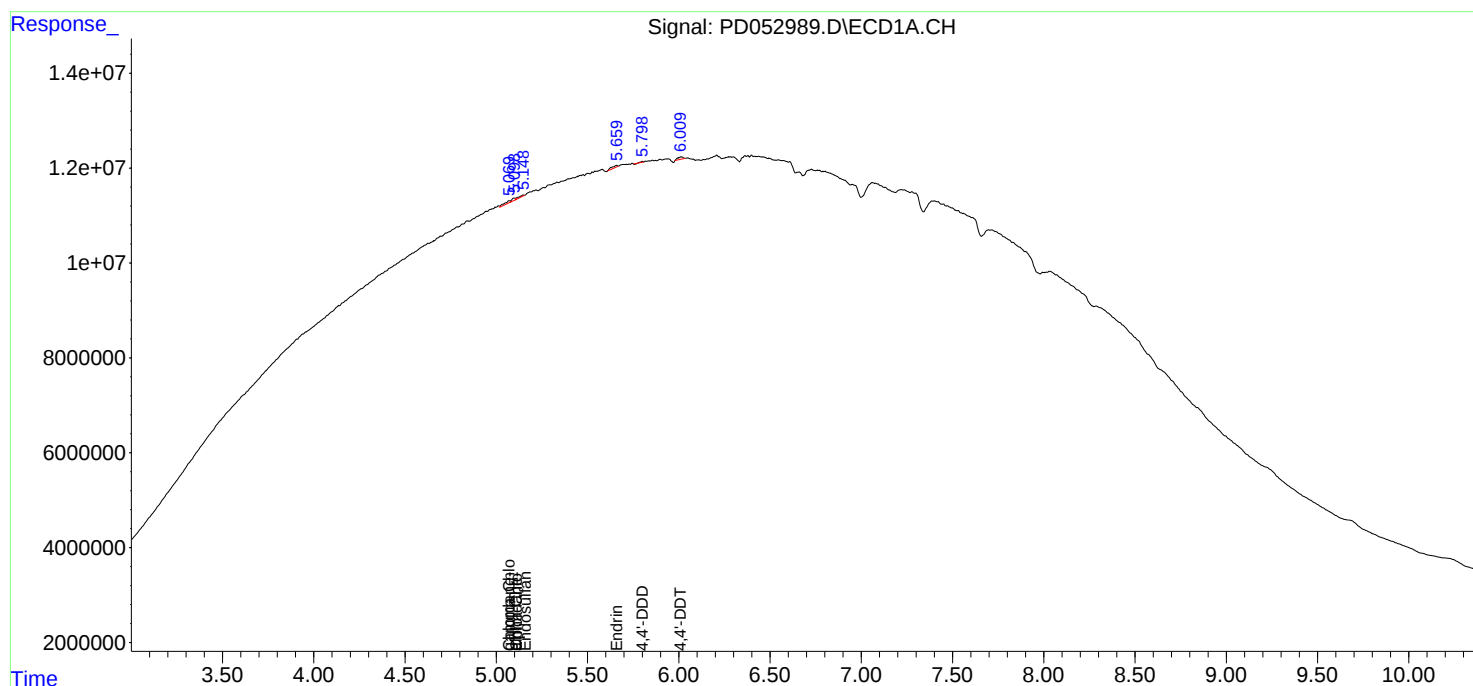


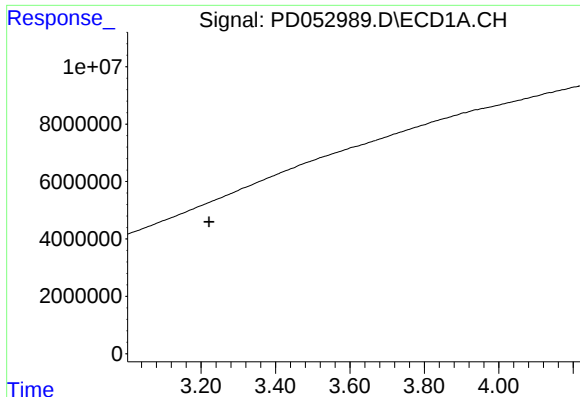

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

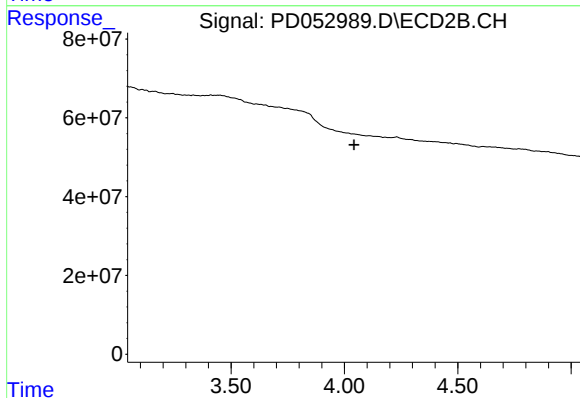


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.043 min
Response: 0
Conc: N.D.

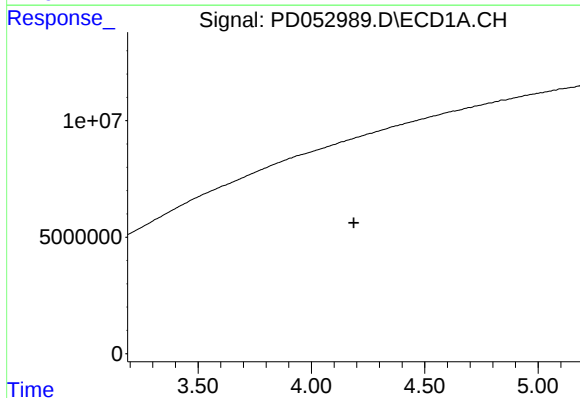


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

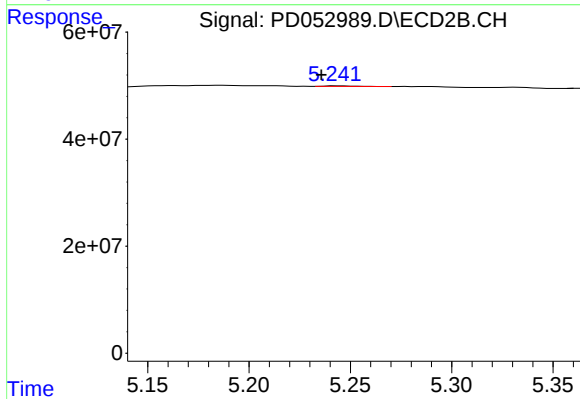

#4 Heptachlor


R.T.: 5.243 min
Delta R.T.: 0.007 min
Response: 1117568
Conc: 0.03 ng/ml

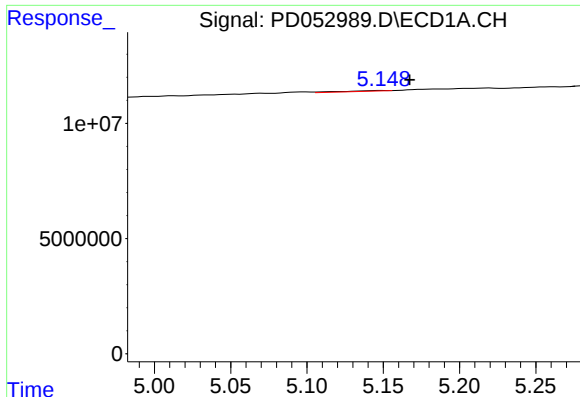

#9 Endosulfan I


R.T.: 5.150 min
Delta R.T.: -0.017 min
Response: 597895
Conc: 0.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

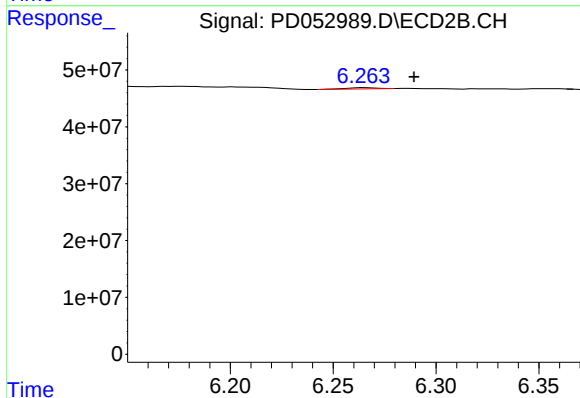


#9 Endosulfan I

R.T.: 6.265 min
Delta R.T.: -0.024 min
Response: 2113734
Conc: 0.07 ng/ml

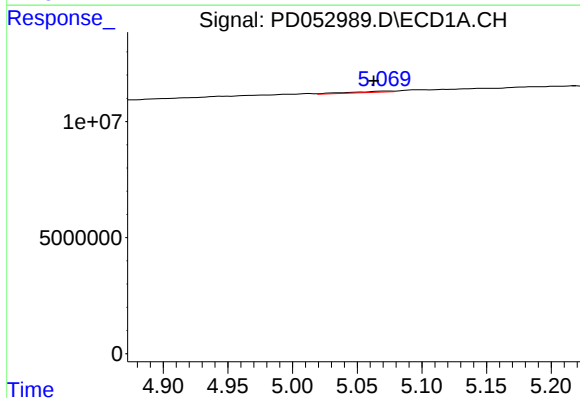


#10 gamma-Chlordane

R.T.: 5.072 min
Delta R.T.: 0.009 min
Response: 1131774
Conc: 0.58 ng/ml

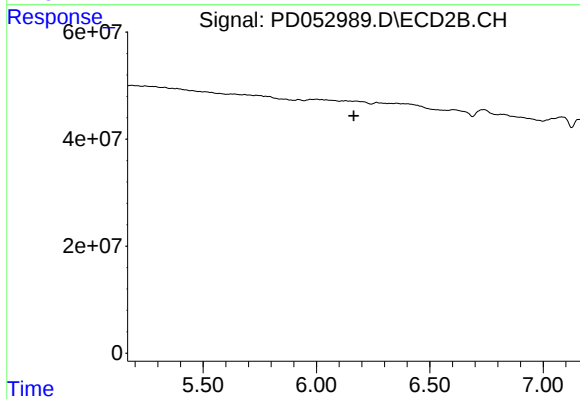

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.165 min
Response: 0
Conc: N.D.

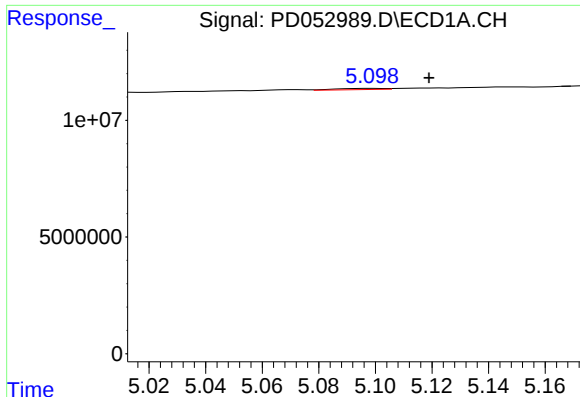

#11 alpha-Chlordane


R.T.: 5.099 min
Delta R.T.: -0.020 min
Response: 640308
Conc: 0.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

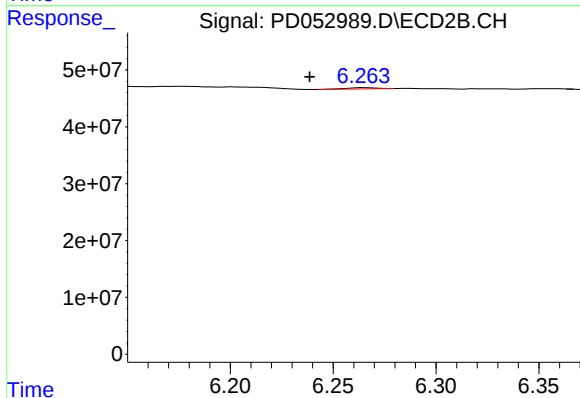


#11 alpha-Chlordane

R.T.: 6.265 min
Delta R.T.: 0.026 min
Response: 2113734
Conc: 0.07 ng/ml

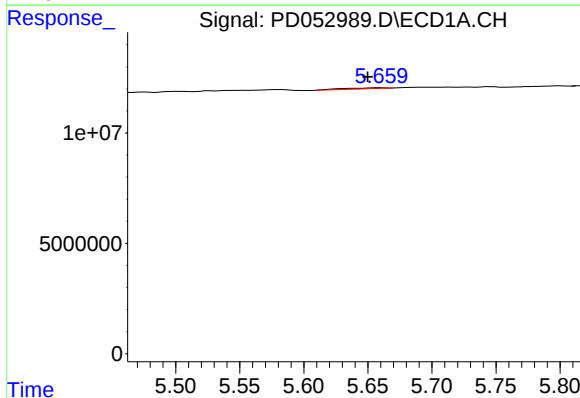


#14 Endrin

R.T.: 5.660 min
Delta R.T.: 0.010 min
Response: 993112
Conc: 0.54 ng/ml

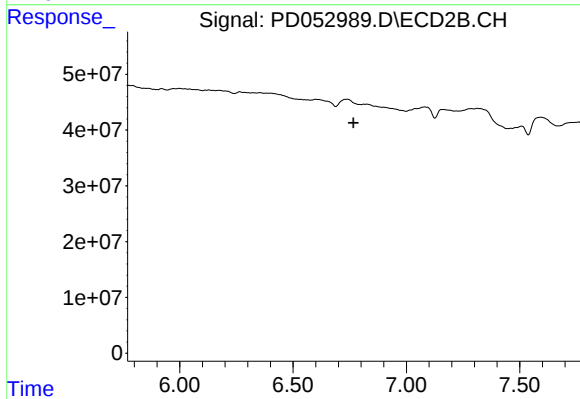

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.767 min
Response: 0
Conc: N.D.

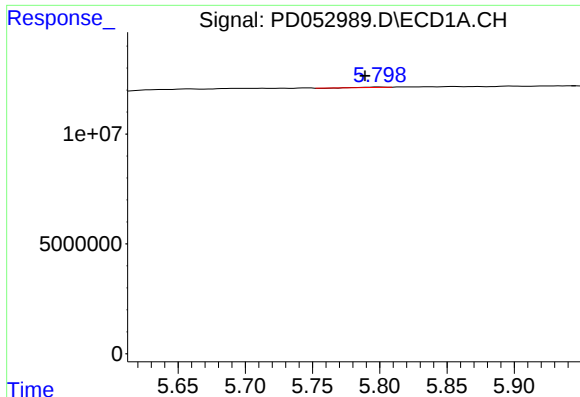

#16 4,4'-DDD


R.T.: 5.800 min
Delta R.T.: 0.011 min
Response: 54451
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

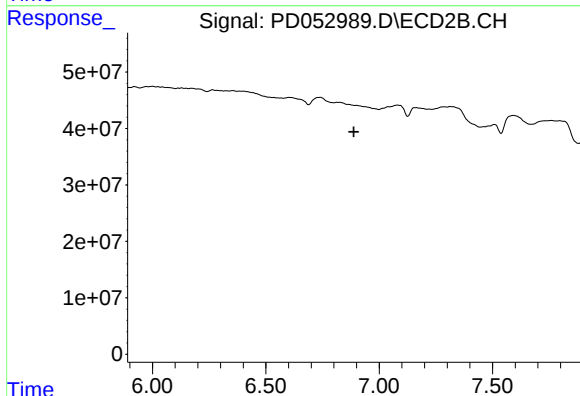


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.888 min
Response: 0
Conc: N.D.

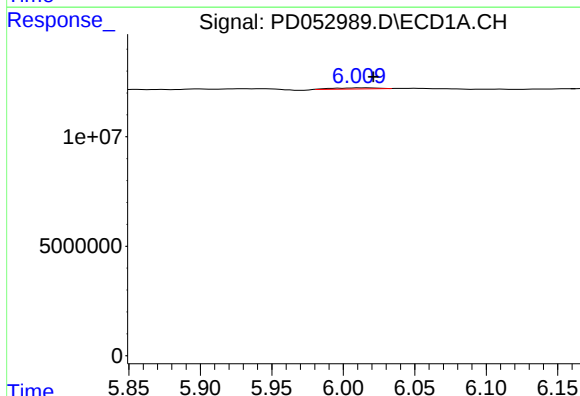


#17 4,4'-DDT

R.T.: 6.012 min
Delta R.T.: -0.009 min
Response: 1018457
Conc: 0.71 ng/ml

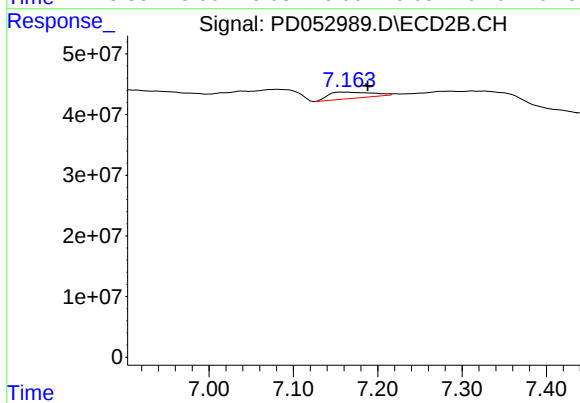

#17 4,4'-DDT


R.T.: 7.164 min
Delta R.T.: -0.024 min
Response: 37385996
Conc: 2.01 ng/ml

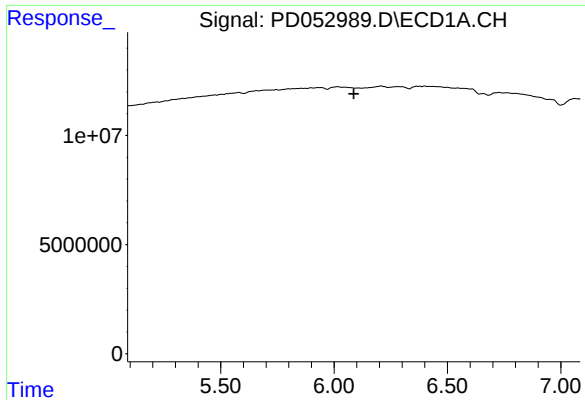

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

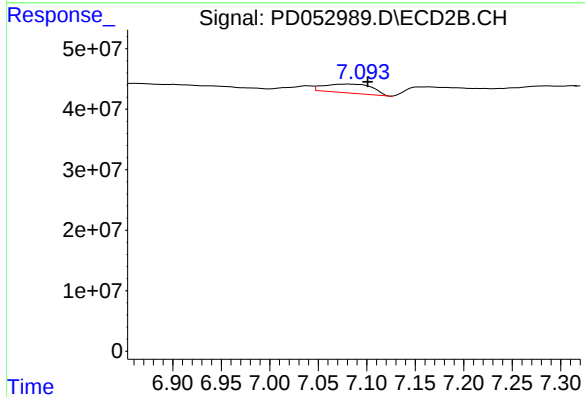


#18 Endrin aldehyde

R.T.: 7.081 min
Delta R.T.: -0.020 min
Response: 51301331
Conc: 2.49 ng/ml

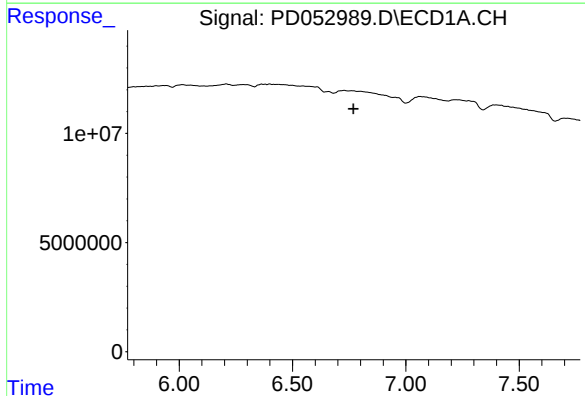


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.770 min
Response: 0
Conc: N.D.

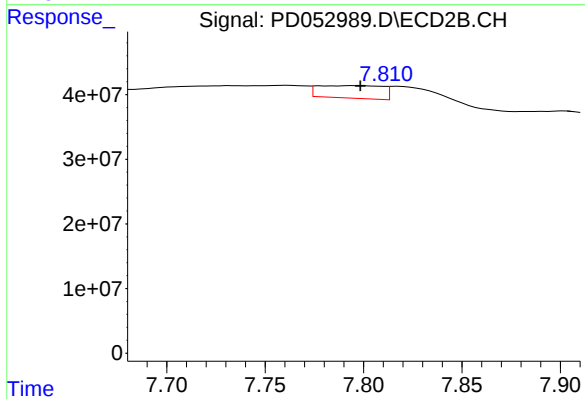

#21 Endrin ketone


R.T.: 7.796 min
Delta R.T.: -0.002 min
Response: 44059519
Conc: 2.15 ng/ml

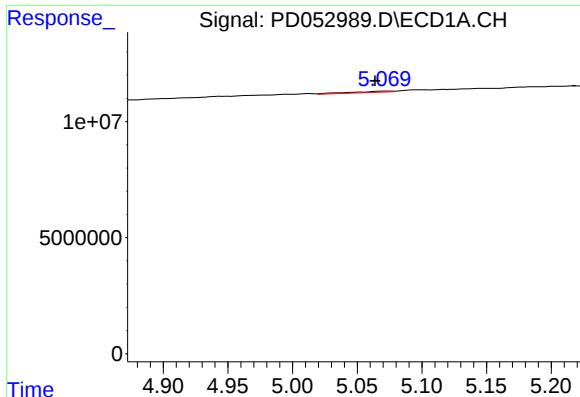

#25 Chlordane-3


R.T.: 5.072 min
Delta R.T.: 0.008 min
Response: 1131774
Conc: 5.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

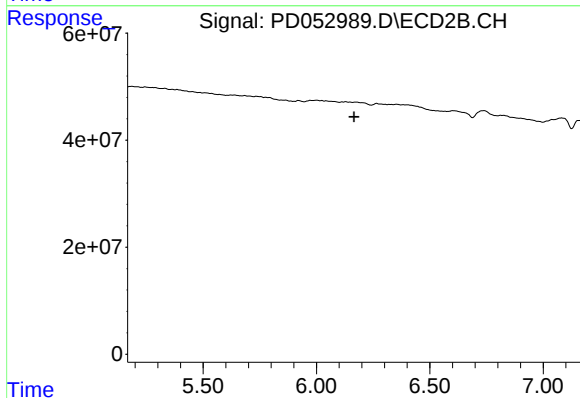


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.166 min
Response: 0
Conc: N.D.

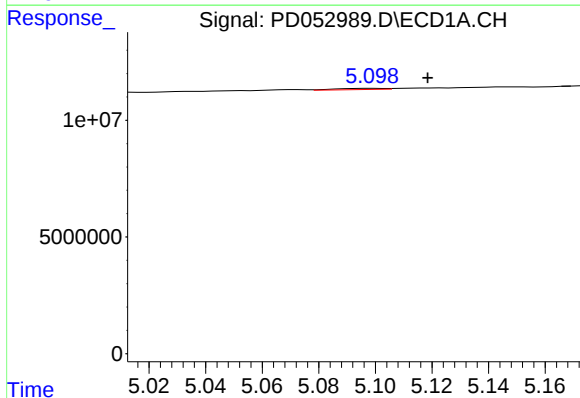

#26 Chlordane-4

R.T.: 5.099 min
Delta R.T.: -0.019 min
Response: 640308
Conc: 3.02 ng/ml

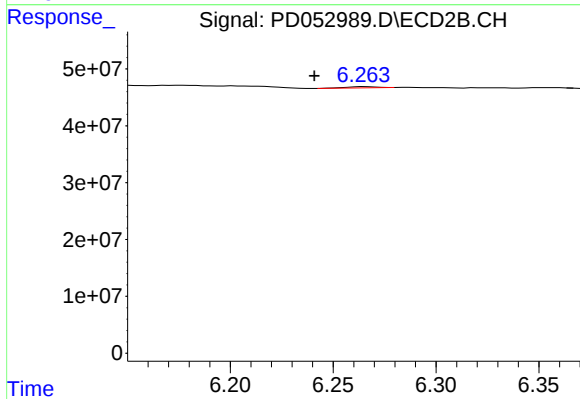

#26 Chlordane-4

R.T.: 6.265 min
Delta R.T.: 0.024 min
Response: 2113734
Conc: 0.42 ng/ml

