

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
 Data File : PD052990.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2019 8:20
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:26:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.222	4.041	24940782	532.6E6	17.873	18.375
28)	SA Decachlor...	7.819	9.163	24176469	238.3E6	18.140	15.326
Target Compounds							
5)	MB Aldrin	0.000	5.529	0	12349877	N.D.	0.334 #
12)	B 4,4'-DDE	0.000	6.409	0	23683441	N.D.	0.776 #
14)	MA Endrin	0.000	6.777	0	36421907	N.D.	1.453 #
15)	B Endosulfa...	0.000	6.982	0	559411	N.D.	0.022 #
17)	MA 4,4'-DDT	0.000	7.187	0	7336159	N.D.	0.394 #
19)	B Endosulfa...	6.323f	0.000	429900	0	0.280	N.D. #
22)	Mirex	0.000	8.266	0	40920604	N.D.	3.173 #
24)	Chlordane-2	0.000	5.505	0	15299067	N.D.	10.924 #
27)	Chlordane-5	0.000	7.051	0	24236882	N.D.	26.270 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
Data File : PD052990.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2019 8:20
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:26:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

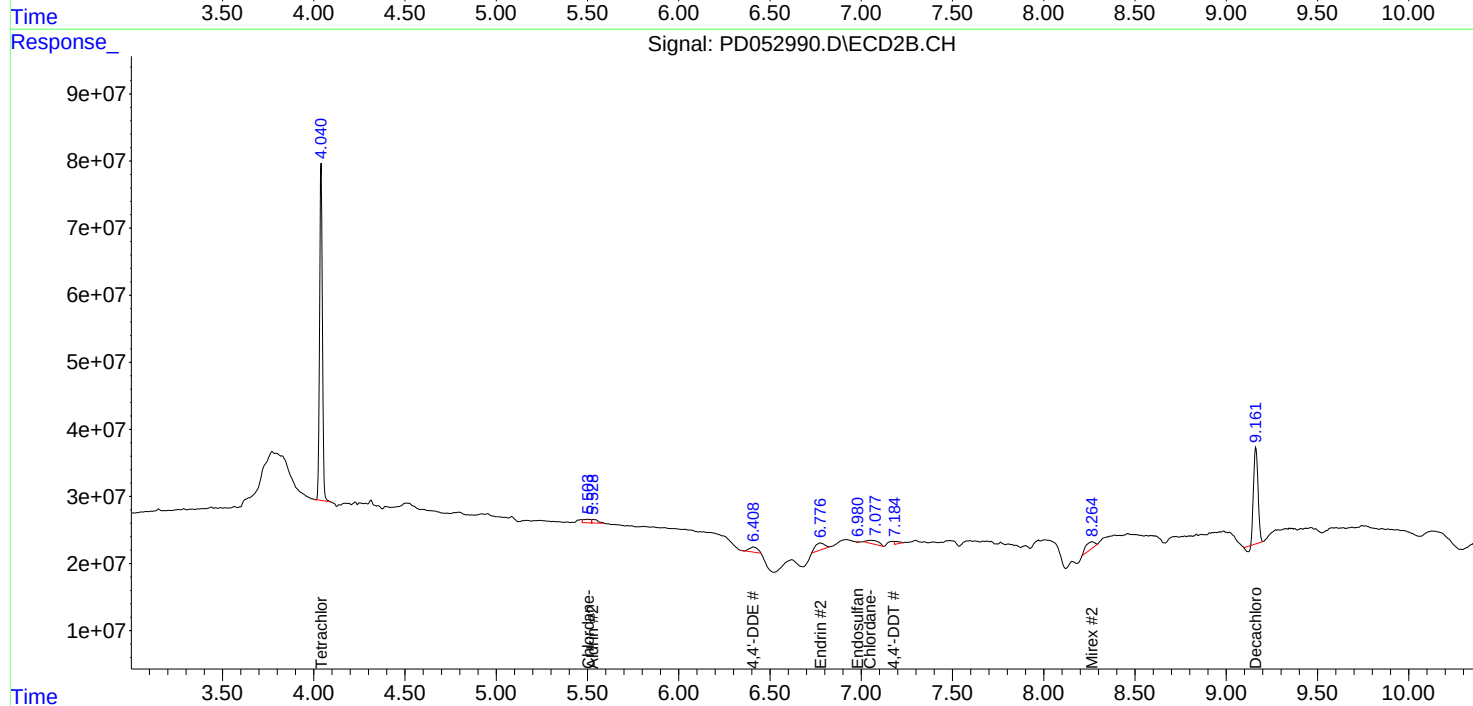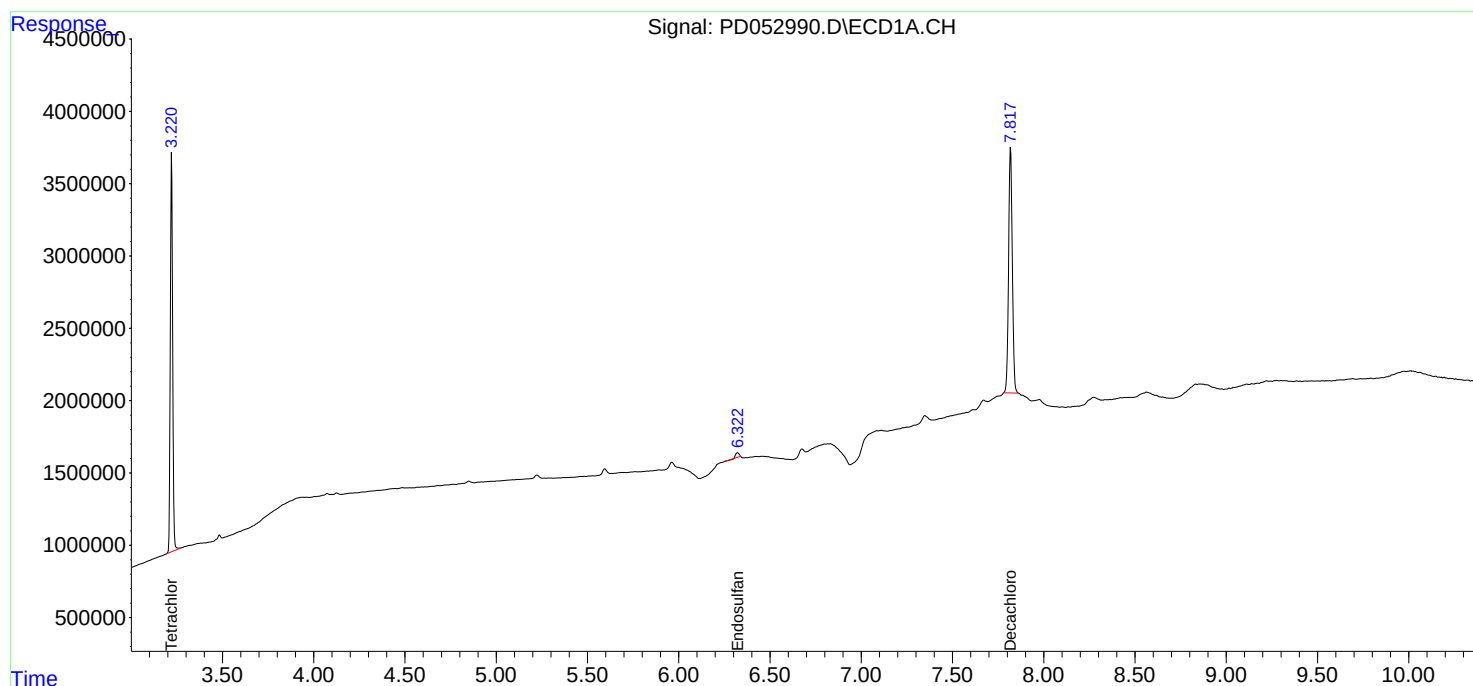


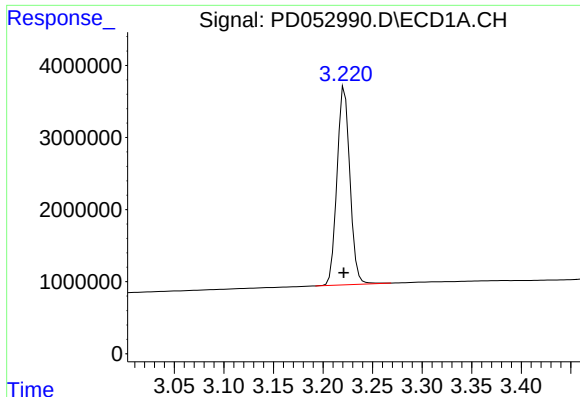

#1 Tetrachloro-m-xylene


R.T.: 3.222 min
Delta R.T.: 0.000 min
Response: 24940782
Conc: 17.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

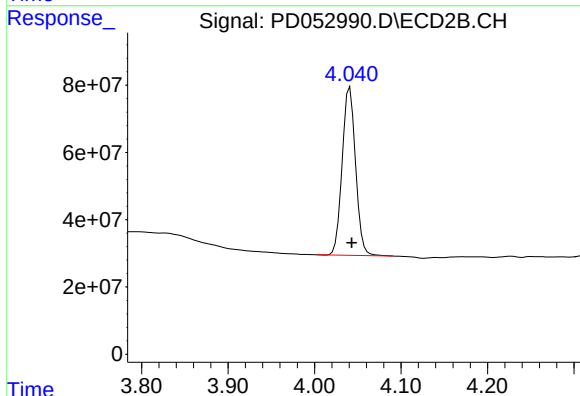


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 532589325
Conc: 18.38 ng/ml

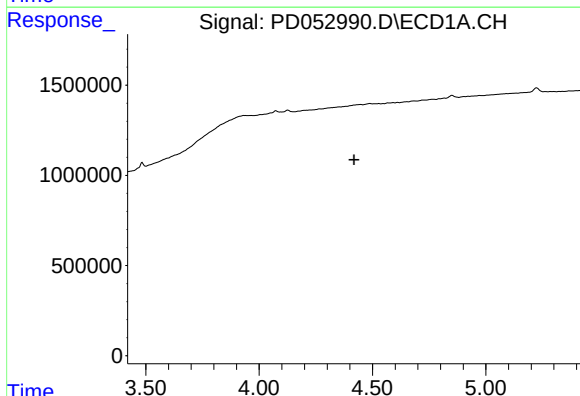


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.418 min
Response: 0
Conc: N.D.

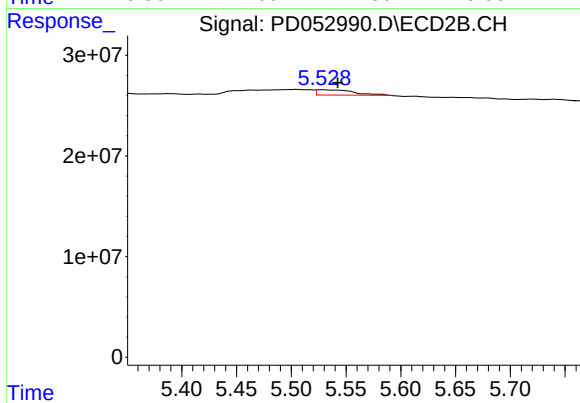

#5 Aldrin


R.T.: 5.529 min
Delta R.T.: -0.013 min
Response: 12349877
Conc: 0.33 ng/ml

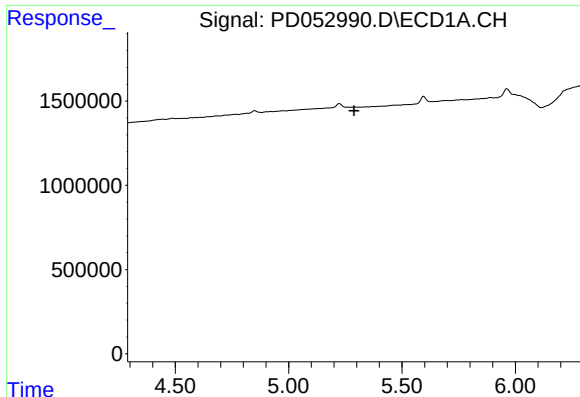

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.288 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

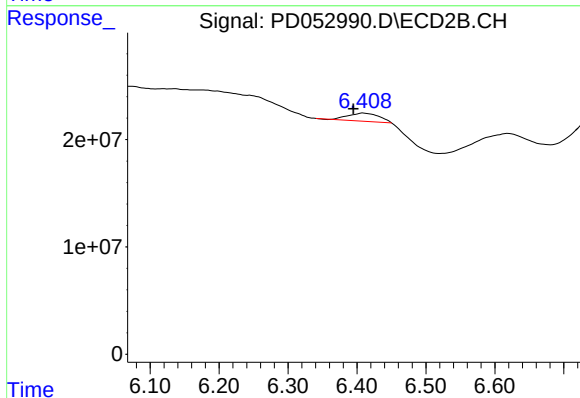


#12 4,4'-DDE

R.T.: 6.409 min
Delta R.T.: 0.014 min
Response: 23683441
Conc: 0.78 ng/ml

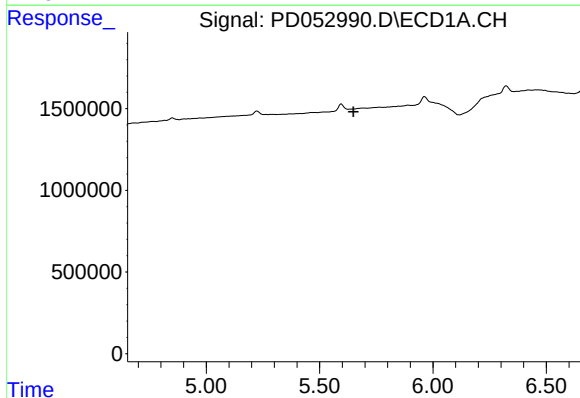


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.650 min
Response: 0
Conc: N.D.

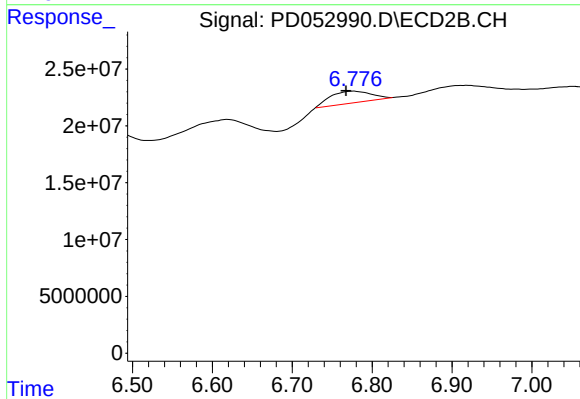

#14 Endrin


R.T.: 6.777 min
Delta R.T.: 0.009 min
Response: 36421907
Conc: 1.45 ng/ml

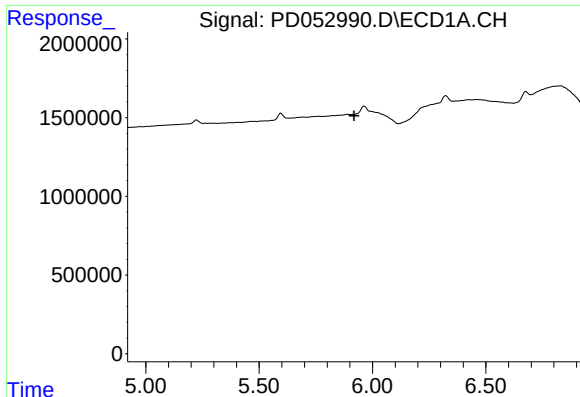

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

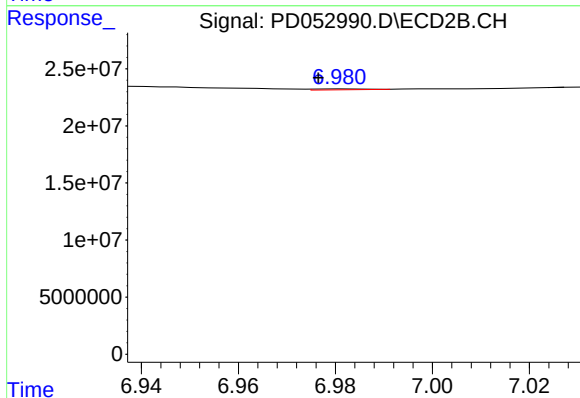


#15 Endosulfan II

R.T.: 6.982 min
Delta R.T.: 0.005 min
Response: 559411
Conc: 0.02 ng/ml

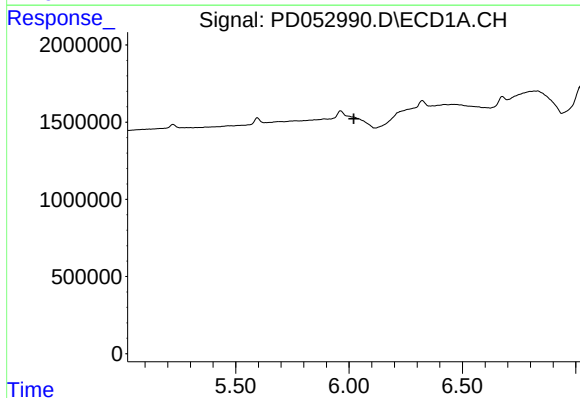


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

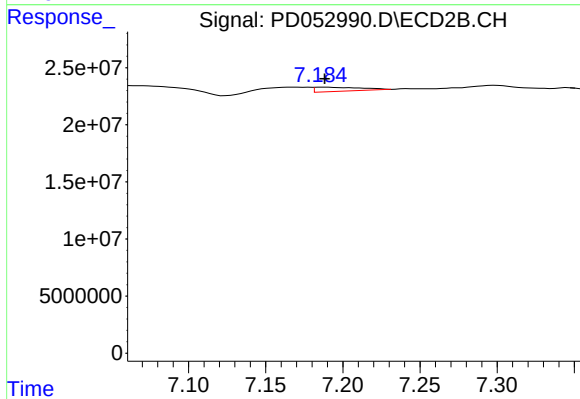

#17 4,4'-DDT


R.T.: 7.187 min
Delta R.T.: -0.002 min
Response: 7336159
Conc: 0.39 ng/ml

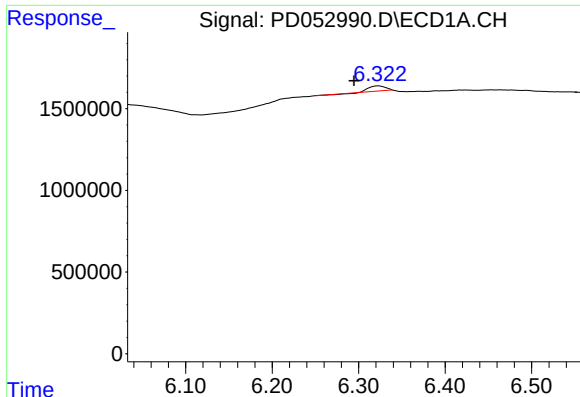

#19 Endosulfan Sulfate


R.T.: 6.323 min
Delta R.T.: 0.028 min
Response: 429900
Conc: 0.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

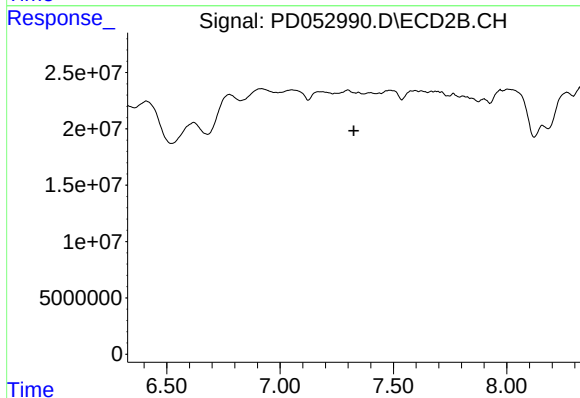


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.326 min
Response: 0
Conc: N.D.

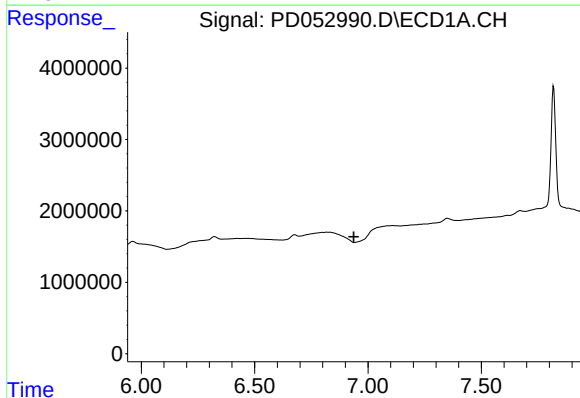


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 6.938 min
Response: 0
Conc: N.D.

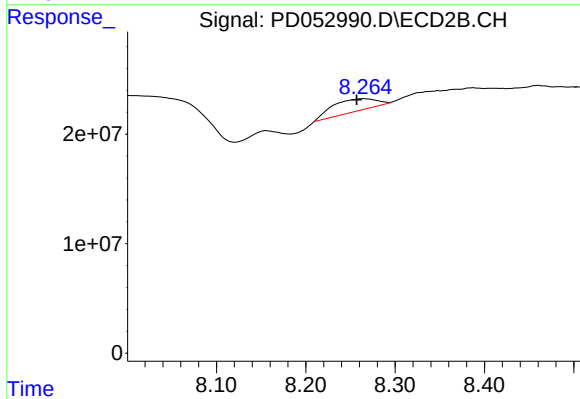

#22 Mirex


R.T.: 8.266 min
Delta R.T.: 0.009 min
Response: 40920604
Conc: 3.17 ng/ml

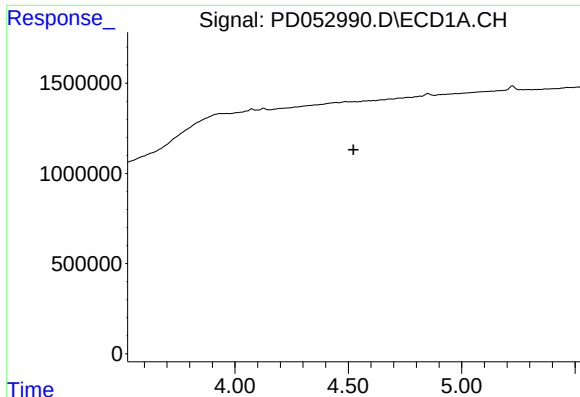

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

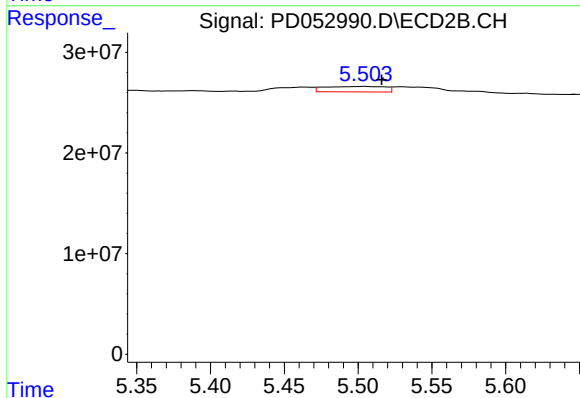


#24 Chlordane-2

R.T.: 5.505 min
Delta R.T.: -0.011 min
Response: 15299067
Conc: 10.92 ng/ml

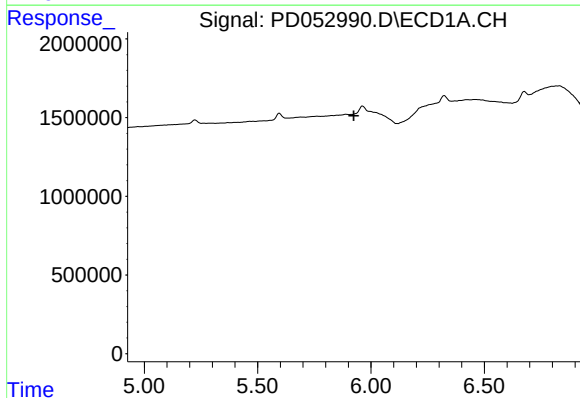


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 5.924 min
Response: 0
Conc: N.D.

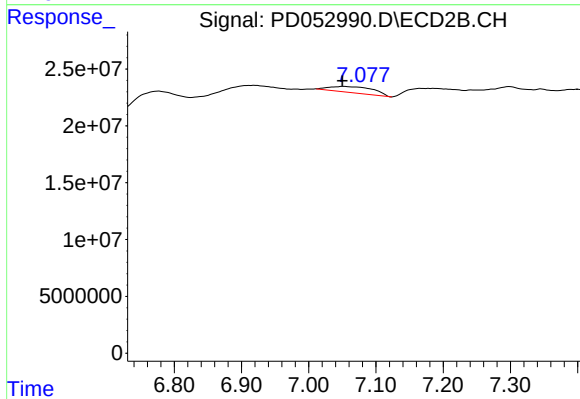

#27 Chlordane-5


R.T.: 7.051 min
Delta R.T.: 0.001 min
Response: 24236882
Conc: 26.27 ng/ml

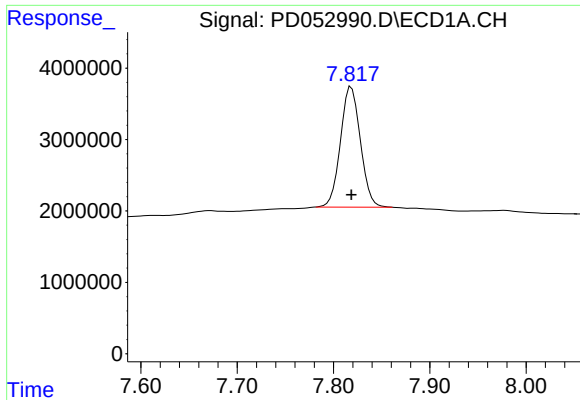

#28 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 24176469
Conc: 18.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

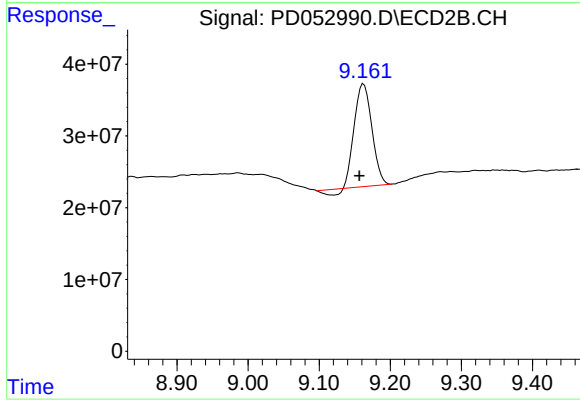

#28 Decachlorobiphenyl

R.T.: 9.163 min
Delta R.T.: 0.006 min
Response: 238334047
Conc: 15.33 ng/ml