

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
 Data File : PD053002.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2019 11:30
 Operator : AJ\SJ
 Sample : K2199-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OR-03-041819-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:29:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.221	4.041	30013133	643.7E6	21.508	22.209
28)	SA Decachlor...	7.818	9.163	20290546	267.2E6	15.224	17.184
Target Compounds							
3)	MA gamma-BHC...	3.914	4.698f	1404163	90584365	0.642	2.252 #
4)	MA Heptachlor	0.000	5.248	0	4699380	N.D.	0.118 #
6)	B beta-BHC	0.000	4.915f	0	31611148	N.D.	1.747 #
10)	B gamma-Chl...	0.000	6.160	0	54156790	N.D.	1.693 #
13)	MA Dieldrin	5.389	6.541	870675	3470775	0.450	0.116 #
14)	MA Endrin	5.670f	0.000	2028010	0	1.101	N.D. #
15)	B Endosulfa...	0.000	6.988	0	32856398	N.D.	1.319 #
25)	Chlordane-3	0.000	6.160	0	54156790	N.D.	12.273 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
Data File : PD053002.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2019 11:30
Operator : AJ\SJ
Sample : K2199-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
OR-03-041819-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:29:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

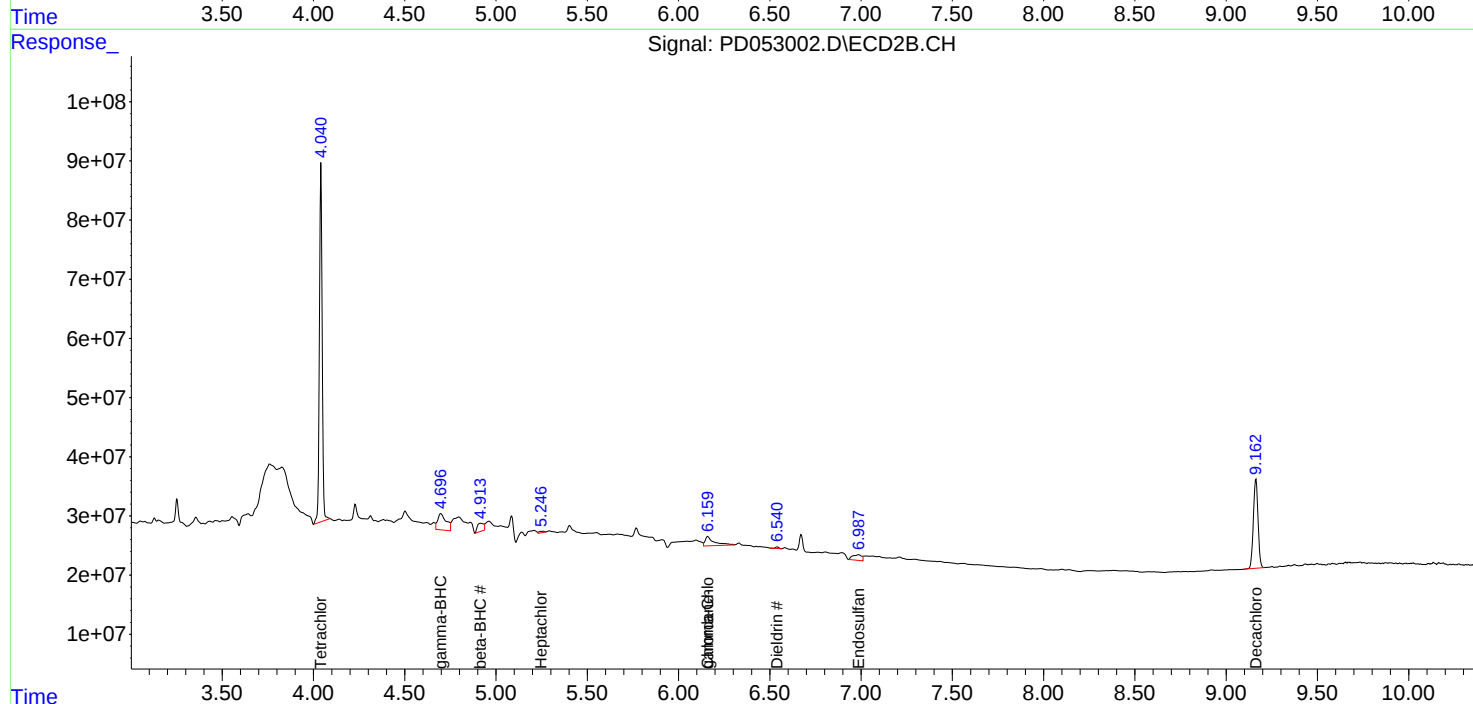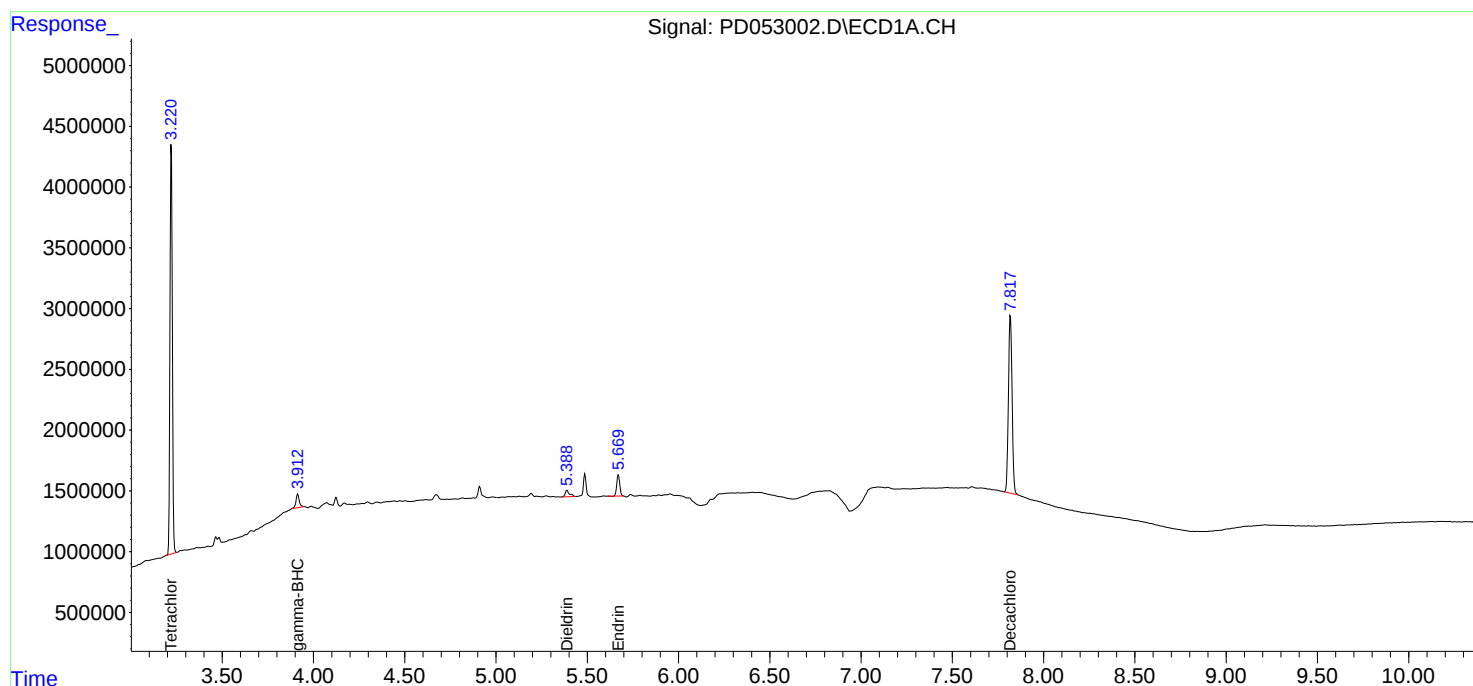


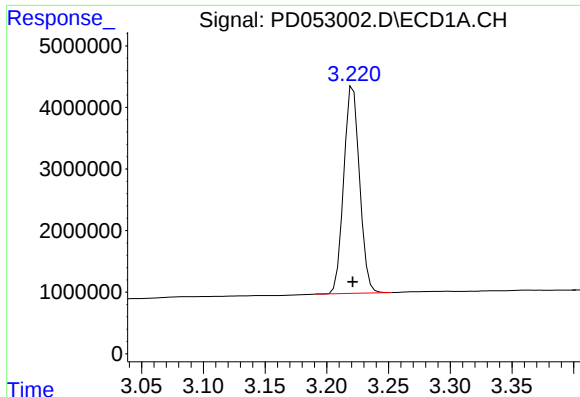

#1 Tetrachloro-m-xylene


R.T.: 3.221 min
Delta R.T.: 0.000 min
Response: 30013133
Conc: 21.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-03-041819-A

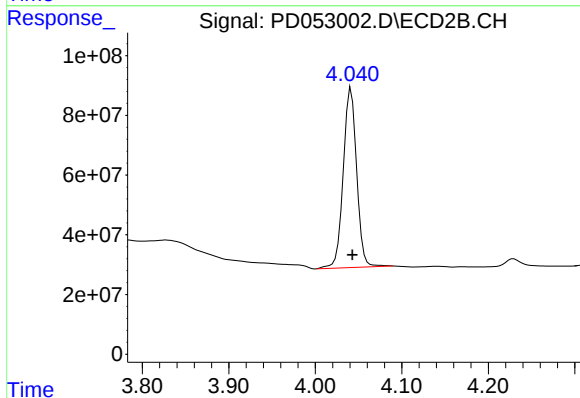


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 643707698
Conc: 22.21 ng/ml

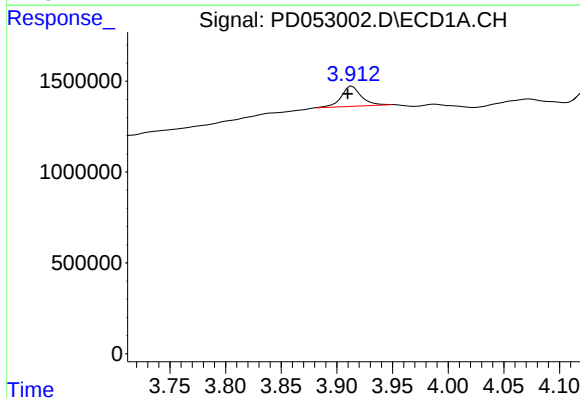


#3 gamma-BHC (Lindane)

R.T.: 3.914 min
Delta R.T.: 0.004 min
Response: 1404163
Conc: 0.64 ng/ml

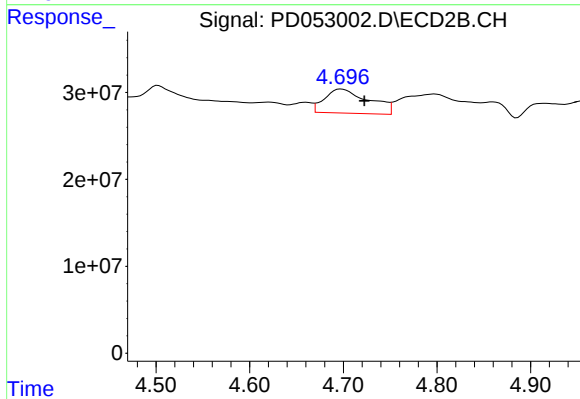

#3 gamma-BHC (Lindane)


R.T.: 4.698 min
Delta R.T.: -0.025 min
Response: 90584365
Conc: 2.25 ng/ml

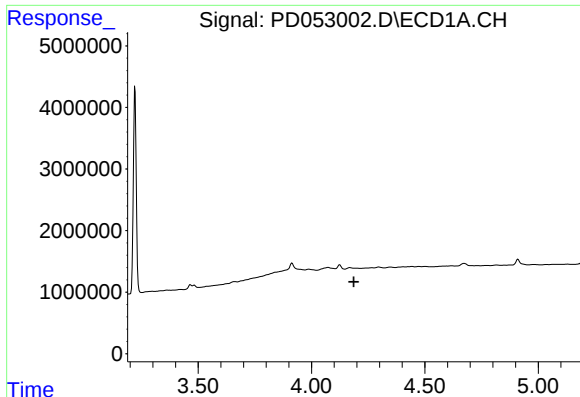

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OR-03-041819-A

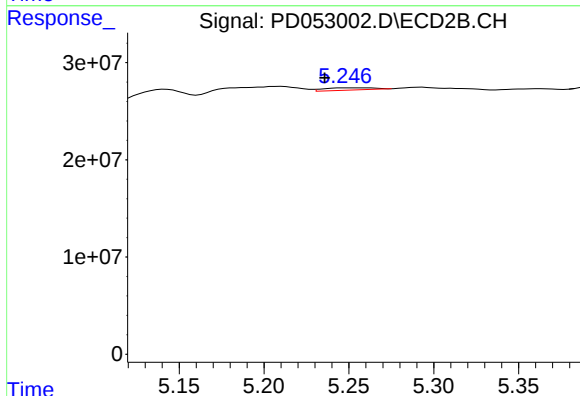


#4 Heptachlor

R.T.: 5.248 min
Delta R.T.: 0.012 min
Response: 4699380
Conc: 0.12 ng/ml

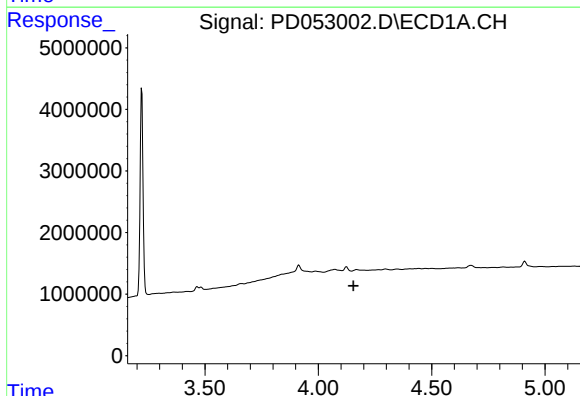


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.156 min
Response: 0
Conc: N.D.

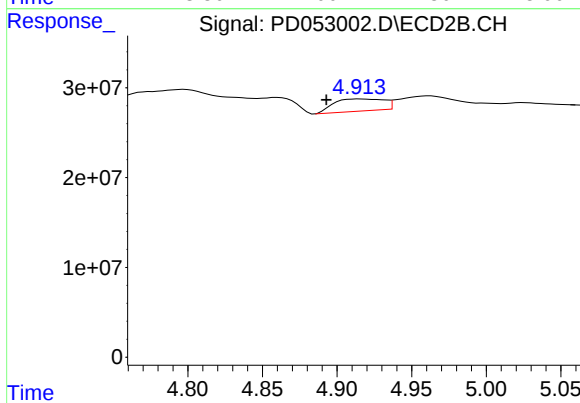

#6 beta-BHC


R.T.: 4.915 min
Delta R.T.: 0.022 min
Response: 31611148
Conc: 1.75 ng/ml

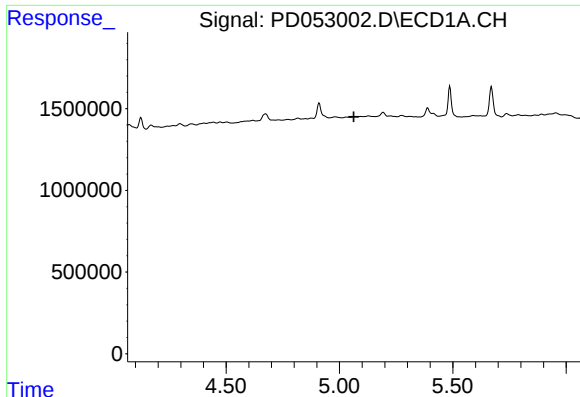

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OR-03-041819-A

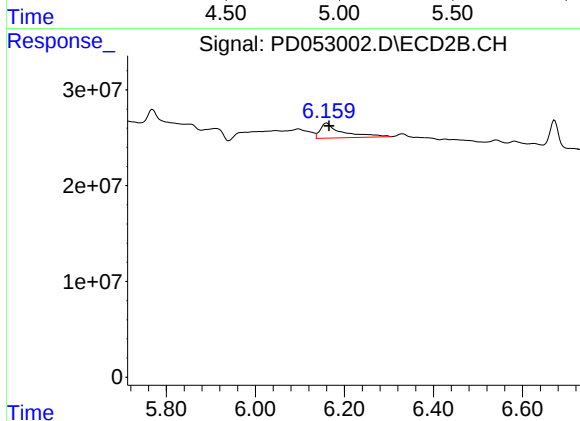


#10 gamma-Chlordane

R.T.: 6.160 min
Delta R.T.: -0.005 min
Response: 54156790
Conc: 1.69 ng/ml

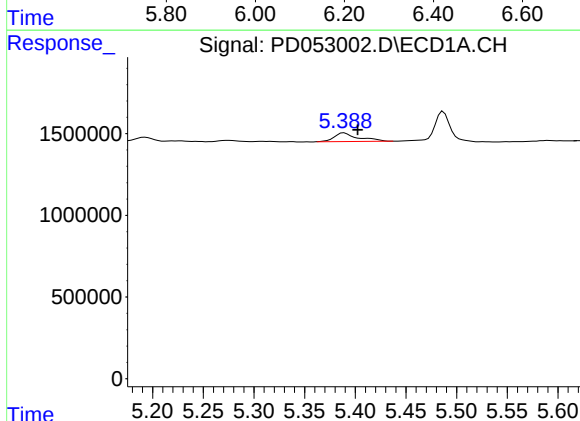


#13 Dieldrin

R.T.: 5.389 min
Delta R.T.: -0.013 min
Response: 870675
Conc: 0.45 ng/ml

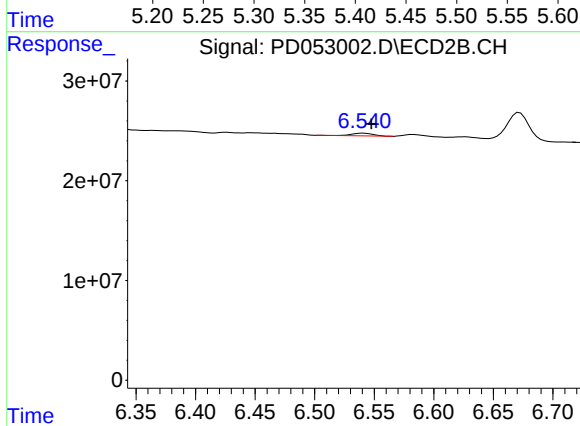

#13 Dieldrin


R.T.: 6.541 min
Delta R.T.: -0.007 min
Response: 3470775
Conc: 0.12 ng/ml

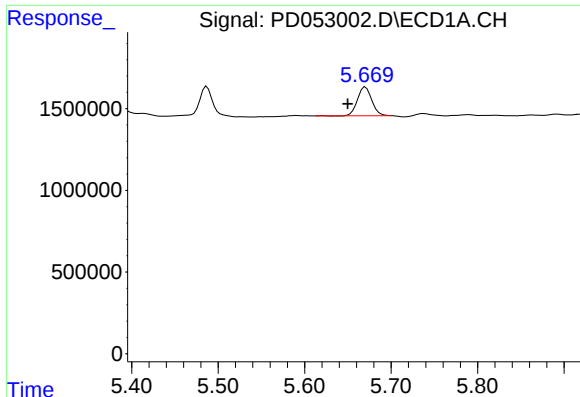

#14 Endrin


R.T.: 5.670 min
Delta R.T.: 0.021 min
Response: 2028010
Conc: 1.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-03-041819-A

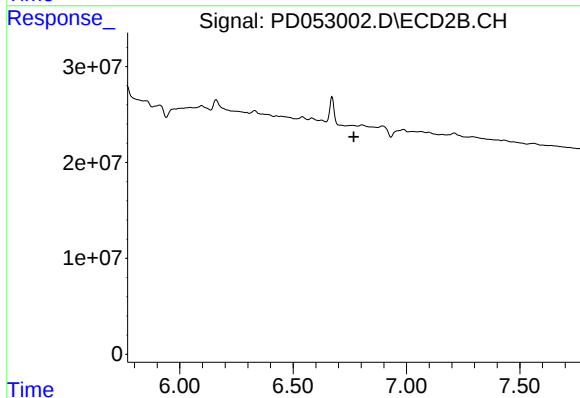


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.767 min
Response: 0
Conc: N.D.

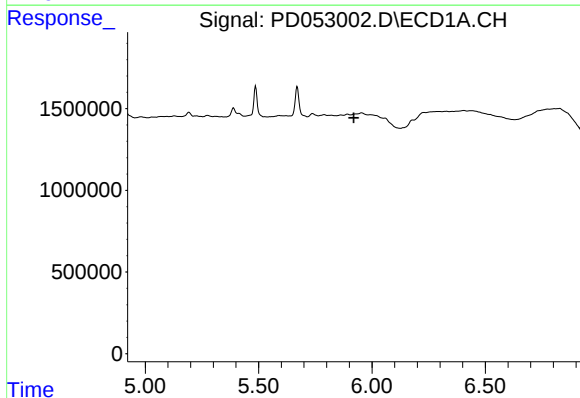


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.919 min
Response: 0
Conc: N.D.

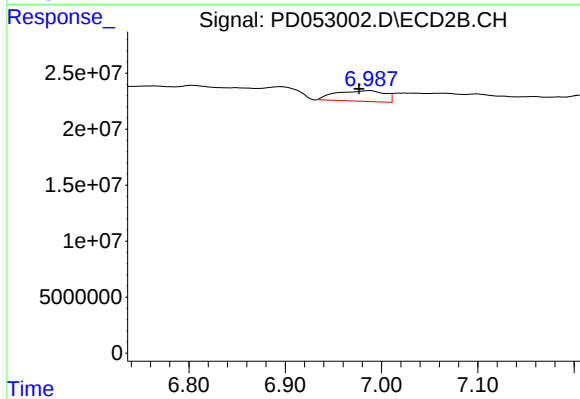

#15 Endosulfan II


R.T.: 6.988 min
Delta R.T.: 0.011 min
Response: 32856398
Conc: 1.32 ng/ml

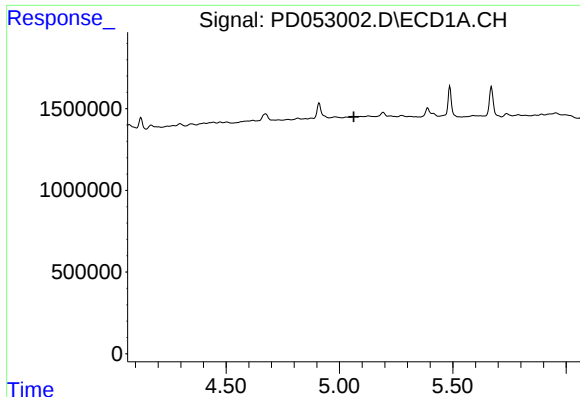

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OR-03-041819-A

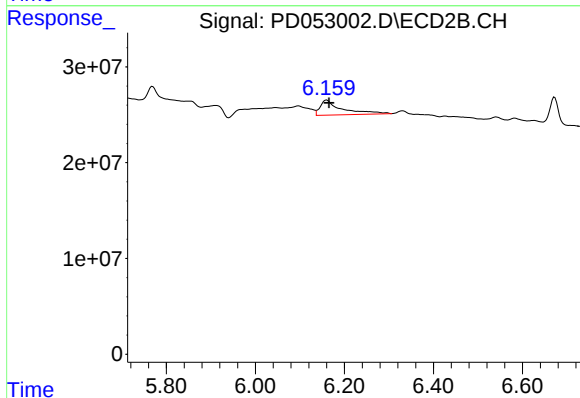


#25 Chlordane-3

R.T.: 6.160 min
Delta R.T.: -0.006 min
Response: 54156790
Conc: 12.27 ng/ml

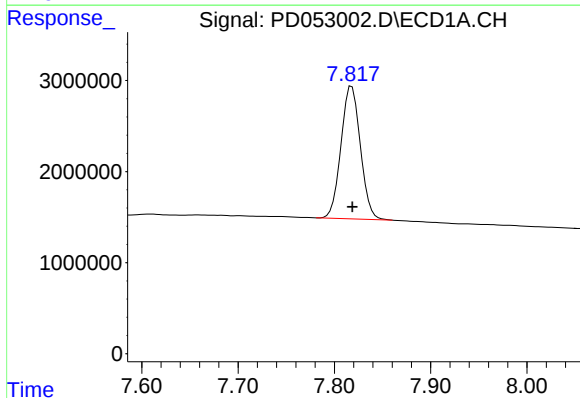

#28 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 20290546
Conc: 15.22 ng/ml

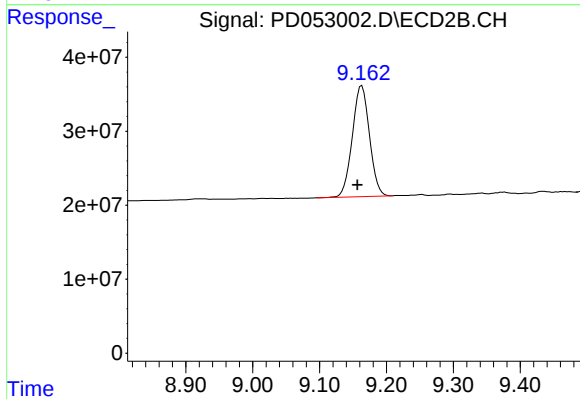

#28 Decachlorobiphenyl

R.T.: 9.163 min
Delta R.T.: 0.007 min
Response: 267239326
Conc: 17.18 ng/ml