

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
 Data File : PD053028.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2019 17:44
 Operator : AJ\SJ
 Sample : K2515-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:34:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.041	30148215	616.8E6	21.605	21.279
28)	SA Decachlor...	7.814	9.160	28493755	375.4E6	21.380	24.139
Target Compounds							
3)	MA gamma-BHC...	3.916	0.000	854203	0	0.391	N.D. #
4)	MA Heptachlor	0.000	5.240	0	5880046	N.D.	0.148 #
10)	B gamma-Chl...	0.000	6.179	0	4920476	N.D.	0.154 #
14)	MA Endrin	5.668f	0.000	987304	0	0.536	N.D. #
15)	B Endosulfa...	0.000	6.986	0	28076134	N.D.	1.127 #
24)	Chlordane-2	0.000	5.501f	0	3659306	N.D.	2.613 #
25)	Chlordane-3	0.000	6.179	0	4920476	N.D.	1.115 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
Data File : PD053028.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2019 17:44
Operator : AJ\SJ
Sample : K2515-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:34:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

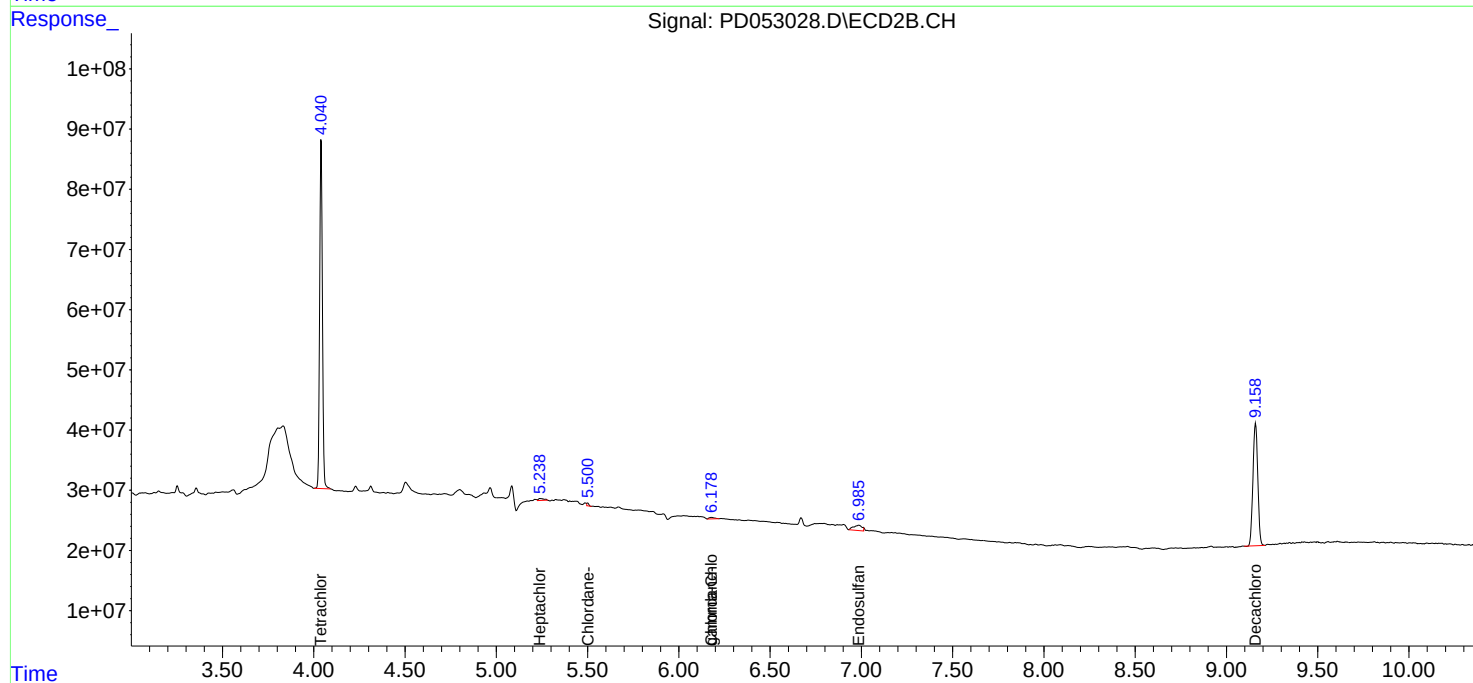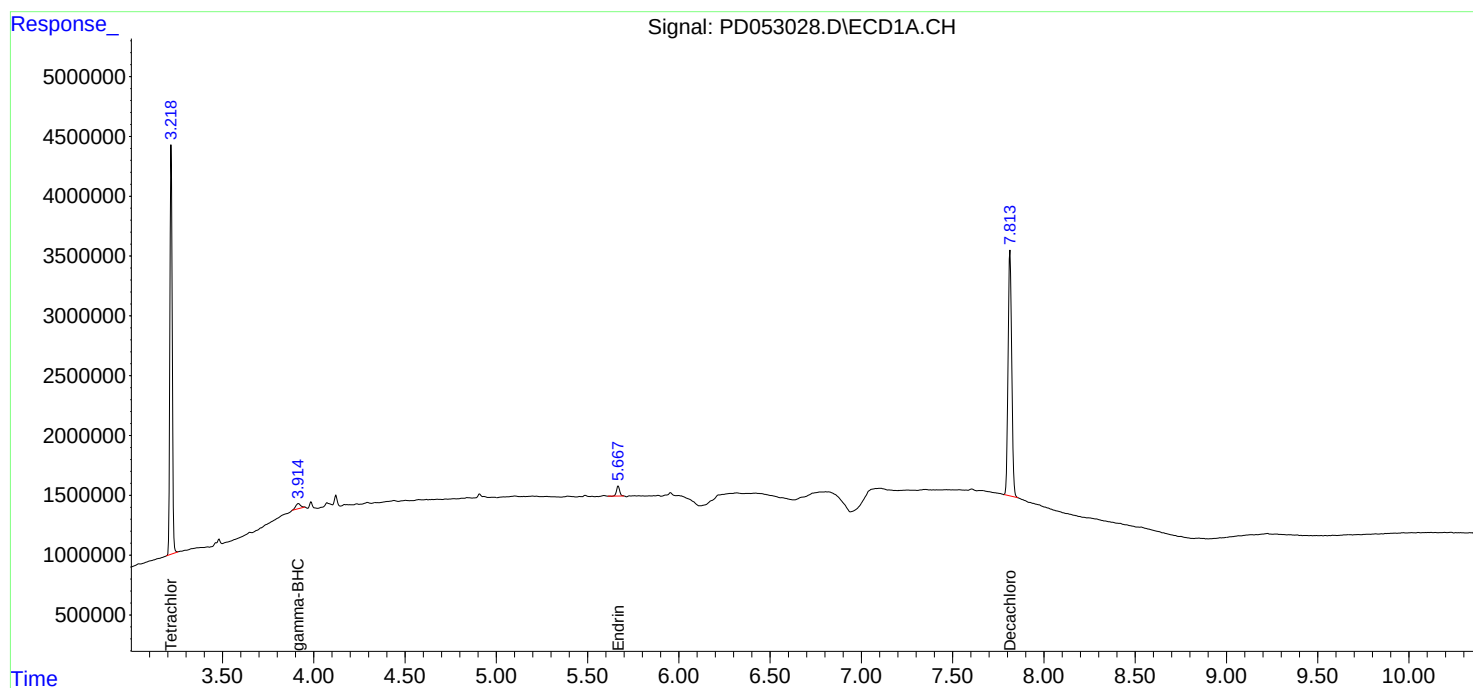


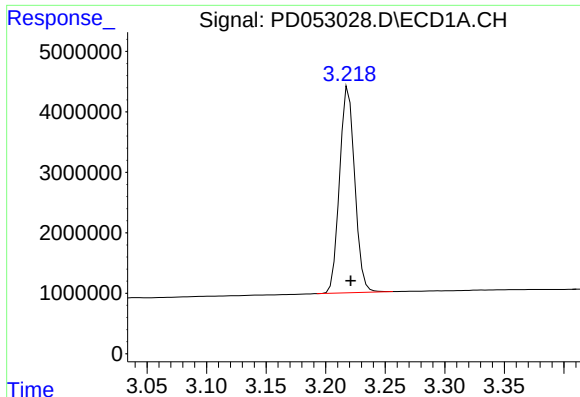

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: -0.002 min
Response: 30148215
Conc: 21.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-15

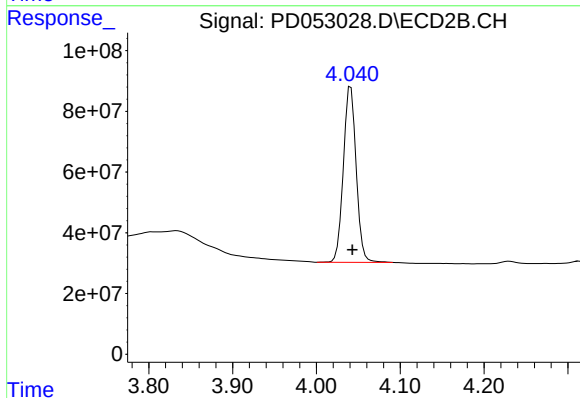


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 616761909
Conc: 21.28 ng/ml

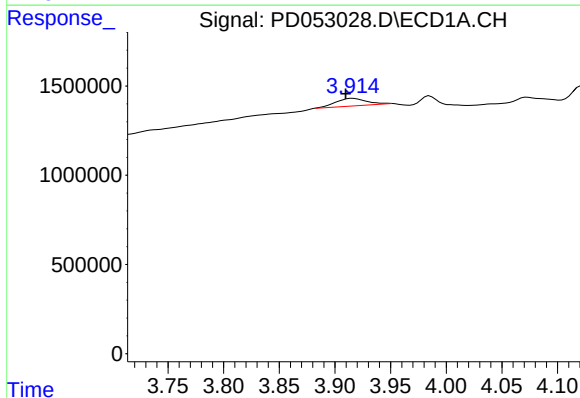


#3 gamma-BHC (Lindane)

R.T.: 3.916 min
Delta R.T.: 0.007 min
Response: 854203
Conc: 0.39 ng/ml

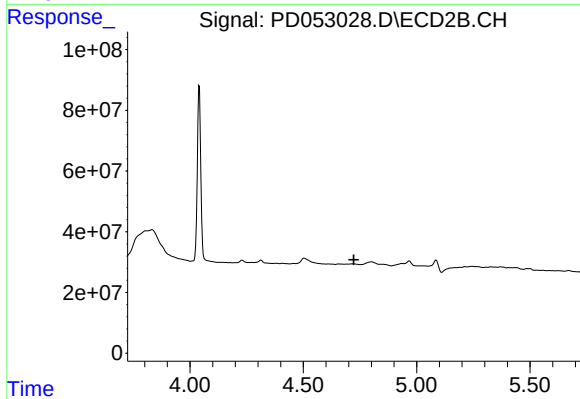

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.723 min
Response: 0
Conc: N.D.

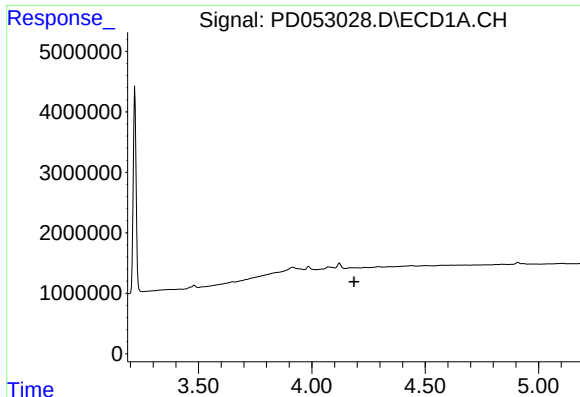

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-15

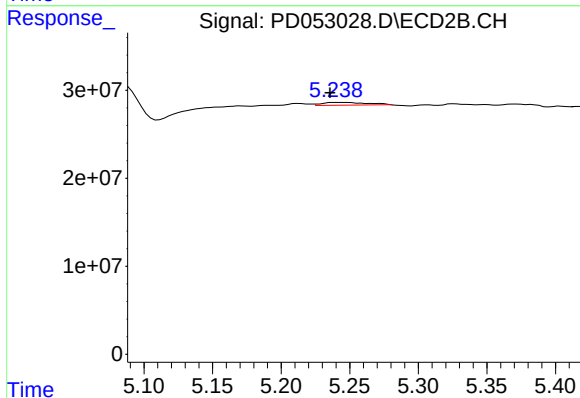


#4 Heptachlor

R.T.: 5.240 min
Delta R.T.: 0.004 min
Response: 5880046
Conc: 0.15 ng/ml

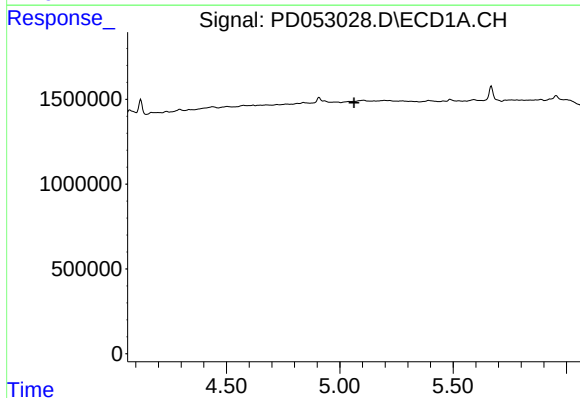


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

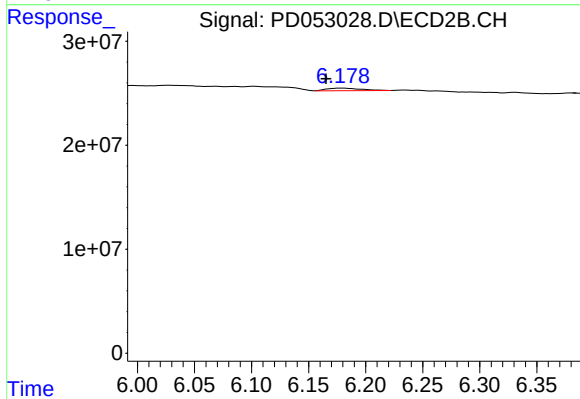

#10 gamma-Chlordane


R.T.: 6.179 min
Delta R.T.: 0.014 min
Response: 4920476
Conc: 0.15 ng/ml

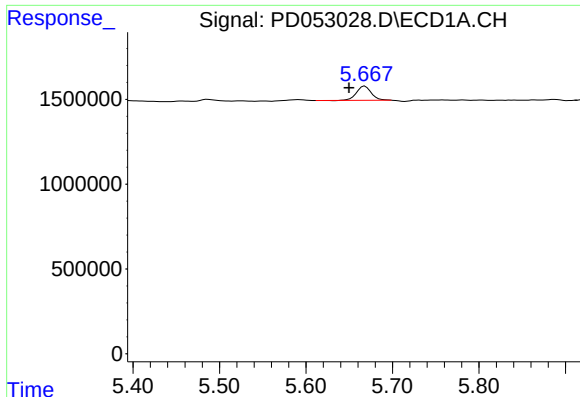

#14 Endrin


R.T.: 5.668 min
Delta R.T.: 0.018 min
Response: 987304
Conc: 0.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-15

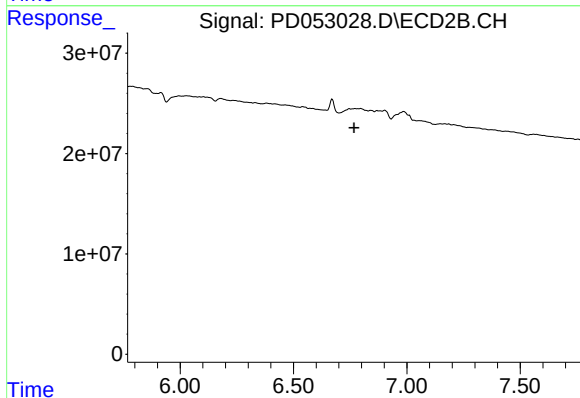


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.767 min
Response: 0
Conc: N.D.

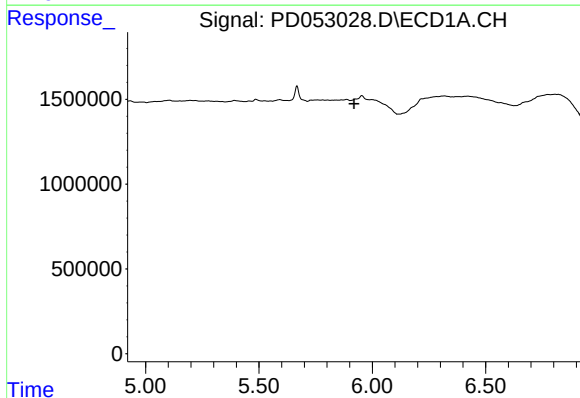


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.919 min
Response: 0
Conc: N.D.

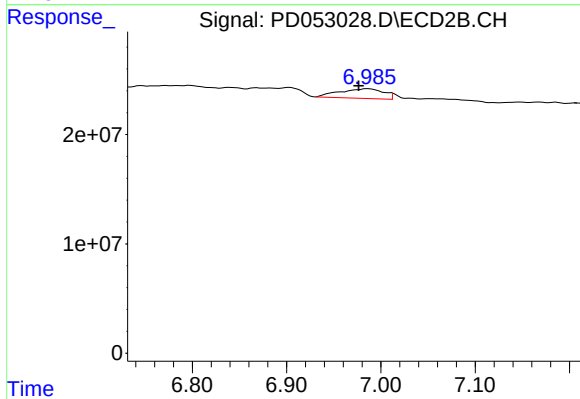

#15 Endosulfan II


R.T.: 6.986 min
Delta R.T.: 0.010 min
Response: 28076134
Conc: 1.13 ng/ml

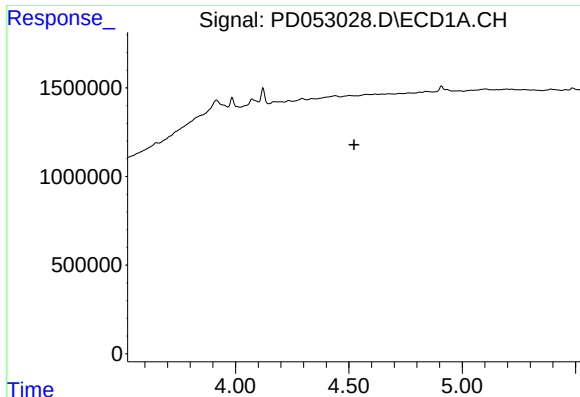

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
TP-15

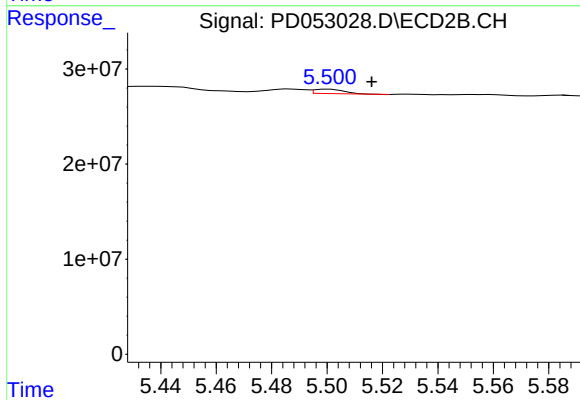


#24 Chlordane-2

R.T.: 5.501 min
Delta R.T.: -0.015 min
Response: 3659306
Conc: 2.61 ng/ml

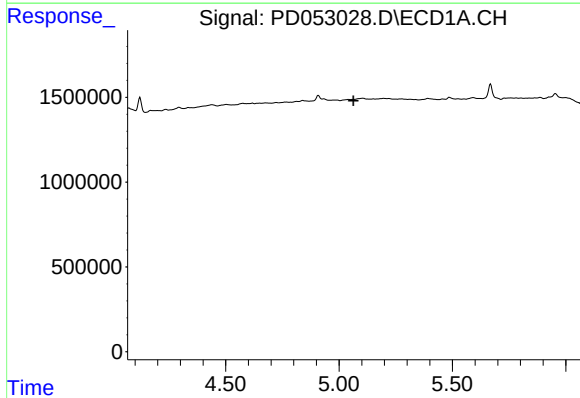


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

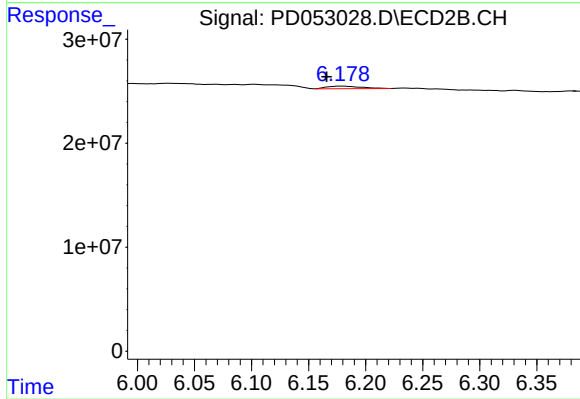

#25 Chlordane-3


R.T.: 6.179 min
Delta R.T.: 0.013 min
Response: 4920476
Conc: 1.12 ng/ml

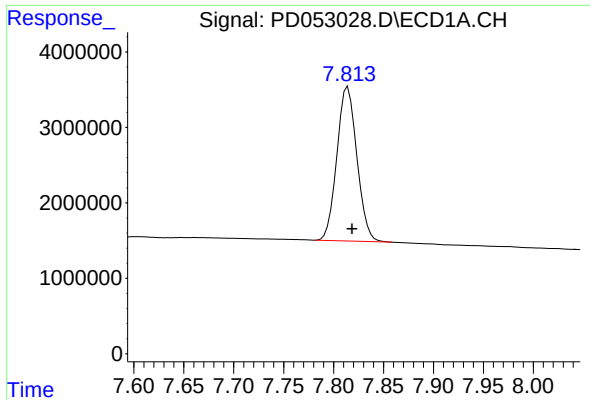

#28 Decachlorobiphenyl

R.T.: 7.814 min
Delta R.T.: -0.004 min
Response: 28493755
Conc: 21.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-15

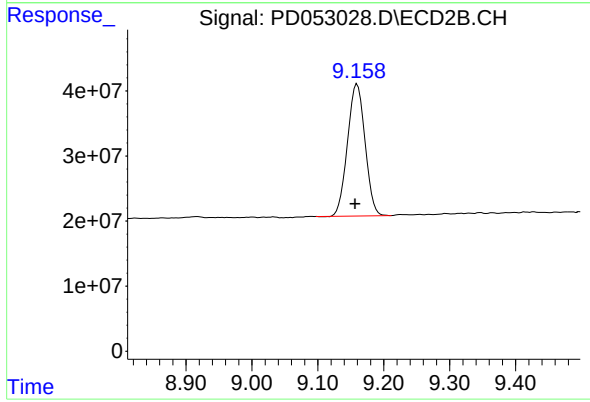

#28 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: 0.003 min
Response: 375391811
Conc: 24.14 ng/ml