

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
 Data File : PD053018.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2019 15:23
 Operator : AJ\SJ
 Sample : K2475-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-TRACK-74-75

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:32:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.040	30588210	629.1E6	21.920	21.704
28)	SA Decachlor...	7.815	9.159	23348567	317.2E6	17.519	20.399

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042219\
Data File : PD053018.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2019 15:23
Operator : AJ\SJ
Sample : K2475-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-TRACK-74-75

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:32:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

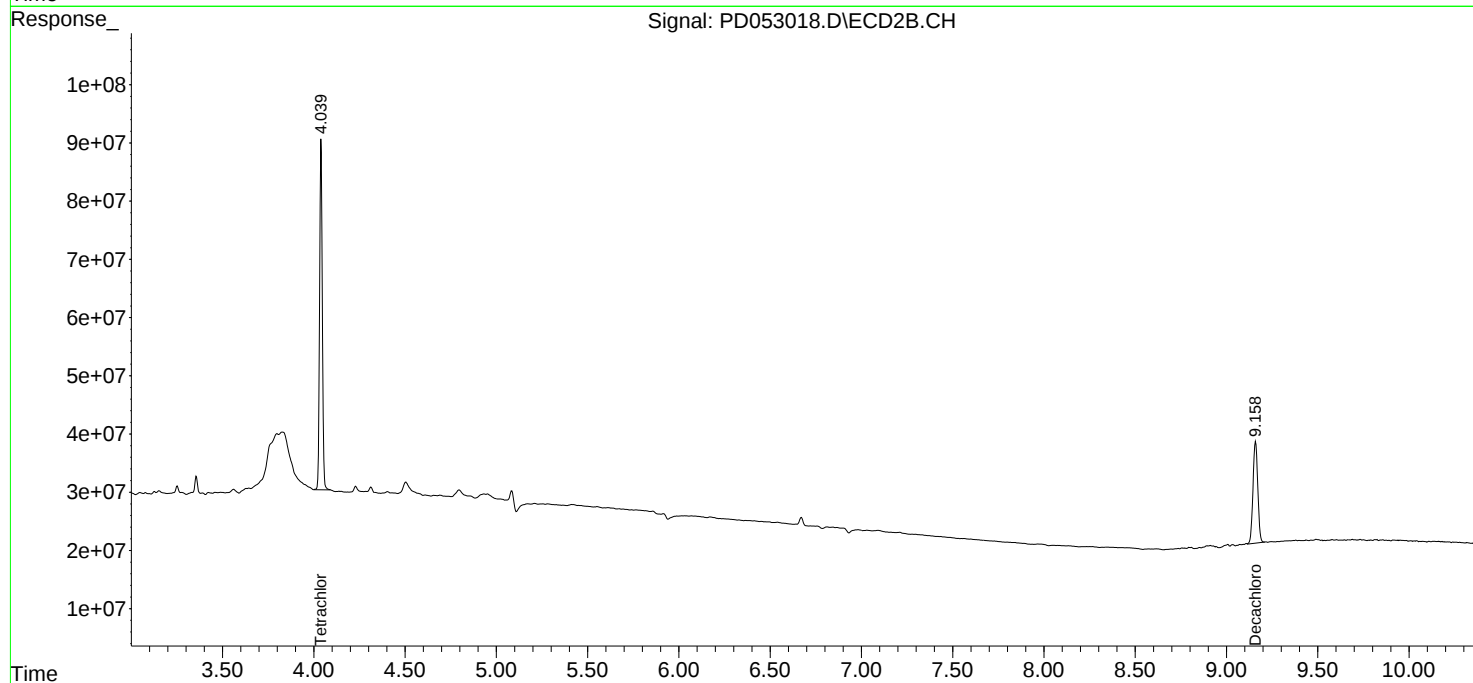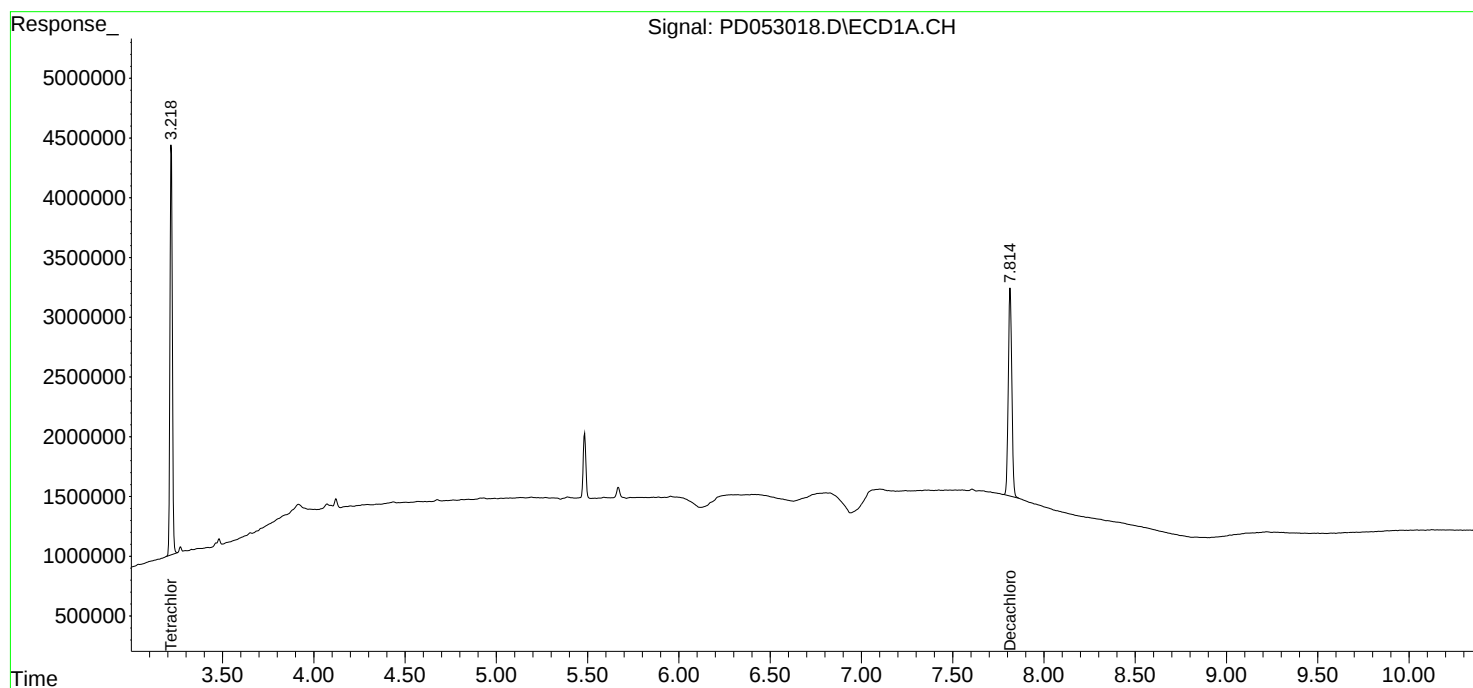


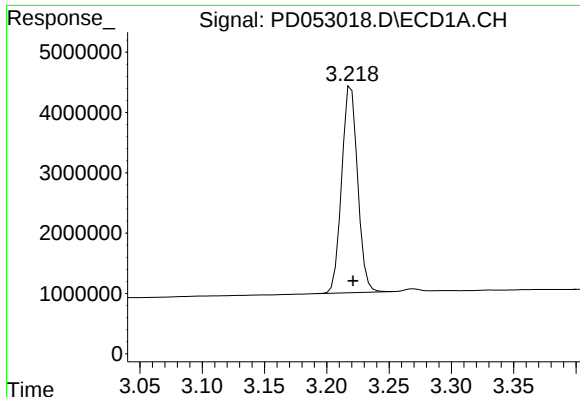

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: -0.001 min
Response: 30588210
Conc: 21.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-TRACK-74-75

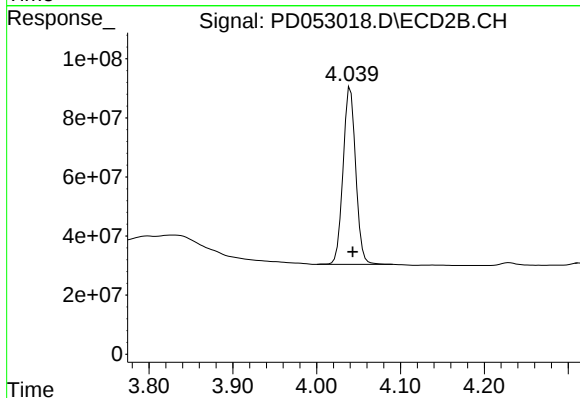


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: -0.003 min
Response: 629058795
Conc: 21.70 ng/ml

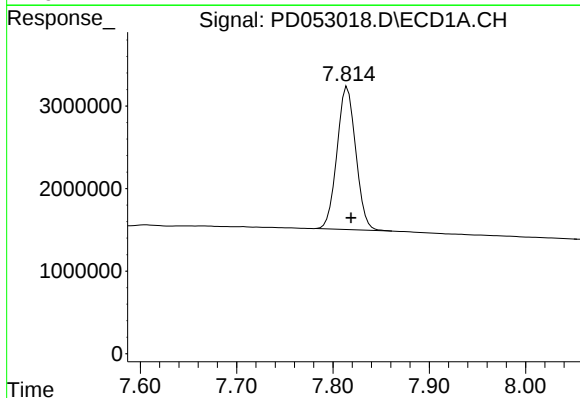

#28 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: -0.004 min
Response: 23348567
Conc: 17.52 ng/ml

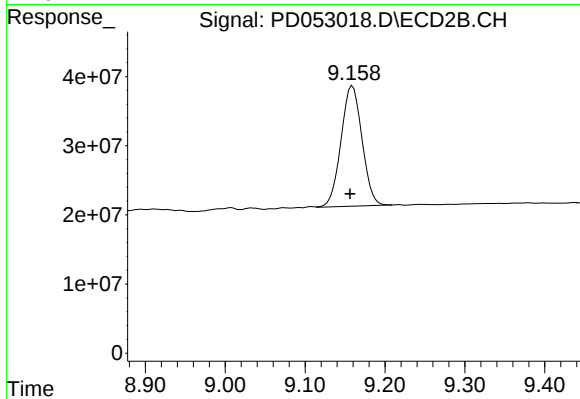

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.003 min
Response: 317233745
Conc: 20.40 ng/ml