

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 18:30
 Operator : AR\AJ
 Sample : M2106-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:07:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	19937276	228.4E6	23.812	26.282
28)	SA Decachlor...	8.256	9.040	25498003	196.1E6	20.723	20.774
Target Compounds							
3)	MA gamma-BHC...	4.237f	0.000	3943780	0	3.322	N.D. #
5)	MB Aldrin	4.746f	5.498f	43200701	-5813616	35.996	N.D. #
9)	A Endosulfan I	0.000	6.234f	0	78774373	N.D.	7.267 #
15)	B Endosulfa...	0.000	6.874f	0	56023425	N.D.	5.901 #
18)	B Endrin al...	0.000	7.019	0	4226052	N.D.	0.537 #
19)	B Endosulfa...	0.000	7.211f	0	15053081	N.D.	1.502 #
21)	B Endrin ke...	0.000	7.705	0	25773200	N.D.	2.541 #
22)	Mirex	0.000	8.193f	0	498046	N.D.	0.077 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 18:30
Operator : AR\AJ
Sample : M2106-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:07:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

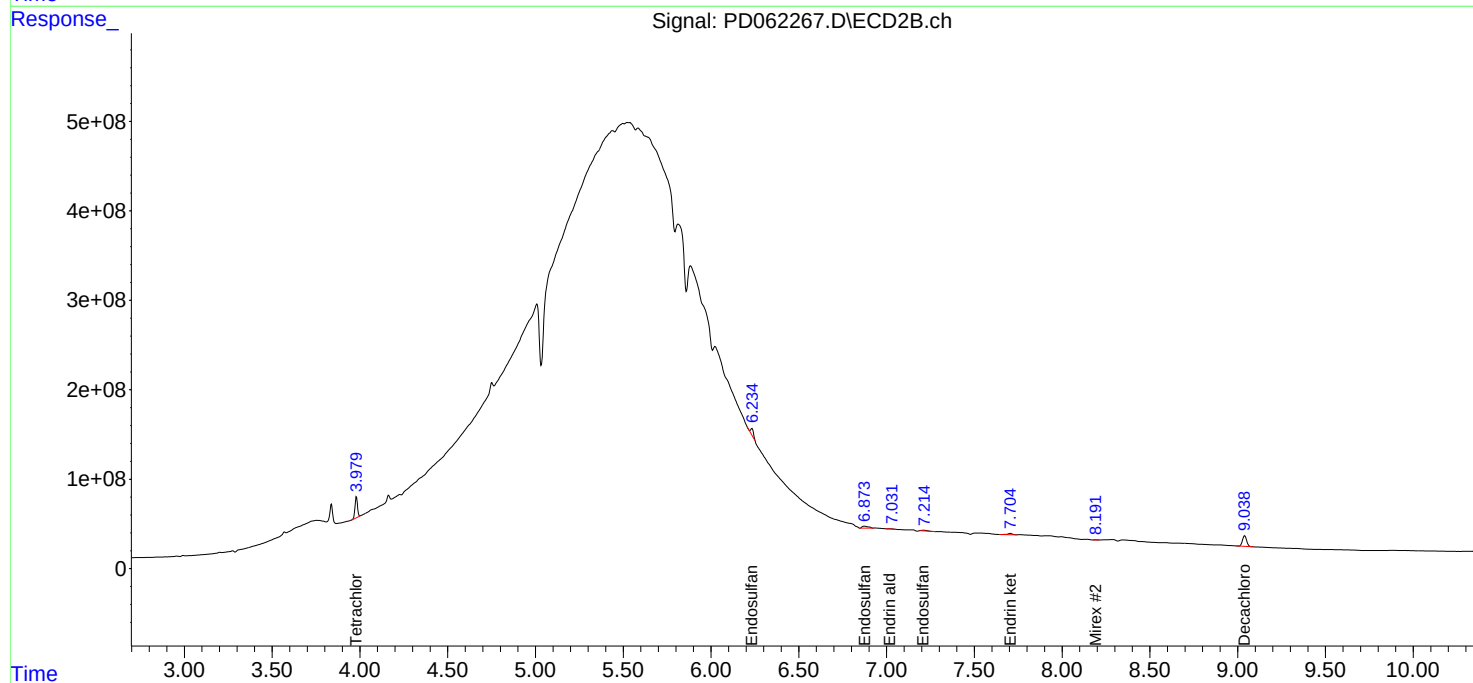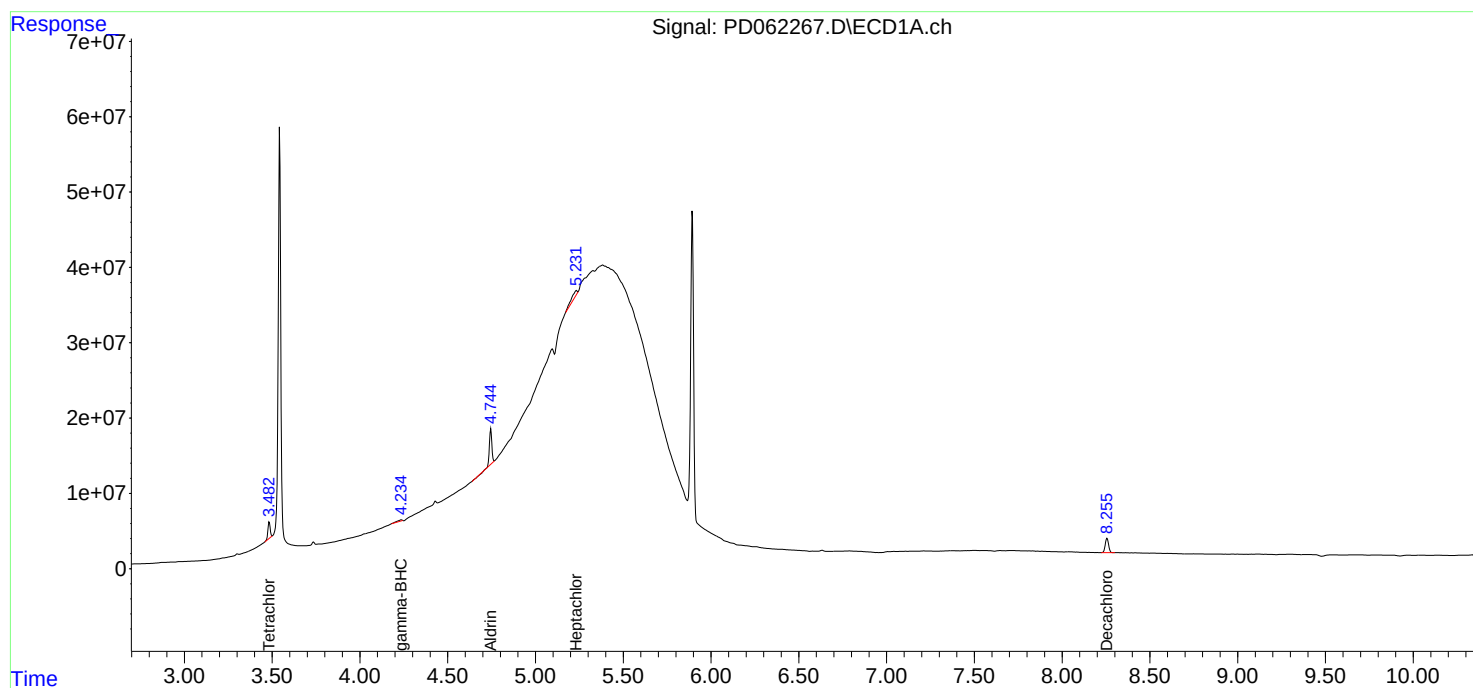


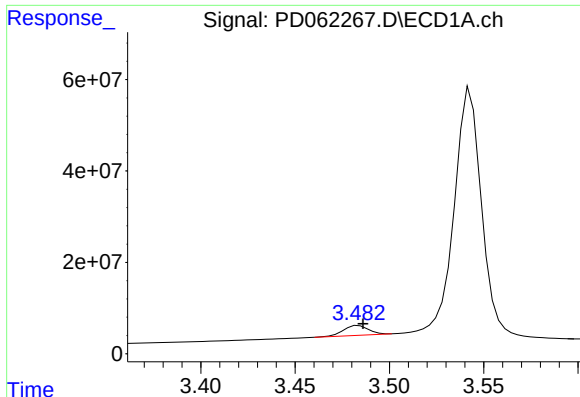

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 19937276
Conc: 23.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

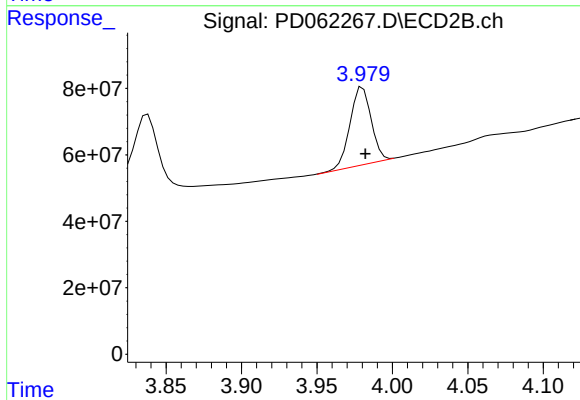


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 228361313
Conc: 26.28 ng/ml

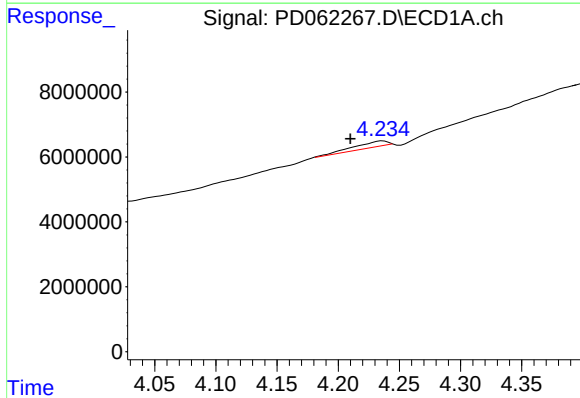


#3 gamma-BHC (Lindane)

R.T.: 4.237 min
Delta R.T.: 0.026 min
Response: 3943780
Conc: 3.32 ng/ml

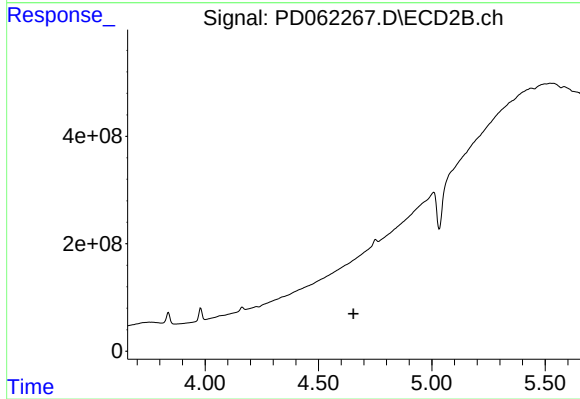

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.655 min
Response: 0
Conc: N.D.

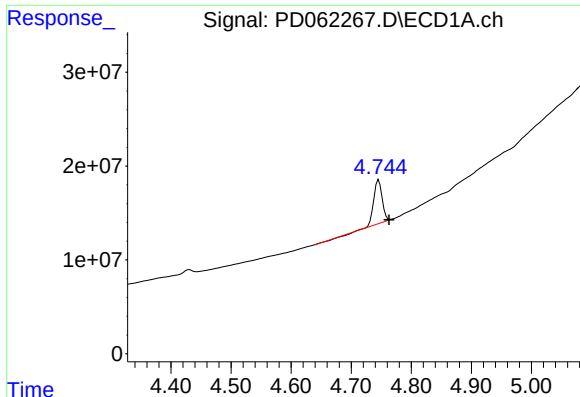

#5 Aldrin


R.T.: 4.746 min
Delta R.T.: -0.018 min
Response: 43200701
Conc: 36.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

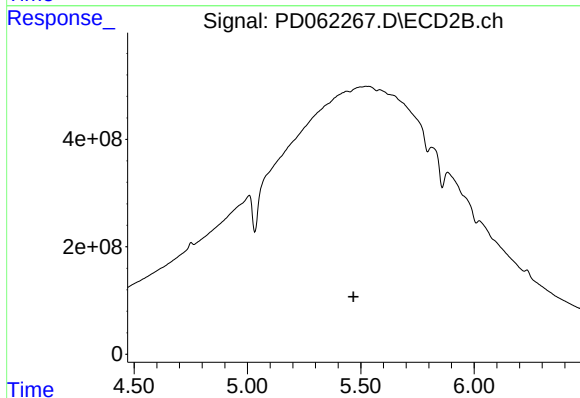


#5 Aldrin

R.T.: 5.498 min
Delta R.T.: 0.030 min
Response: -5813616
Conc: N.D.

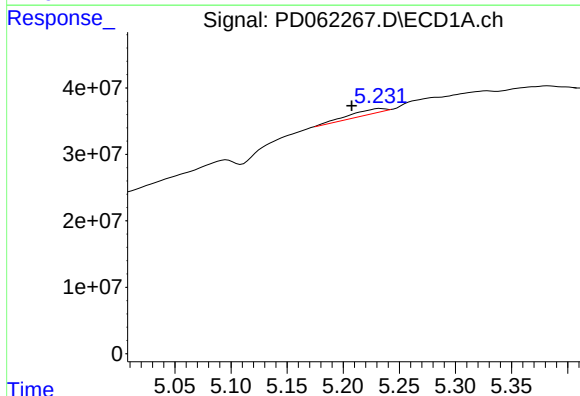


#8 Heptachlor epoxide

R.T.: 5.233 min
Delta R.T.: 0.026 min
Response: 16514313
Conc: 14.41 ng/ml

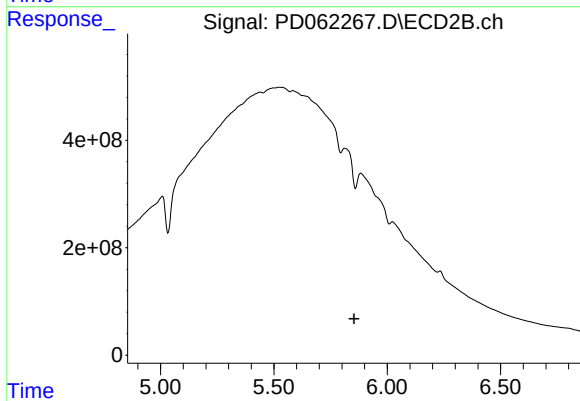

#8 Heptachlor epoxide


R.T.: 5.883 min
Delta R.T.: 0.030 min
Response: -383618462
Conc: N.D.

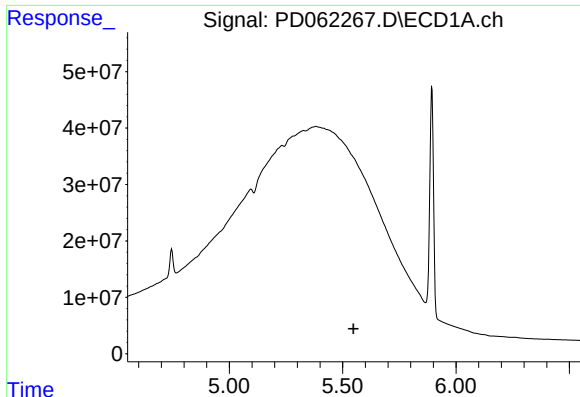

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

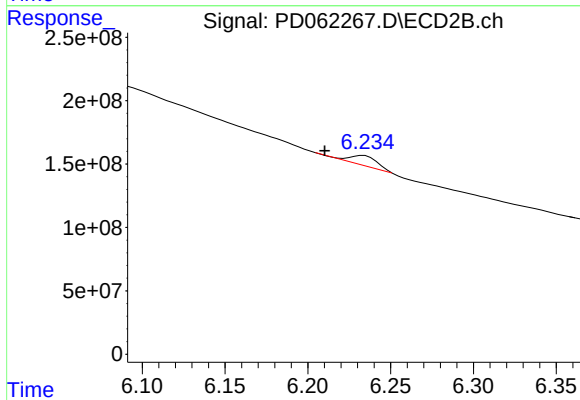


#9 Endosulfan I

R.T.: 6.234 min
Delta R.T.: 0.024 min
Response: 78774373
Conc: 7.27 ng/ml

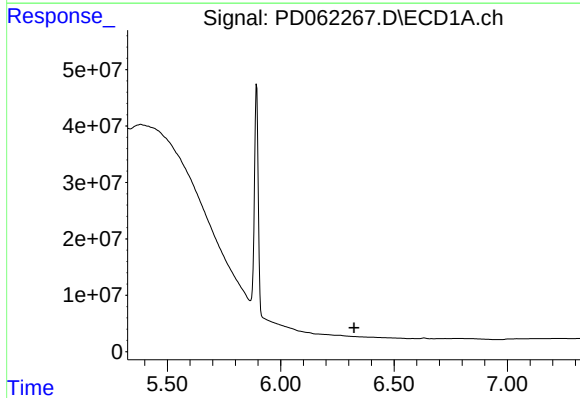


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

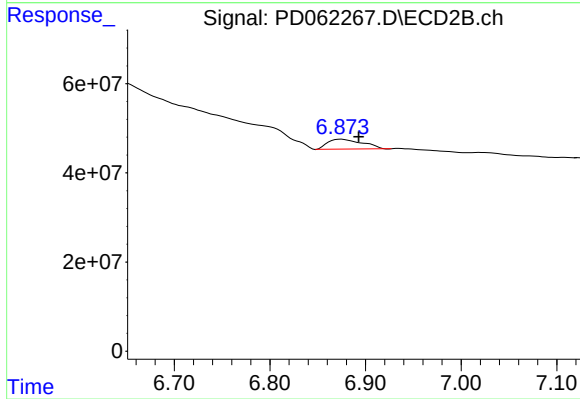

#15 Endosulfan II


R.T.: 6.874 min
Delta R.T.: -0.019 min
Response: 56023425
Conc: 5.90 ng/ml

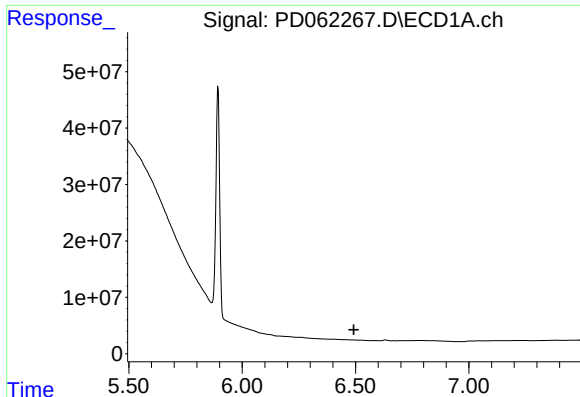

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

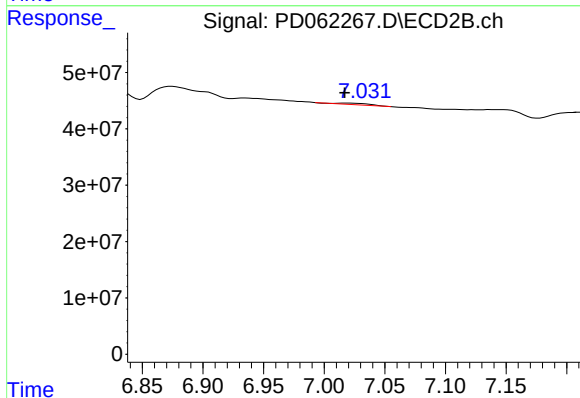


#18 Endrin aldehyde

R.T.: 7.019 min
Delta R.T.: 0.003 min
Response: 4226052
Conc: 0.54 ng/ml

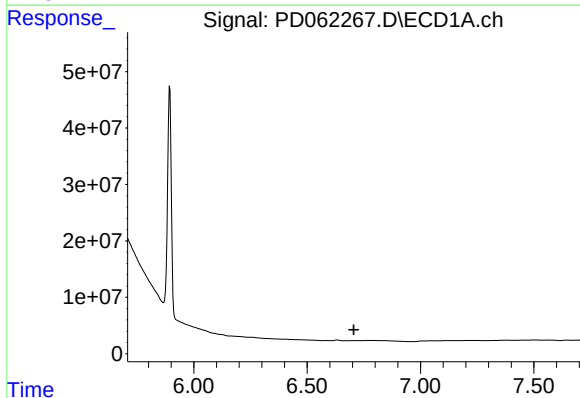


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

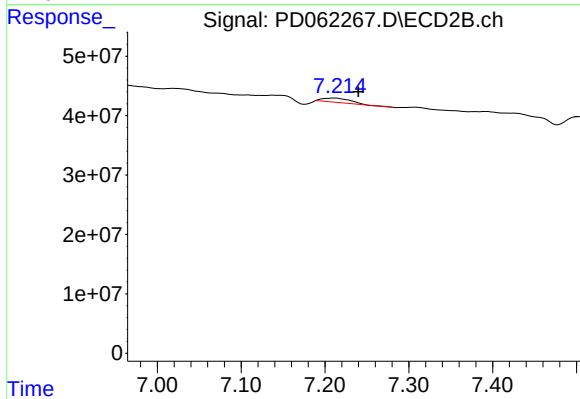

#19 Endosulfan Sulfate


R.T.: 7.211 min
Delta R.T.: -0.029 min
Response: 15053081
Conc: 1.50 ng/ml

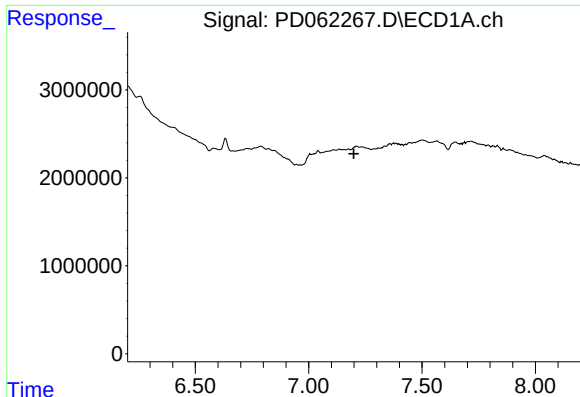

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

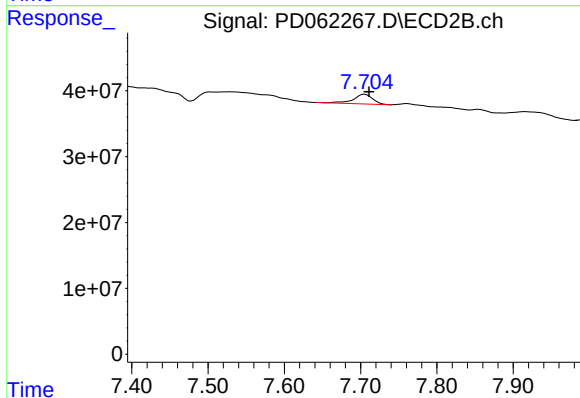


#21 Endrin ketone

R.T.: 7.705 min
Delta R.T.: -0.006 min
Response: 25773200
Conc: 2.54 ng/ml

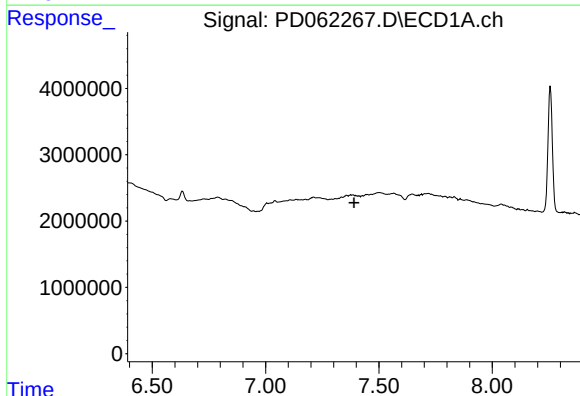


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

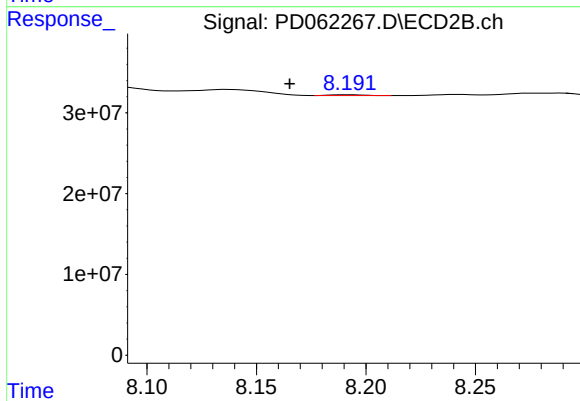

#22 Mirex


R.T.: 8.193 min
Delta R.T.: 0.027 min
Response: 498046
Conc: 0.08 ng/ml

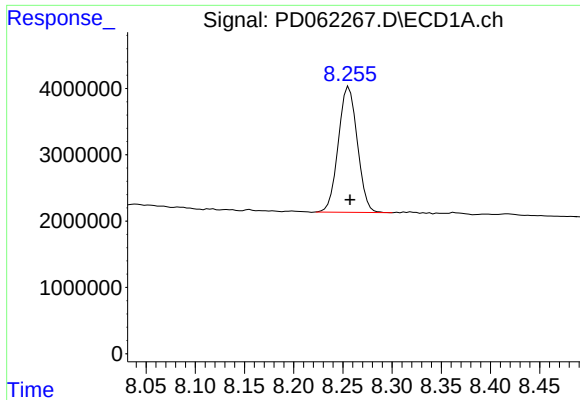

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 25498003
Conc: 20.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

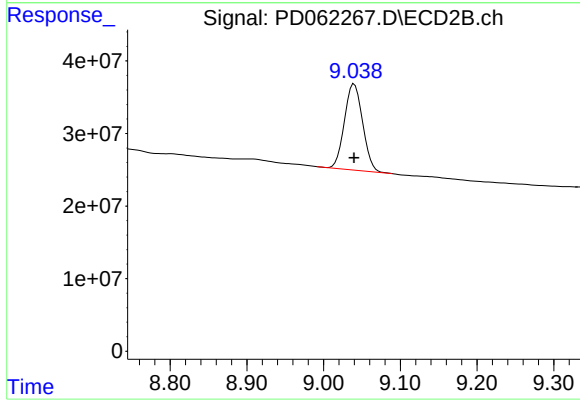

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 196122102
Conc: 20.77 ng/ml