

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 19:26
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:08:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	18827421	231.8E6	22.486	26.673
28)	SA Decachlor...	8.256	9.041	26517867	203.4E6	21.552	21.550
Target Compounds							
2)	A alpha-BHC	3.923	4.370	13560573	171.7E6	10.737	12.768
3)	MA gamma-BHC...	4.208	4.654	13327314	167.5E6	11.225	13.430
5)	MB Aldrin	0.000	5.473	0	398497	N.D.	0.032 #
6)	B beta-BHC	4.459	4.824	7022583	70762859	12.878	13.700
7)	B delta-BHC	0.000	5.015f	0	13615506	N.D.	1.029 #
8)	B Heptachlo...	0.000	5.849	0	15500609	N.D.	1.309 #
10)	B gamma-Chl...	0.000	6.095	0	1887057	N.D.	0.159 #
11)	B alpha-Chl...	0.000	6.177f	0	430592	N.D.	0.038 #
12)	B 4,4'-DDE	0.000	6.317	0	2564738	N.D.	0.223 #
13)	MA Dieldrin	0.000	6.470	0	10082196	N.D.	0.873 #
14)	MA Endrin	6.049	6.684	58702178	551.9E6	57.131	55.768
15)	B Endosulfa...	0.000	6.900	0	4379768	N.D.	0.461 #
16)	A 4,4'-DDD	6.172	6.806	4066937	44071293	4.370	4.654
17)	MA 4,4'-DDT	6.414	7.105	110.1E6	1000.2E6	122.211	104.716
18)	B Endrin al...	0.000	7.017	0	5067144	N.D.	0.644 #
20)	A Methoxychlor	6.961	7.563	138.7E6	1157.4E6	293.463	256.740
21)	B Endrin ke...	7.198	7.711	4047265	28177526	3.171	2.778
22)	Mirex	0.000	8.181f	0	3566981	N.D.	0.553 #
25)	Chlordane-3	0.000	6.095	0	1887057	N.D.	1.138 #
26)	Chlordane-4	0.000	6.177f	0	430592	N.D.	0.224 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 19:26
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:08:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

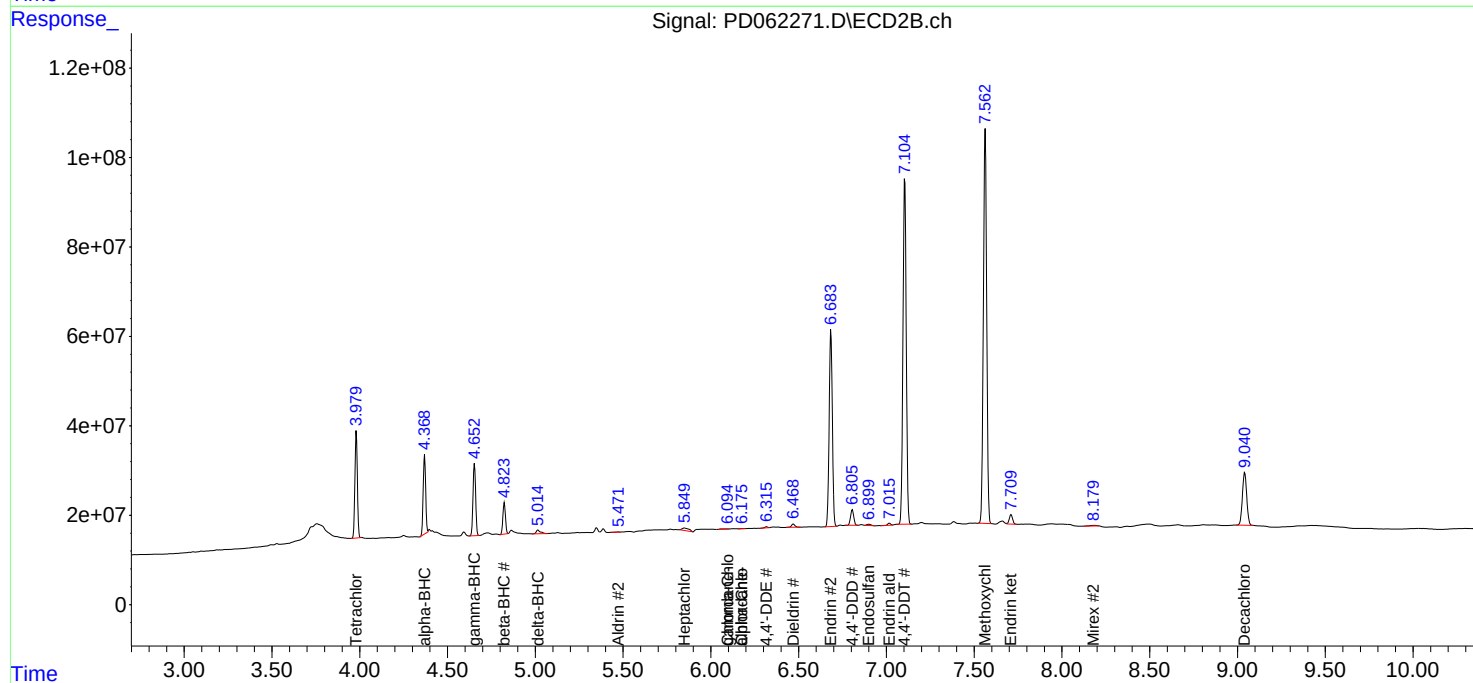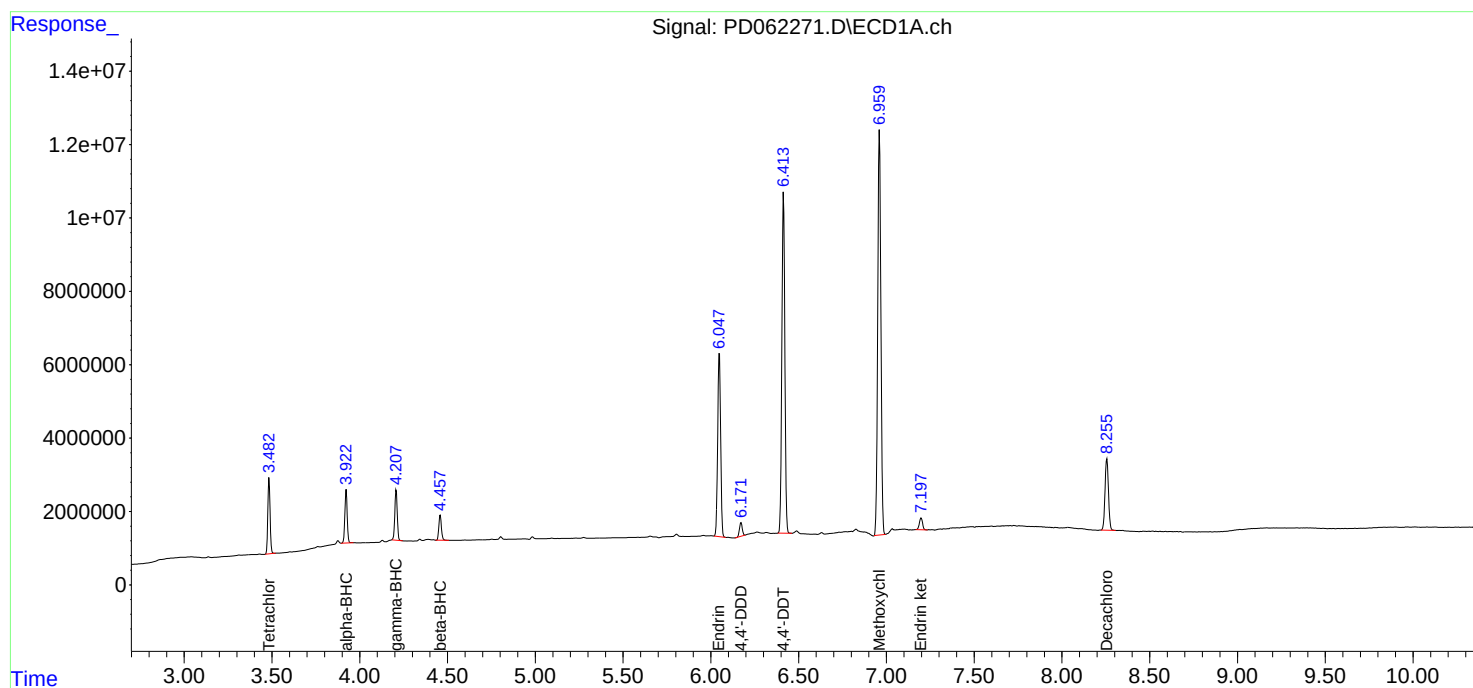


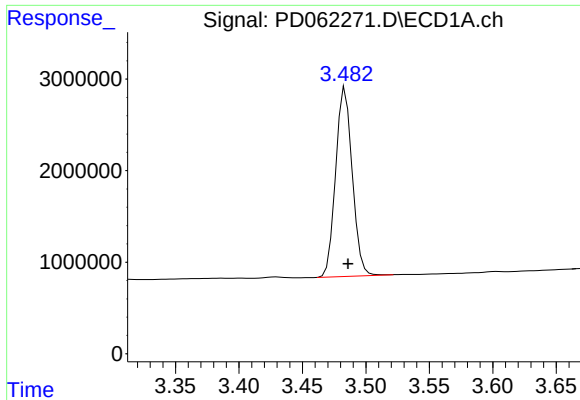

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 18827421
Conc: 22.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

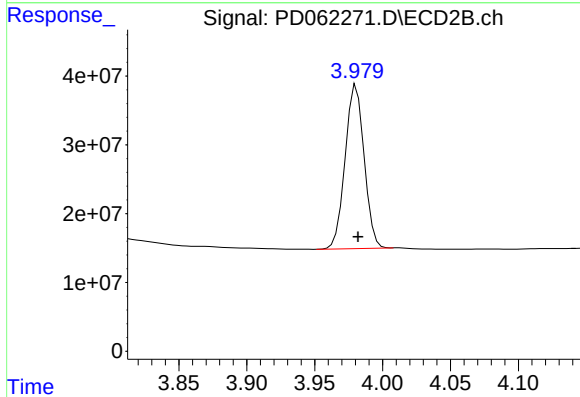


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 231756284
Conc: 26.67 ng/ml

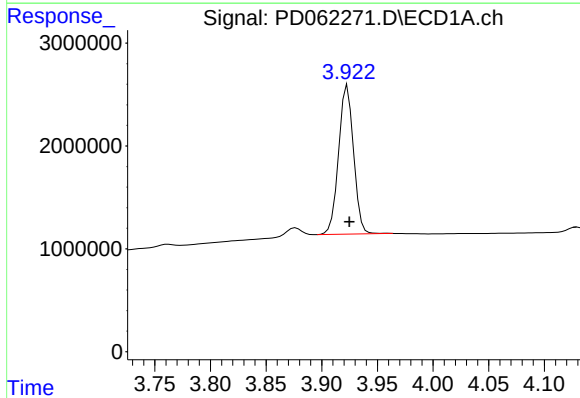


#2 alpha-BHC

R.T.: 3.923 min
Delta R.T.: -0.002 min
Response: 13560573
Conc: 10.74 ng/ml

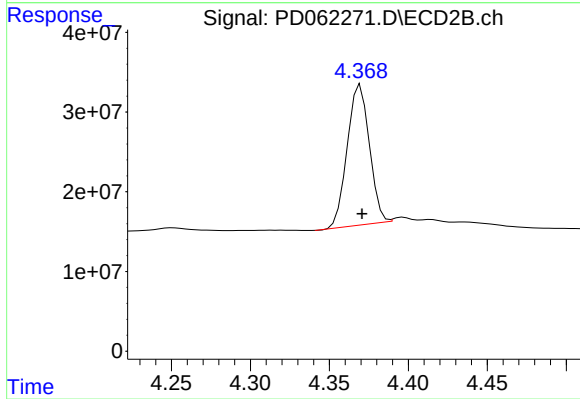

#2 alpha-BHC


R.T.: 4.370 min
Delta R.T.: -0.001 min
Response: 171742315
Conc: 12.77 ng/ml

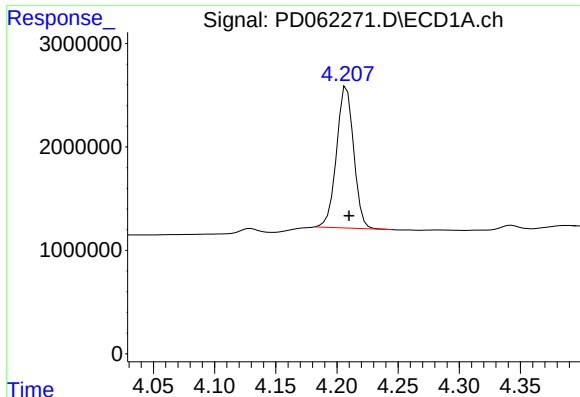

#3 gamma-BHC (Lindane)


R.T.: 4.208 min
Delta R.T.: -0.002 min
Response: 13327314
Conc: 11.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

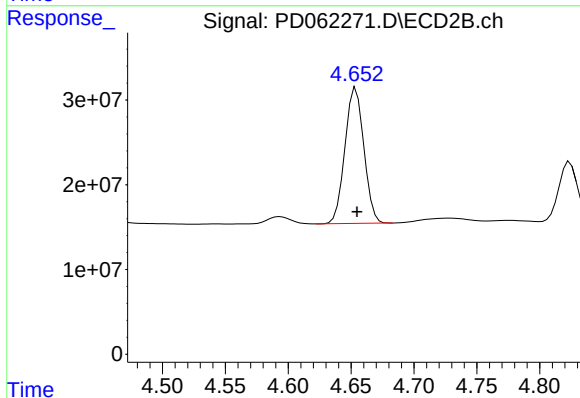


#3 gamma-BHC (Lindane)

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 167529019
Conc: 13.43 ng/ml

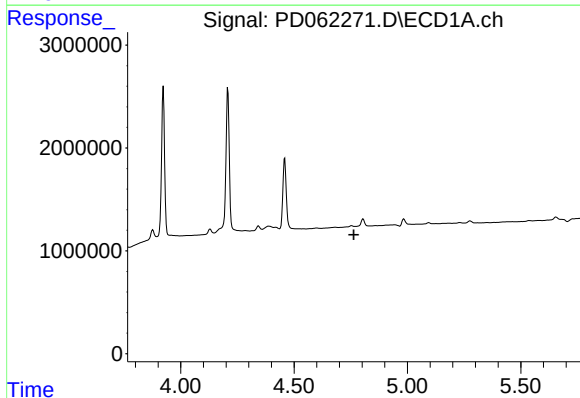


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.763 min
Response: 0
Conc: N.D.

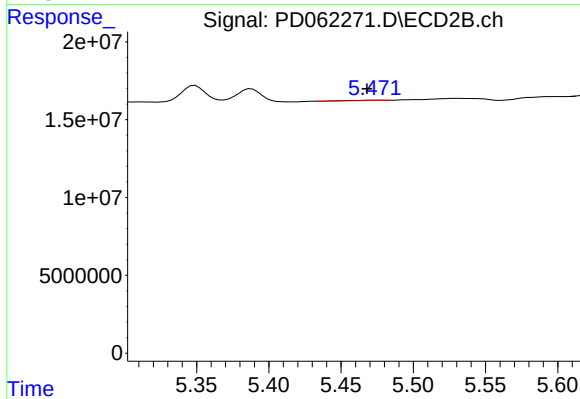

#5 Aldrin


R.T.: 5.473 min
Delta R.T.: 0.005 min
Response: 398497
Conc: 0.03 ng/ml

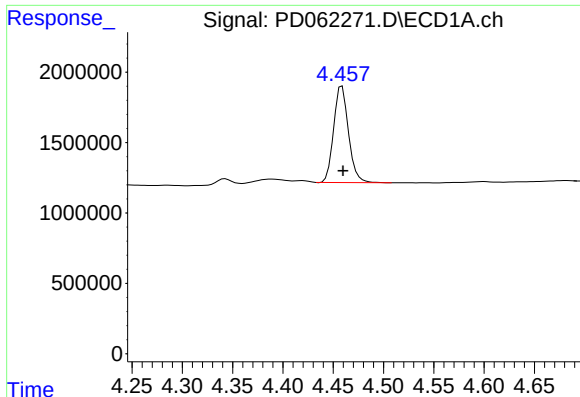

#6 beta-BHC


R.T.: 4.459 min
Delta R.T.: -0.001 min
Response: 7022583
Conc: 12.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

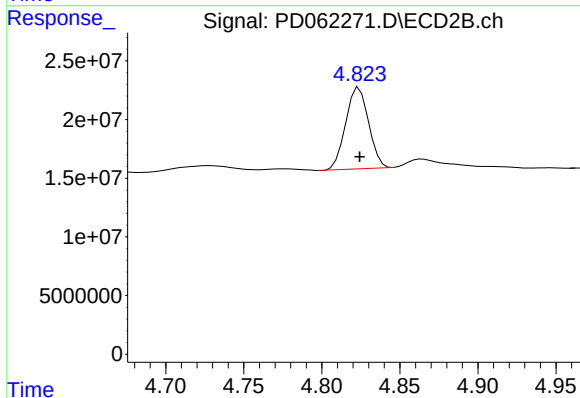


#6 beta-BHC

R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 70762859
Conc: 13.70 ng/ml

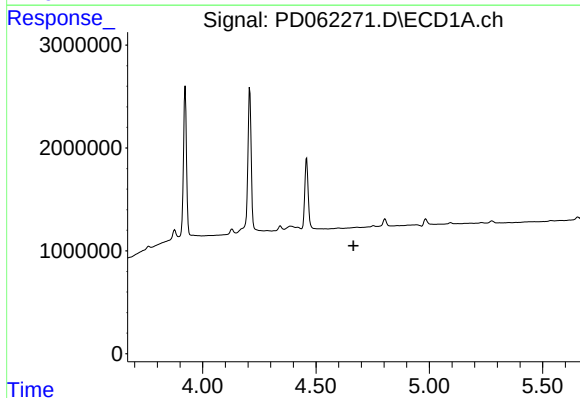


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

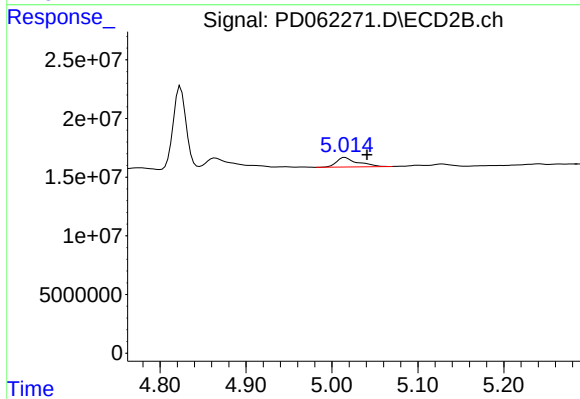

#7 delta-BHC


R.T.: 5.015 min
Delta R.T.: -0.026 min
Response: 13615506
Conc: 1.03 ng/ml

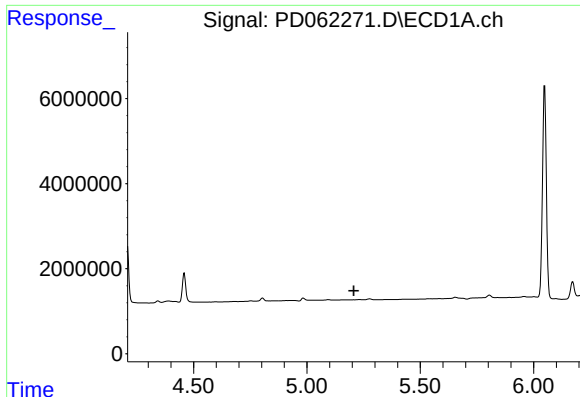

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

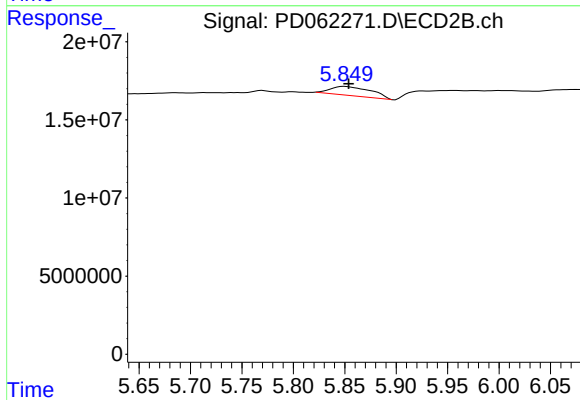


#8 Heptachlor epoxide

R.T.: 5.849 min
Delta R.T.: -0.005 min
Response: 15500609
Conc: 1.31 ng/ml

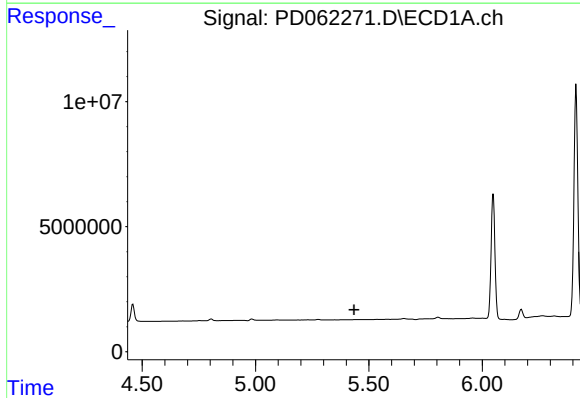


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

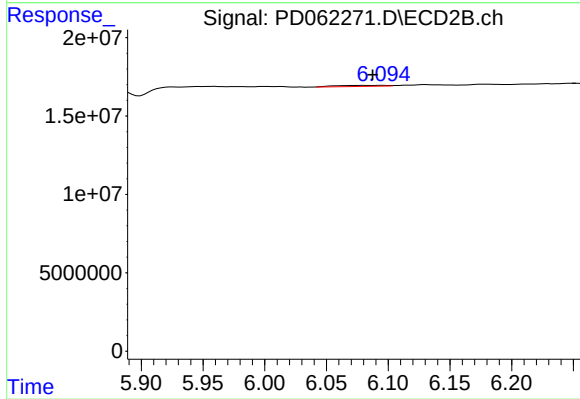

#10 gamma-Chlordane


R.T.: 6.095 min
Delta R.T.: 0.008 min
Response: 1887057
Conc: 0.16 ng/ml

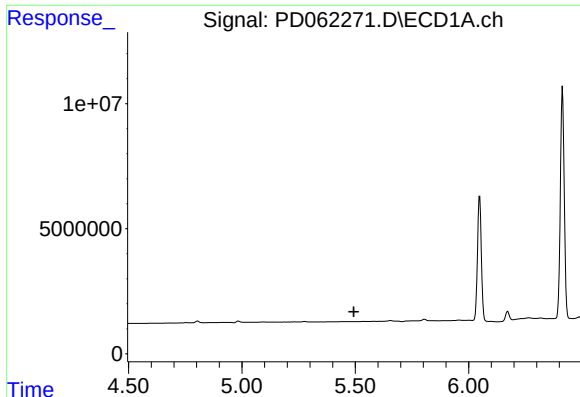

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

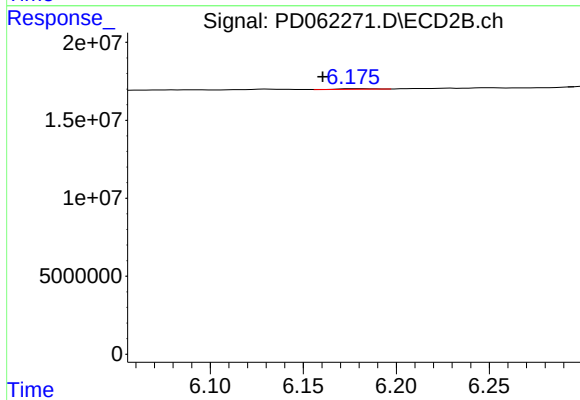


#11 alpha-Chlordane

R.T.: 6.177 min
Delta R.T.: 0.017 min
Response: 430592
Conc: 0.04 ng/ml

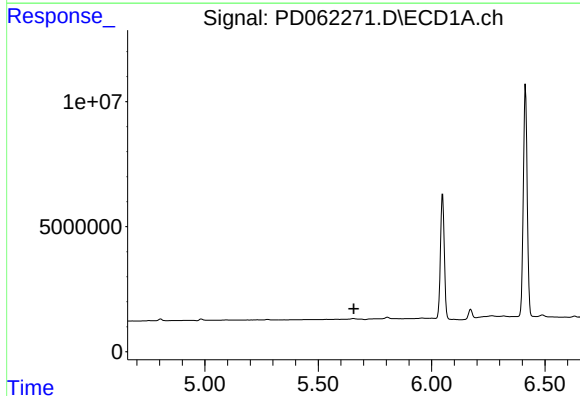


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.657 min
Response: 0
Conc: N.D.

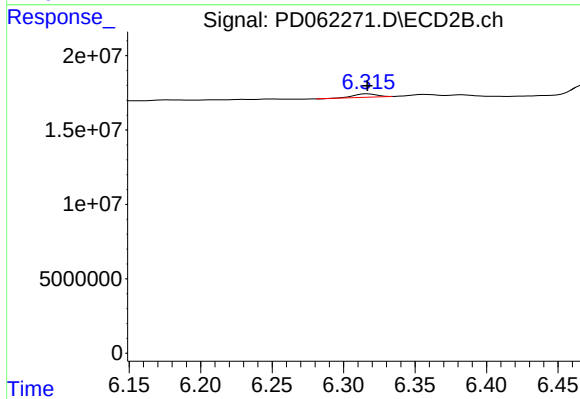

#12 4,4'-DDE


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 2564738
Conc: 0.22 ng/ml

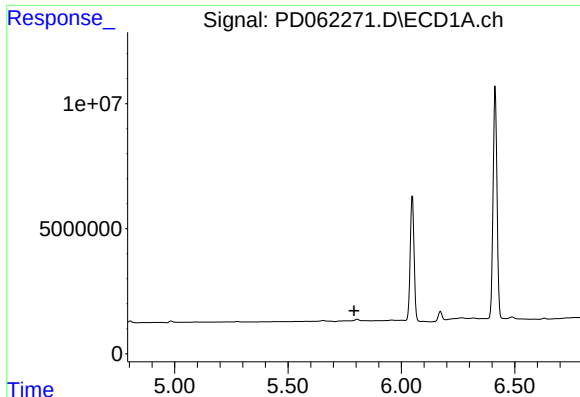

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.792 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

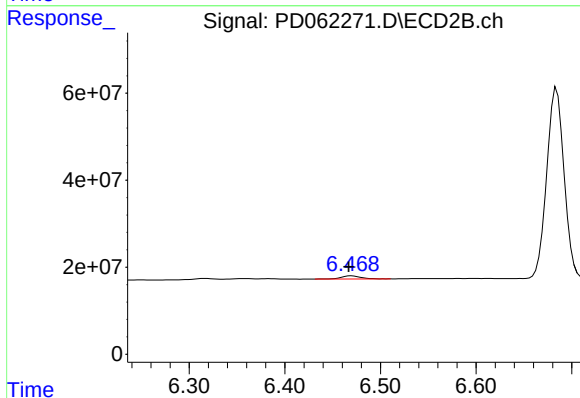


#13 Dieldrin

R.T.: 6.470 min
Delta R.T.: 0.003 min
Response: 10082196
Conc: 0.87 ng/ml

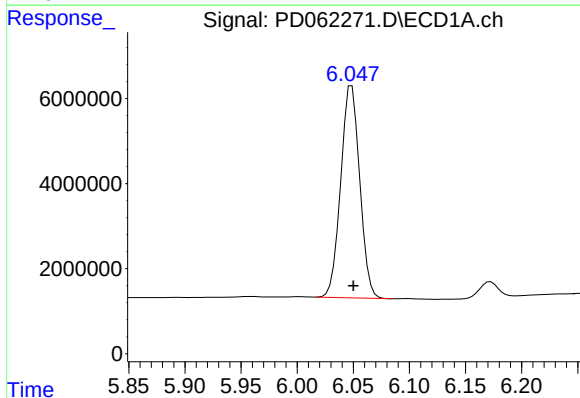


#14 Endrin

R.T.: 6.049 min
Delta R.T.: -0.002 min
Response: 58702178
Conc: 57.13 ng/ml

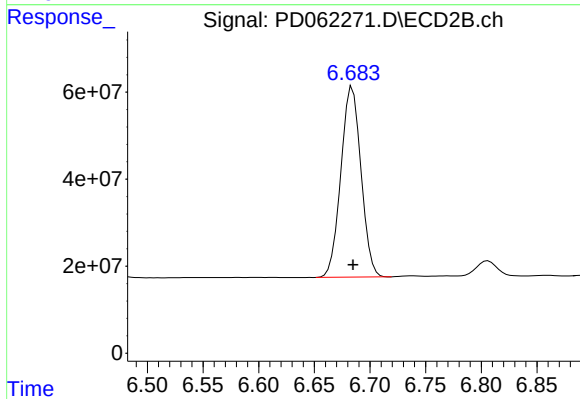

#14 Endrin


R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 551895136
Conc: 55.77 ng/ml

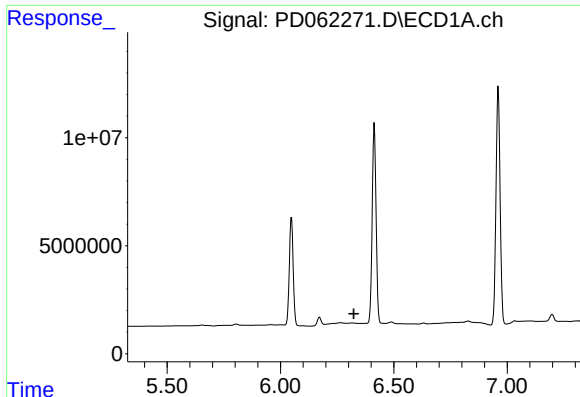

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

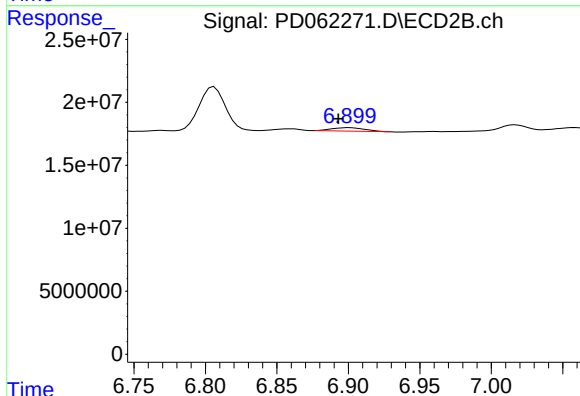


#15 Endosulfan II

R.T.: 6.900 min
Delta R.T.: 0.007 min
Response: 4379768
Conc: 0.46 ng/ml

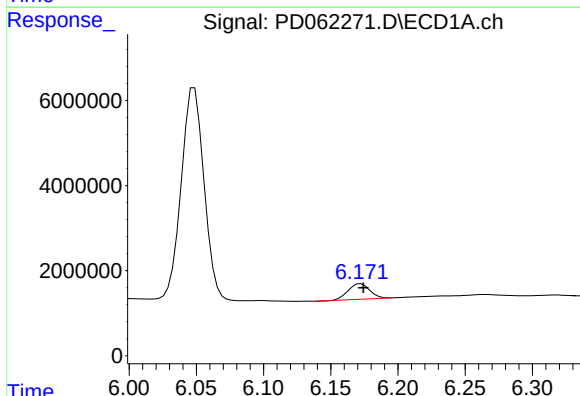


#16 4,4'-DDD

R.T.: 6.172 min
Delta R.T.: -0.002 min
Response: 4066937
Conc: 4.37 ng/ml

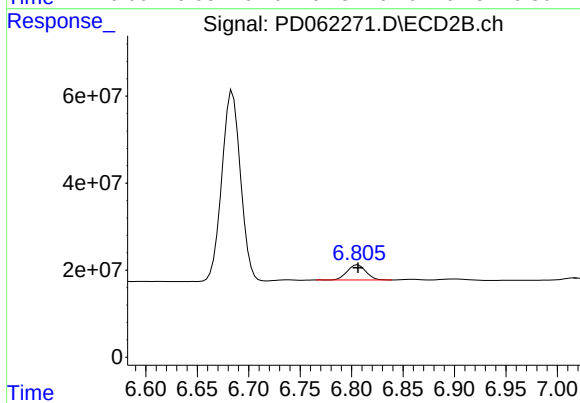

#16 4,4'-DDD


R.T.: 6.806 min
Delta R.T.: 0.000 min
Response: 44071293
Conc: 4.65 ng/ml

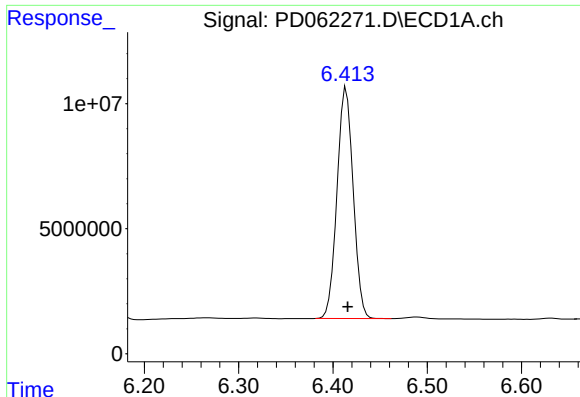

#17 4,4'-DDT


R.T.: 6.414 min
Delta R.T.: -0.002 min
Response: 110078470
Conc: 122.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

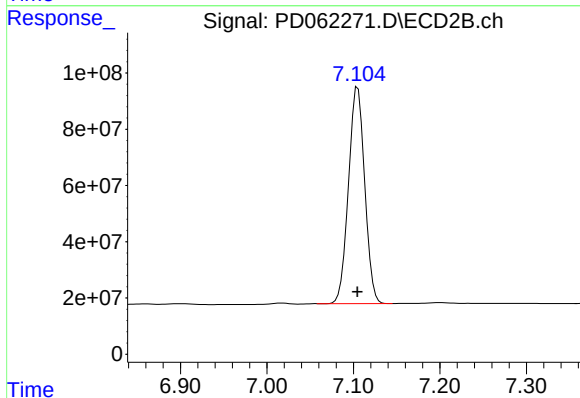


#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 1000207235
Conc: 104.72 ng/ml

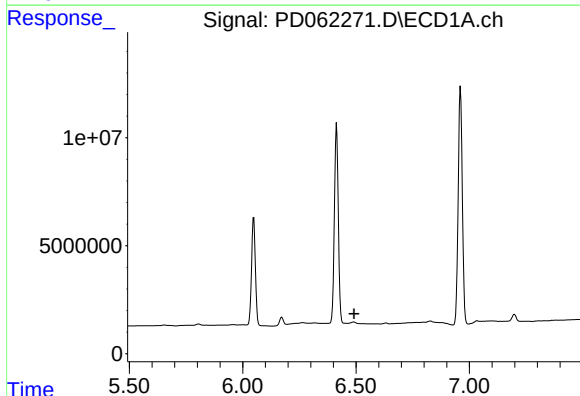


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.492 min
Response: 0
Conc: N.D.

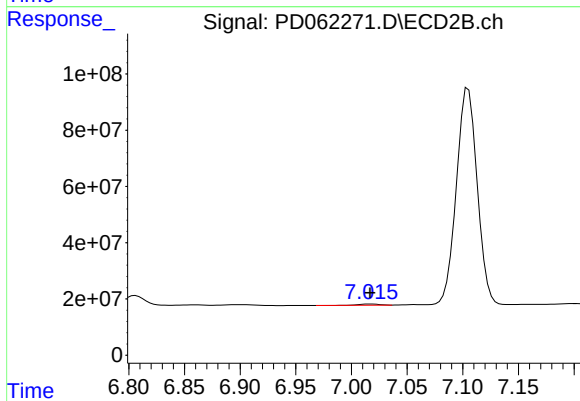

#18 Endrin aldehyde


R.T.: 7.017 min
Delta R.T.: 0.000 min
Response: 5067144
Conc: 0.64 ng/ml

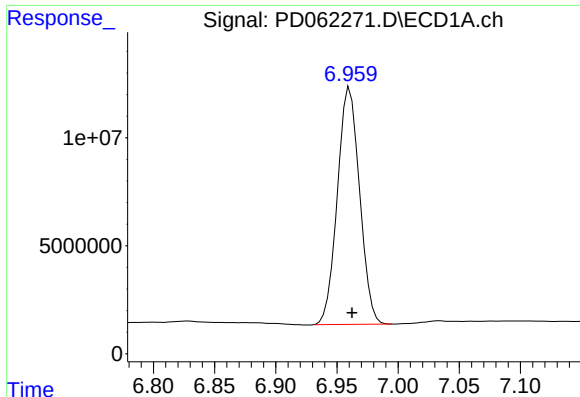

#20 Methoxychlor


R.T.: 6.961 min
Delta R.T.: -0.002 min
Response: 138661569
Conc: 293.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

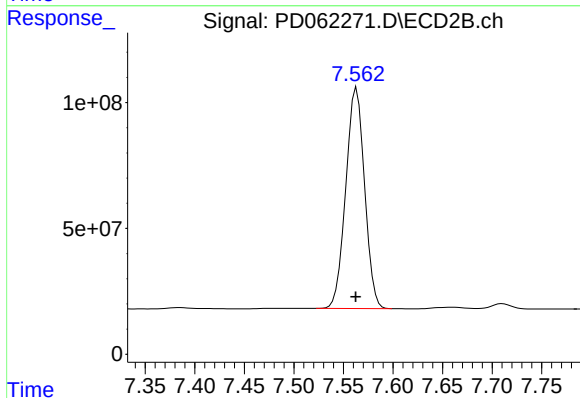


#20 Methoxychlor

R.T.: 7.563 min
Delta R.T.: 0.000 min
Response: 1157360544
Conc: 256.74 ng/ml

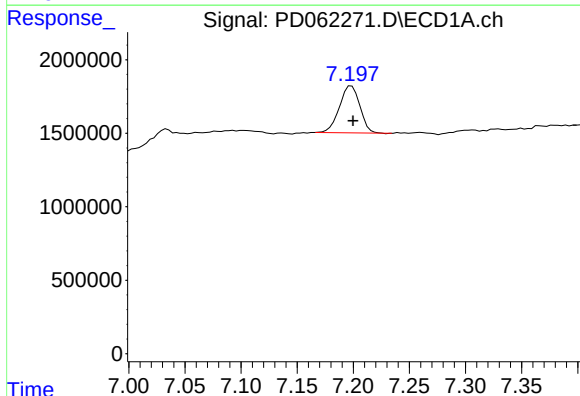


#21 Endrin ketone

R.T.: 7.198 min
Delta R.T.: -0.001 min
Response: 4047265
Conc: 3.17 ng/ml

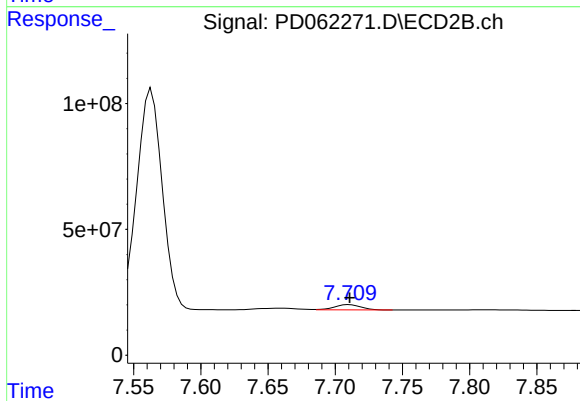

#21 Endrin ketone

R.T.: 7.711 min
Delta R.T.: 0.000 min
Response: 28177526
Conc: 2.78 ng/ml

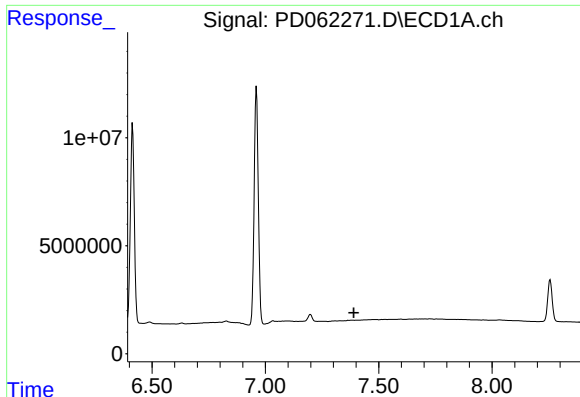

#22 Mirex


R.T.: 0.000 min

Exp R.T.: 7.390 min

Response: 0

Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

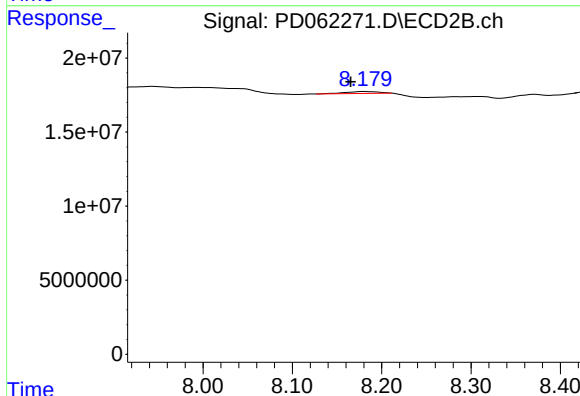


#22 Mirex

R.T.: 8.181 min

Delta R.T.: 0.015 min

Response: 3566981

Conc: 0.55 ng/ml

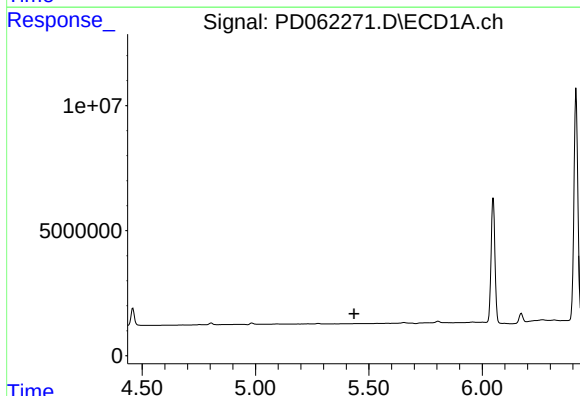


#25 Chlordane-3

R.T.: 0.000 min

Exp R.T.: 5.435 min

Response: 0

Conc: N.D.

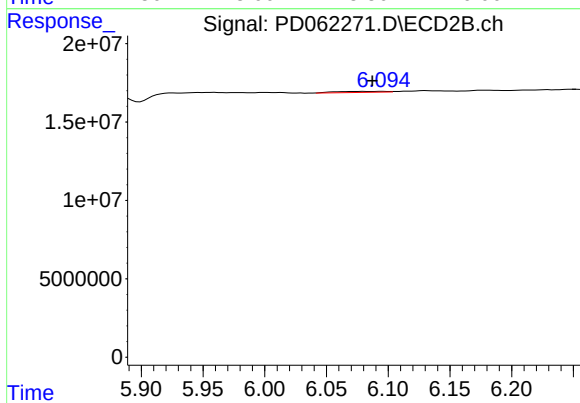


#25 Chlordane-3

R.T.: 6.095 min

Delta R.T.: 0.008 min

Response: 1887057


Conc: 1.14 ng/ml

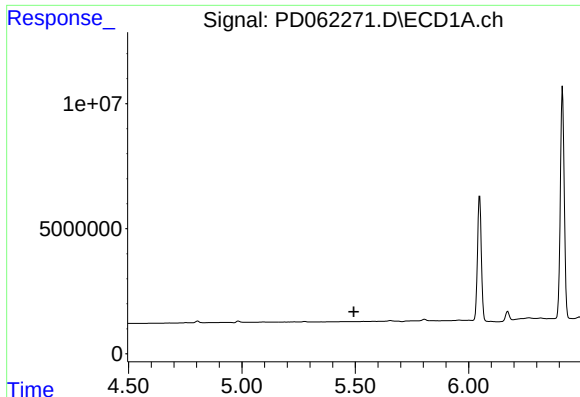

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

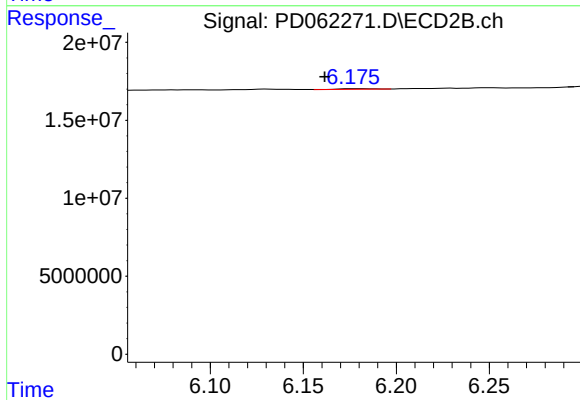


#26 Chlordane-4

R.T.: 6.177 min
Delta R.T.: 0.016 min
Response: 430592
Conc: 0.22 ng/ml

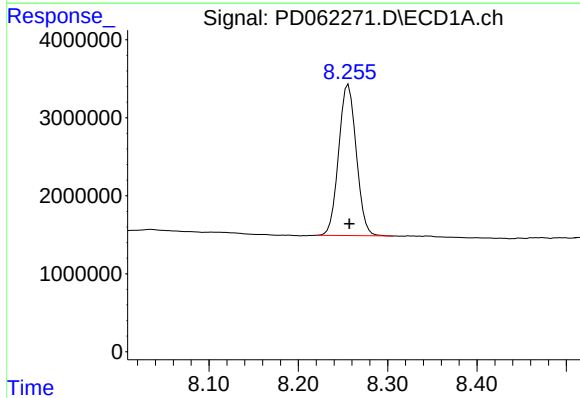

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 26517867
Conc: 21.55 ng/ml

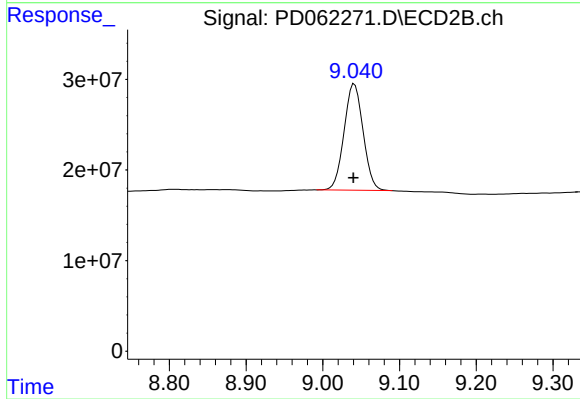

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.001 min
Response: 203441920
Conc: 21.55 ng/ml