

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 20:21
 Operator : AR\AJ
 Sample : M2106-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:09:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	6972442	83993488	8.327	9.667
28)	SA Decachlor...	8.256	9.041	15388418	120.1E6	12.507	12.720
Target Compounds							
5)	MB Aldrin	4.746f	5.487f	10305140	38806023	8.587	3.118 #
6)	B beta-BHC	4.429f	4.804f	1086101	1342103	1.992	0.260 #
8)	B Heptachlo...	5.230f	0.000	8406235	0	7.333	N.D. #
9)	A Endosulfan I	0.000	6.235f	0	33397077	N.D.	3.081 #
16)	A 4,4'-DDD	0.000	6.809	0	7250212	N.D.	0.766 #
17)	MA 4,4'-DDT	0.000	7.077f	0	7018974	N.D.	0.735 #
19)	B Endosulfa...	0.000	7.212f	0	3197606	N.D.	0.319 #
22)	Mirex	0.000	8.191f	0	12468686	N.D.	1.935 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 20:21
Operator : AR\AJ
Sample : M2106-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:09:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

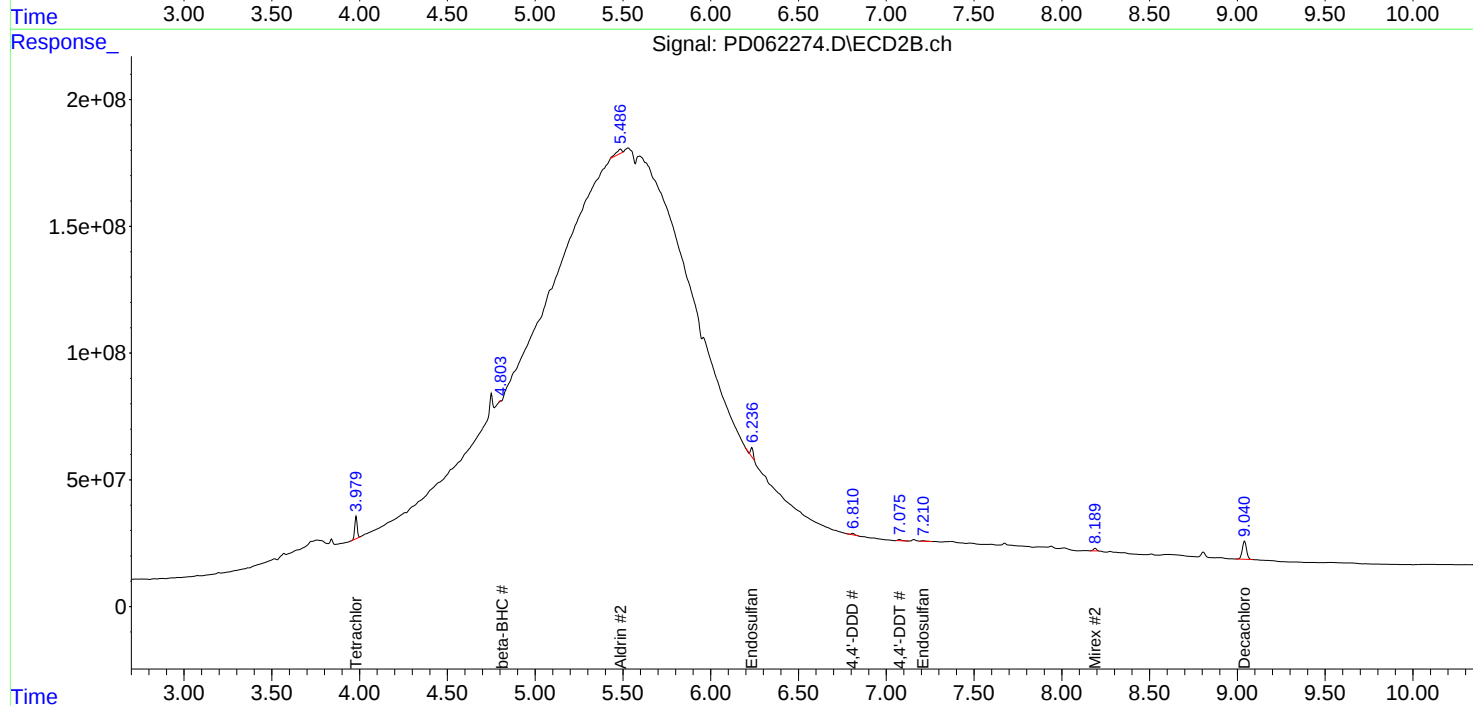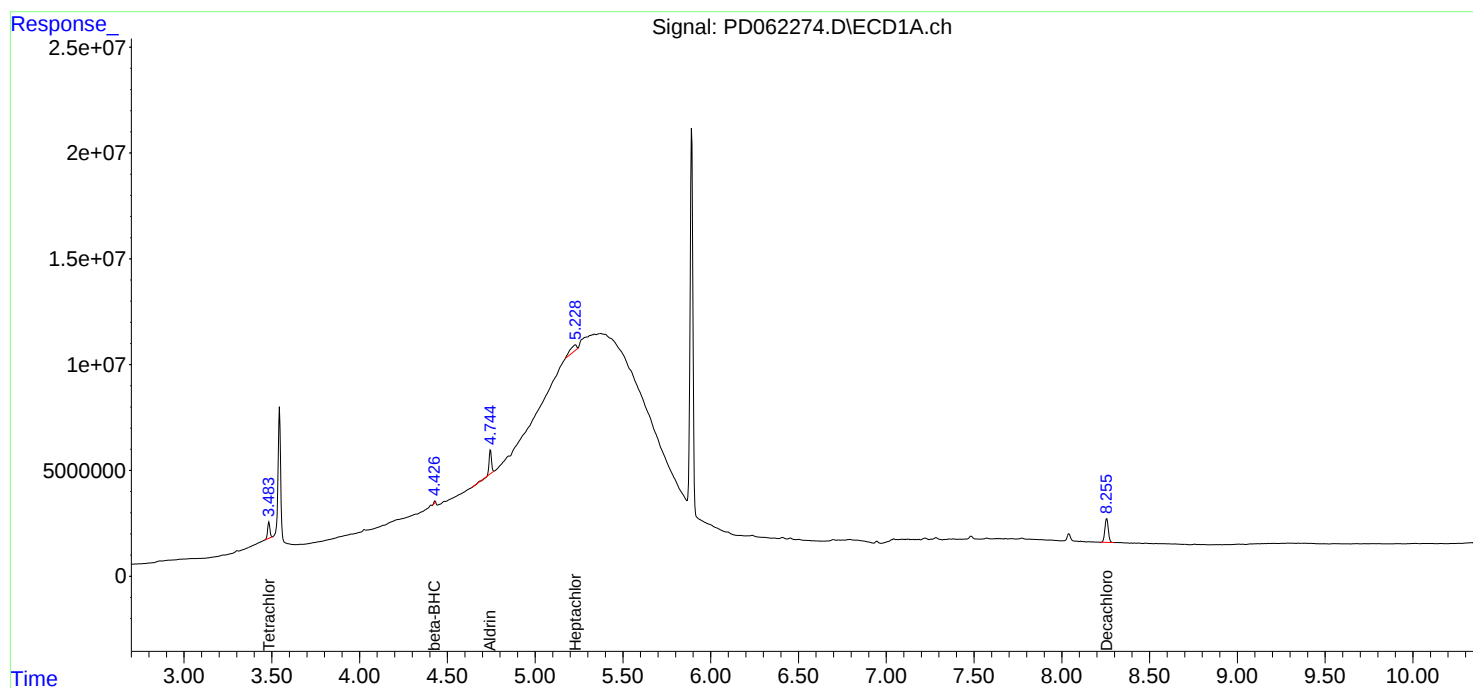


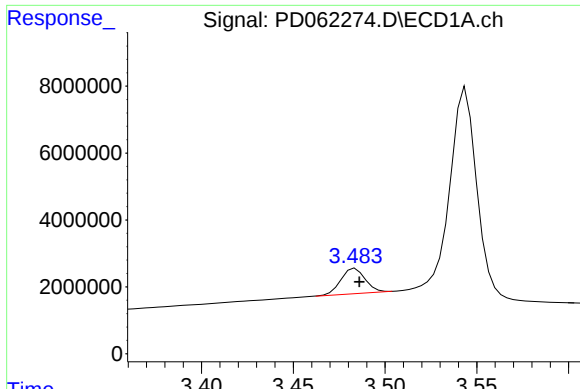

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 6972442
Conc: 8.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

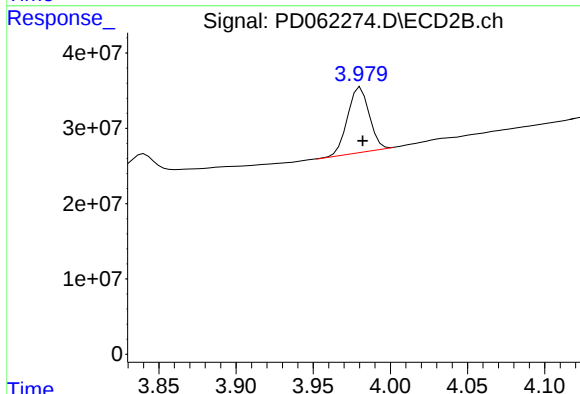


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 83993488
Conc: 9.67 ng/ml

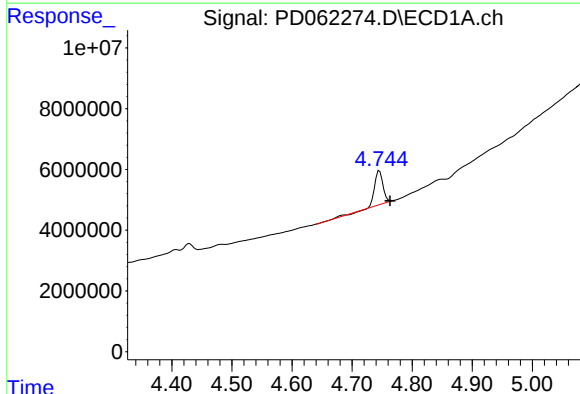


#5 Aldrin

R.T.: 4.746 min
Delta R.T.: -0.018 min
Response: 10305140
Conc: 8.59 ng/ml

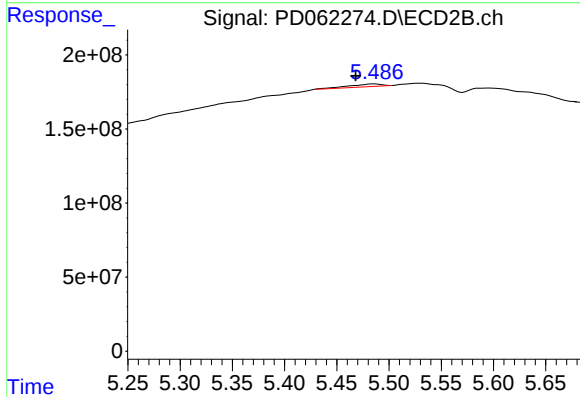

#5 Aldrin


R.T.: 5.487 min
Delta R.T.: 0.019 min
Response: 38806023
Conc: 3.12 ng/ml

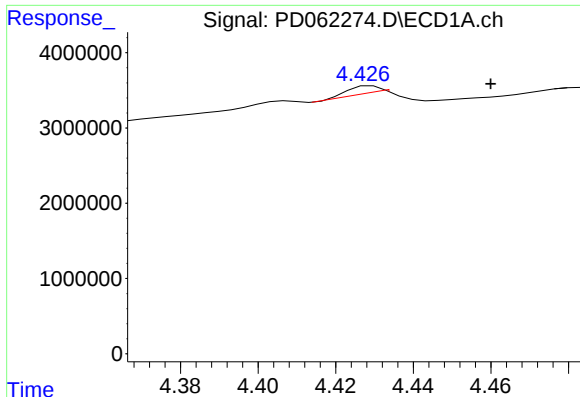

#6 beta-BHC


R.T.: 4.429 min
Delta R.T.: -0.031 min
Response: 1086101
Conc: 1.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

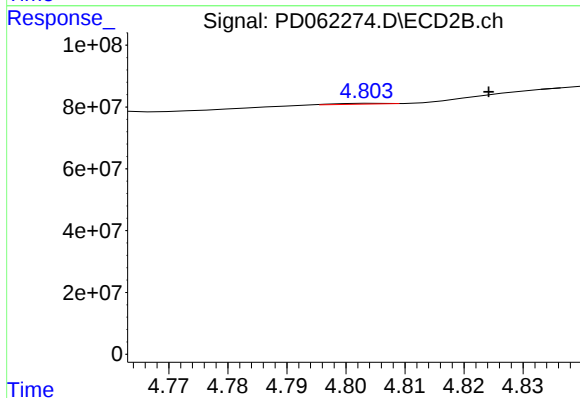


#6 beta-BHC

R.T.: 4.804 min
Delta R.T.: -0.020 min
Response: 1342103
Conc: 0.26 ng/ml

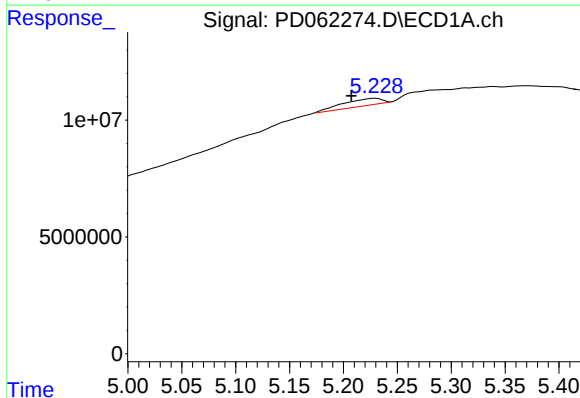


#8 Heptachlor epoxide

R.T.: 5.230 min
Delta R.T.: 0.022 min
Response: 8406235
Conc: 7.33 ng/ml

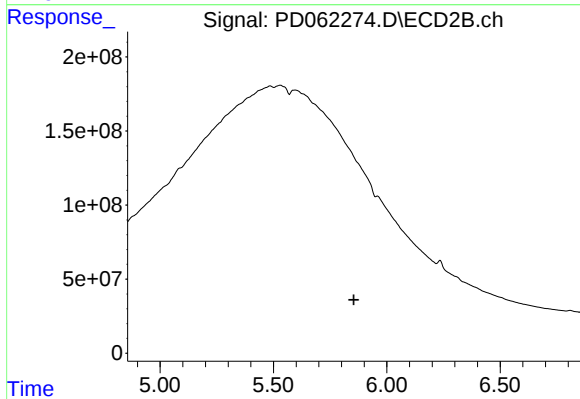

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.854 min
Response: 0
Conc: N.D.

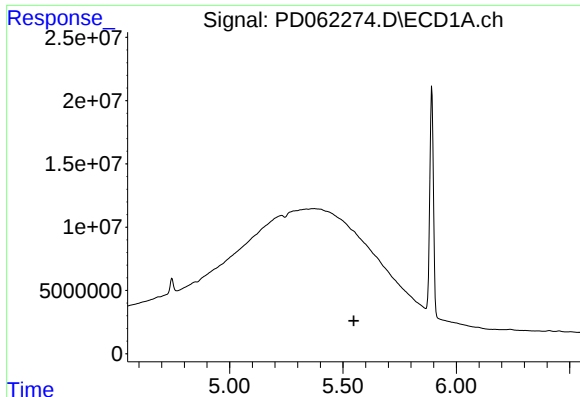

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

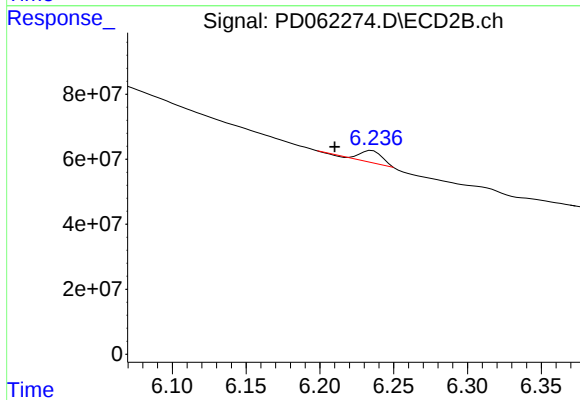


#9 Endosulfan I

R.T.: 6.235 min
Delta R.T.: 0.025 min
Response: 33397077
Conc: 3.08 ng/ml

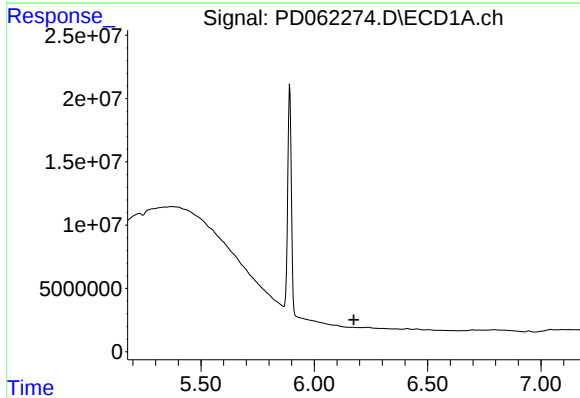


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.174 min
Response: 0
Conc: N.D.

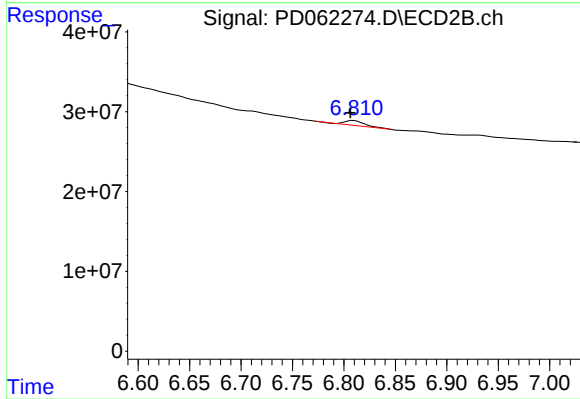

#16 4,4'-DDD


R.T.: 6.809 min
Delta R.T.: 0.003 min
Response: 7250212
Conc: 0.77 ng/ml

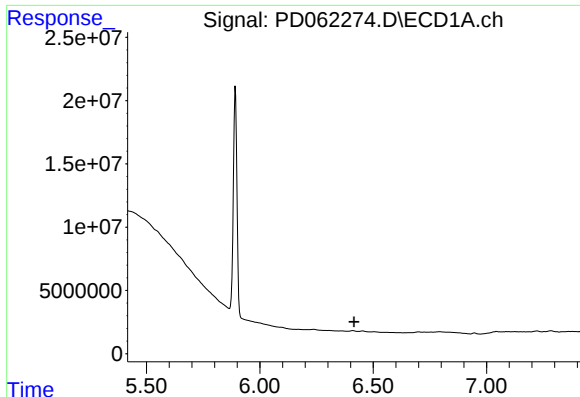

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

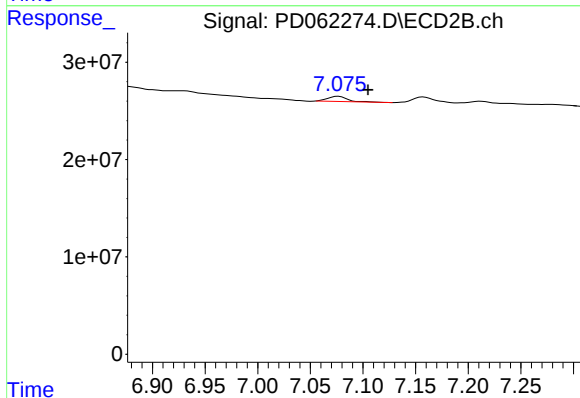


#17 4,4'-DDT

R.T.: 7.077 min
Delta R.T.: -0.028 min
Response: 7018974
Conc: 0.73 ng/ml

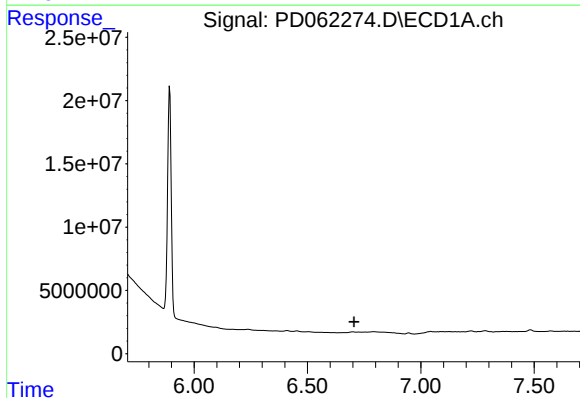


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

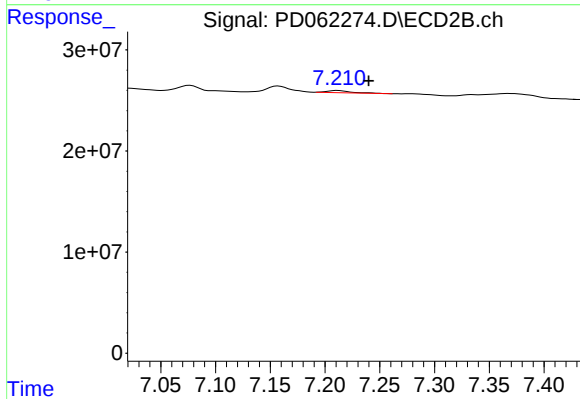

#19 Endosulfan Sulfate


R.T.: 7.212 min
Delta R.T.: -0.028 min
Response: 3197606
Conc: 0.32 ng/ml

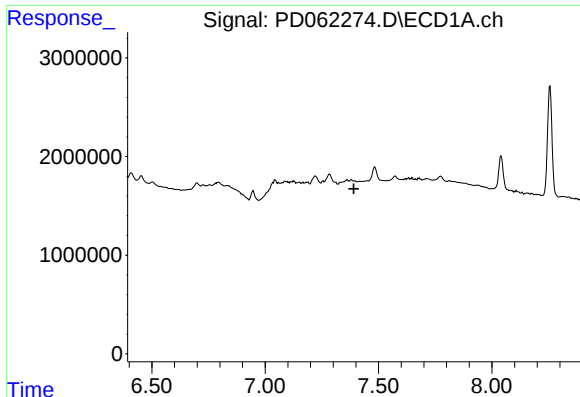

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

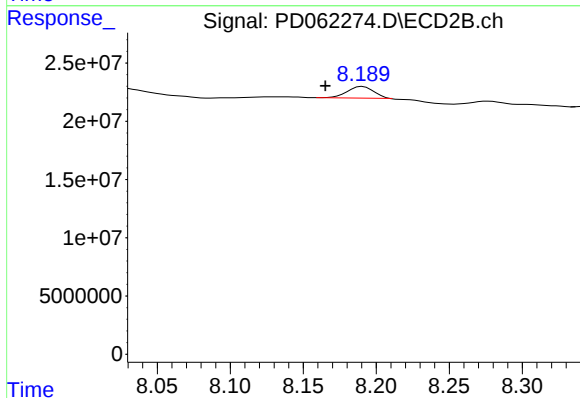


#22 Mirex

R.T.: 8.191 min
Delta R.T.: 0.026 min
Response: 12468686
Conc: 1.93 ng/ml

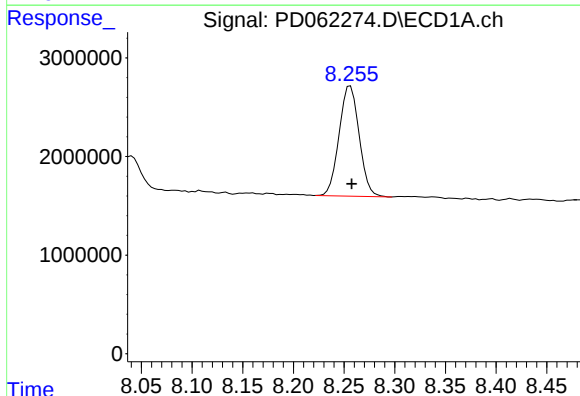

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.001 min
Response: 15388418
Conc: 12.51 ng/ml

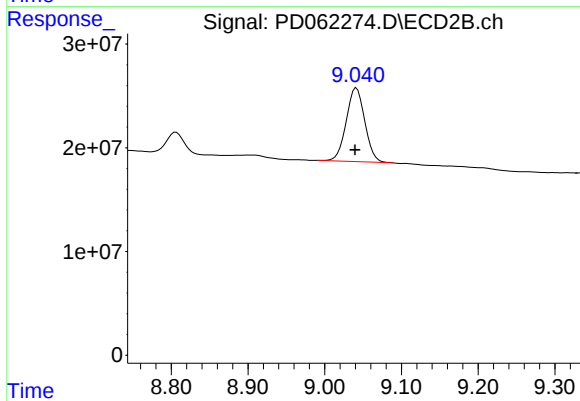

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.001 min
Response: 120079606
Conc: 12.72 ng/ml