

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 11:46
 Operator : AR\AJ
 Sample : M2098-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HR-01-042021

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:50:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:00:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	11830461	141.6E6	14.129	16.298
28)	SA Decachlor...	8.258	9.042	18329908	144.5E6	14.897	15.311
Target Compounds							
12)	B 4,4'-DDE	5.654	6.314	564220	9990179	0.502m	0.867 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 11:46
Operator : AR\AJ
Sample : M2098-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HR-01-042021


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:00:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

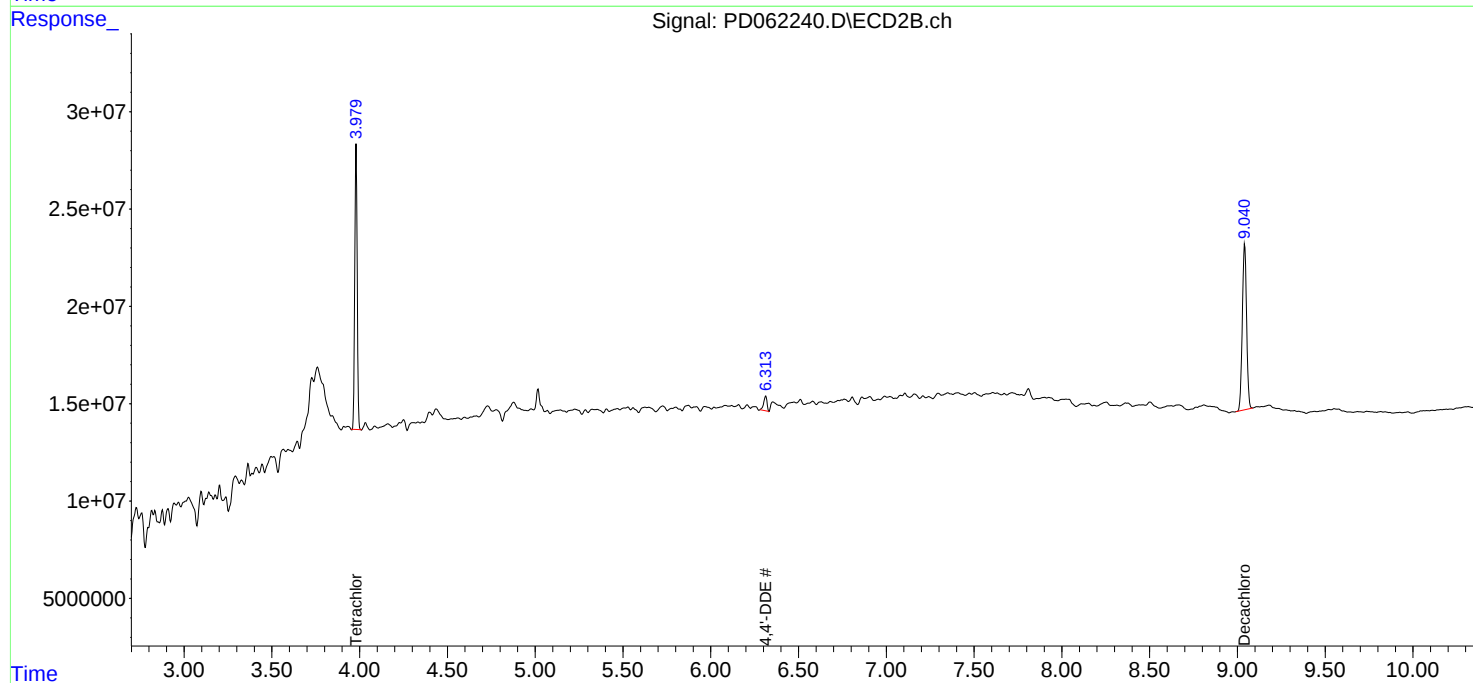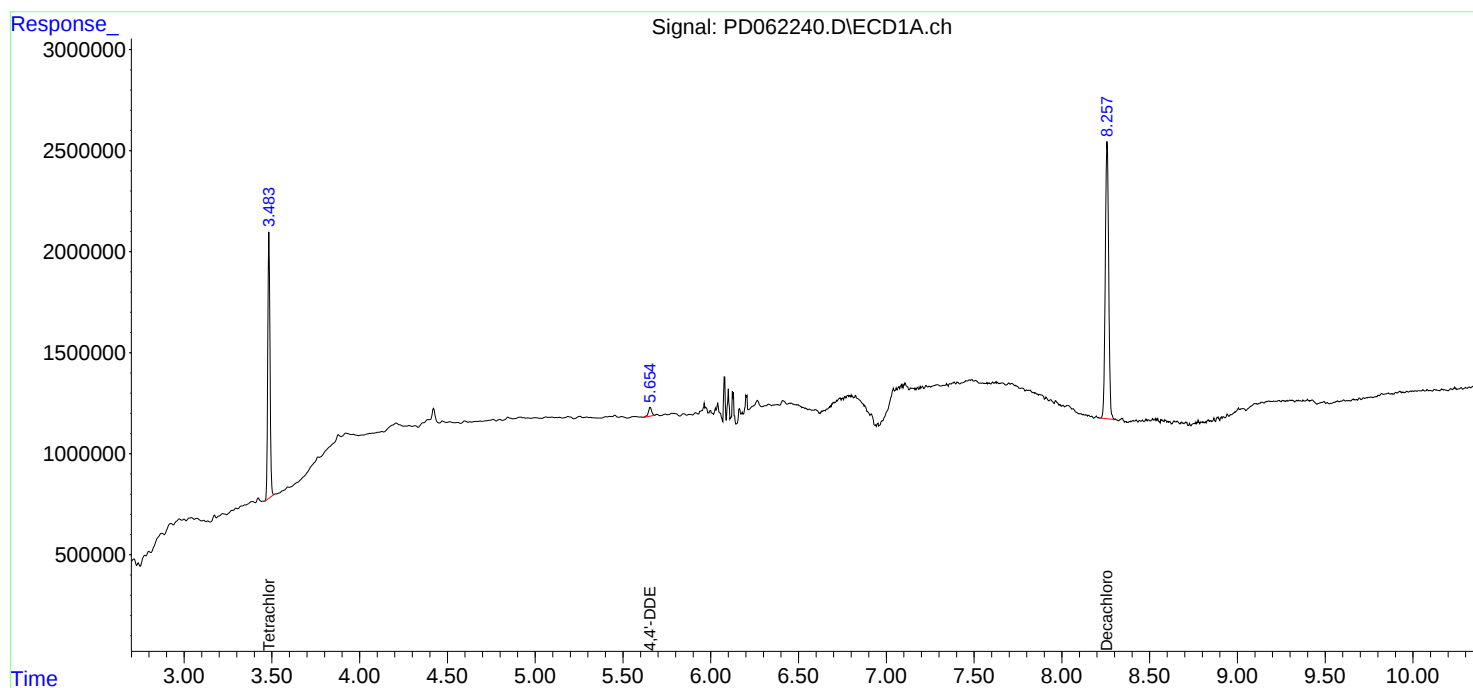

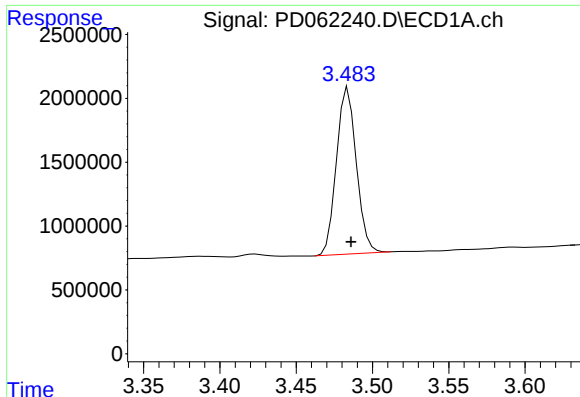


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 11830461
Conc: 14.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
HR-01-042021


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:33 PM

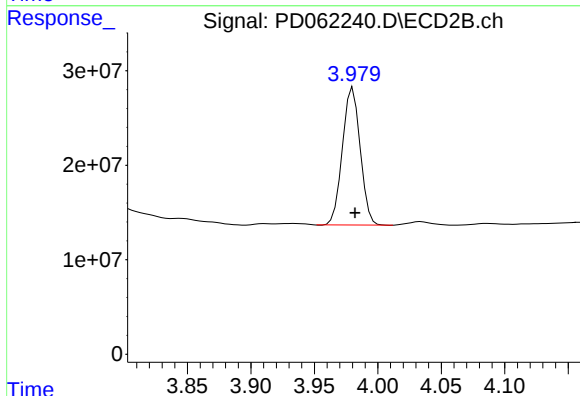


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 141609380
Conc: 16.30 ng/ml

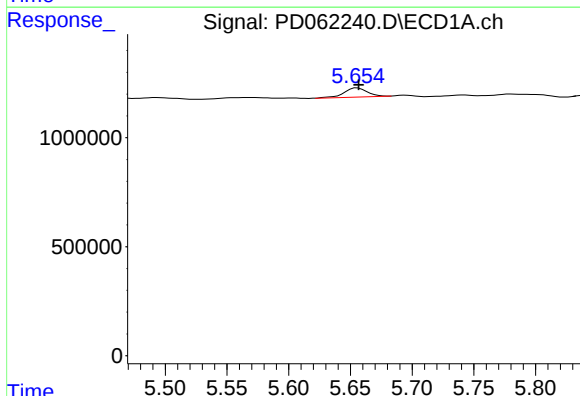


#12 4,4'-DDE

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 564220
Conc: 0.50 ng/ml m

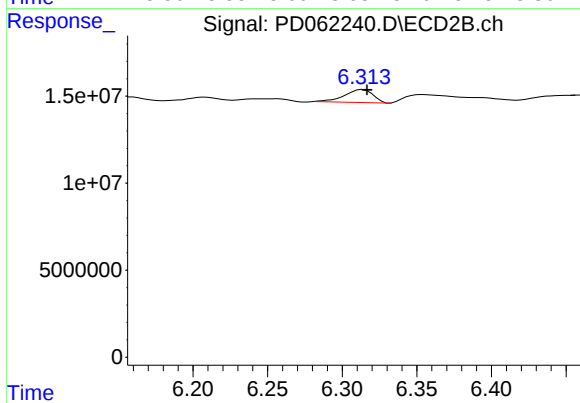

#12 4,4'-DDE

R.T.: 6.314 min
Delta R.T.: -0.003 min
Response: 9990179
Conc: 0.87 ng/ml

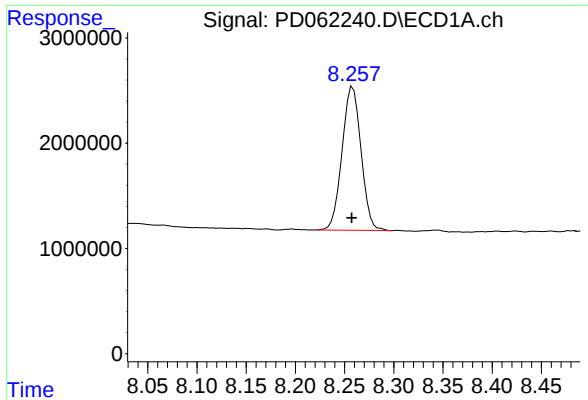


#28 Decachlorobiphenyl

R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 18329908
Conc: 14.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
HR-01-042021

Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:33 PM

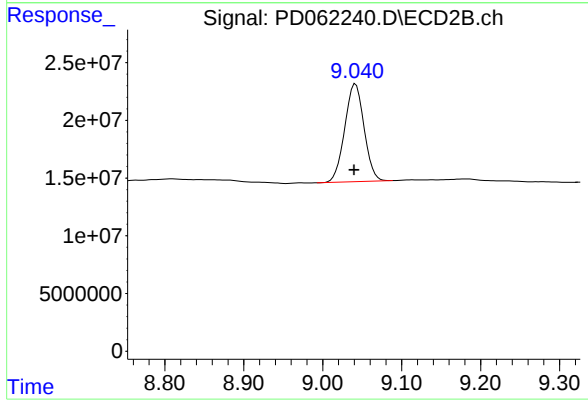

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 144543663
Conc: 15.31 ng/ml