

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 12:14
 Operator : AR\AJ
 Sample : M2099-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:50:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:01:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.979	11887495	123.5E6	14.198	14.208m
28)	SA Decachlor...	8.257	9.041	16173355	114.5E6	13.144	12.126m
Target Compounds							
12)	B 4,4'-DDE	5.653	6.314	1168988	14258818	1.040m	1.237

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 12:14
Operator : AR\AJ
Sample : M2099-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:01:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

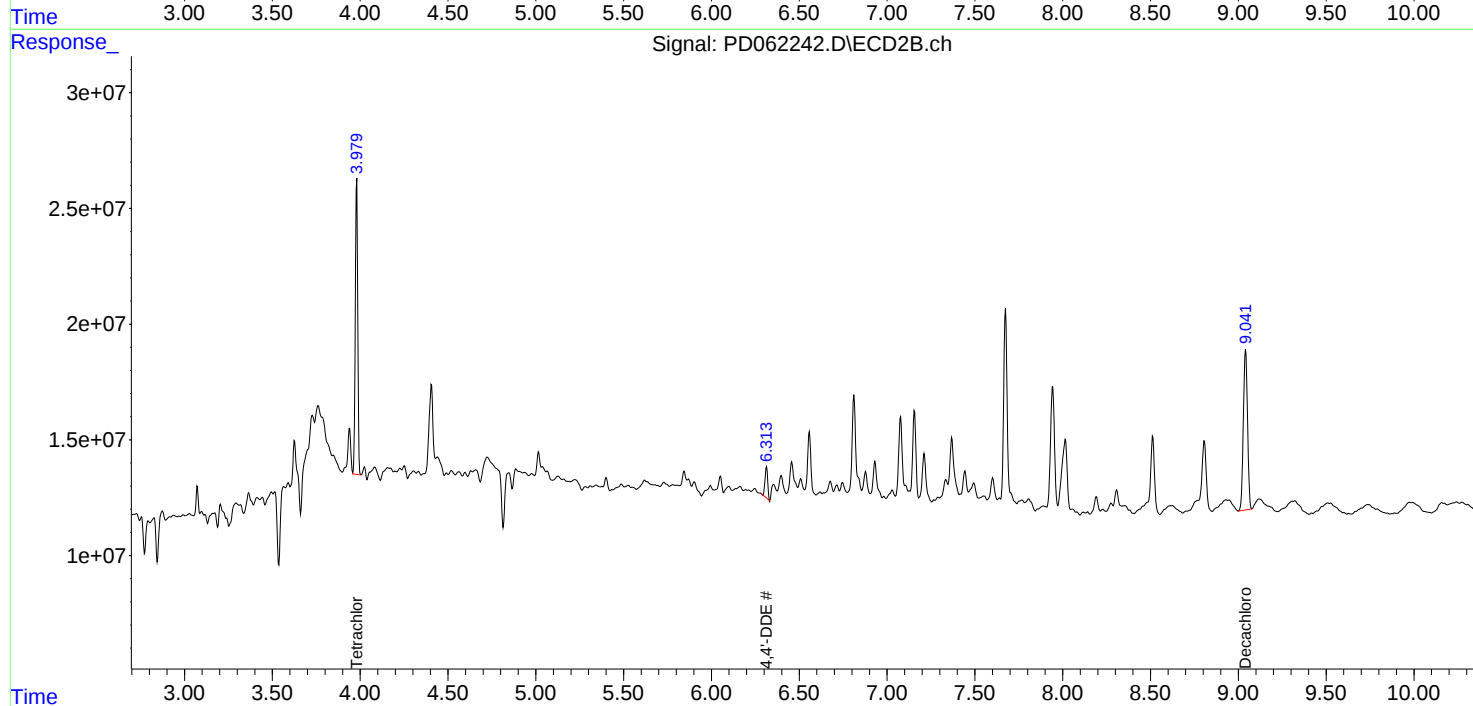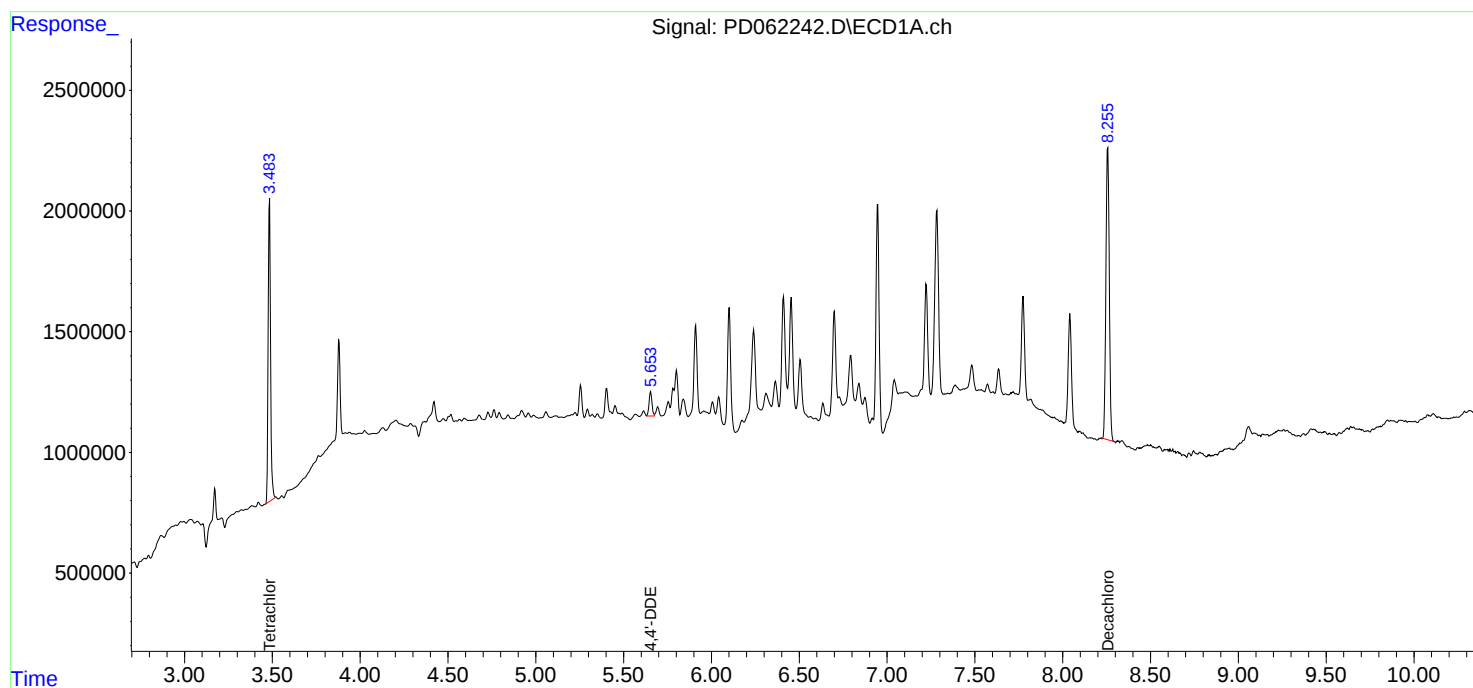

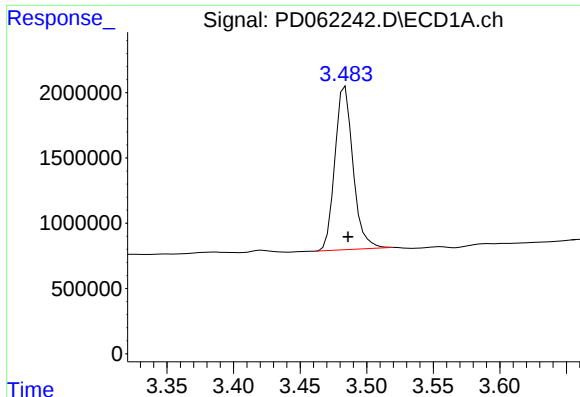


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 11887495
Conc: 14.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:35 PM

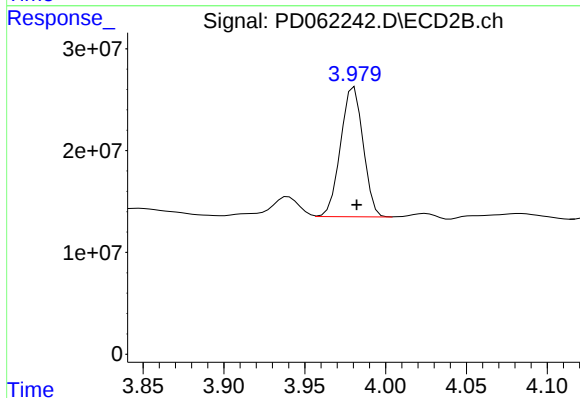


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.003 min
Response: 123452669
Conc: 14.21 ng/ml m

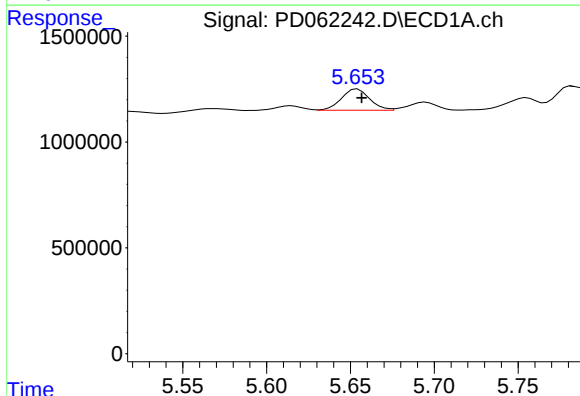


#12 4,4'-DDE

R.T.: 5.653 min
Delta R.T.: -0.004 min
Response: 1168988
Conc: 1.04 ng/ml m

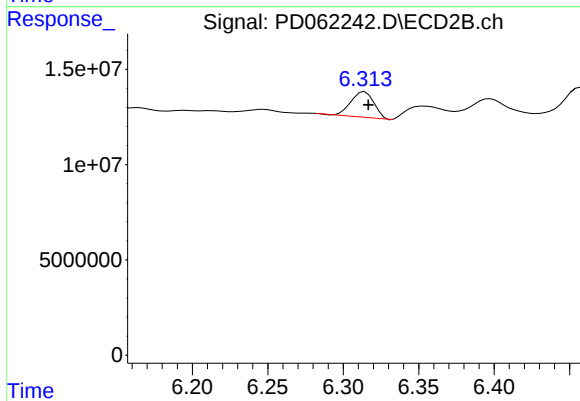

#12 4,4'-DDE

R.T.: 6.314 min
Delta R.T.: -0.002 min
Response: 14258818
Conc: 1.24 ng/ml

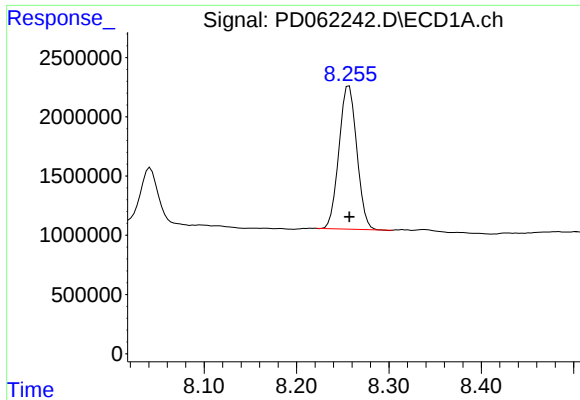


#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 16173355
Conc: 13.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:35 PM

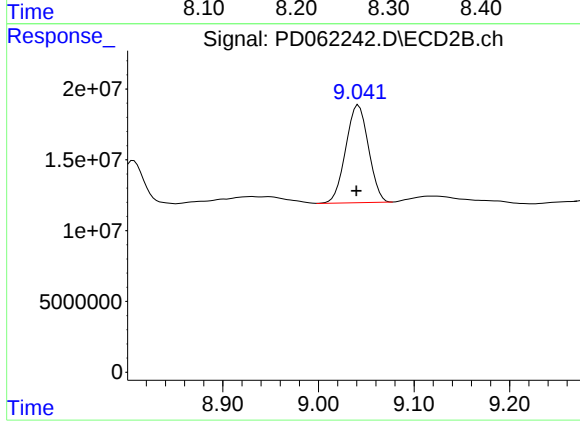

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 114475090
Conc: 12.13 ng/ml m