

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 12:42
 Operator : AR\AJ
 Sample : M2099-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Ankita
 4/23/2021 6:55:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:01:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.484	3.979	11096548	125.7E6	13.253	14.469m
28) SA Decachlor...	8.257	9.041	15783934	122.1E6	12.828	12.933
Target Compounds						
12) B 4,4'-DDE	5.653	6.314	1189601	19001178	1.059m	1.649 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 12:42
Operator : AR\AJ
Sample : M2099-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
4/23/2021 6:55:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:01:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

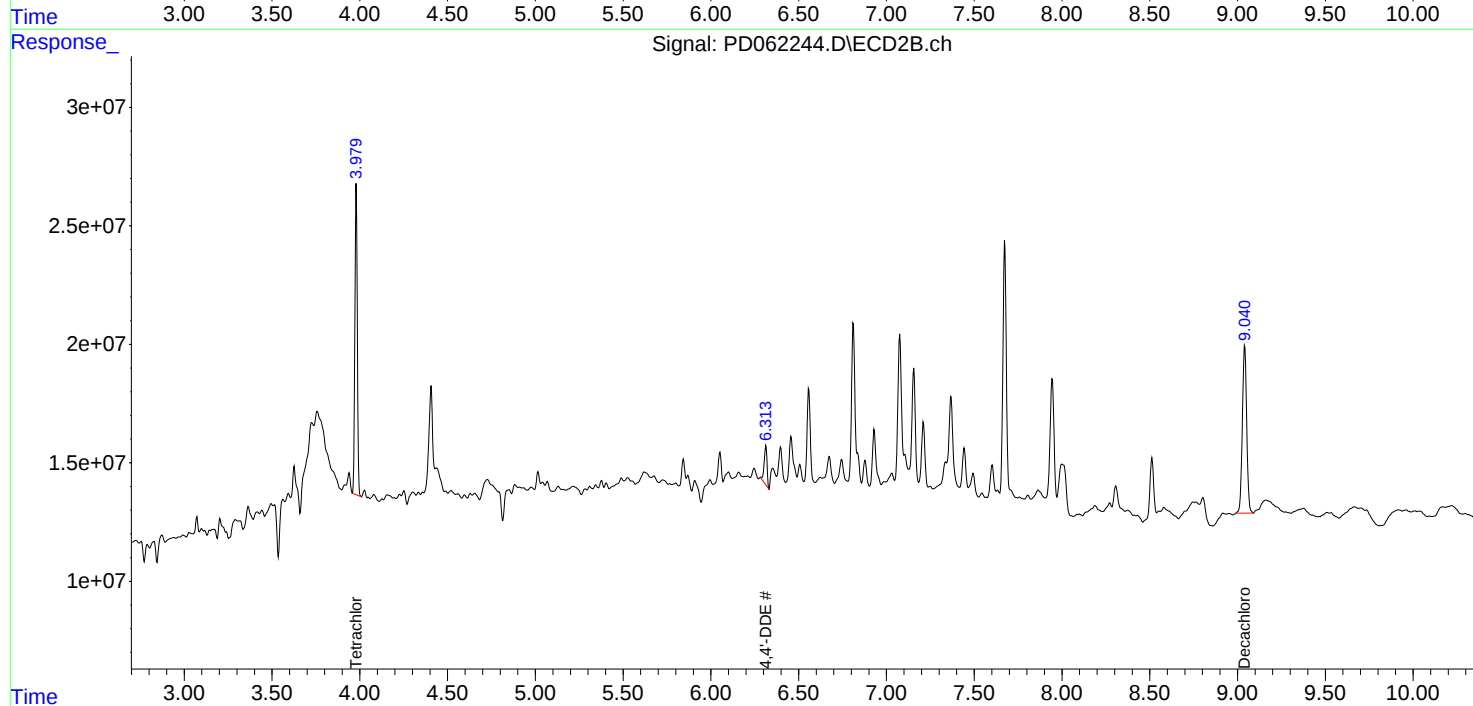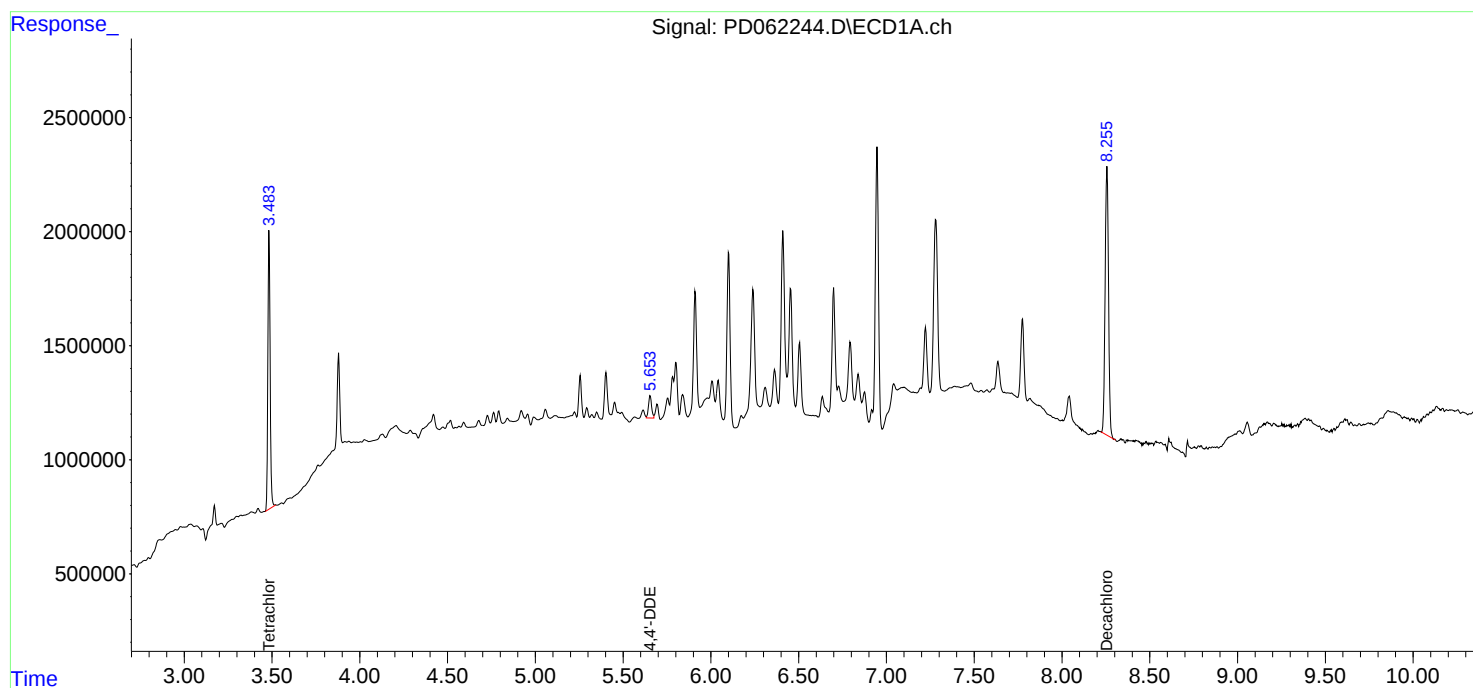

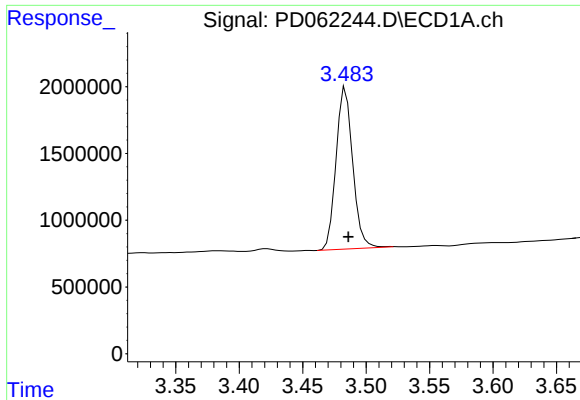


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 11096548
Conc: 13.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
4/23/2021 6:55:53 PM

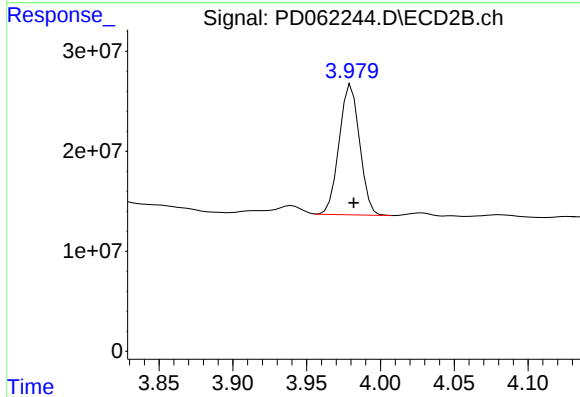


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.003 min
Response: 125720592
Conc: 14.47 ng/ml m

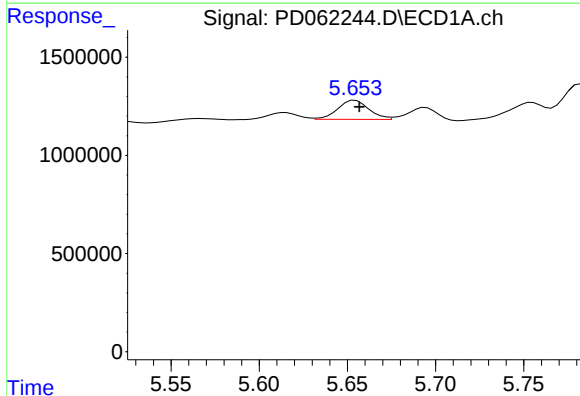


#12 4,4'-DDE

R.T.: 5.653 min
Delta R.T.: -0.004 min
Response: 1189601
Conc: 1.06 ng/ml m

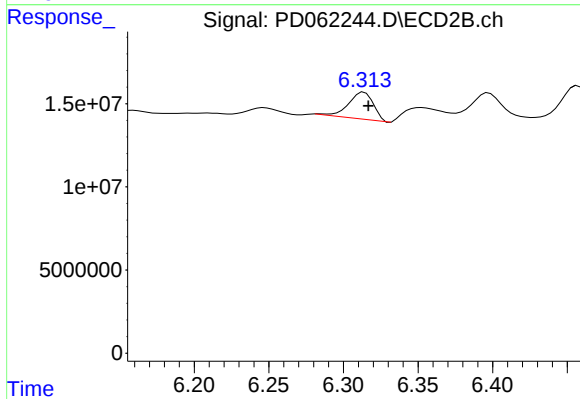

#12 4,4'-DDE

R.T.: 6.314 min
Delta R.T.: -0.003 min
Response: 19001178
Conc: 1.65 ng/ml

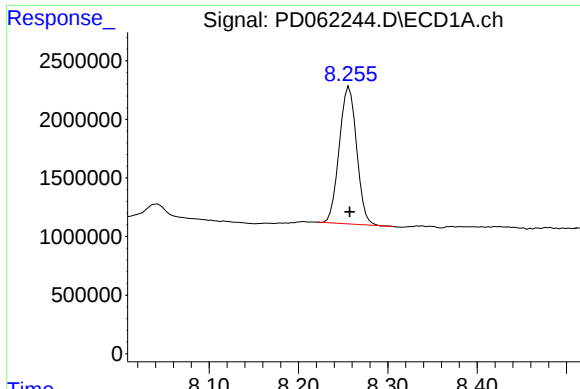


#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 15783934
Conc: 12.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3

Manual Integrations
APPROVED

Ankita
4/23/2021 6:55:53 PM

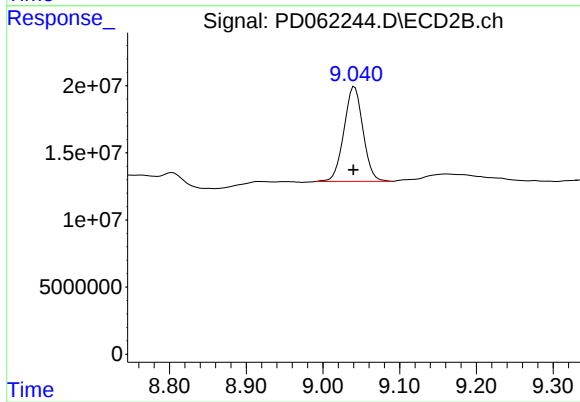

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.001 min
Response: 122092111
Conc: 12.93 ng/ml