

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
 Data File : PD062266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 18:16
 Operator : AR\AJ
 Sample : M2106-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-23-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:50:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 22:07:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.981	18940797	236.9E6	22.621	27.270
28)	SA Decachlor...	8.257	9.043	24246972	190.8E6	19.706	20.211
Target Compounds							
12)	B 4,4'-DDE	5.653	6.316	7017486	76584997	6.245m	6.646
17)	MA 4,4'-DDT	6.413	7.106	10369146	66913666	11.512	7.005 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042221\
Data File : PD062266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 18:16
Operator : AR\AJ
Sample : M2106-04
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-23-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 22:07:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

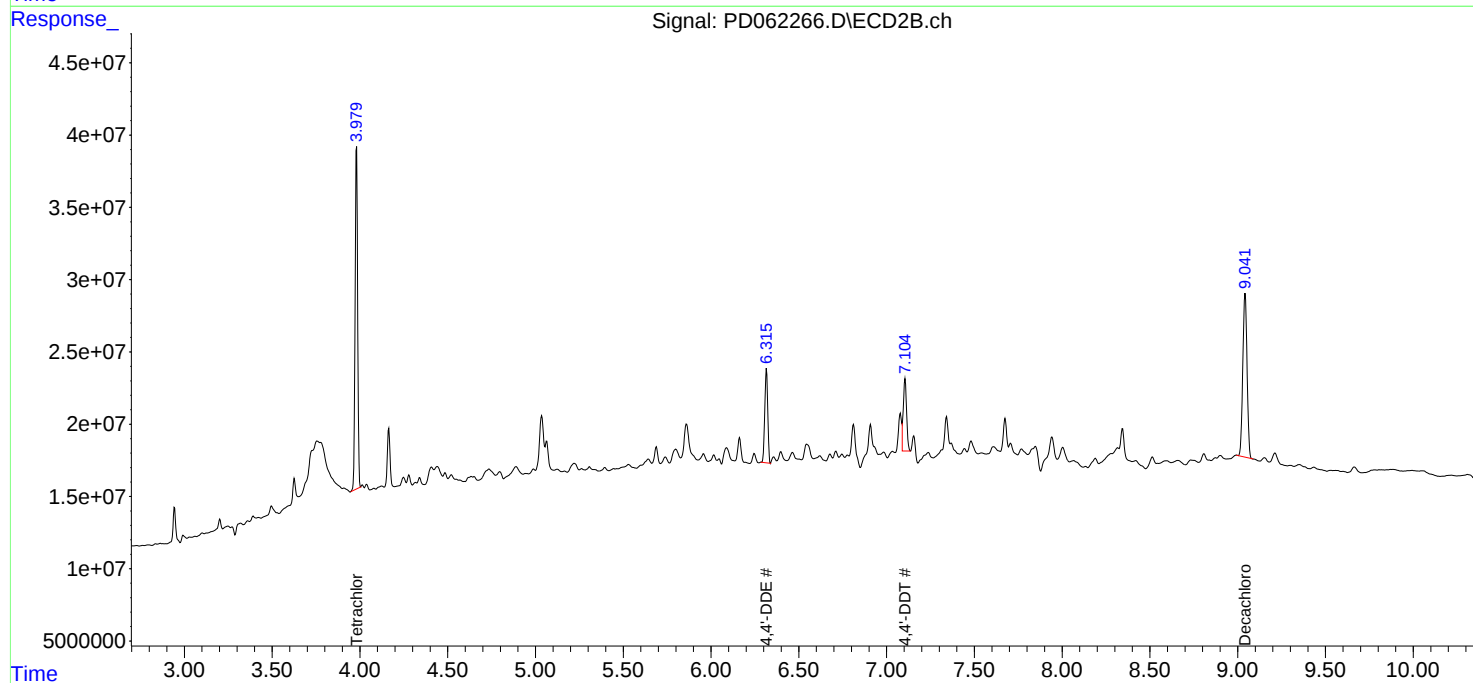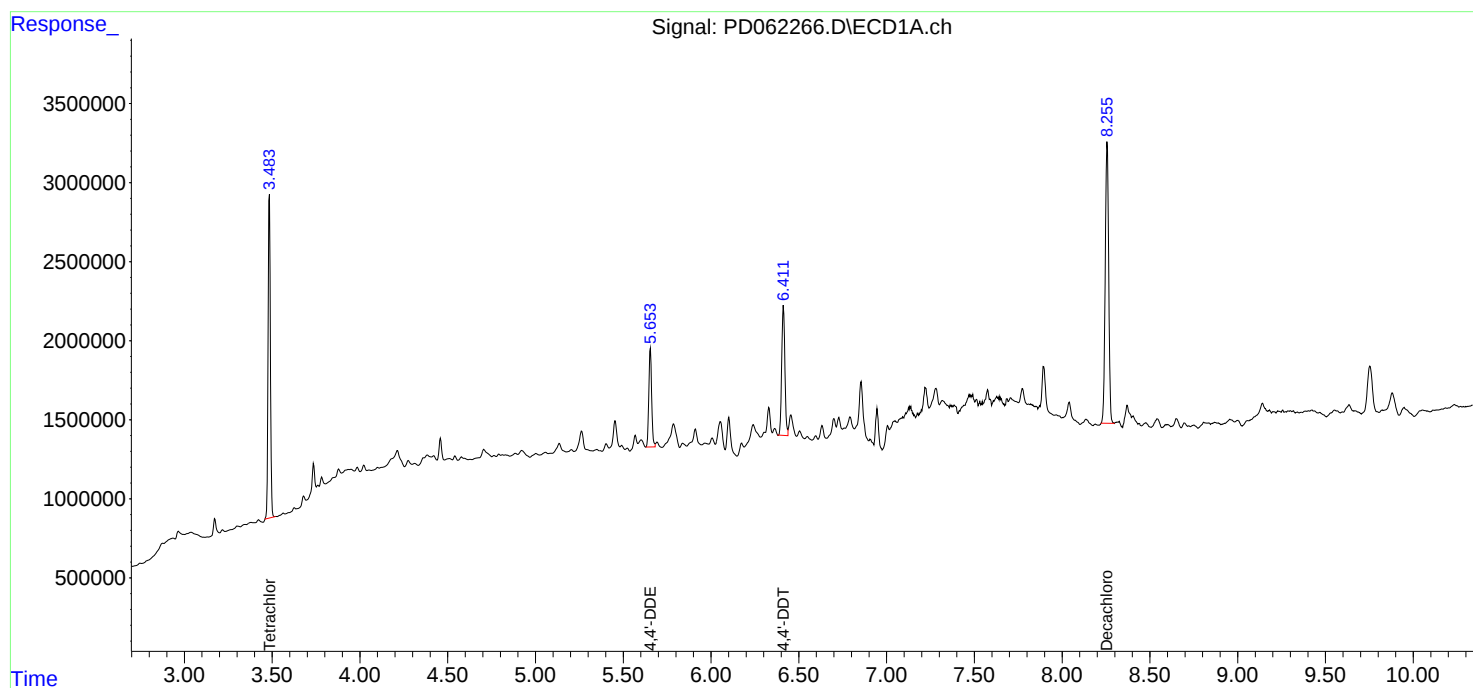

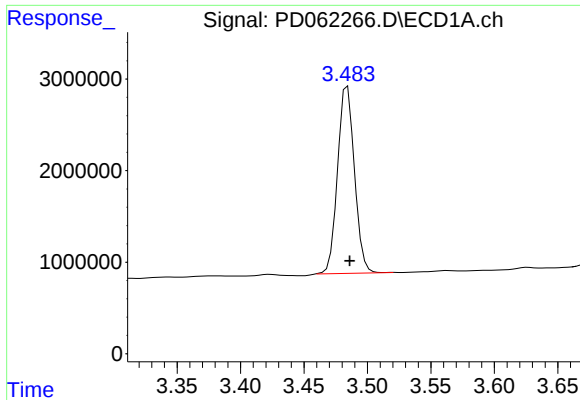


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 18940797
Conc: 22.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-23-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:48 PM

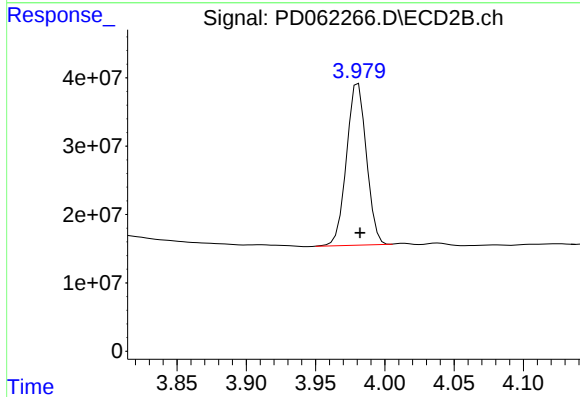


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 236947274
Conc: 27.27 ng/ml

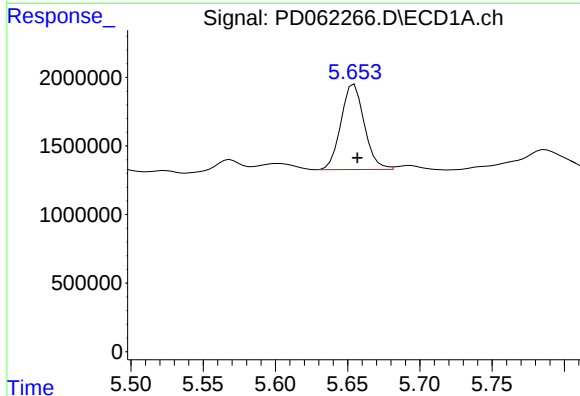


#12 4,4'-DDE

R.T.: 5.653 min
Delta R.T.: -0.004 min
Response: 7017486
Conc: 6.25 ng/ml m

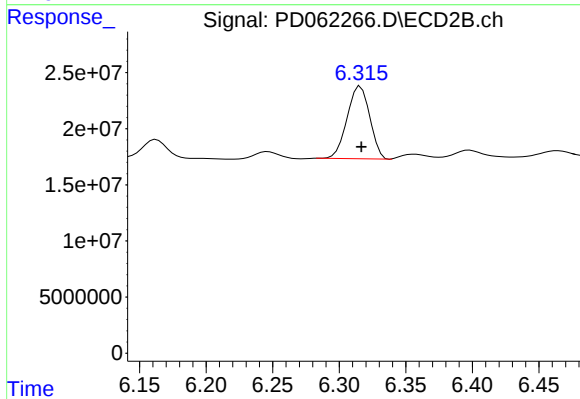

#12 4,4'-DDE

R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 76584997
Conc: 6.65 ng/ml

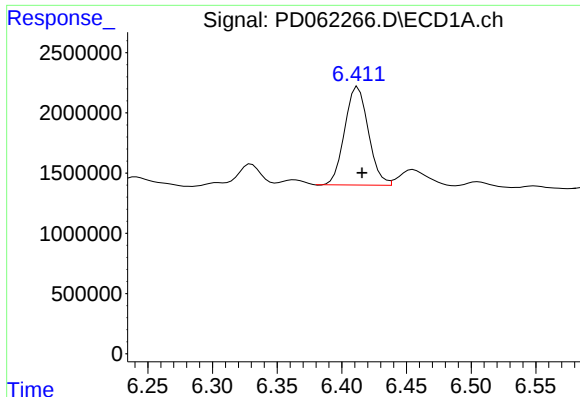


#17 4,4'-DDT

R.T.: 6.413 min
Delta R.T.: -0.003 min
Response: 10369146
Conc: 11.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-23-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:50:48 PM

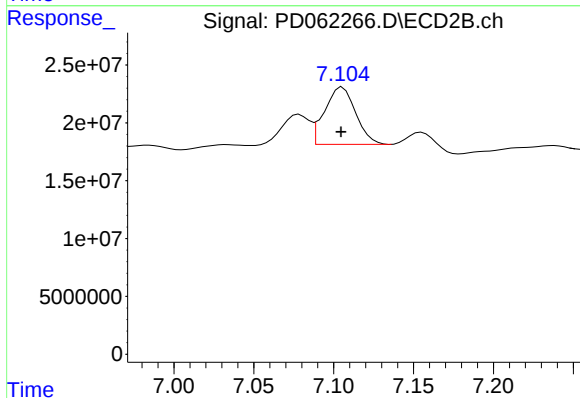


#17 4,4'-DDT

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 66913666
Conc: 7.01 ng/ml

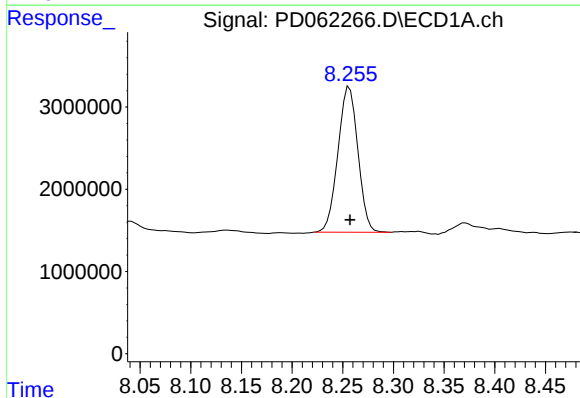

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 24246972
Conc: 19.71 ng/ml

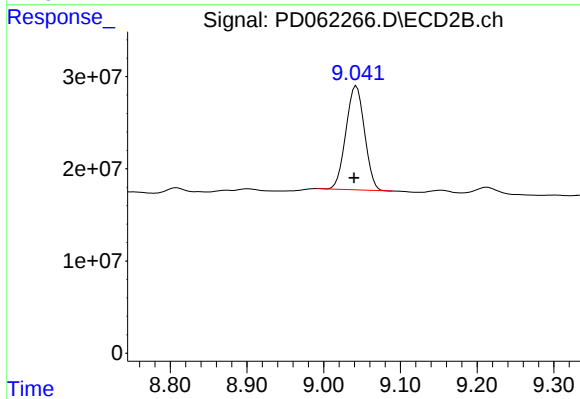

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.003 min
Response: 190800501
Conc: 20.21 ng/ml